


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX013120\  
 Data File : VX014774.D  
 Acq On : 31 Jan 2020 09:16  
 Operator : JC/SP  
 Sample : BFB  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X012220W.M  
 Title : SW846 8260  
 Last Update : Wed Jan 22 12:35:15 2020

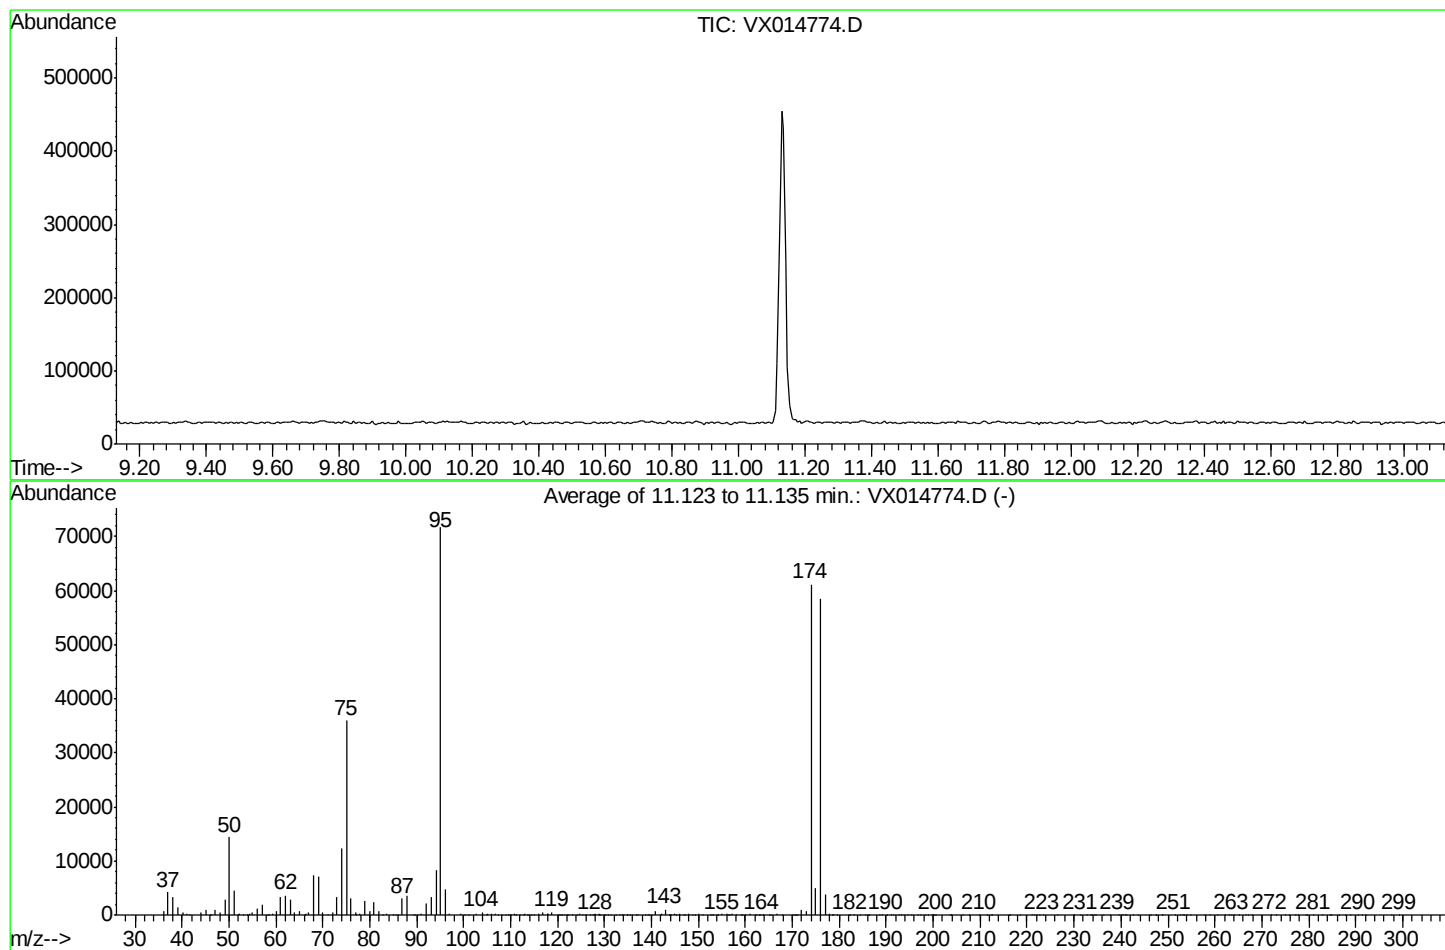

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1669

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 20.1      | 14403   | PASS             |
| 75          | 95           | 30           | 60           | 50.2      | 35964   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 71696   | PASS             |
| 96          | 95           | 5            | 9            | 6.7       | 4795    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.3       | 799     | PASS             |
| 174         | 95           | 50           | 100          | 85.3      | 61133   | PASS             |
| 175         | 174          | 5            | 9            | 8.2       | 5016    | PASS             |
| 176         | 174          | 95           | 101          | 95.8      | 58562   | PASS             |
| 177         | 176          | 5            | 9            | 6.6       | 3878    | PASS             |