

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX013122\
 Data File : VX026670.D
 Acq On : 31 Jan 2022 11:09
 Operator : JC/MD
 Sample : VX0131MBL01
 Misc : 5.0g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0131MBL01

Quant Time: Jan 31 13:56:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 11 14:45:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	134090	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	222986	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	203596	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	88655	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	83666	44.666	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	89.340%
35) Dibromofluoromethane	5.385	113	69624	48.351	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	96.700%
50) Toluene-d8	8.647	98	262246	50.538	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	101.080%
62) 4-Bromofluorobenzene	11.079	95	97278	52.773	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	105.540%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX013122\
Data File : VX026670.D
Acq On : 31 Jan 2022 11:09
Operator : JC/MD
Sample : VX0131MBL01
Misc : 5.0g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0131MBL01

Quant Time: Jan 31 13:56:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 11 14:45:13 2022
Response via : Initial Calibration




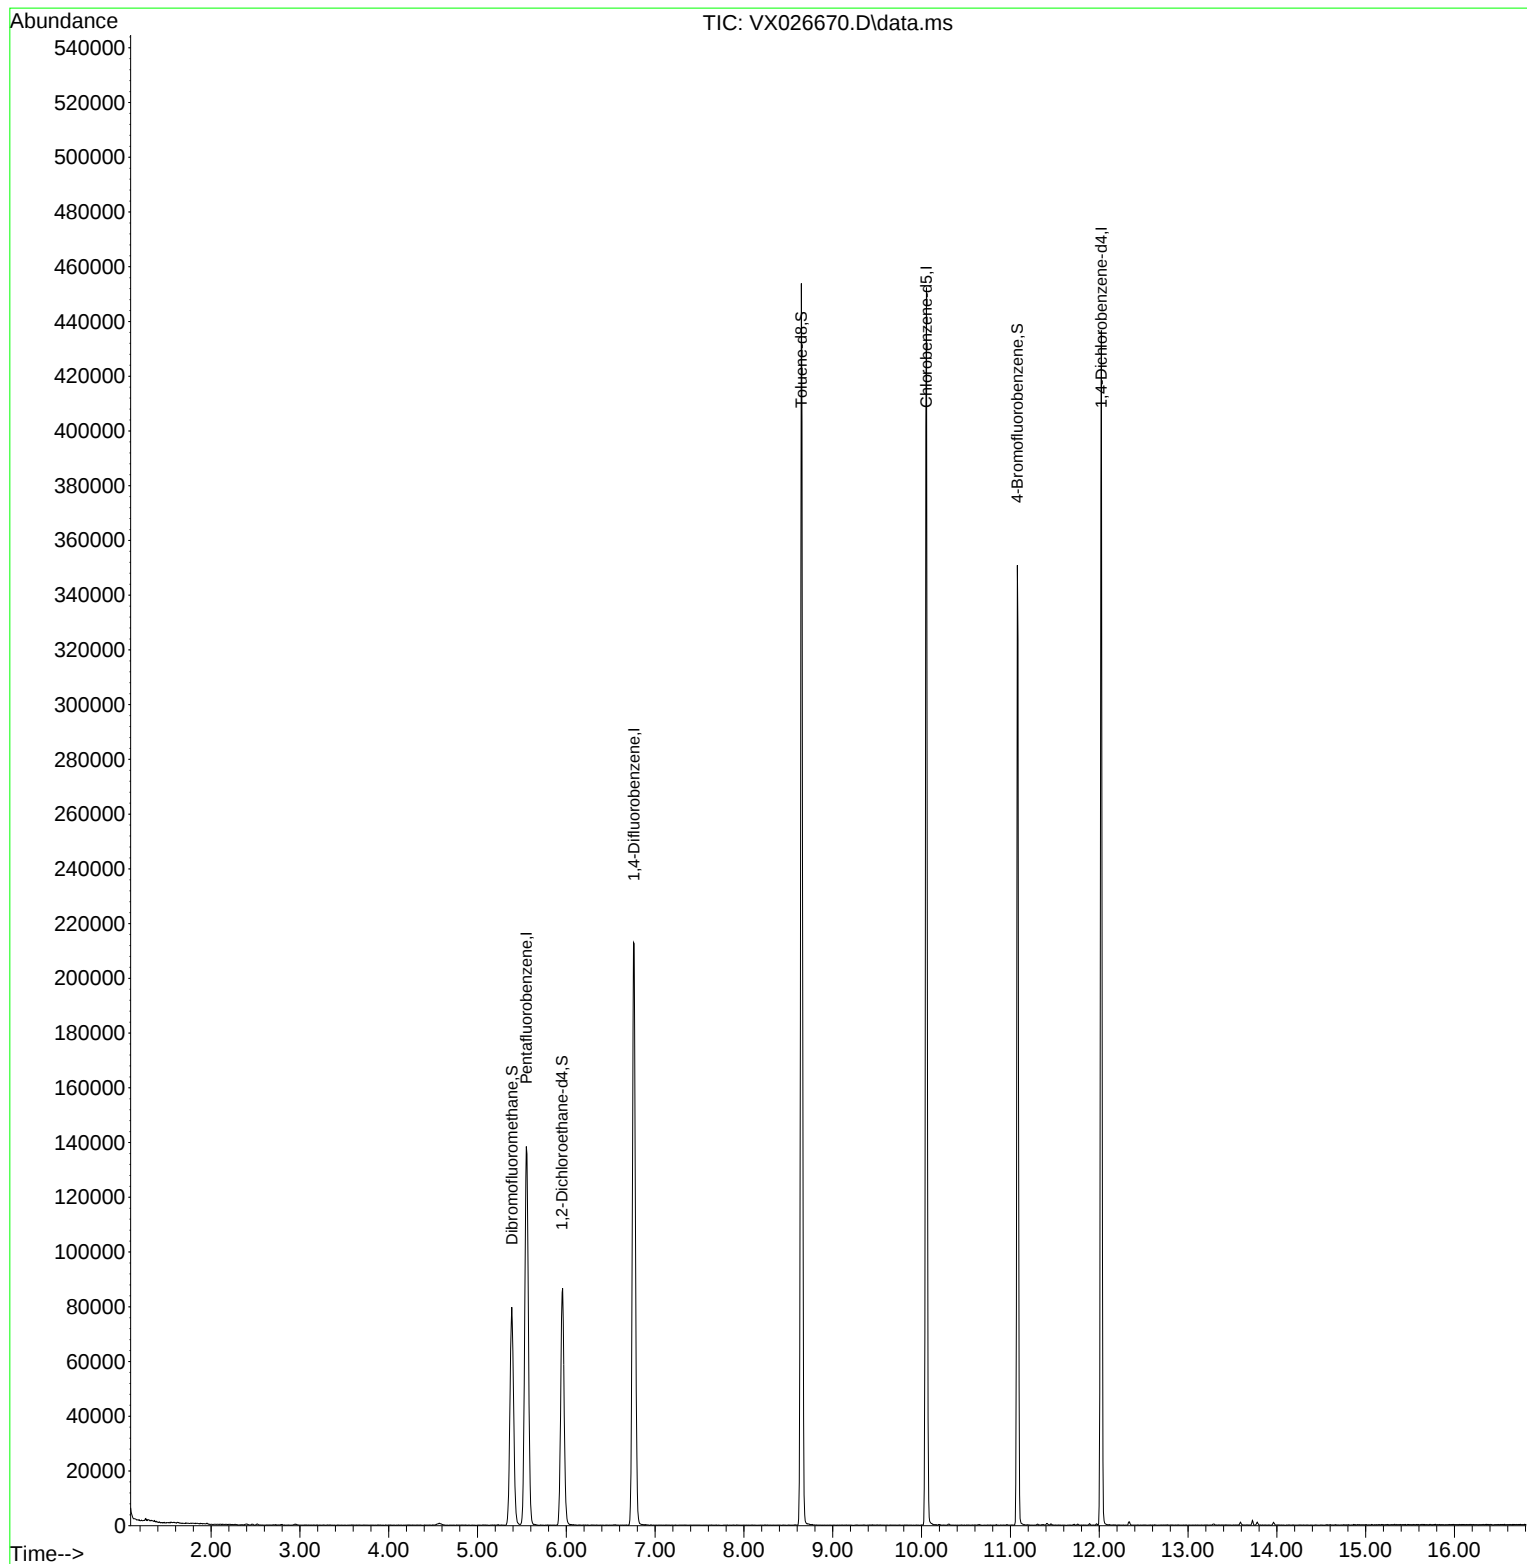


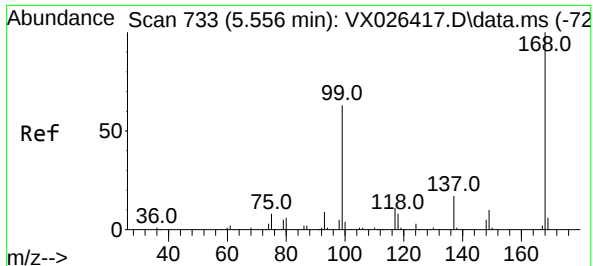

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 713
Delta R.T. -0.006 min
Lab File: VX026670.D
Acq: 31 Jan 2022 11:09




Instrument :
MSVOA_X
ClientSampleId :
VX0131MBL01


Tgt Ion:168 Resp: 134090
Ion Ratio Lower Upper
168 100
99 61.1 50.3 75.5

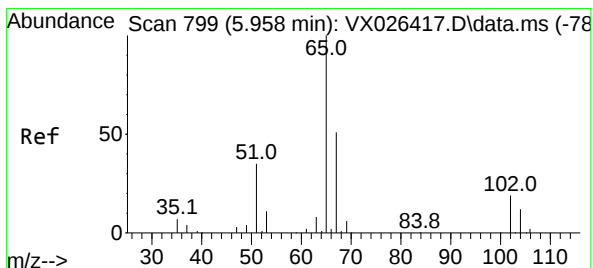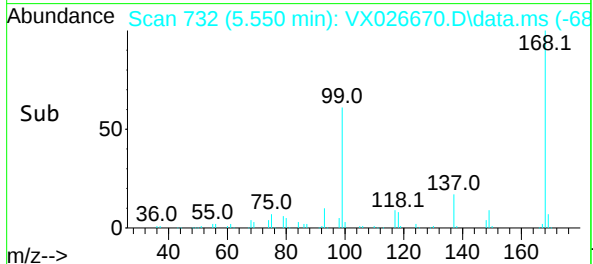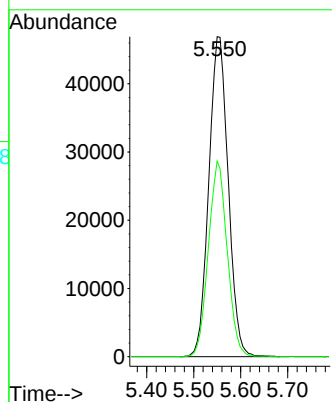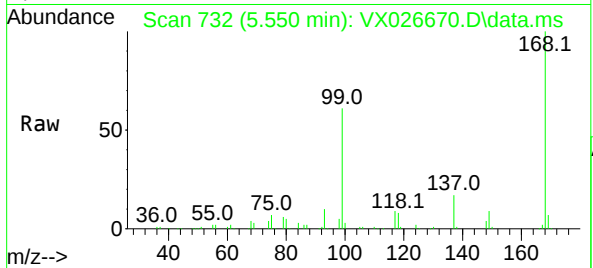

#33
1,2-Dichloroethane-d4
Concen: 44.666 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX026670.D
Acq: 31 Jan 2022 11:09

Tgt Ion: 65 Resp: 83666
Ion Ratio Lower Upper
65 100
67 52.1 0.0 100.8


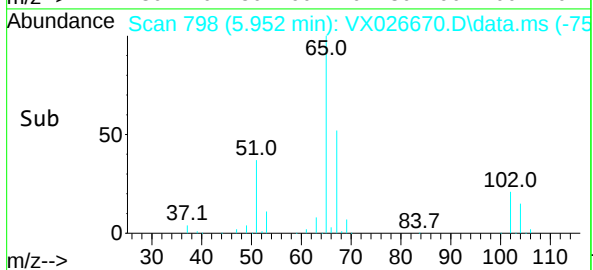
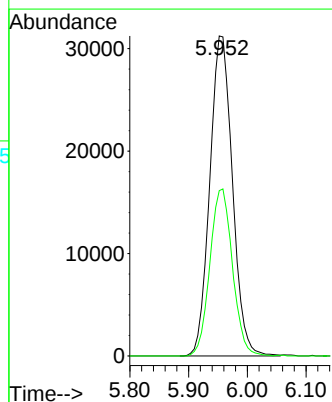
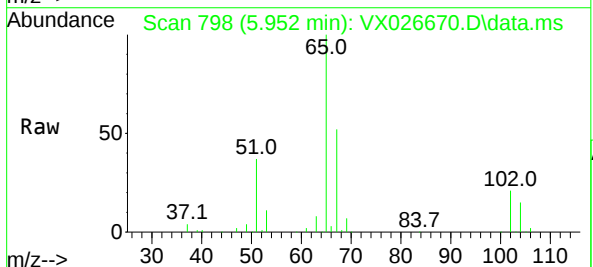


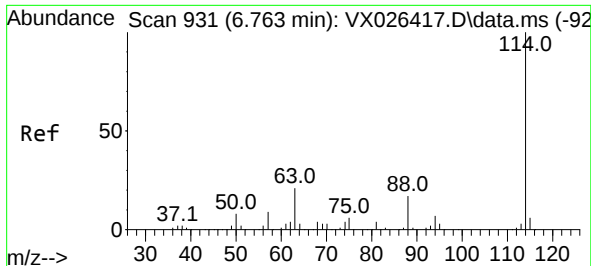

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX026670.D
Acq: 31 Jan 2022 11:09




Instrument :
MSVOA_X
ClientSampleId :
VX0131MBL01


Tgt Ion:114 Resp: 222986
Ion Ratio Lower Upper
114 100
63 21.0 0.0 42.8
88 16.2 0.0 33.0

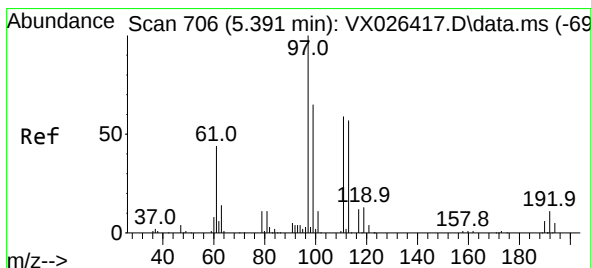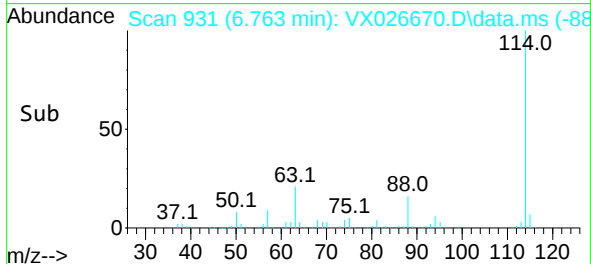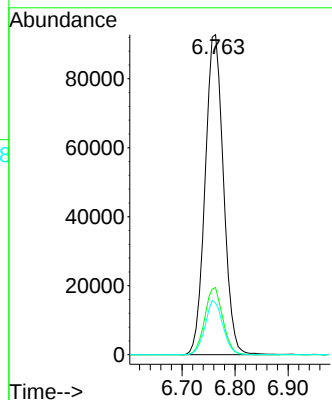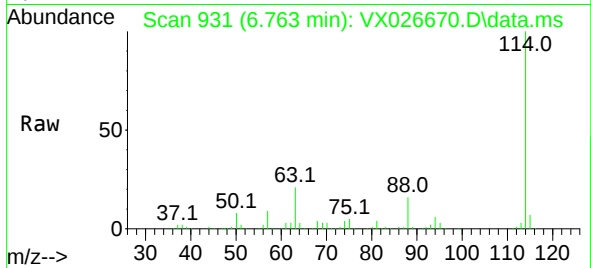

#35
Dibromofluoromethane
Concen: 48.351 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.006 min
Lab File: VX026670.D
Acq: 31 Jan 2022 11:09

Tgt Ion:113 Resp: 69624
Ion Ratio Lower Upper
113 100
111 102.7 81.2 121.8
192 19.7 15.0 22.4


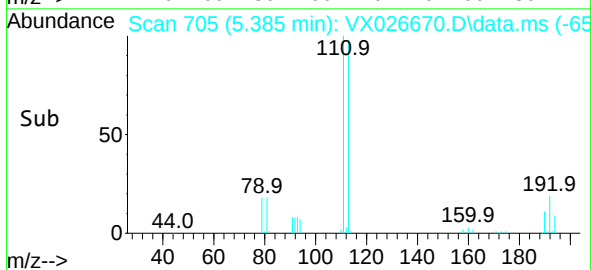
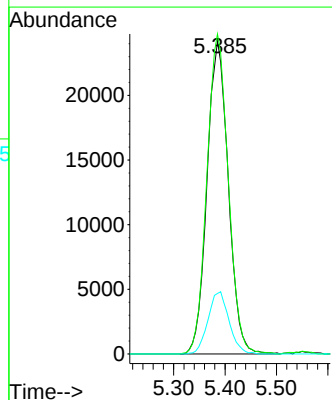
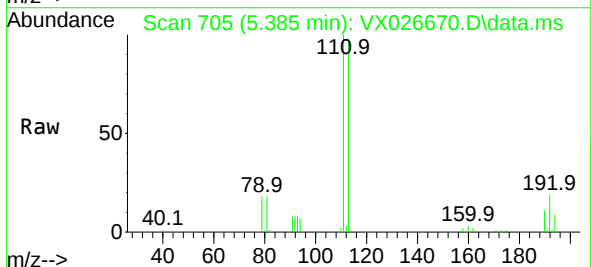


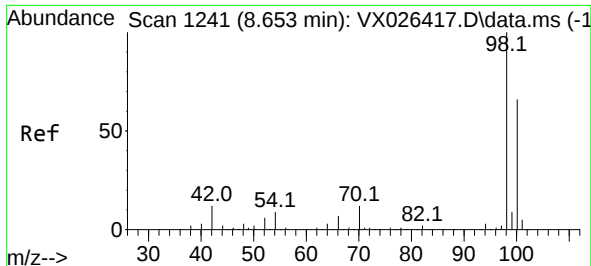

#50
Toluene-d8
Concen: 50.538 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX026670.D
Acq: 31 Jan 2022 11:09




Instrument :
MSVOA_X
ClientSampleId :
VX0131MBL01


Tgt Ion: 98 Resp: 262246
Ion Ratio Lower Upper
98 100
100 66.5 53.2 79.8

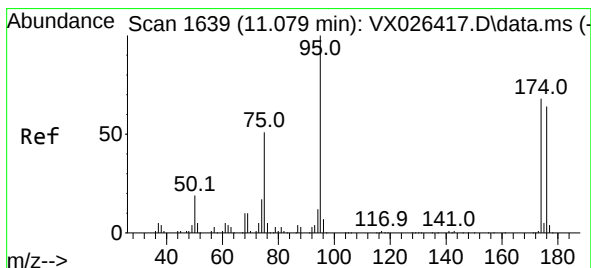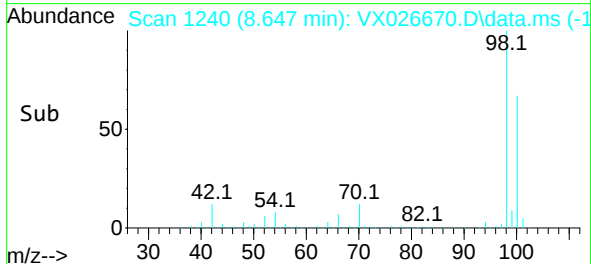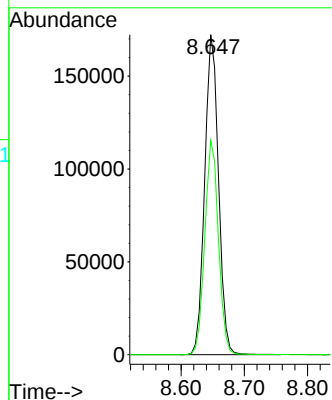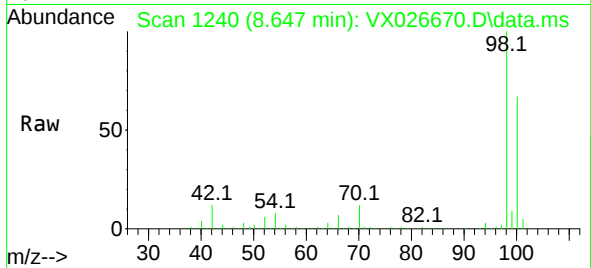

#62
4-Bromofluorobenzene
Concen: 52.773 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX026670.D
Acq: 31 Jan 2022 11:09

Tgt Ion: 95 Resp: 97278
Ion Ratio Lower Upper
95 100
174 75.0 0.0 148.6
176 73.3 0.0 141.4


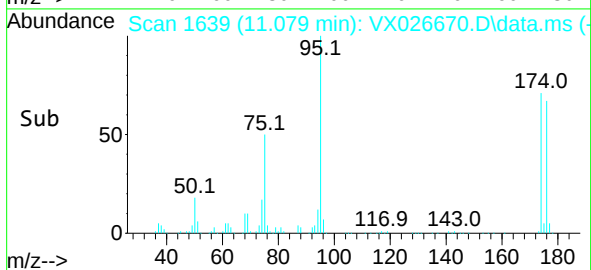
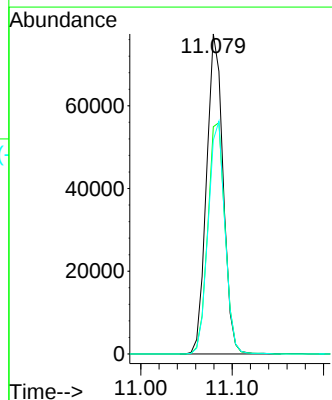
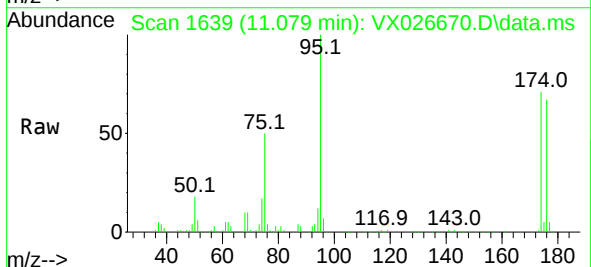


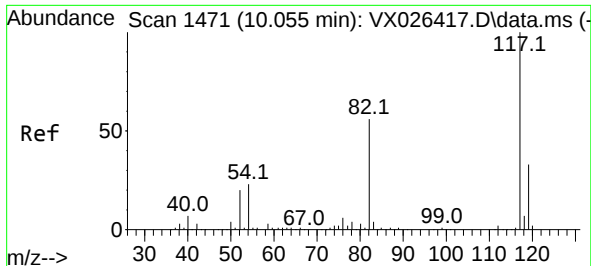

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX026670.D
Acq: 31 Jan 2022 11:09

Instrument :
MSVOA_X
ClientSampleId :
VX0131MBL01

Tgt Ion:117 Resp: 203596
Ion Ratio Lower Upper
117 100
82 55.3 45.2 67.8
119 31.9 26.2 39.2

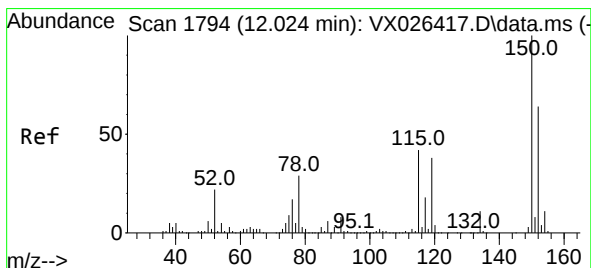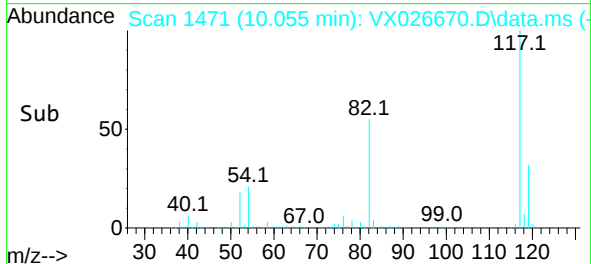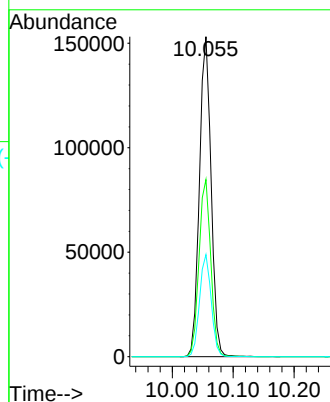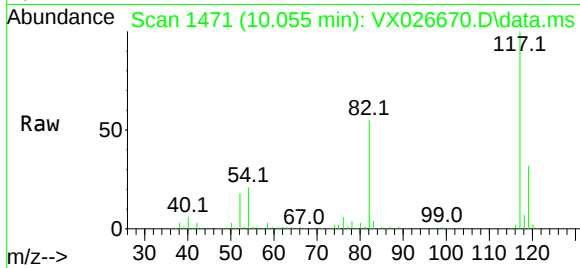

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX026670.D
Acq: 31 Jan 2022 11:09

Tgt Ion:152 Resp: 88655
Ion Ratio Lower Upper
152 100
115 59.6 44.2 132.6
150 155.9 0.0 348.2

