

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX013122\
 Data File : VX026694.D
 Acq On : 31 Jan 2022 20:30
 Operator : JC/MD
 Sample : N1335-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MH-4D

Quant Time: Feb 01 06:32:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 11 14:45:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	123497	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	209909	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	194412	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	86883	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	80522	46.675	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	93.360%
35) Dibromofluoromethane	5.391	113	65530	48.343	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	96.680%
50) Toluene-d8	8.653	98	250427	51.267	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	102.540%
62) 4-Bromofluorobenzene	11.079	95	93153	53.683	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	107.360%
Target Compounds						
					Qvalue	
16) Acetone	2.386	43	12616	14.340	ug/l	95
20) Methylene Chloride	2.794	84	1562	1.075	ug/l	90
43) Isopropyl Acetate	6.342	43	11416	3.265	ug/l	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX013122\
Data File : VX026694.D
Acq On : 31 Jan 2022 20:30
Operator : JC/MD
Sample : N1335-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MH-4D

Quant Time: Feb 01 06:32:08 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 11 14:45:13 2022
Response via : Initial Calibration




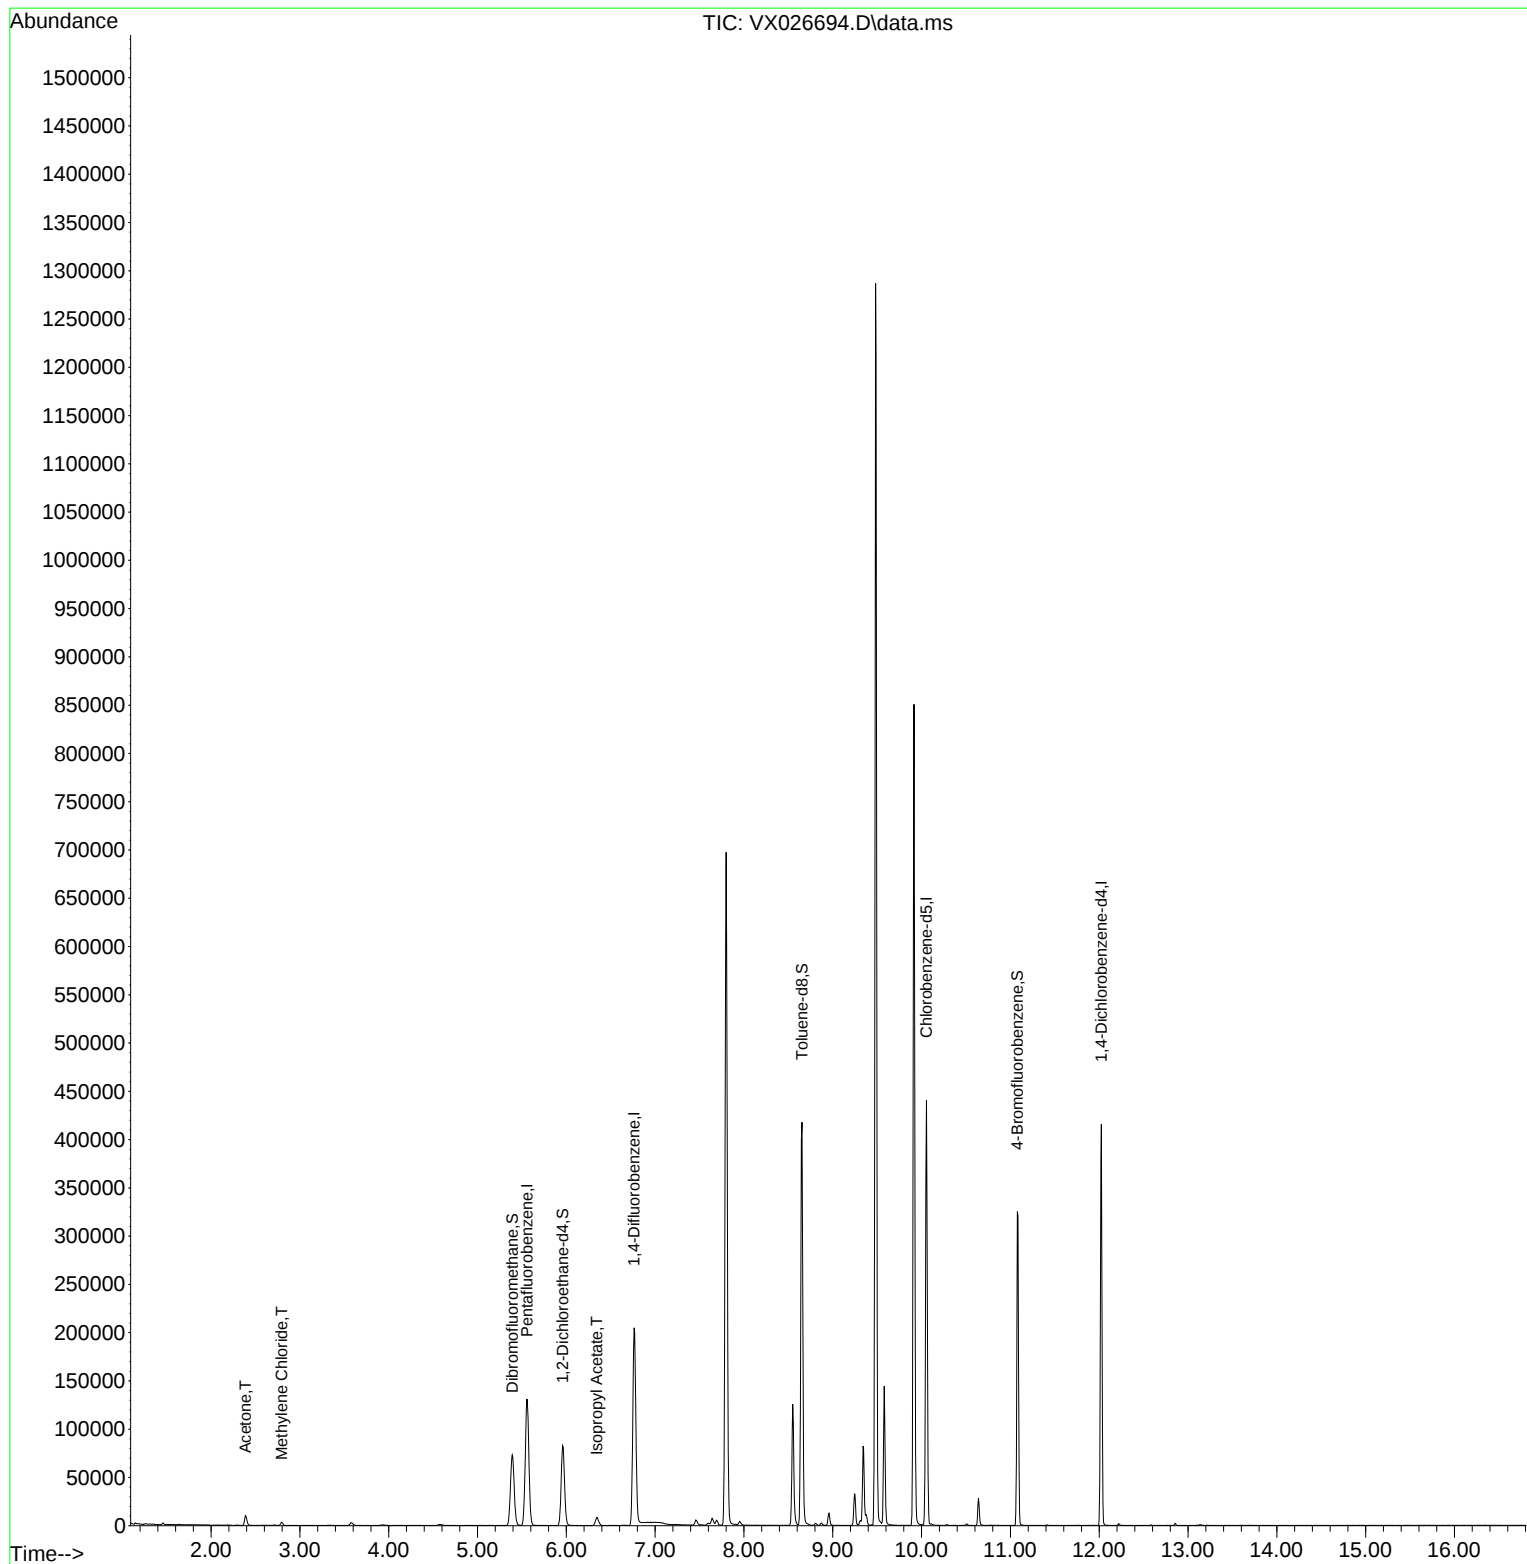




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX026694.D
Acq: 31 Jan 2022 20:30




Instrument :
MSVOA_X
ClientSampleId :
MH-4D


Tgt Ion:168 Resp: 123497
Ion Ratio Lower Upper
168 100
99 61.0 50.3 75.5

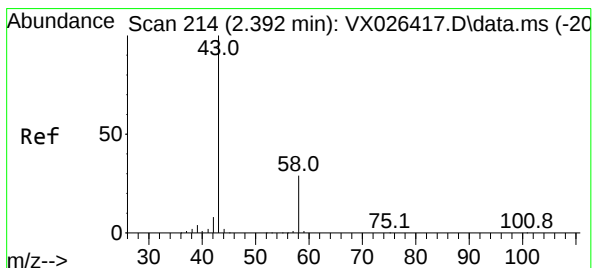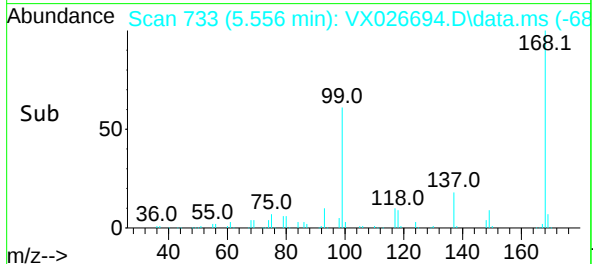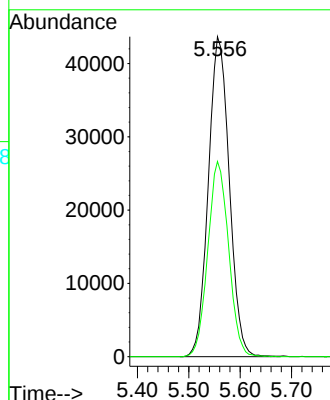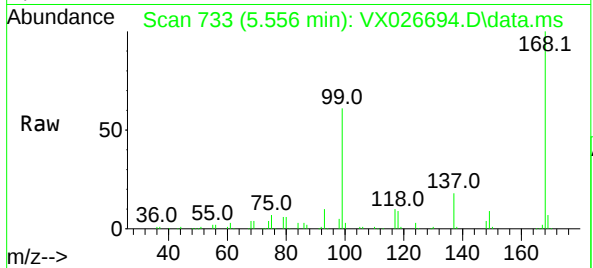

#16
Acetone
Concen: 14.340 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX026694.D
Acq: 31 Jan 2022 20:30

Tgt Ion: 43 Resp: 12616
Ion Ratio Lower Upper
43 100
58 31.4 23.0 34.6

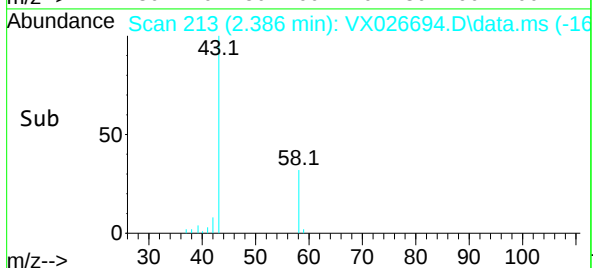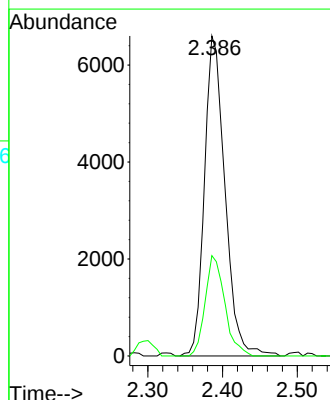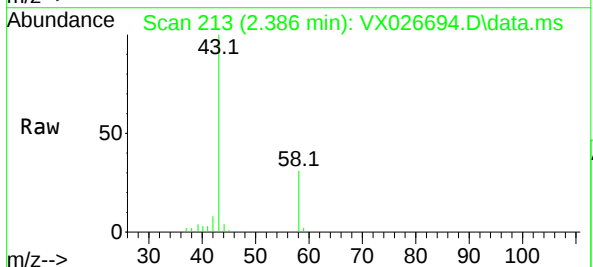




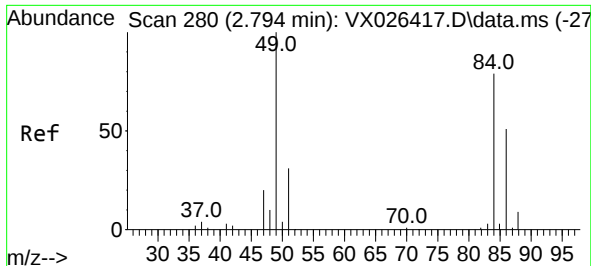


#20
Methylene Chloride
Concen: 1.075 ug/l
RT: 2.794 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX026694.D
Acq: 31 Jan 2022 20:30

Instrument :
MSVOA_X
ClientSampleId :
MH-4D

Tgt Ion: 84 Resp: 1562




Ion	Ratio	Lower	Upper
84	100		
49	108.6	101.5	152.3
51	36.3	31.2	46.8
86	63.6	51.3	76.9

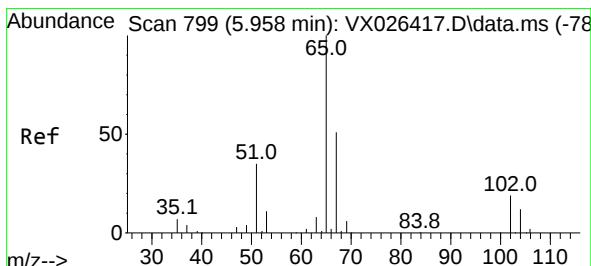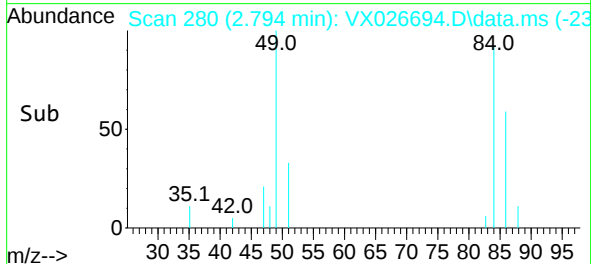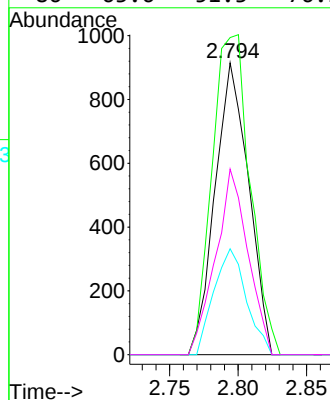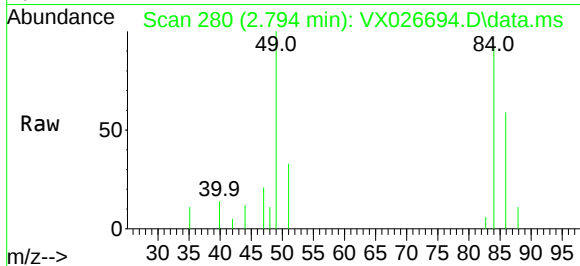


#33
1,2-Dichloroethane-d4
Concen: 46.675 ug/l
RT: 5.958 min Scan# 799
Delta R.T. -0.000 min
Lab File: VX026694.D
Acq: 31 Jan 2022 20:30

Tgt Ion: 65 Resp: 80522

Ion	Ratio	Lower	Upper
65	100		
67	51.8	0.0	100.8


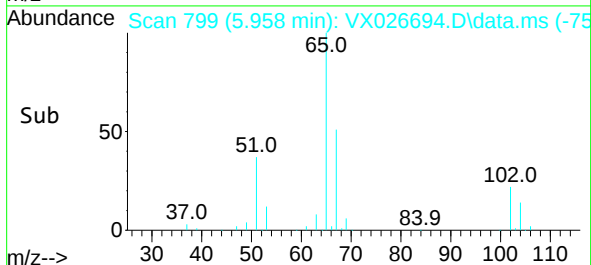
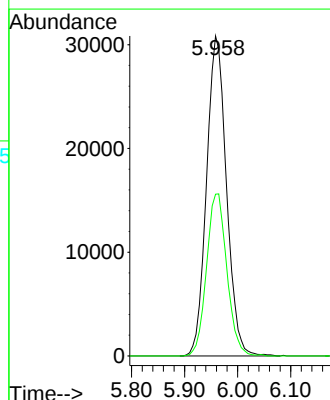
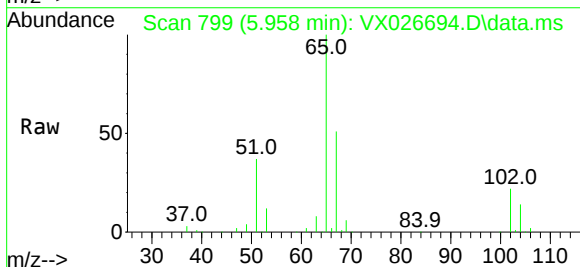


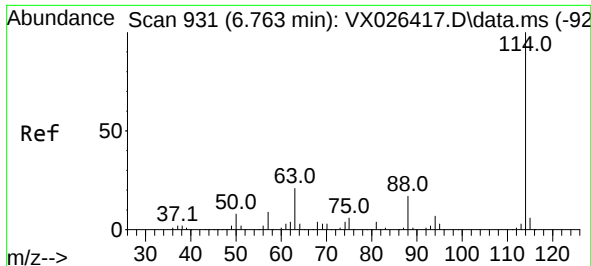

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX026694.D
Acq: 31 Jan 2022 20:30




Instrument :
MSVOA_X
ClientSampleId :
MH-4D


Tgt Ion:114 Resp: 209909
Ion Ratio Lower Upper
114 100
63 21.5 0.0 42.8
88 16.4 0.0 33.0

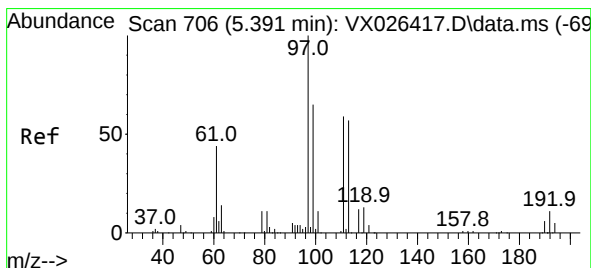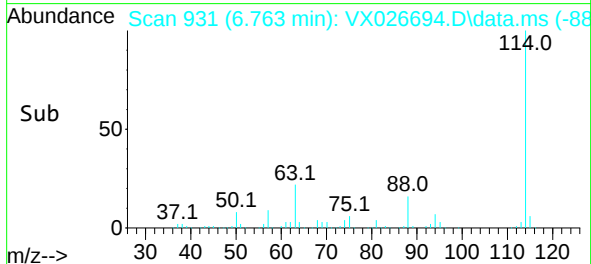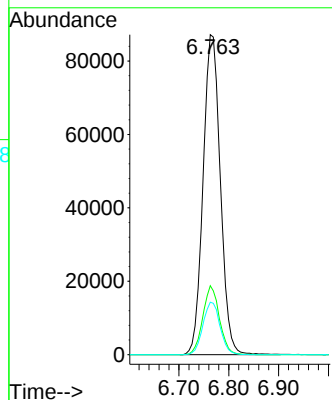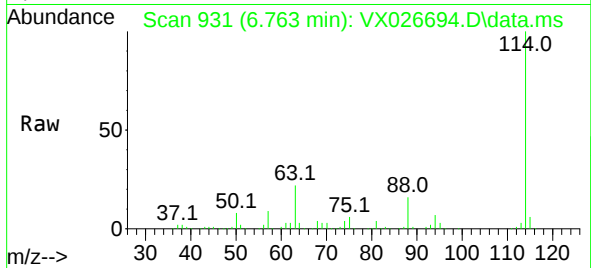

#35
Dibromofluoromethane
Concen: 48.343 ug/l
RT: 5.391 min Scan# 706
Delta R.T. -0.000 min
Lab File: VX026694.D
Acq: 31 Jan 2022 20:30

Tgt Ion:113 Resp: 65530
Ion Ratio Lower Upper
113 100
111 102.6 81.2 121.8
192 19.0 15.0 22.4


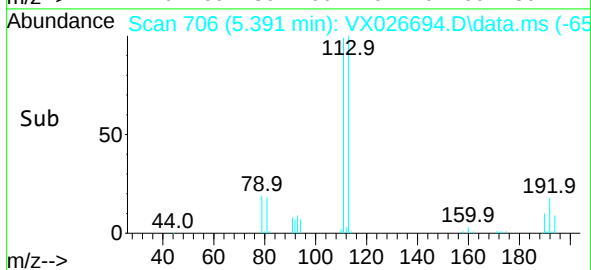
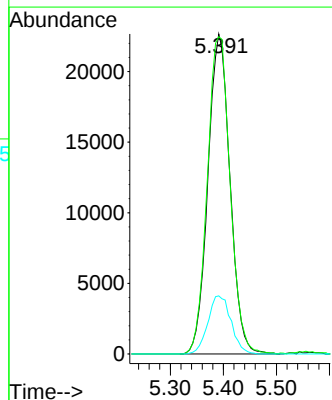
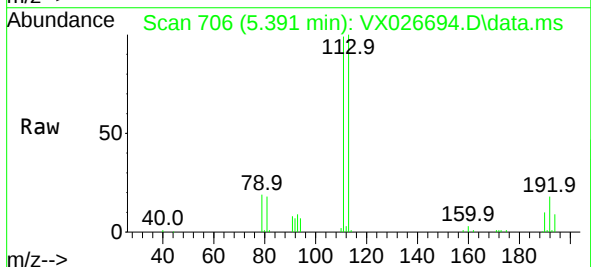


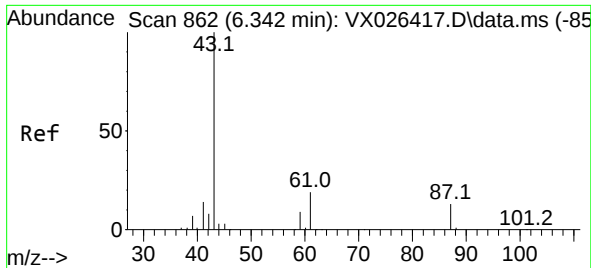

#43
Isopropyl Acetate
Concen: 3.265 ug/l
RT: 6.342 min Scan# 862
Delta R.T. -0.000 min
Lab File: VX026694.D
Acq: 31 Jan 2022 20:30




Instrument :
MSVOA_X
ClientSampleId :
MH-4D


Tgt Ion: 43 Resp: 11416
Ion Ratio Lower Upper
43 100
61 20.6 15.4 23.0
87 12.6 10.2 15.2

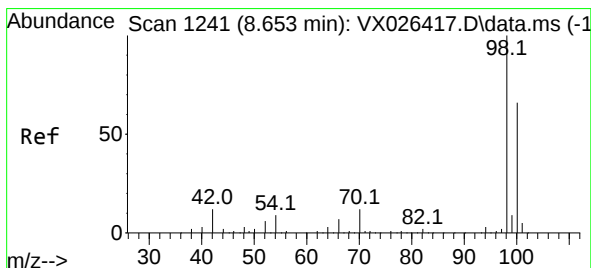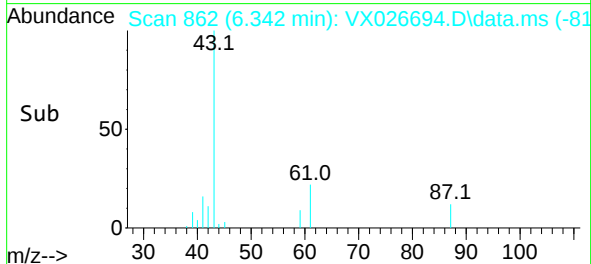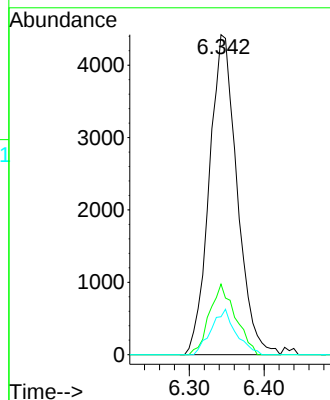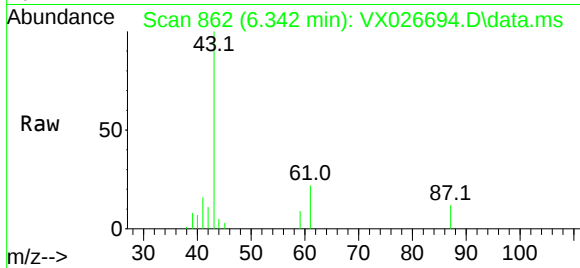

#50
Toluene-d8
Concen: 51.267 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX026694.D
Acq: 31 Jan 2022 20:30

Tgt Ion: 98 Resp: 250427
Ion Ratio Lower Upper
98 100
100 65.6 53.2 79.8


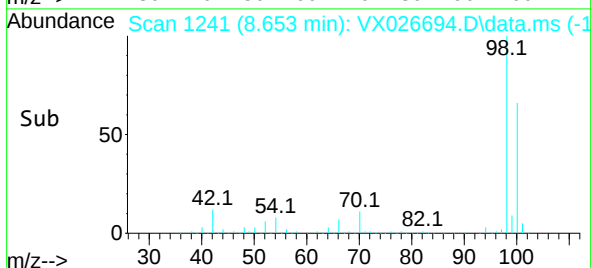
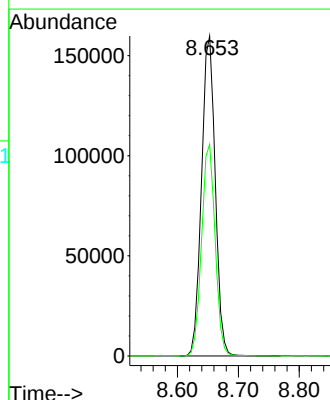
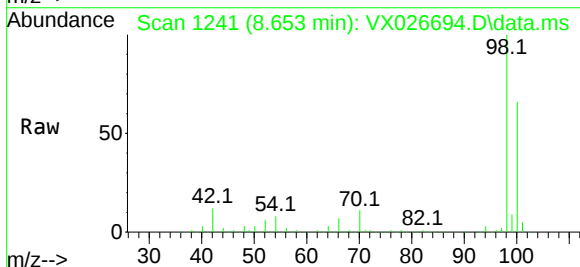


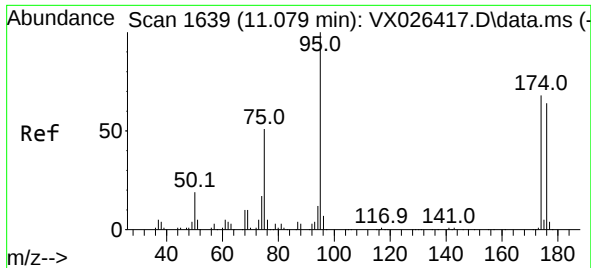

#62
4-Bromofluorobenzene
Concen: 53.683 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX026694.D
Acq: 31 Jan 2022 20:30




Instrument :
MSVOA_X
ClientSampleId :
MH-4D


Tgt Ion: 95 Resp: 93153
Ion Ratio Lower Upper
95 100
174 75.1 0.0 148.6
176 73.1 0.0 141.4

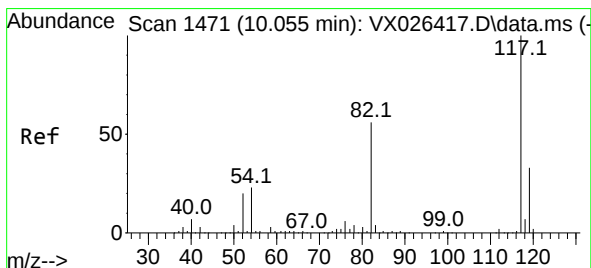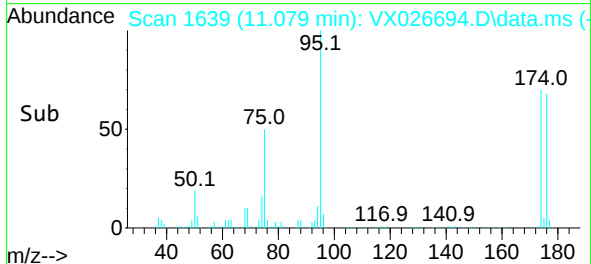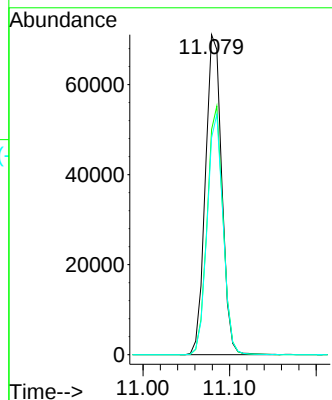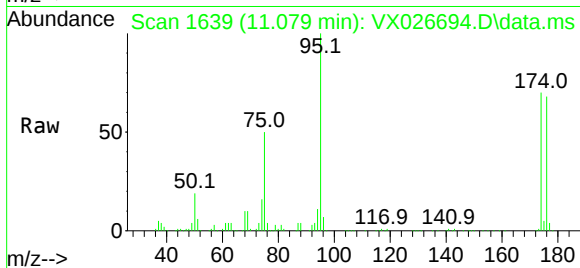

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX026694.D
Acq: 31 Jan 2022 20:30

Tgt Ion: 117 Resp: 194412
Ion Ratio Lower Upper
117 100
82 56.1 45.2 67.8
119 31.9 26.2 39.2

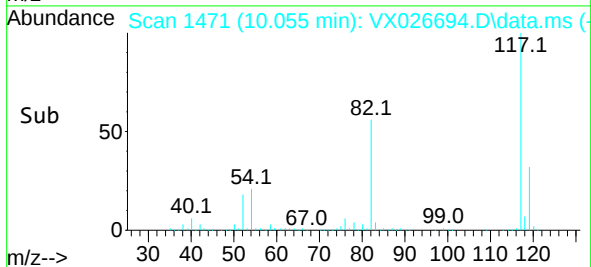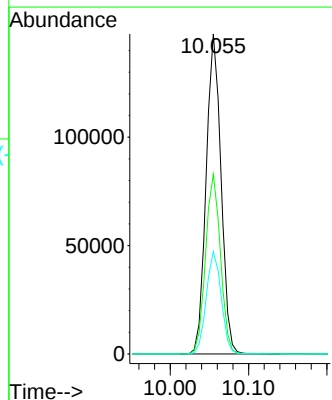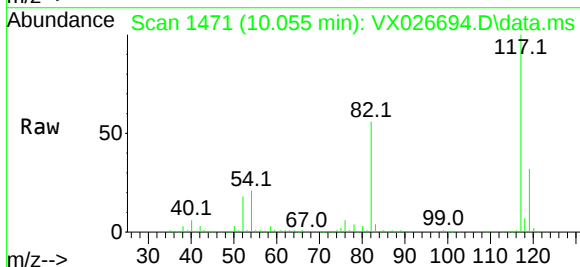

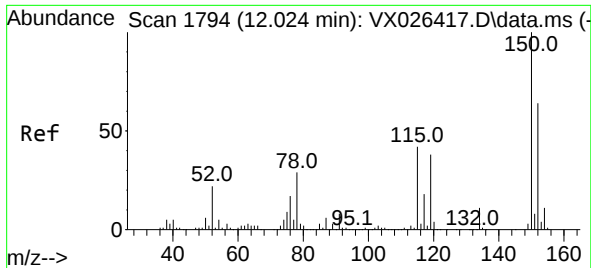

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: VX026694.D
 Acq: 31 Jan 2022 20:30

Instrument :
 MSVOA_X
 ClientSampleId :
 MH-4D

Tgt Ion:152 Resp: 86883
 Ion Ratio Lower Upper
 152 100
 115 59.6 44.2 132.6
 150 155.2 0.0 348.2

