


BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX013123\
Data File : VX033957.D
Acq On : 31 Jan 2023 08:29
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
Title : SW846 8260
Last Update : Wed Jan 11 14:48:42 2023

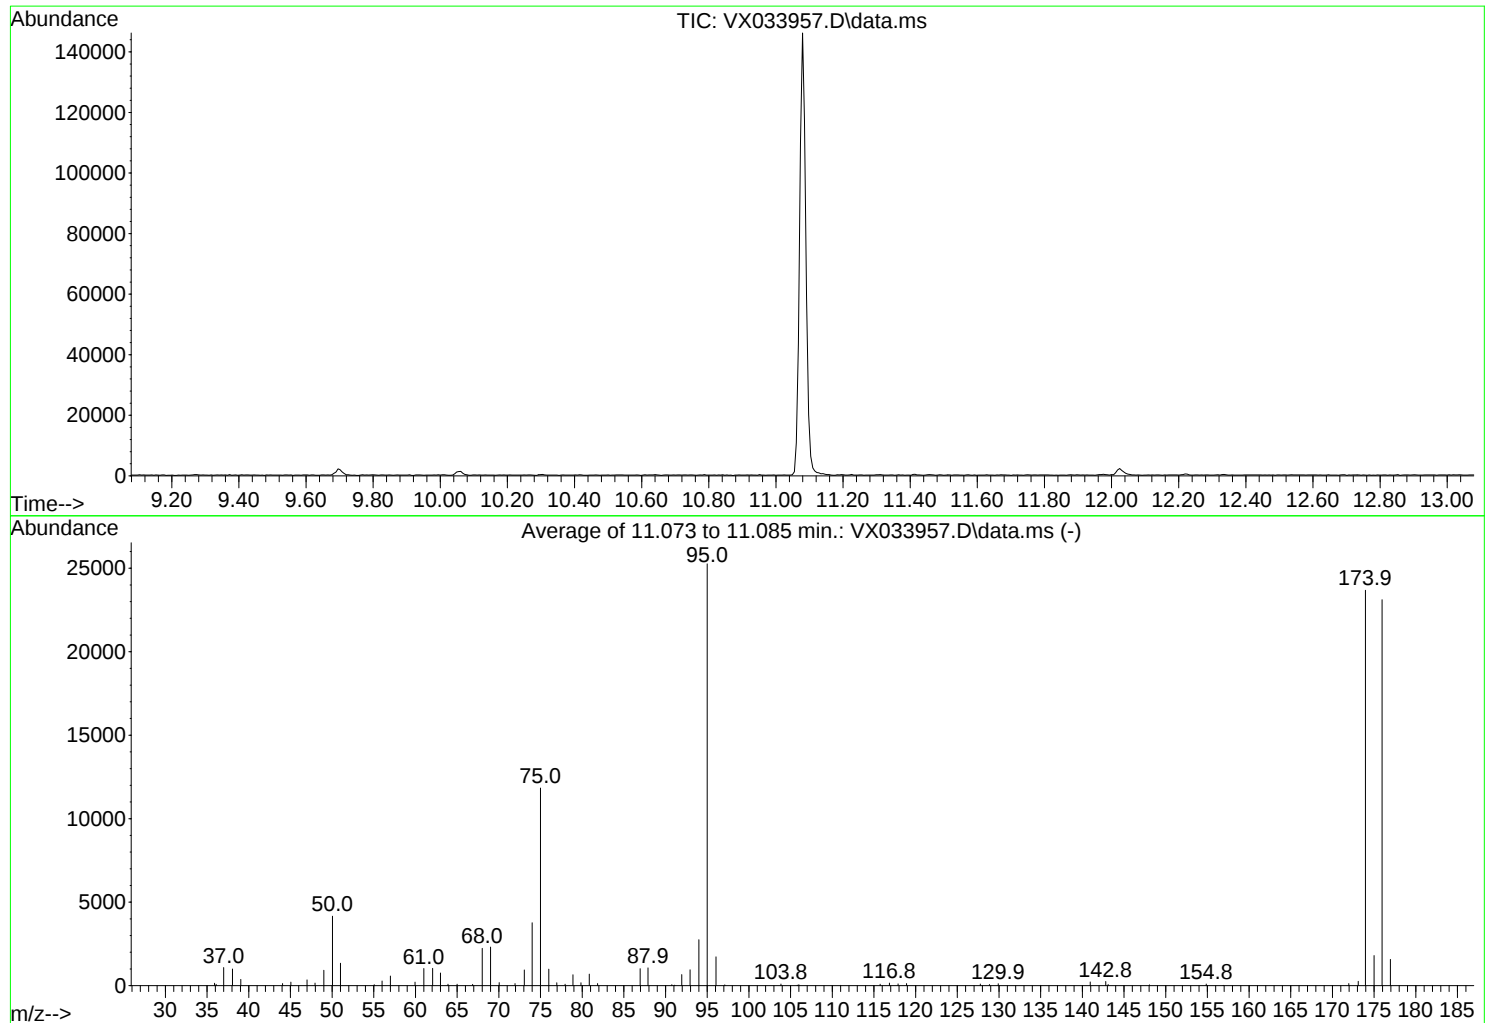

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	4164	PASS
75	95	30	60	46.9	11839	PASS
95	95	100	100	100.0	25264	PASS
96	95	5	9	6.8	1729	PASS
173	174	0.00	2	1.1	258	PASS
174	95	50	100	93.7	23677	PASS
175	174	5	9	7.6	1801	PASS
176	174	95	101	97.6	23115	PASS
177	176	5	9	6.8	1573	PASS