

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX013124\
 Data File : VX040052.D
 Acq On : 31 Jan 2024 17:00
 Operator : JC/MD
 Sample : P1282-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 1241

Quant Time: Feb 01 04:24:53 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X013024W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jan 31 07:12:04 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	76239	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	147184	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	144603	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	78867	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	60003	48.903	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	97.800%		
35) Dibromofluoromethane	5.385	113	47225	47.134	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	94.260%		
50) Toluene-d8	8.647	98	182877	48.807	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	97.620%		
62) 4-Bromofluorobenzene	11.079	95	74816	51.856	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	103.720%		
Target Compounds						Qvalue
3) Chloromethane	1.306	50	190	0.233	ug/l #	43
11) Tert butyl alcohol	2.946	59	4705	21.134	ug/l #	86
13) Acrolein	2.239	56	136	0.638	ug/l #	14
16) Acetone	2.373	43	53651	93.323	ug/l	95
17) Carbon Disulfide	2.514	76	646	0.258	ug/l #	76
18) Methyl Acetate	2.703	43	9494	6.971	ug/l	99
20) Methylene Chloride	2.788	84	562	0.550	ug/l #	78
25) 2-Butanone	4.562	43	20429	25.563	ug/l	96
31) Cyclohexane	5.550	56	2053	1.336	ug/l #	42
36) 1,1-Dichloropropene	5.556	75	7292	5.032	ug/l #	51
37) Ethyl Acetate	4.562	43	20429	12.909	ug/l #	69
38) Carbon Tetrachloride	5.556	117	8726	6.294	ug/l #	15
40) Benzene	6.037	78	1658	0.393	ug/l #	71
48) Methyl methacrylate	7.574	41	7043	5.729	ug/l #	51
49) 1,4-Dioxane	7.665	88	973	36.423	ug/l #	92
51) 4-Methyl-2-Pentanone	8.580	43	1415	0.831	ug/l	89
52) Toluene	8.720	92	2197	0.835	ug/l	95
59) 2-Hexanone	9.445	43	1574	1.159	ug/l	84
67) Ethyl Benzene	10.195	91	2231	0.416	ug/l	93
68) m/p-Xylenes	10.299	106	3546	1.758	ug/l	88
69) o-Xylene	10.646	106	1791	0.936	ug/l	94
70) Styrene	10.658	104	2934	0.910	ug/l	95
74) N-amyl acetate	10.854	43	924	0.559	ug/l #	7
76) 1,2,3-Trichloropropane	11.079	75	39242	23.365	ug/l #	39
80) 1,3,5-Trimethylbenzene	11.451	105	988	0.203	ug/l	90
81) trans-1,4-Dichloro-2-b...	11.079	75	39242	69.830	ug/l #	5
84) 1,2,4-Trimethylbenzene	11.756	105	4462	0.919	ug/l	79
89) n-Butylbenzene	12.329	91	1738	0.355	ug/l	78
90) Hexachloroethane	12.542	117	53	Below Cal	#	17
93) 1,2,4-Trichlorobenzene	13.591	180	405	0.255	ug/l	85
95) Naphthalene	13.780	128	4039	0.749	ug/l #	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX013124\
Data File : VX040052.D
Acq On : 31 Jan 2024 17:00
Operator : JC/MD
Sample : P1282-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1241

Quant Time: Feb 01 04:24:53 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X013024W.M
Quant Title : SW846 8260
QLast Update : Wed Jan 31 07:12:04 2024
Response via : Initial Calibration




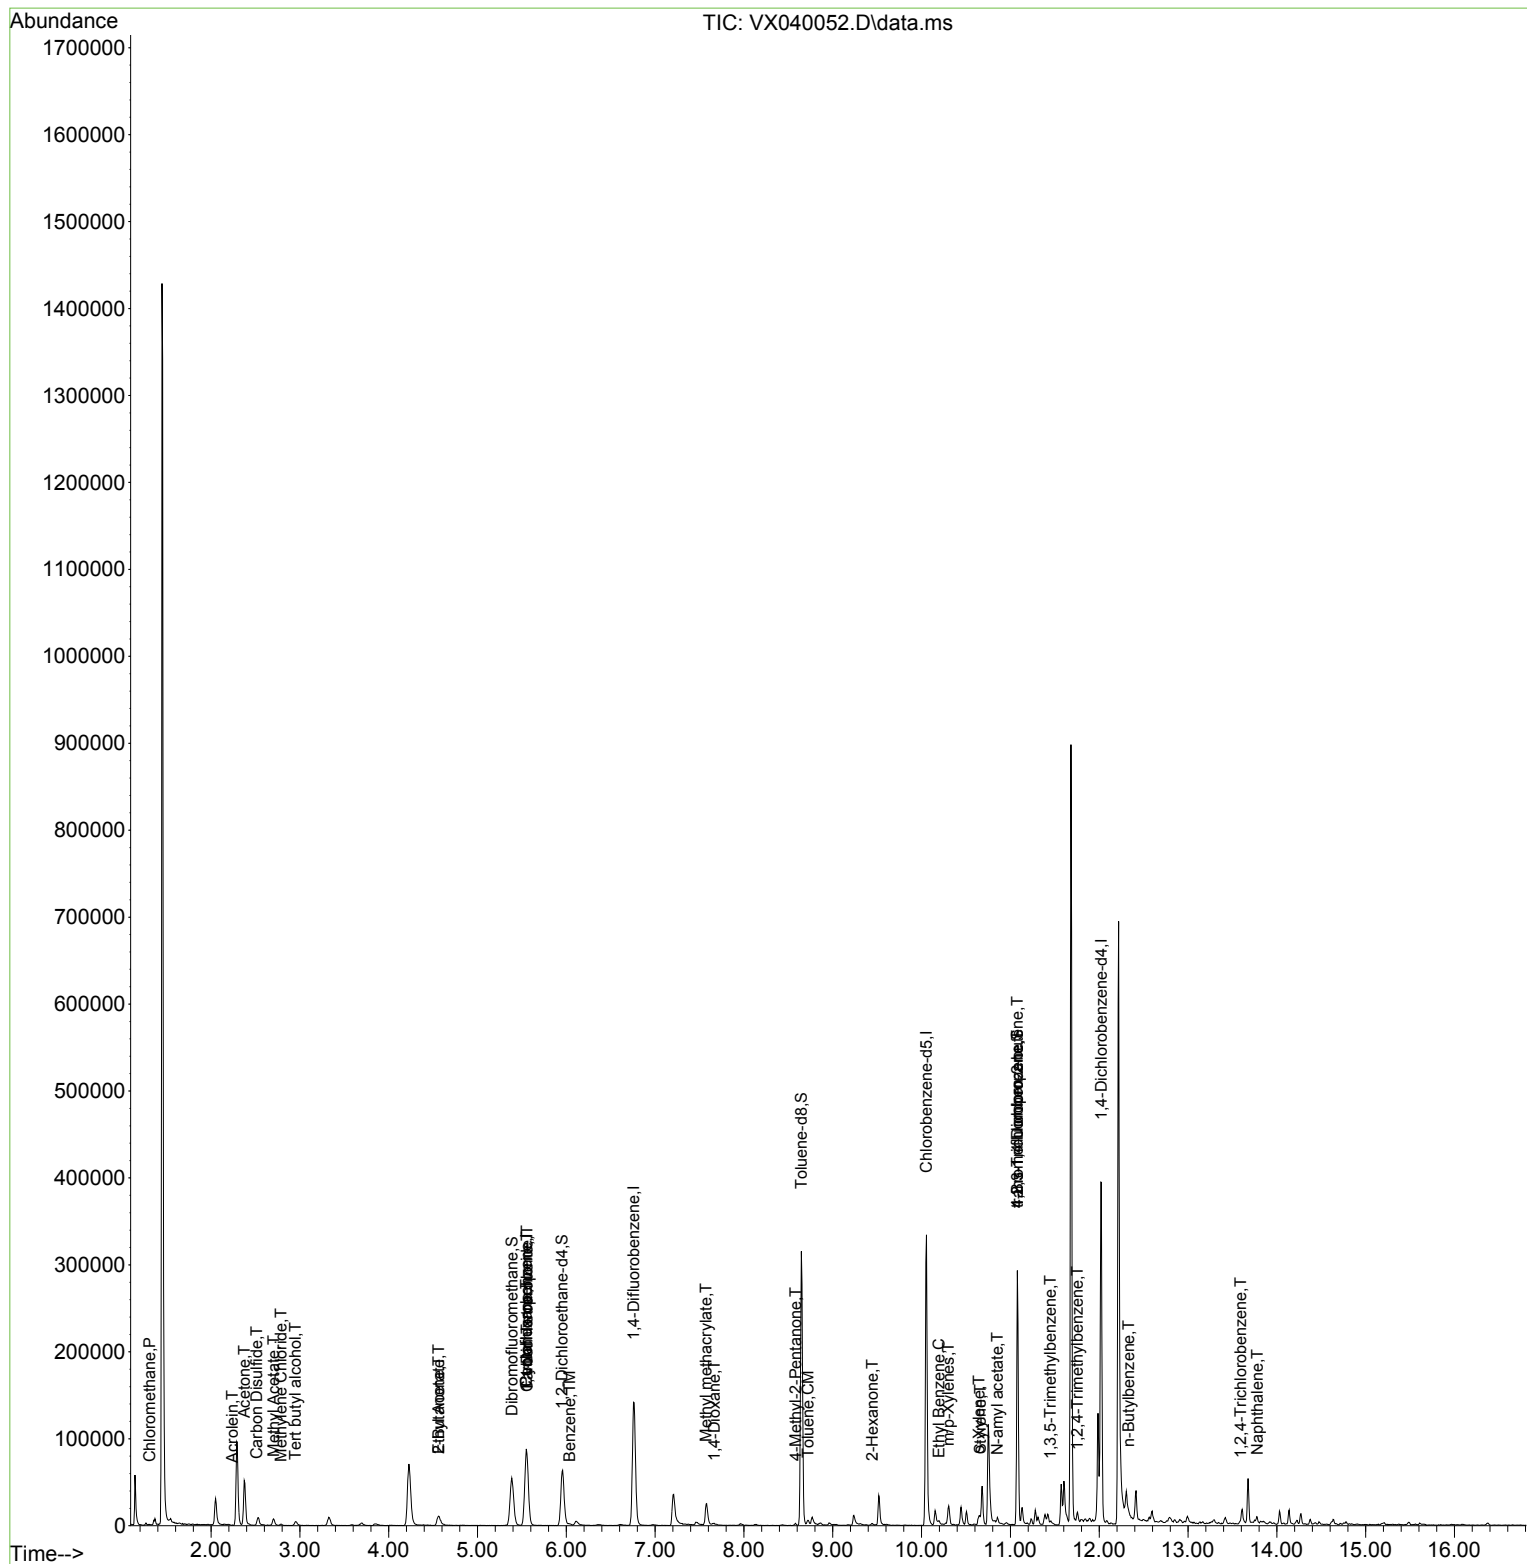




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX040052.D
Acq: 31 Jan 2024 17:00




Instrument :
MSVOA_X
ClientSampleId :
1241


Tgt Ion:168 Resp: 76239
Ion Ratio Lower Upper
168 100
99 64.7 56.6 85.0

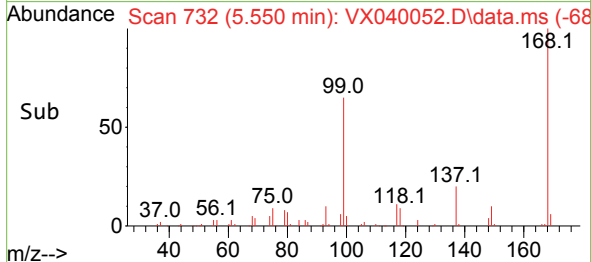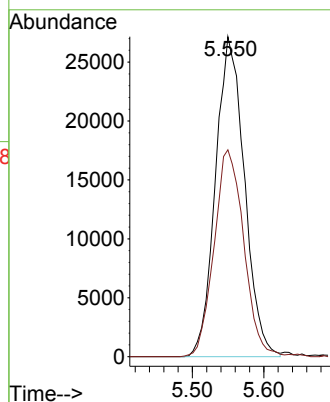

#3
Chloromethane
Concen: 0.233 ug/l
RT: 1.306 min Scan# 36
Delta R.T. 0.012 min
Lab File: VX040052.D
Acq: 31 Jan 2024 17:00

Tgt Ion: 50 Resp: 190
Ion Ratio Lower Upper
50 100
52 0.0 25.5 38.3#


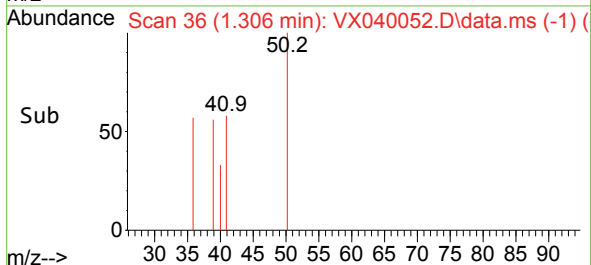

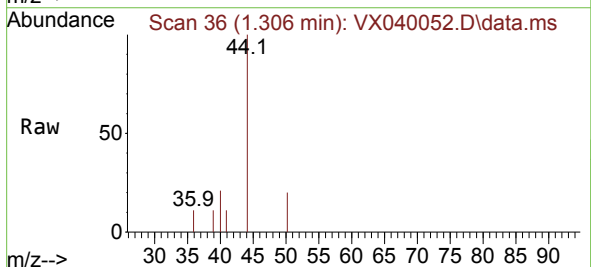




#11
Tert butyl alcohol
Concen: 21.134 ug/l
RT: 2.946 min Scan# 30
Delta R.T. -0.012 min
Lab File: VX040052.D
Acq: 31 Jan 2024 17:00




Instrument :
MSVOA_X
ClientSampleId :
1241


Tgt Ion: 59 Resp: 4705
Ion Ratio Lower Upper
59 100
57 12.2 6.0 9.0#

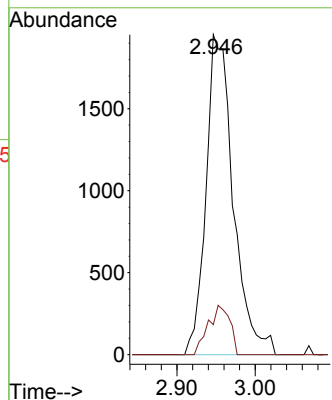

#13
Acrolein
Concen: 0.638 ug/l
RT: 2.239 min Scan# 189
Delta R.T. 0.006 min
Lab File: VX040052.D
Acq: 31 Jan 2024 17:00

Tgt Ion: 56 Resp: 136
Ion Ratio Lower Upper
56 100
55 0.0 57.1 85.7#



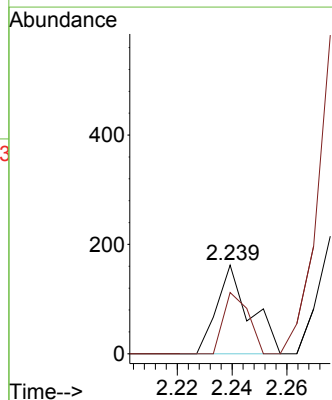





#16
 Acetone
 Concen: 93.323 ug/l
 RT: 2.373 min Scan# 211
 Delta R.T. -0.000 min
 Lab File: VX040052.D
 Acq: 31 Jan 2024 17:00




Instrument :
 MSVOA_X
 ClientSampleId :
 1241


Tgt Ion: 43 Resp: 53651
 Ion Ratio Lower Upper
 43 100
 58 29.8 21.9 32.9

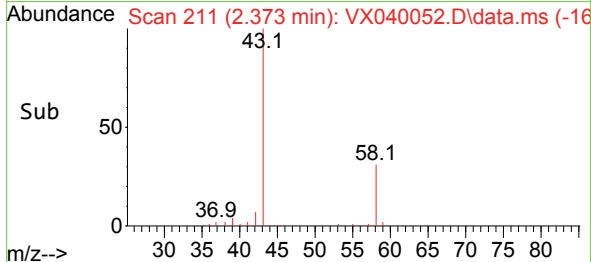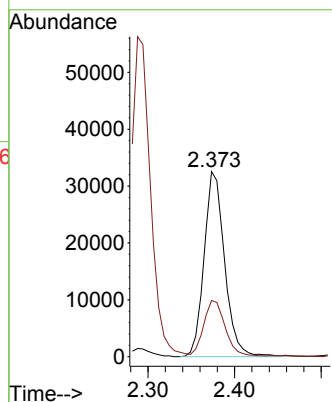

#17
 Carbon Disulfide
 Concen: 0.258 ug/l
 RT: 2.514 min Scan# 234
 Delta R.T. -0.000 min
 Lab File: VX040052.D
 Acq: 31 Jan 2024 17:00

Tgt Ion: 76 Resp: 646
 Ion Ratio Lower Upper
 76 100
 78 0.0 7.0 10.6#


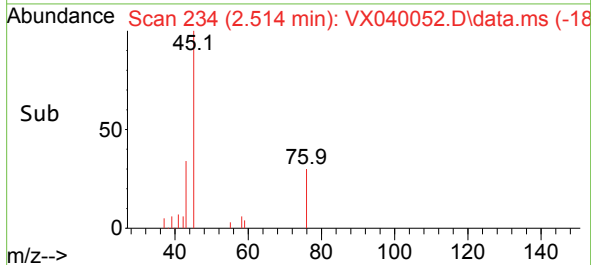
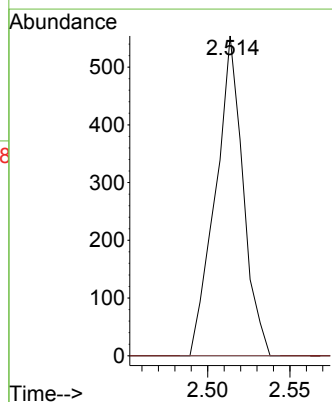
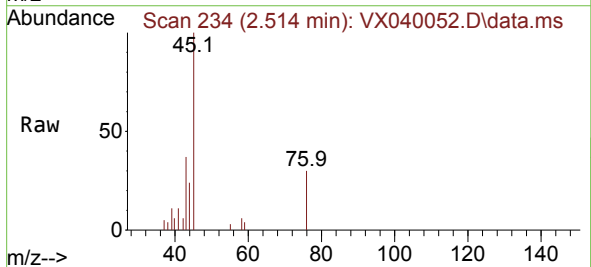




#18
Methyl Acetate
Concen: 6.971 ug/l
RT: 2.703 min Scan# 265
Delta R.T. -0.000 min
Lab File: VX040052.D
Acq: 31 Jan 2024 17:00




Instrument :
MSVOA_X
ClientSampleId :
1241


Tgt Ion: 43 Resp: 9494
Ion Ratio Lower Upper
43 100
74 22.7 17.8 26.8

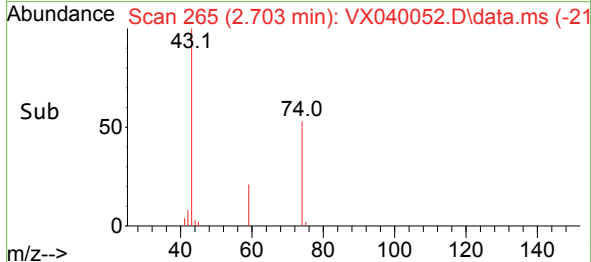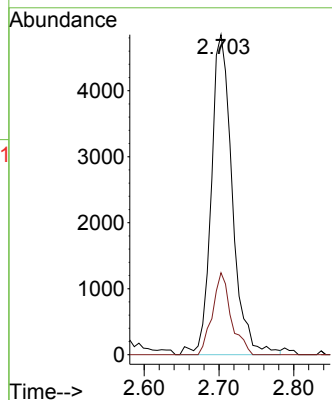

#20
Methylene Chloride
Concen: 0.550 ug/l
RT: 2.788 min Scan# 279
Delta R.T. -0.000 min
Lab File: VX040052.D
Acq: 31 Jan 2024 17:00

Tgt Ion: 84 Resp: 562
Ion Ratio Lower Upper
84 100
49 99.1 103.6 155.4#
51 49.8 33.8 50.6
86 45.3 49.4 74.0#


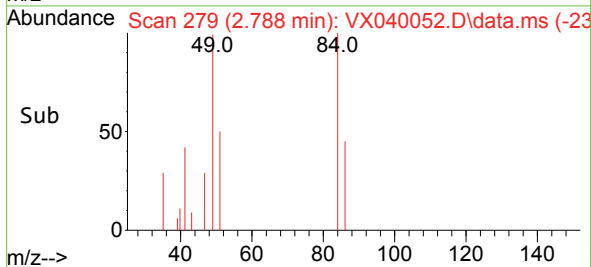
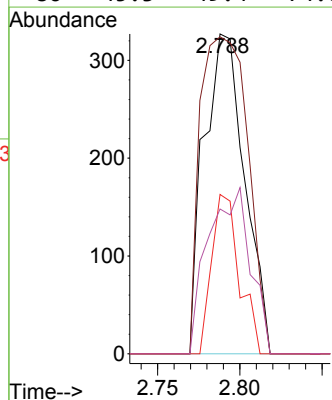
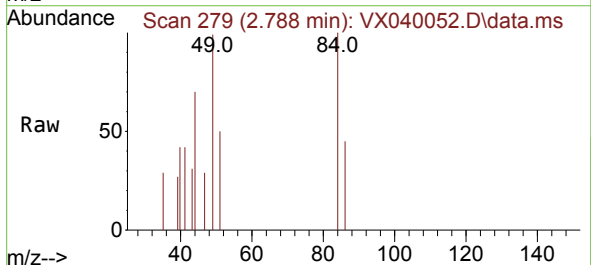




#25
2-Butanone
Concen: 25.563 ug/l
RT: 4.562 min Scan# 51
Delta R.T. 0.012 min
Lab File: VX040052.D
Acq: 31 Jan 2024 17:00




Instrument :
MSVOA_X
ClientSampleId :
1241


Tgt Ion: 43 Resp: 20429
Ion Ratio Lower Upper
43 100
72 26.3 19.4 29.2

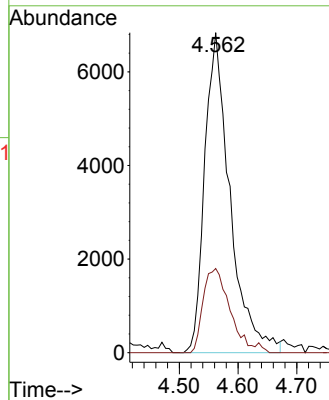

#31
Cyclohexane
Concen: 1.336 ug/l
RT: 5.550 min Scan# 732
Delta R.T. 0.085 min
Lab File: VX040052.D
Acq: 31 Jan 2024 17:00

Tgt Ion: 56 Resp: 2053
Ion Ratio Lower Upper
56 100
69 129.5 23.4 35.2#
84 93.3 65.9 98.9

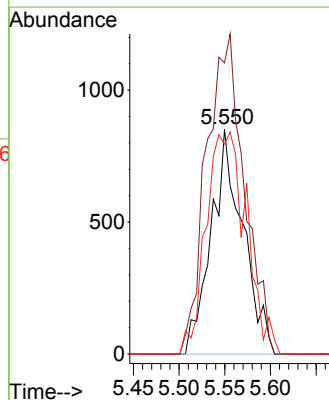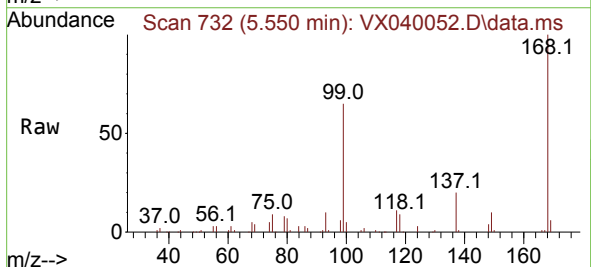



#33

1,2-Dichloroethane-d4

Concen: 48.903 ug/l

RT: 5.952 min Scan# 798

Delta R.T. -0.000 min

Lab File: VX040052.D

Acq: 31 Jan 2024 17:00

Instrument :

MSVOA_X

ClientSampleId :





1241

Tgt Ion: 65 Resp: 60003

Ion Ratio Lower Upper

65 100

67 53.1 0.0 100.2



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. -0.006 min

Lab File: VX040052.D

Acq: 31 Jan 2024 17:00




Tgt Ion: 114 Resp: 147184


Ion Ratio Lower Upper

114 100

63 19.9 0.0 45.0

88 16.0 0.0 36.6


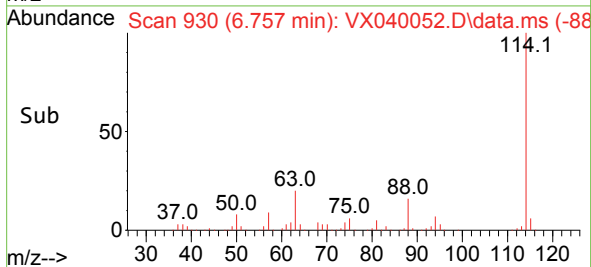

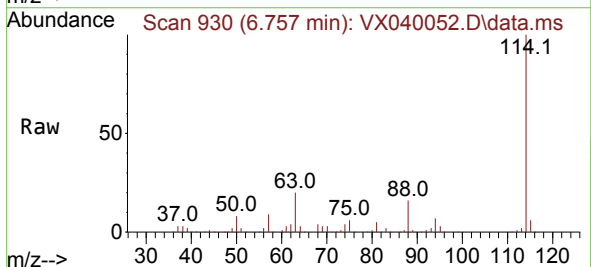


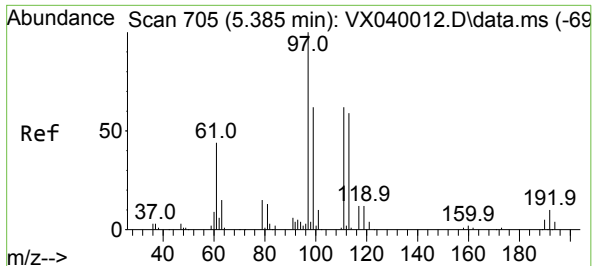

#35
Dibromofluoromethane
Concen: 47.134 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX040052.D
Acq: 31 Jan 2024 17:00




Instrument :
MSVOA_X
ClientSampleId :
1241


Tgt Ion:113 Resp: 47225
Ion Ratio Lower Upper
113 100
111 101.1 82.9 124.3
192 16.5 13.3 19.9

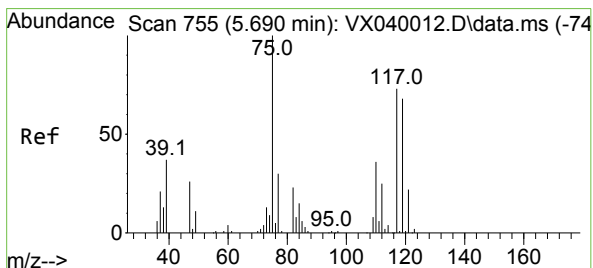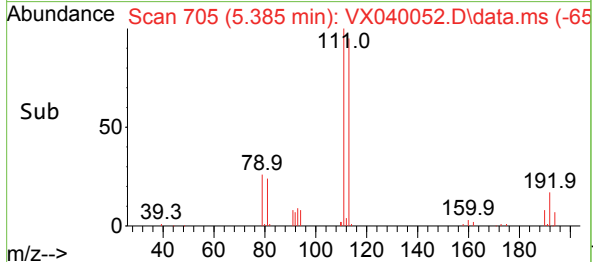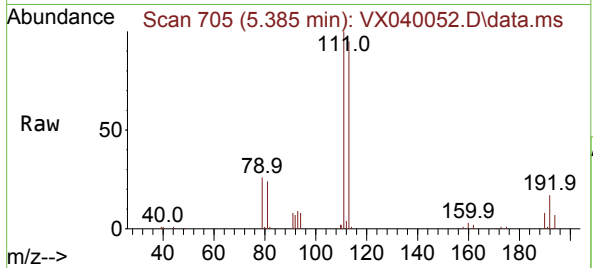

#36
1,1-Dichloropropene
Concen: 5.032 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.134 min
Lab File: VX040052.D
Acq: 31 Jan 2024 17:00

Tgt Ion: 75 Resp: 7292
Ion Ratio Lower Upper
75 100
110 10.0 17.0 50.9#
77 0.0 24.7 37.1#

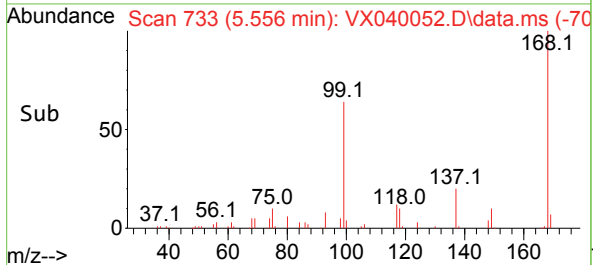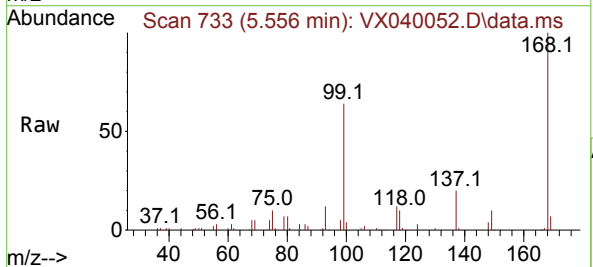



#37

Ethyl Acetate

Concen: 12.909 ug/l

RT: 4.562 min Scan# 51

Delta R.T. -0.153 min

Lab File: VX040052.D


Acq: 31 Jan 2024 17:00

Instrument :

MSVOA_X

ClientSampleId :

1241






Tgt Ion: 43 Resp: 20429

Ion Ratio Lower Upper

43 100

61 0.0 10.6 16.0#

70 0.2 8.3 12.5#

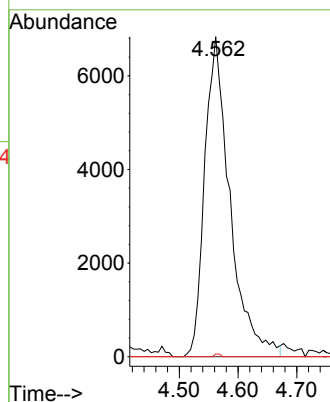

#38

Carbon Tetrachloride

Concen: 6.294 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.122 min

Lab File: VX040052.D

Acq: 31 Jan 2024 17:00




Tgt Ion: 117 Resp: 8726


Ion Ratio Lower Upper

117 100

119 4.9 78.2 117.2#

121 0.0 24.4 36.6#

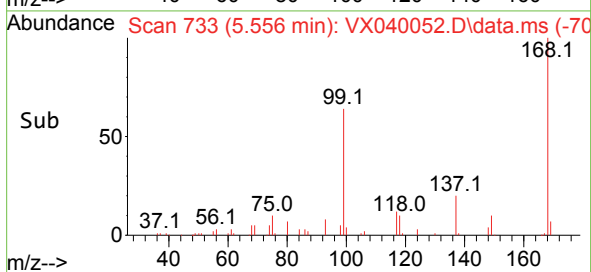

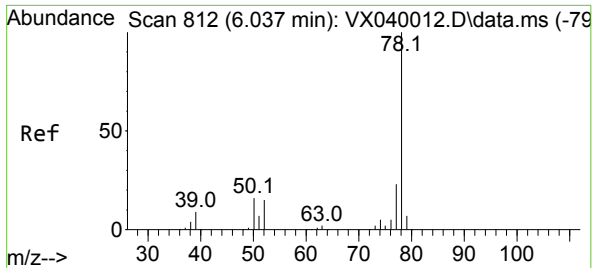

#40

Benzene

Concen: 0.393 ug/l

RT: 6.037 min Scan# 81

Delta R.T. -0.000 min

Lab File: VX040052.D

Acq: 31 Jan 2024 17:00

Instrument :

MSVOA_X

ClientSampleId :





1241

Tgt Ion: 78 Resp: 1658

Ion Ratio Lower Upper

78 100

77 38.2 19.3 28.9#

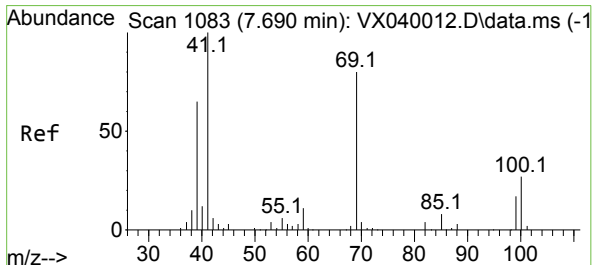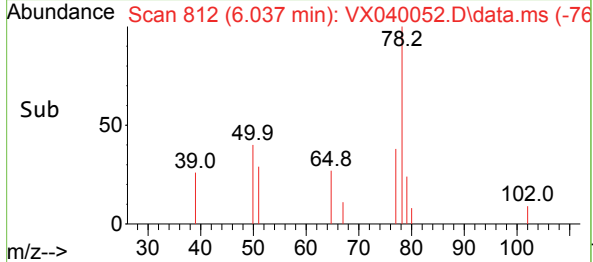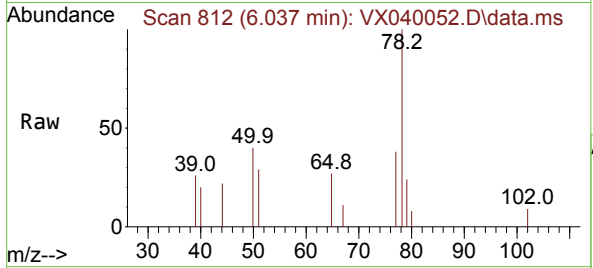

#48

Methyl methacrylate

Concen: 5.729 ug/l

RT: 7.574 min Scan# 1064

Delta R.T. -0.116 min

Lab File: VX040052.D

Acq: 31 Jan 2024 17:00




Tgt Ion: 41 Resp: 7043


Ion Ratio Lower Upper

41 100

69 0.0 59.2 88.8#

39 60.2 47.7 71.5


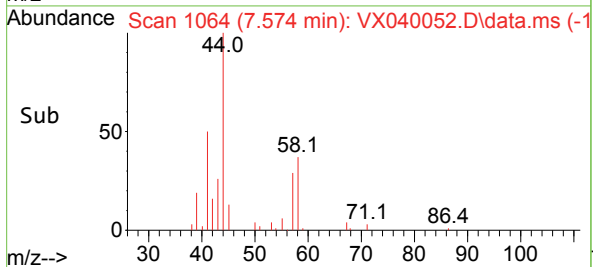
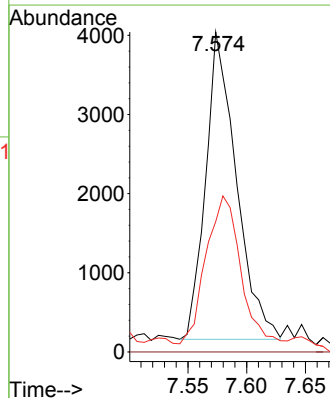
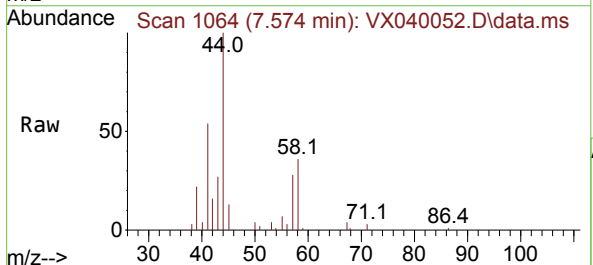




#49
1,4-Dioxane
Concen: 36.423 ug/l
RT: 7.665 min Scan# 1077
Delta R.T. 0.012 min
Lab File: VX040052.D
Acq: 31 Jan 2024 17:00




Instrument :
MSVOA_X
ClientSampleId :
1241


Tgt Ion: 88 Resp: 973
Ion Ratio Lower Upper
88 100
43 20.5 0.0 0.0#
58 81.9 60.1 90.1

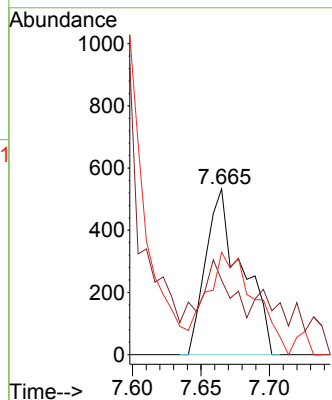

#50
Toluene-d8
Concen: 48.807 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.000 min
Lab File: VX040052.D
Acq: 31 Jan 2024 17:00

Tgt Ion: 98 Resp: 182877
Ion Ratio Lower Upper
98 100
100 64.1 53.1 79.7



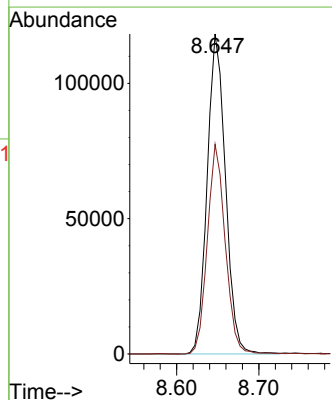





#51
4-Methyl-2-Pentanone
Concen: 0.831 ug/l
RT: 8.580 min Scan# 1229
Delta R.T. 0.006 min
Lab File: VX040052.D
Acq: 31 Jan 2024 17:00




Instrument :
MSVOA_X
ClientSampleId :
1241


Tgt Ion: 43 Resp: 1415
Ion Ratio Lower Upper
43 100
58 31.5 30.4 45.6

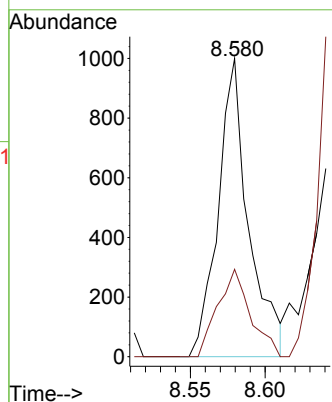

#52
Toluene
Concen: 0.835 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. 0.006 min
Lab File: VX040052.D
Acq: 31 Jan 2024 17:00

Tgt Ion: 92 Resp: 2197
Ion Ratio Lower Upper
92 100
91 174.9 134.2 201.2


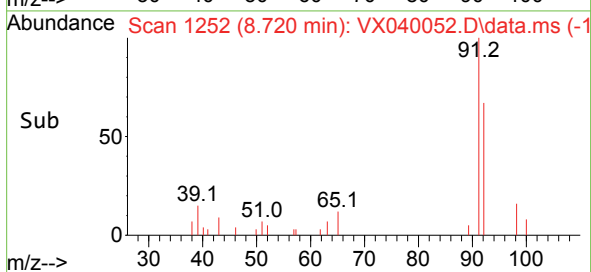
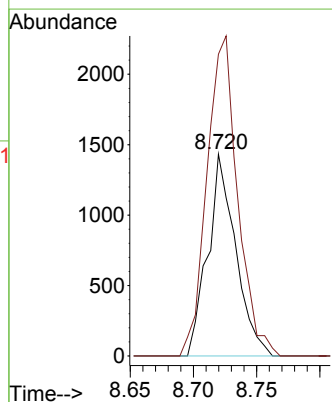
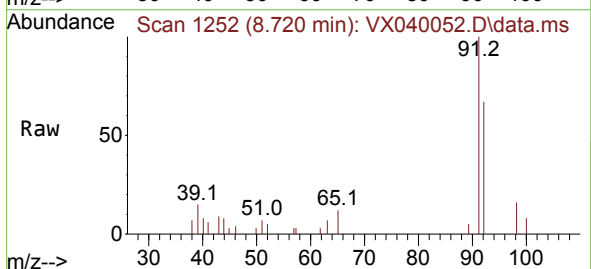




#59
2-Hexanone
Concen: 1.159 ug/l
RT: 9.445 min Scan# 11
Delta R.T. 0.018 min
Lab File: VX040052.D
Acq: 31 Jan 2024 17:00




Instrument :
MSVOA_X
ClientSampleId :
1241


Tgt Ion: 43 Resp: 1574
Ion Ratio Lower Upper
43 100
58 41.4 26.2 78.5

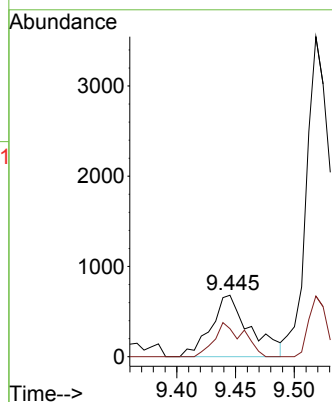

#62
4-Bromofluorobenzene
Concen: 51.856 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX040052.D
Acq: 31 Jan 2024 17:00

Tgt Ion: 95 Resp: 74816
Ion Ratio Lower Upper
95 100
174 70.7 0.0 135.6
176 69.1 0.0 131.0


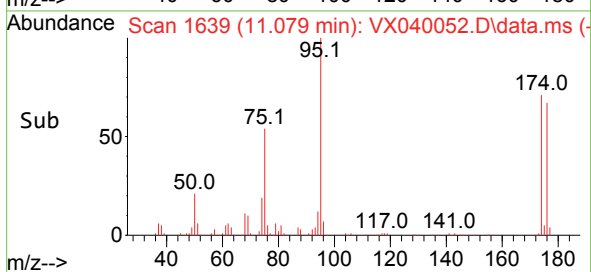
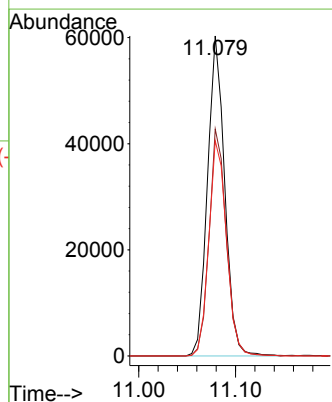





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX040052.D
Acq: 31 Jan 2024 17:00




Instrument :
MSVOA_X
ClientSampleId :
1241


Tgt Ion:117 Resp: 144603
Ion Ratio Lower Upper
117 100
82 56.3 46.2 69.4
119 30.4 25.5 38.3

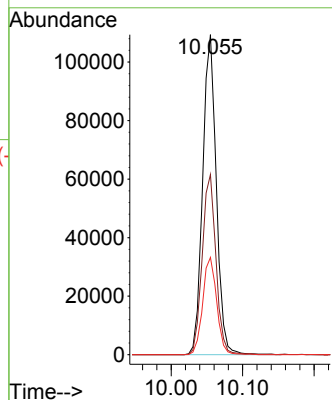

#67
Ethyl Benzene
Concen: 0.416 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. -0.000 min
Lab File: VX040052.D
Acq: 31 Jan 2024 17:00

Tgt Ion: 91 Resp: 2231
Ion Ratio Lower Upper
91 100
106 27.1 24.9 37.3



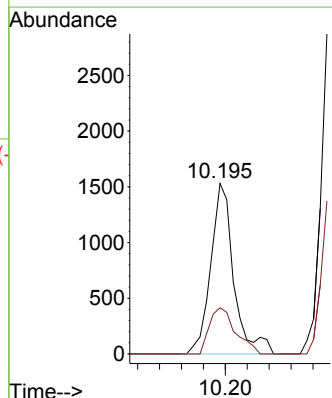
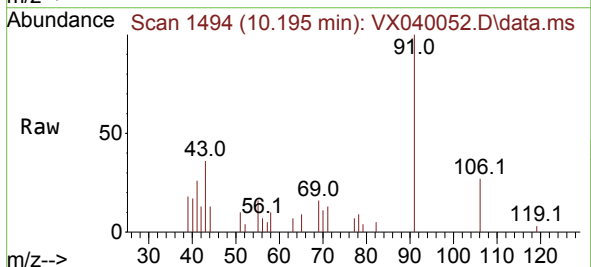




#68
m/p-Xylenes
Concen: 1.758 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.000 min
Lab File: VX040052.D
Acq: 31 Jan 2024 17:00




Instrument :
MSVOA_X
ClientSampleId :
1241


Tgt Ion:106 Resp: 3546
Ion Ratio Lower Upper
106 100
91 188.9 165.5 248.3



#69
o-Xylene
Concen: 0.936 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. 0.006 min
Lab File: VX040052.D
Acq: 31 Jan 2024 17:00

Tgt Ion:106 Resp: 1791
Ion Ratio Lower Upper
106 100
91 207.9 108.9 326.8









#70
Styrene
Concen: 0.910 ug/l
RT: 10.658 min Scan# 11
Delta R.T. 0.005 min
Lab File: VX040052.D
Acq: 31 Jan 2024 17:00




Instrument :
MSVOA_X
ClientSampleId :
1241


Tgt Ion:104 Resp: 2934
Ion Ratio Lower Upper
104 100
78 51.7 43.6 65.4
103 59.4 43.6 65.4

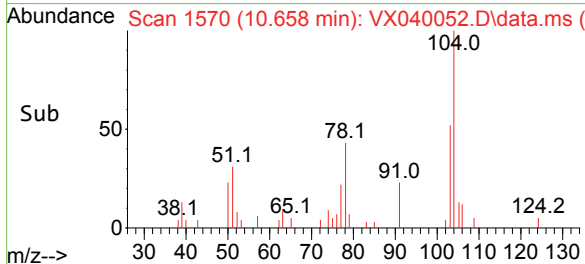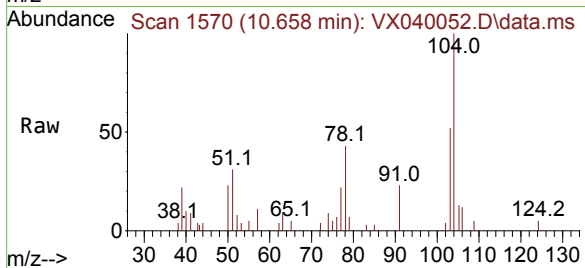

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.006 min
Lab File: VX040052.D
Acq: 31 Jan 2024 17:00

Tgt Ion:152 Resp: 78867
Ion Ratio Lower Upper
152 100
115 61.8 43.3 129.9
150 157.4 0.0 345.0

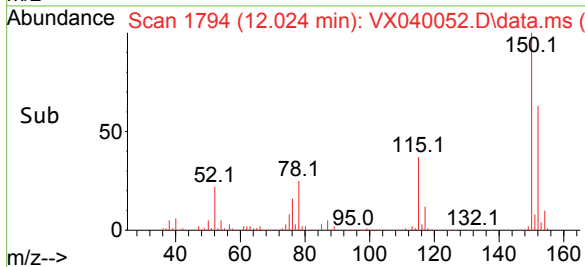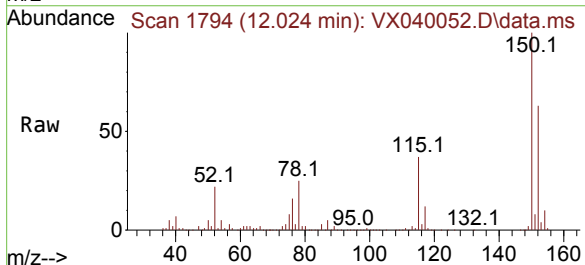



#74

N-amy1 acetate

Concen: 0.559 ug/l

RT: 10.854 min Scan# 1

Delta R.T. 0.012 min

Lab File: VX040052.D

Acq: 31 Jan 2024 17:00

Instrument :

MSVOA_X

ClientSampleId :

1241

Tgt Ion: 43 Resp: 924





Ion Ratio Lower Upper

43 100

70 131.5 32.9 49.3#

55 0.0 19.3 28.9#

61 0.0 18.8 28.2#



#76

1,2,3-Trichloropropane

Concen: 23.365 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.159 min

Lab File: VX040052.D




Acq: 31 Jan 2024 17:00


Tgt Ion: 75 Resp: 39242

Ion Ratio Lower Upper

75 100

77 1.3 19.1 57.5#





#80

1,3,5-Trimethylbenzene

Concen: 0.203 ug/l

RT: 11.451 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX040052.D

Acq: 31 Jan 2024 17:00

Instrument :

MSVOA_X

ClientSampleId :





1241

Tgt Ion:105 Resp: 988

Ion Ratio Lower Upper

105 100

120 54.9 24.1 72.3

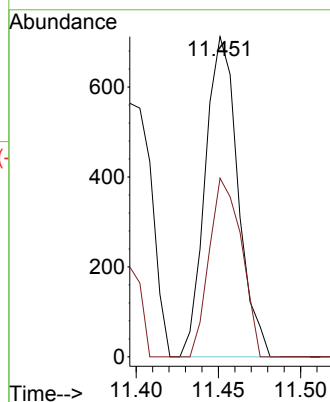

#81

trans-1,4-Dichloro-2-butene

Concen: 69.830 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.061 min

Lab File: VX040052.D

Acq: 31 Jan 2024 17:00




Tgt Ion: 75 Resp: 39242


Ion Ratio Lower Upper

75 100

53 0.0 90.5 135.7#

89 0.0 36.9 55.3#





#84

1,2,4-Trimethylbenzene

Concen: 0.919 ug/l

RT: 11.756 min Scan# 1749

Delta R.T. 0.006 min

Lab File: VX040052.D

Acq: 31 Jan 2024 17:00

Instrument :

MSVOA_X

ClientSampleId :





1241

Tgt Ion:105 Resp: 4462

Ion Ratio Lower Upper

105 100

120 29.3 21.2 63.6

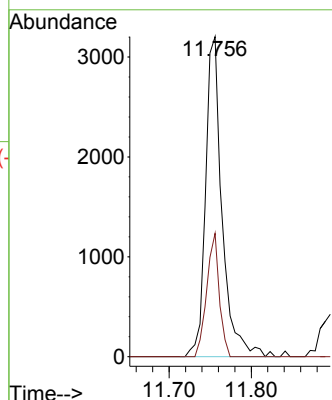

#89

n-Butylbenzene

Concen: 0.355 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. -0.000 min

Lab File: VX040052.D

Acq: 31 Jan 2024 17:00




Tgt Ion: 91 Resp: 1738


Ion Ratio Lower Upper

91 100

92 33.1 27.4 82.0

134 27.4 12.6 37.8

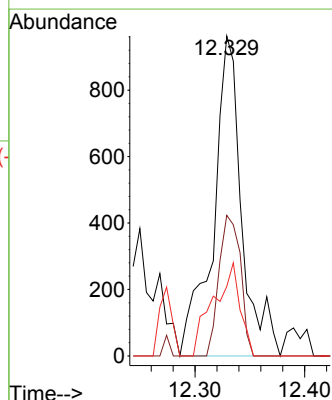



#90

Hexachloroethane

Concen: Below Cal

RT: 12.542 min Scan# 11

Delta R.T. 0.006 min

Lab File: VX040052.D

Acq: 31 Jan 2024 17:00

Instrument :

MSVOA_X

ClientSampleId :





1241

Tgt Ion:117 Resp: 53

Ion Ratio Lower Upper

117 100

201 0.0 32.9 98.6#

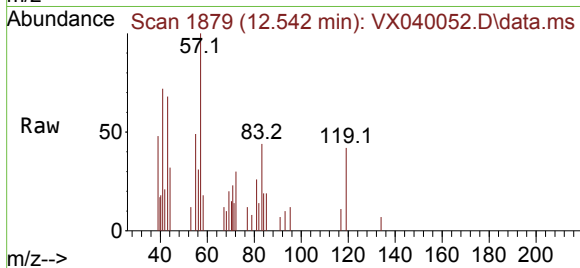

#93

1,2,4-Trichlorobenzene

Concen: 0.255 ug/l

RT: 13.591 min Scan# 2051

Delta R.T. 0.006 min

Lab File: VX040052.D

Acq: 31 Jan 2024 17:00




Tgt Ion:180 Resp: 405


Ion Ratio Lower Upper

180 100

182 86.7 48.3 144.8


145 51.6 18.0 54.0

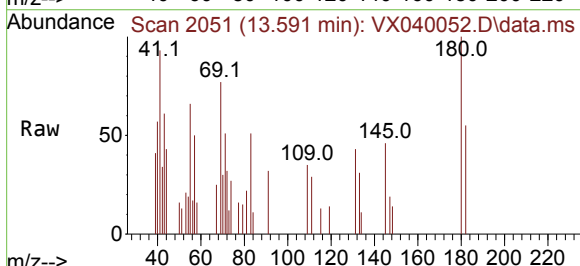

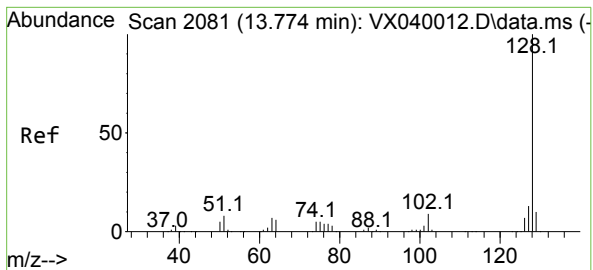

#95
 Naphthalene
 Concen: 0.749 ug/l
 RT: 13.780 min Scan# 20
 Delta R.T. 0.006 min
 Lab File: VX040052.D
 Acq: 31 Jan 2024 17:00

Instrument :
 MSVOA_X
 ClientSampleId :
 1241

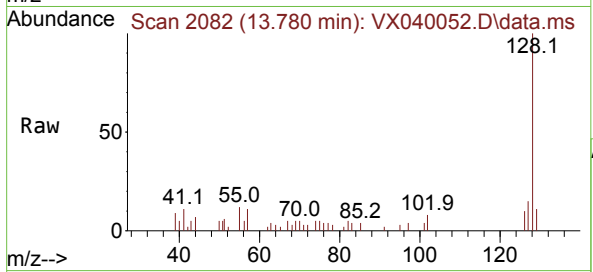

Tgt Ion:	128	Resp:	4039
Ion	Ratio	Lower	Upper
128	100		
127	15.4	10.3	15.5
129	8.2	8.8	13.2#

