

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX013125\
 Data File : VX044789.D
 Acq On : 31 Jan 2025 12:22
 Operator : JC/MD
 Sample : Q1189-19ME
 Misc : 10.58g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Feb 03 07:32:41 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Feb 03 07:31:09 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	280614	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	246465	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	111914	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	54772	25.930	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	51.860%#
7) Chloroethane-d5	1.715	69	18707	23.312	ug/L	0.07
Spiked Amount	50.000	Range	70 - 130	Recovery	=	46.620%#
11) 1,1-Dichloroethene-d2	2.282	65	38657	42.815	ug/L	-0.01
Spiked Amount	50.000	Range	60 - 125	Recovery	=	85.620%
21) 2-Butanone-d5	4.483	46	103933	115.095	ug/L	0.03
Spiked Amount	100.000	Range	40 - 130	Recovery	=	115.100%
24) Chloroform-d	5.050	84	168369	45.361	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.720%
26) 1,2-Dichloroethane-d4	5.952	65	106522	47.812	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.620%
32) Benzene-d6	5.964	84	372326	48.314	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.620%
36) 1,2-Dichloropropane-d6	7.306	67	117778	48.285	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	96.560%
41) Toluene-d8	8.647	98	327842	48.066	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.140%
43) trans-1,3-Dichloroprop...	8.952	79	51970	44.916	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.840%
47) 2-Hexanone-d5	9.391	63	70557	97.737	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	97.740%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	149469	49.311	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	98.620%
66) 1,2-Dichlorobenzene-d4	12.317	152	111070	50.722	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.440%
Target Compounds						Qvalue
15) Methyl Acetate	2.715	43	6482	3.111	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX013125\
Data File : VX044789.D
Acq On : 31 Jan 2025 12:22
Operator : JC/MD
Sample : Q1189-19ME
Misc : 10.58g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Feb 03 07:32:41 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Feb 03 07:31:09 2025
Response via : Initial Calibration

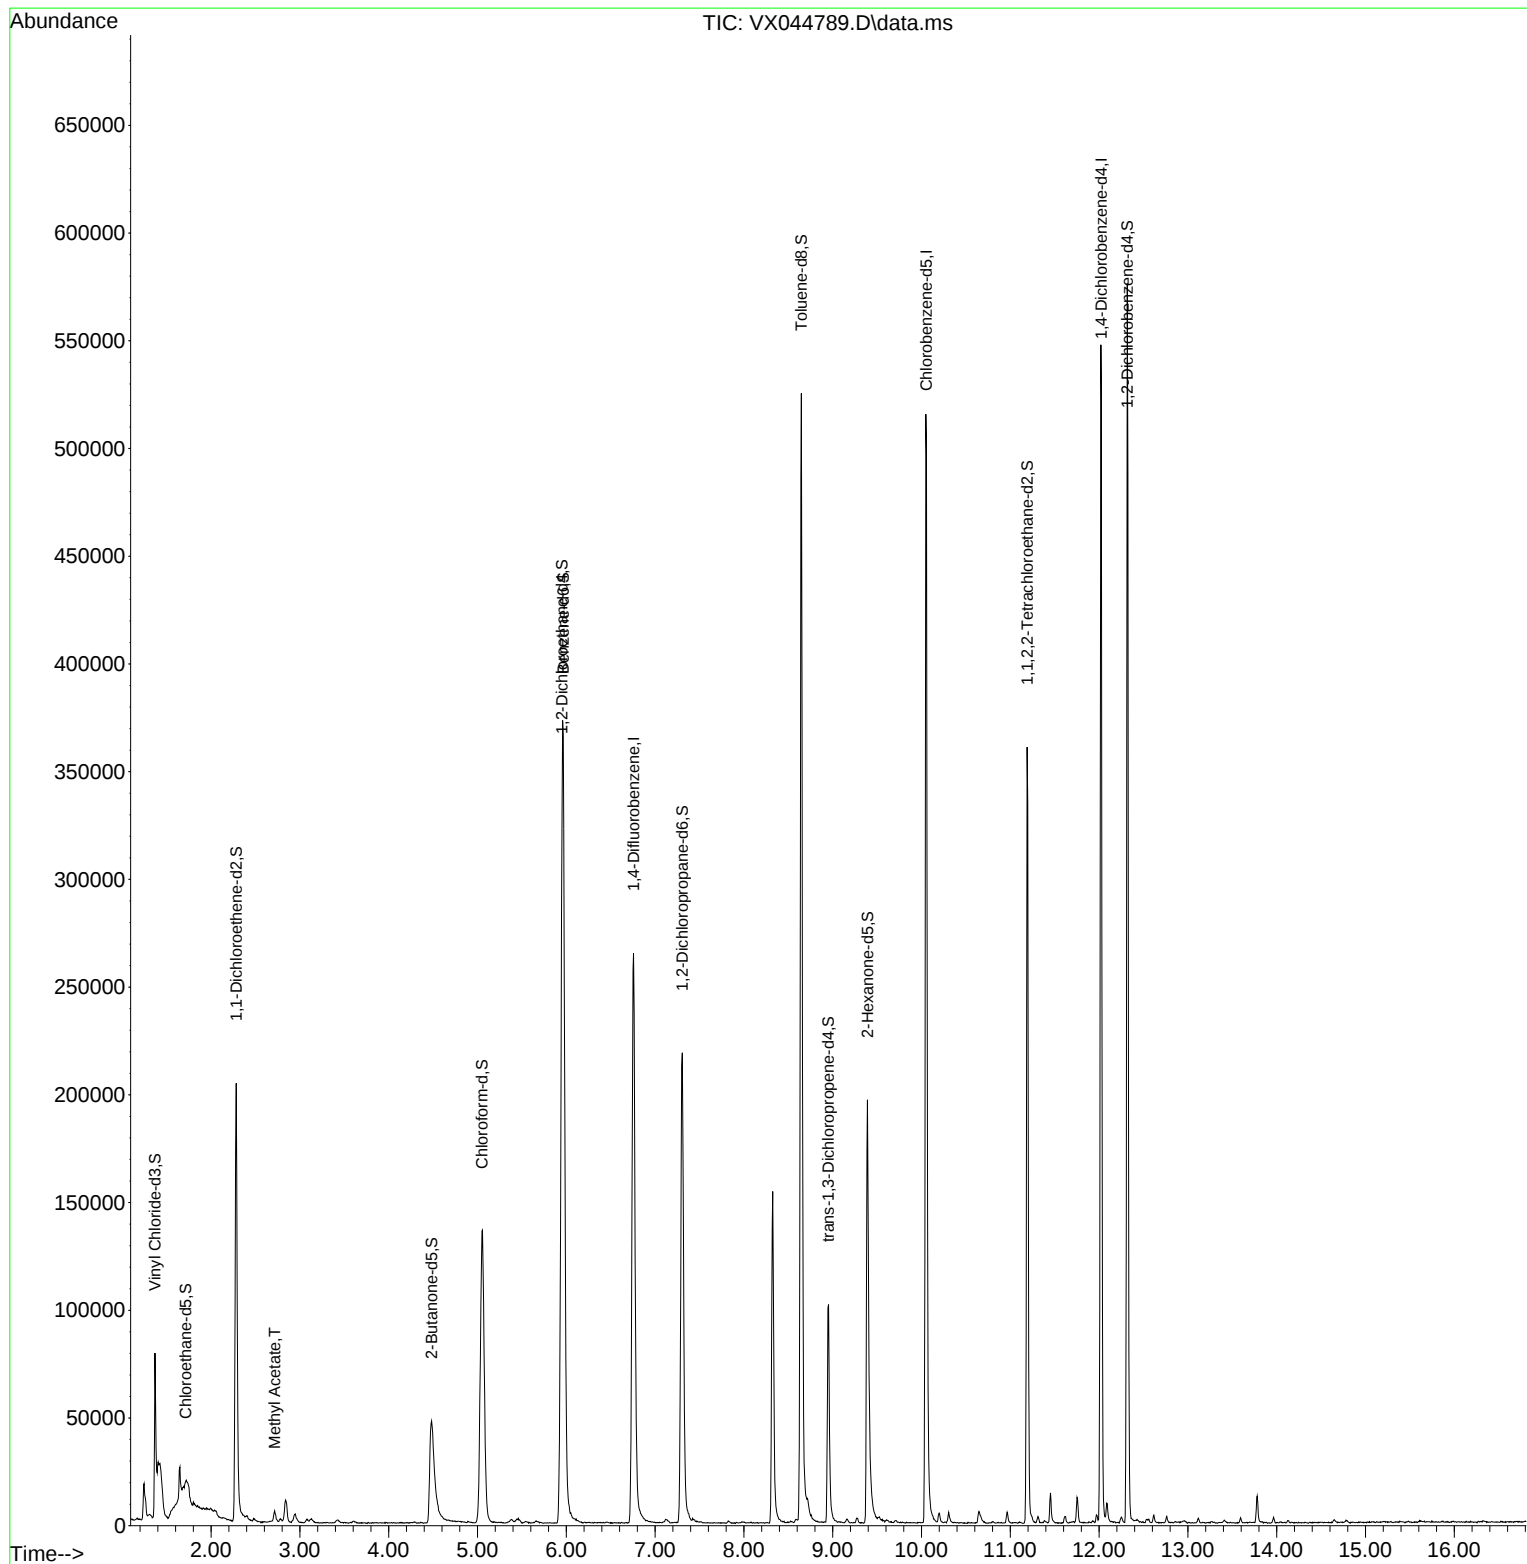

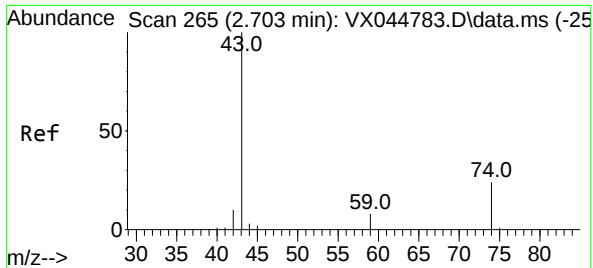

#15
Methyl Acetate
Concen: 3.111 ug/L
RT: 2.715 min Scan# 2
Delta R.T. 0.012 min
Lab File: VX044789.D
Acq: 31 Jan 2025 12:22

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion: 43 Resp: 6482
Ion Ratio Lower Upper
43 100
74 22.5 19.7 29.5

