
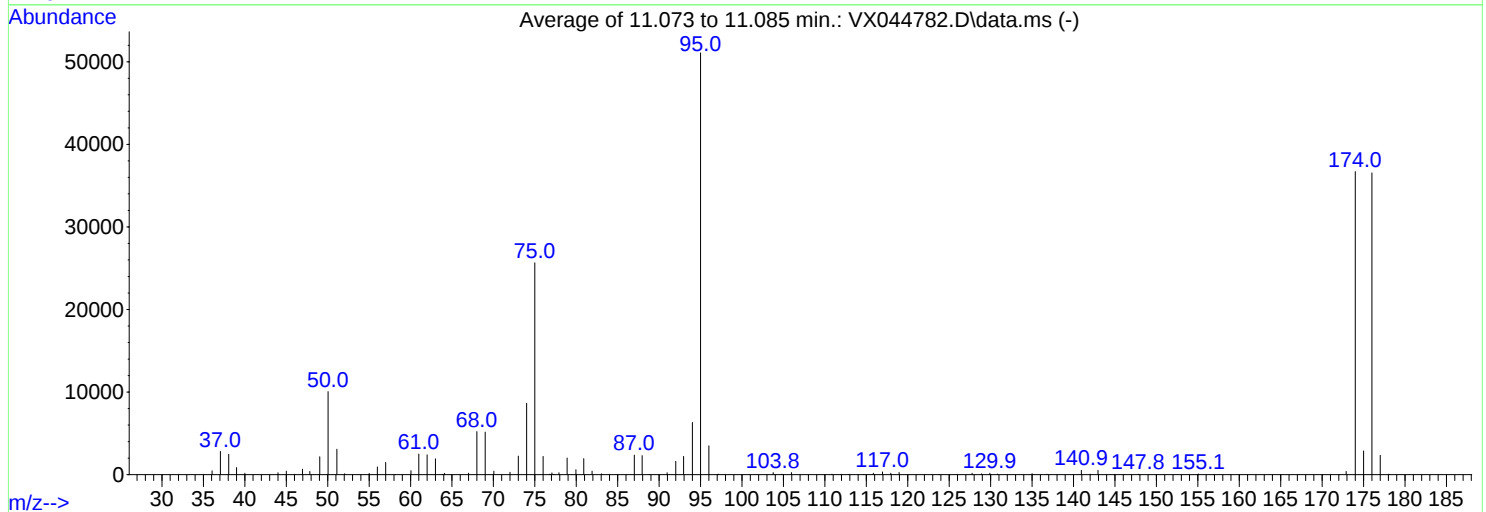


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX013125\
Data File : VX044782.D
Acq On : 31 Jan 2025 09:09
Operator : JC/MD
Sample : BFB716
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB716

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM012825WMA.M
Title : VOC Analysis
Last Update : Mon Feb 03 07:31:09 2025

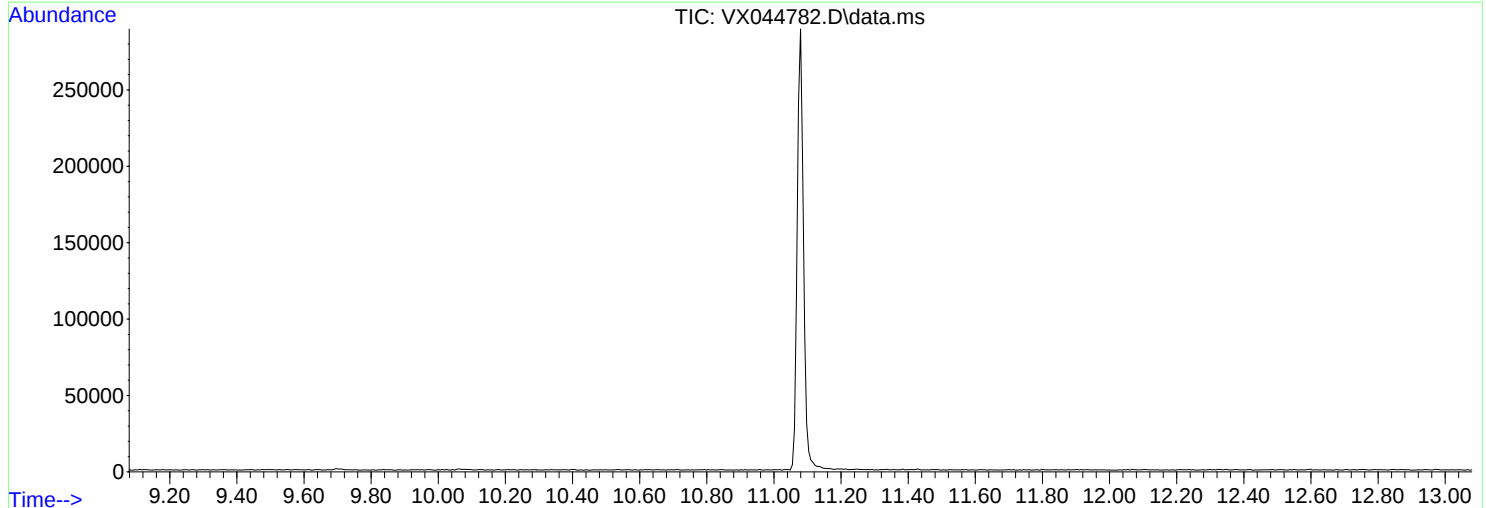

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	10062	PASS
75	95	30	80	50.2	25653	PASS
95	95	100	100	100.0	51085	PASS
96	95	5	9	6.8	3494	PASS
173	174	0.00	2	1.1	397	PASS
174	95	50	120	71.9	36712	PASS
175	174	5	9	7.8	2872	PASS
176	174	95	101	99.6	36552	PASS
177	176	5	9	6.4	2354	PASS

m/z	Abundance
39.00	75.0
40.00	751.0
41.10	94.0
44.00	517.0

Instrument :
MSVOA_X
ClientSampleId :
BFB716

m/z	Abundance
36.10	515.0
37.10	3162.0
38.00	2880.0
39.00	977.0
40.00	880.0
44.00	677.0
45.00	570.0
46.00	71.0
46.90	587.0
47.80	444.0
49.00	2267.0
50.10	11037.0
51.10	3490.0
52.00	125.0
55.00	197.0
56.00	1110.0
57.00	1590.0
58.20	70.0
60.00	531.0
61.00	2912.0
62.00	2520.0
63.00	2132.0
63.90	200.0
67.00	190.0
68.00	5476.0
69.00	5826.0
70.00	440.0
72.00	245.0
73.00	2374.0
74.00	9272.0
75.00	27168.0
76.00	2299.0
77.00	340.0
77.90	287.0
78.90	2008.0
79.90	591.0
80.90	2224.0
81.90	508.0
83.00	84.0
87.00	2459.0
88.00	2093.0
90.90	237.0
92.00	1717.0
93.00	2240.0
94.00	6293.0
95.00	51632.0
96.00	3819.0
97.00	121.0
103.80	253.0
104.80	114.0
105.90	298.0
110.90	75.0
114.70	83.0
115.90	168.0
117.00	301.0
118.00	153.0
119.00	260.0
127.80	162.0
128.80	125.0
129.90	214.0
130.80	69.0
135.00	79.0
136.80	62.0
140.90	560.0
142.00	98.0
142.90	504.0
144.90	53.0
146.10	54.0
147.80	81.0
154.90	102.0
172.10	68.0
172.90	357.0
174.00	31488.0
175.00	2616.0
176.00	31128.0
177.00	2161.0
178.10	63.0

Instrument :
MSVOA_X
ClientSampleId :
BFB716

m/z	Abundance
36.10	562.0
37.10	3148.0
38.10	2931.0
39.00	1233.0
40.00	993.0
44.00	904.0
45.00	429.0
46.00	55.0
47.00	747.0
47.90	506.0
49.10	2578.0
50.00	11896.0
51.10	3635.0
52.10	134.0
55.00	126.0
56.00	1076.0
57.00	1753.0
60.10	518.0
61.00	2857.0
62.00	2805.0
63.00	2151.0
64.10	165.0
66.90	234.0
68.00	6290.0
69.00	5831.0
70.10	528.0
72.00	394.0
73.00	2703.0
74.00	10108.0
75.00	30064.0
76.00	2648.0
77.10	292.0
78.00	308.0
78.90	2520.0
80.00	768.0
80.90	2189.0
81.90	467.0
83.10	84.0
87.00	2701.0
88.00	2964.0
88.80	53.0
91.00	247.0
92.00	1847.0
93.00	2705.0
94.00	7632.0
95.00	61216.0
96.00	4193.0
97.20	132.0
103.80	254.0
104.80	71.0
106.00	222.0
110.80	86.0
112.90	51.0
114.70	64.0
115.80	265.0
116.90	316.0
117.90	227.0
118.90	276.0
123.80	68.0
127.70	203.0
128.90	121.0
129.90	208.0
130.80	81.0
135.00	101.0
136.80	87.0
140.90	615.0
142.00	66.0
143.00	634.0
145.00	63.0
147.80	104.0
155.10	120.0
156.90	58.0
172.70	293.0
173.00	304.0
174.00	44128.0
175.00	3398.0
176.00	44240.0
177.00	2710.0
178.00	84.0

Instrument :
MSVOA_X
ClientSampleId :
BFB716

m/z	Abundance
35.90	309.0
37.00	2116.0
38.00	1600.0
39.00	549.0
40.00	931.0
44.00	644.0
45.00	305.0
47.00	636.0
47.90	237.0
49.00	1661.0
50.00	7253.0
51.00	2107.0
52.00	69.0
55.00	168.0
56.00	596.0
57.00	1070.0
60.00	419.0
61.00	1731.0
62.00	1885.0
63.00	1447.0
64.10	276.0
67.10	85.0
68.00	3865.0
69.00	3833.0
70.00	339.0
72.00	221.0
73.00	1680.0
74.00	6552.0
75.00	19728.0
76.00	1666.0
76.80	187.0
77.30	127.0
77.80	133.0
78.90	1529.0
80.00	418.0
81.00	1418.0
81.90	330.0
83.00	108.0
87.00	1948.0
87.90	1856.0
90.90	219.0
92.00	1239.0
92.90	1697.0
94.00	5030.0
95.00	40408.0
96.00	2469.0
97.10	69.0
103.70	279.0
105.90	255.0
111.90	61.0
112.90	51.0
115.80	111.0
116.90	352.0
118.00	162.0
118.90	290.0
127.70	149.0
129.00	70.0
129.90	122.0
130.80	106.0
135.00	146.0
141.00	425.0
143.00	428.0
148.00	93.0
155.10	92.0
173.00	238.0
174.00	34520.0
175.00	2602.0
176.00	34288.0
177.00	2190.0
178.00	51.0

Instrument :
MSVOA_X
ClientSampleId :
BFB716