



Dichlorodifluoromethane

Response Ratio

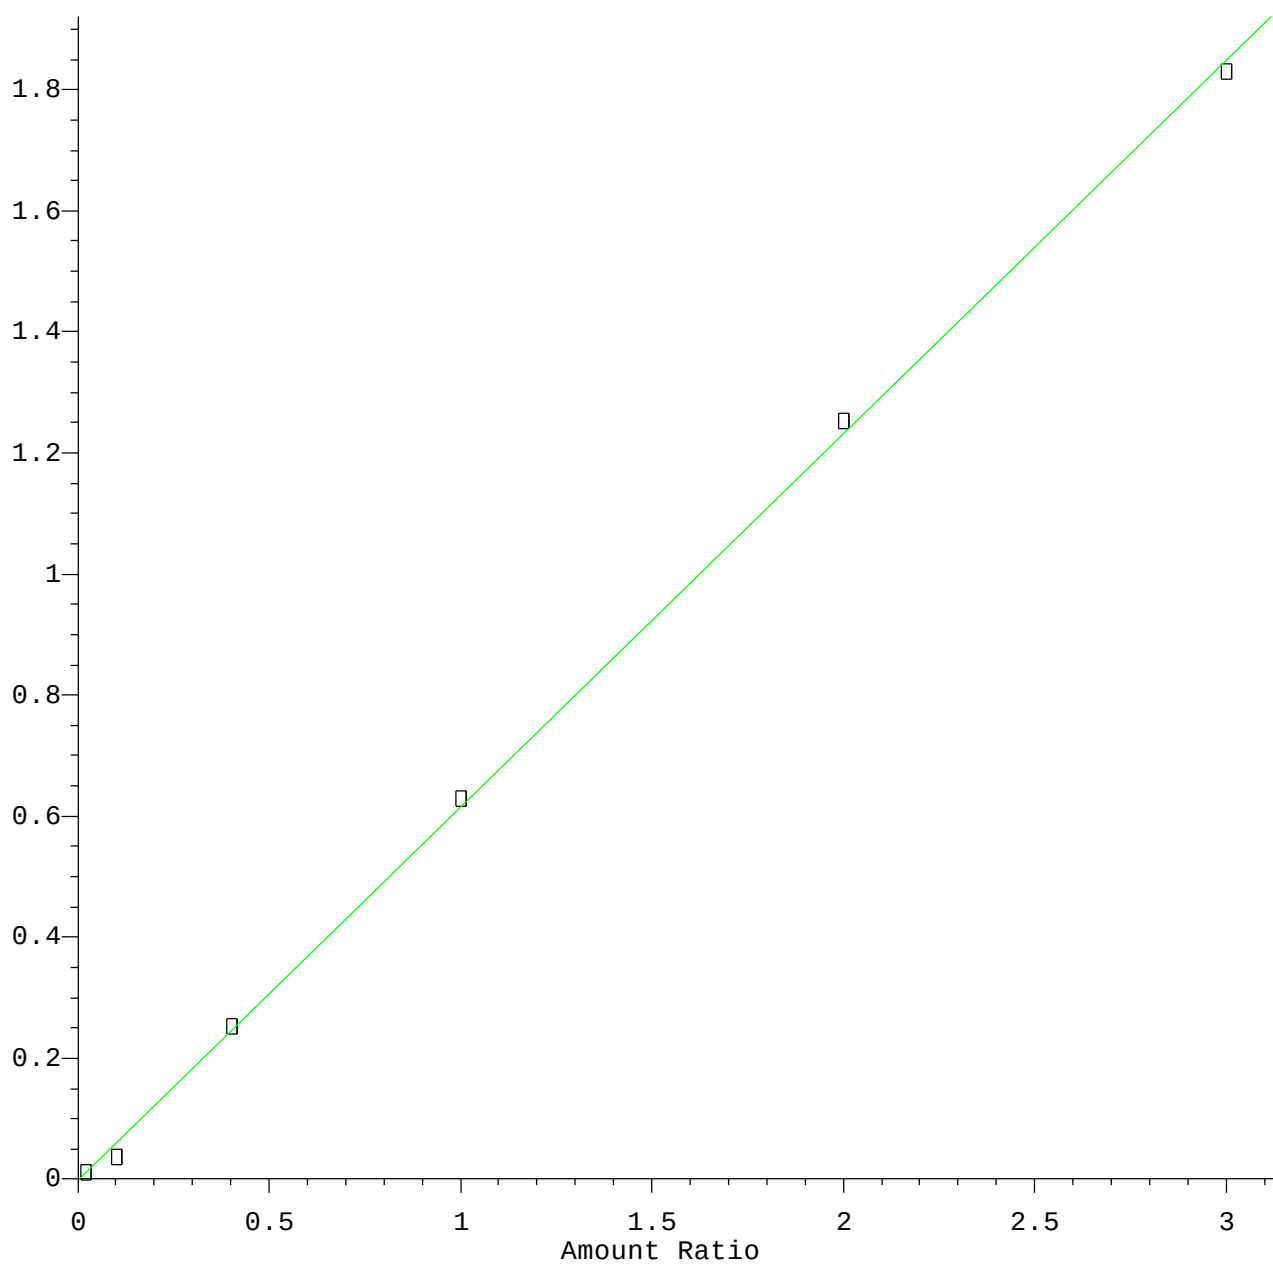


Resp Ratio = $6.17 \times 10^{-1} \times \text{Amt} - 2.19 \times 10^{-3}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
Calibration Table Last Updated: Sat Feb 02 01:32:36 2019

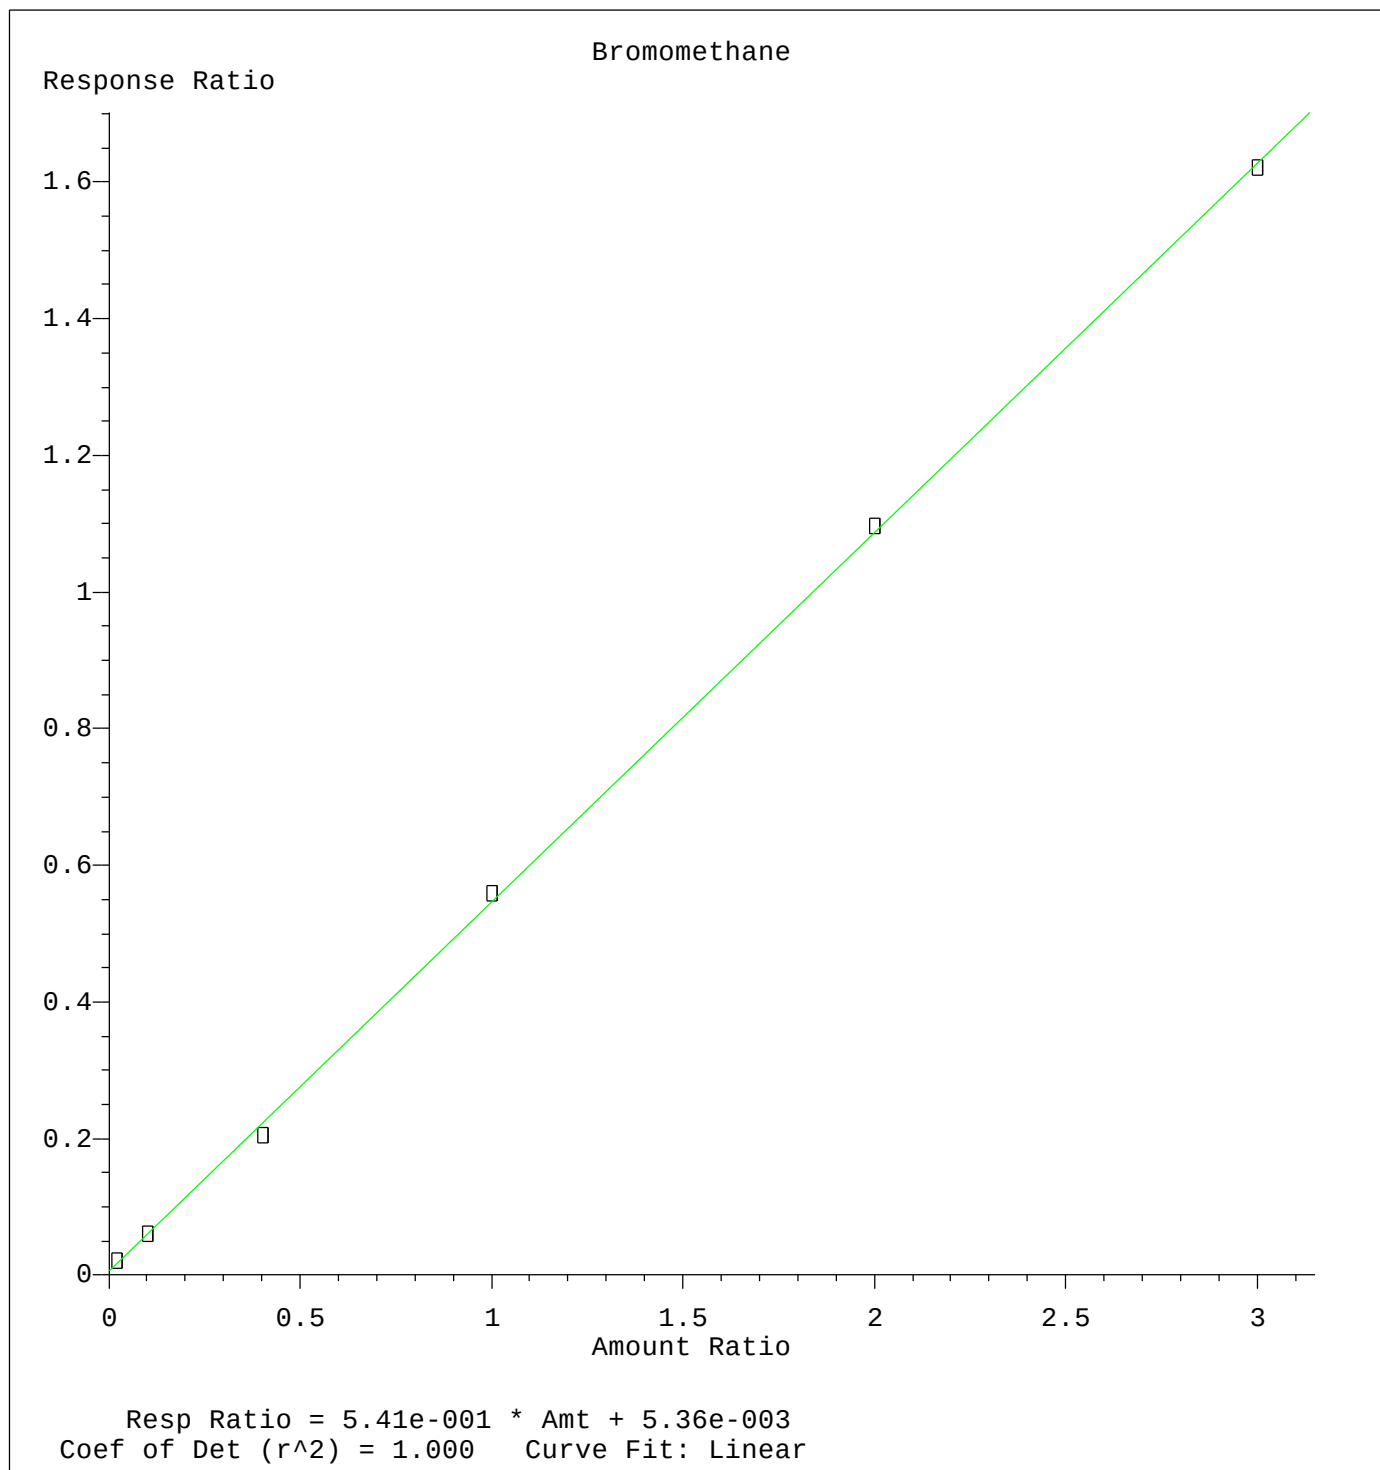


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
Calibration Table Last Updated: Sat Feb 02 01:32:36 2019

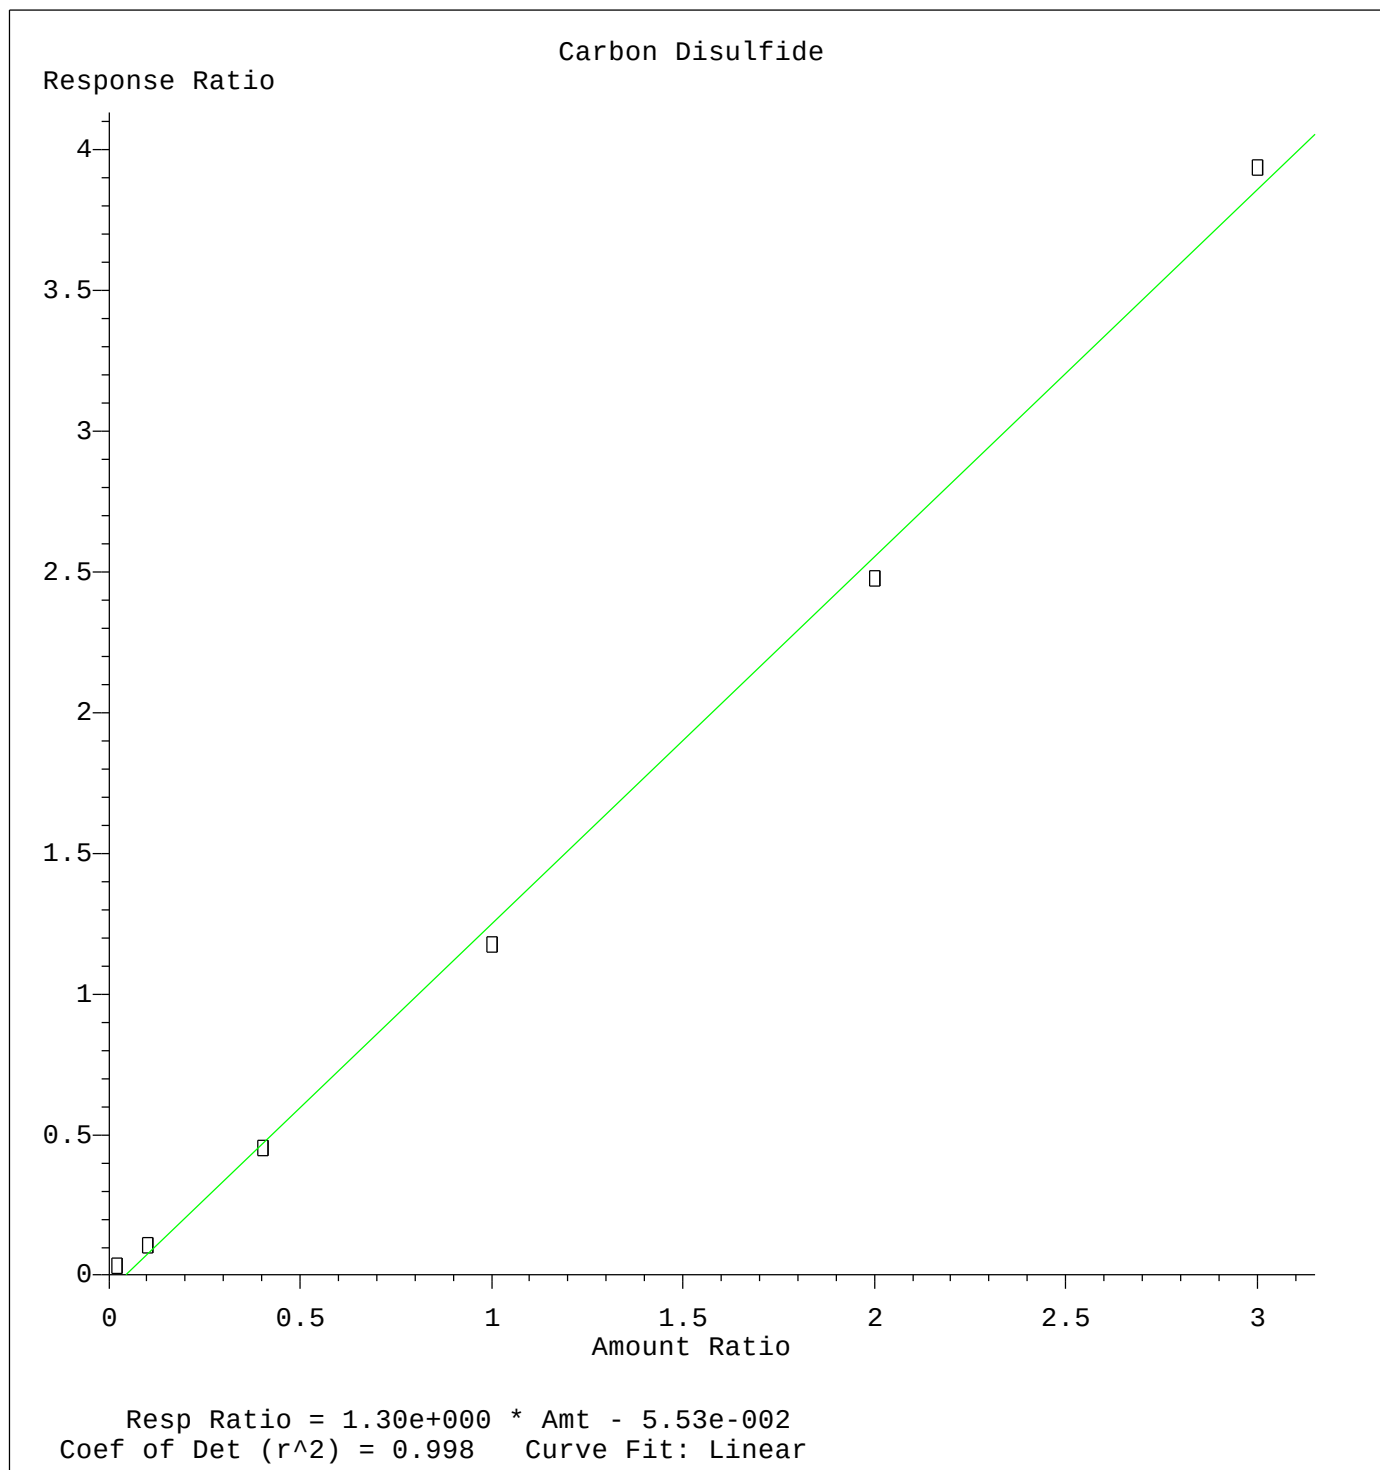


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
Calibration Table Last Updated: Sat Feb 02 01:32:36 2019

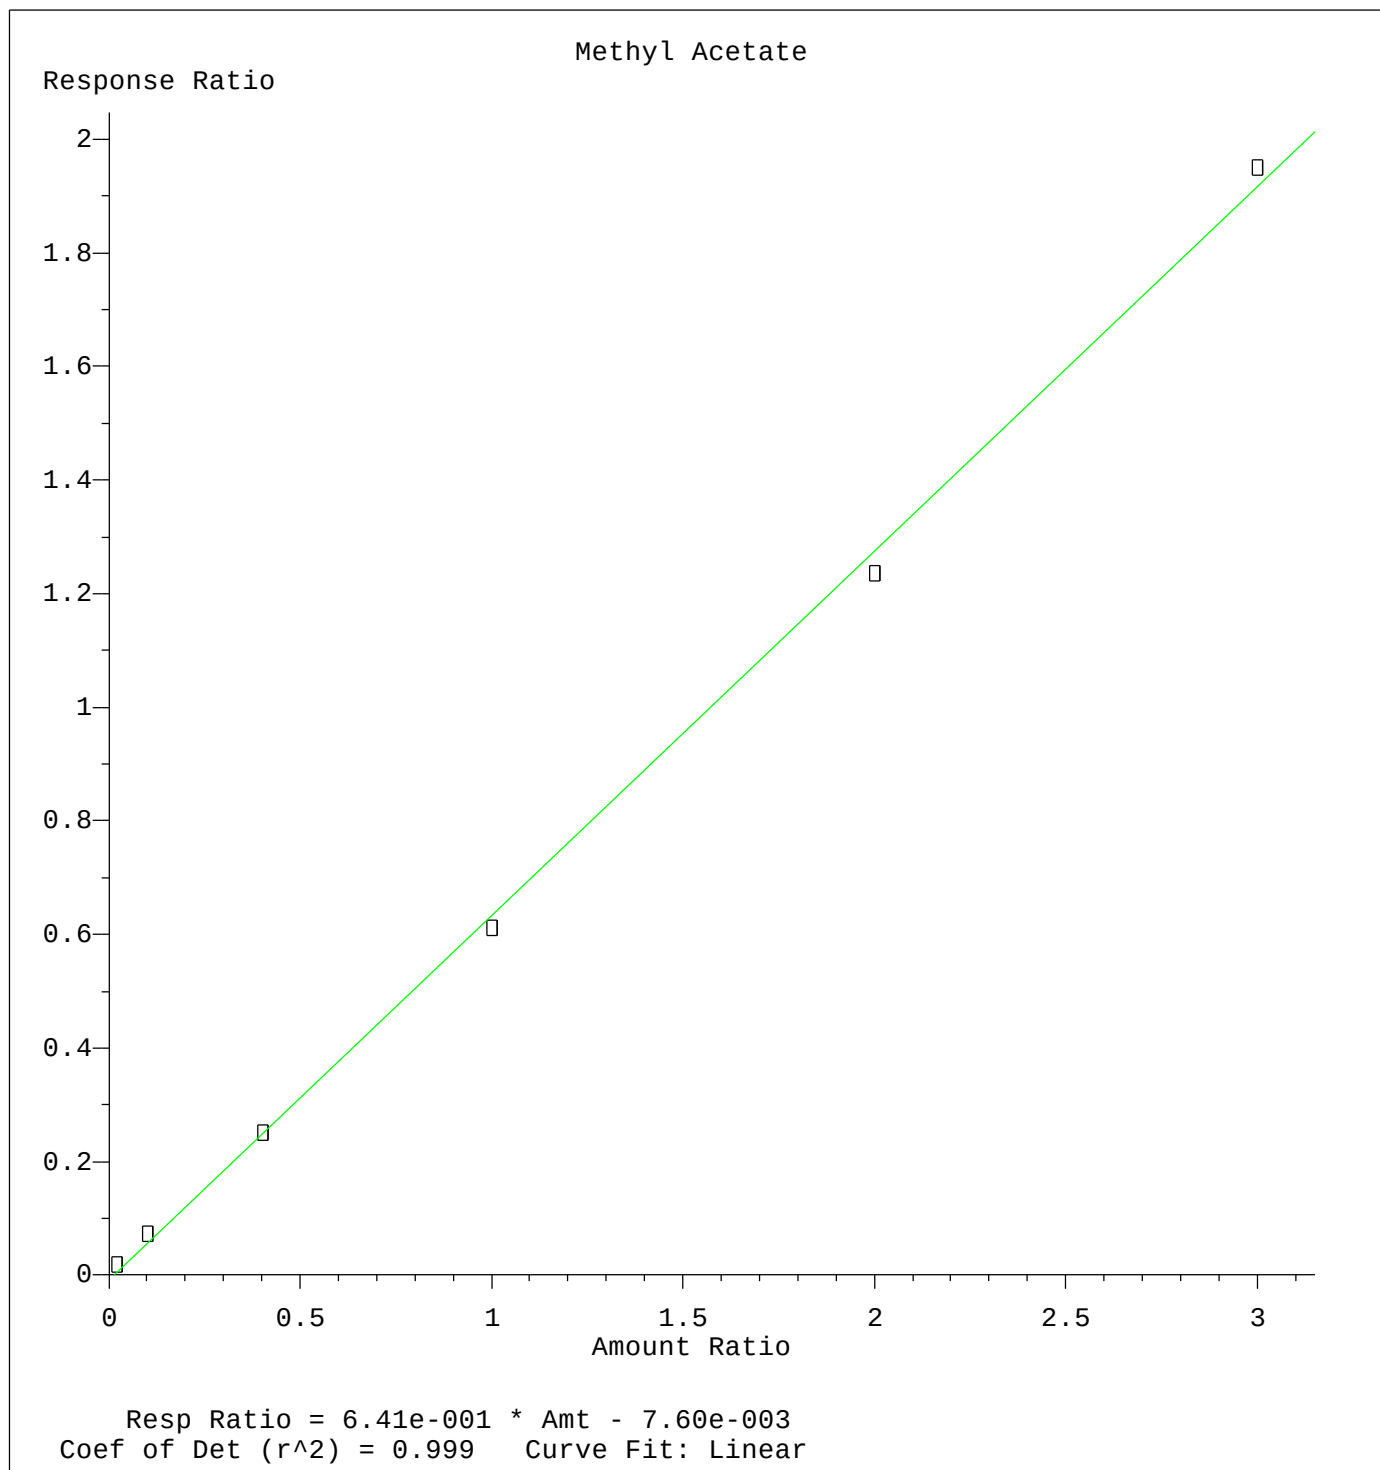


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
Calibration Table Last Updated: Sat Feb 02 01:32:36 2019

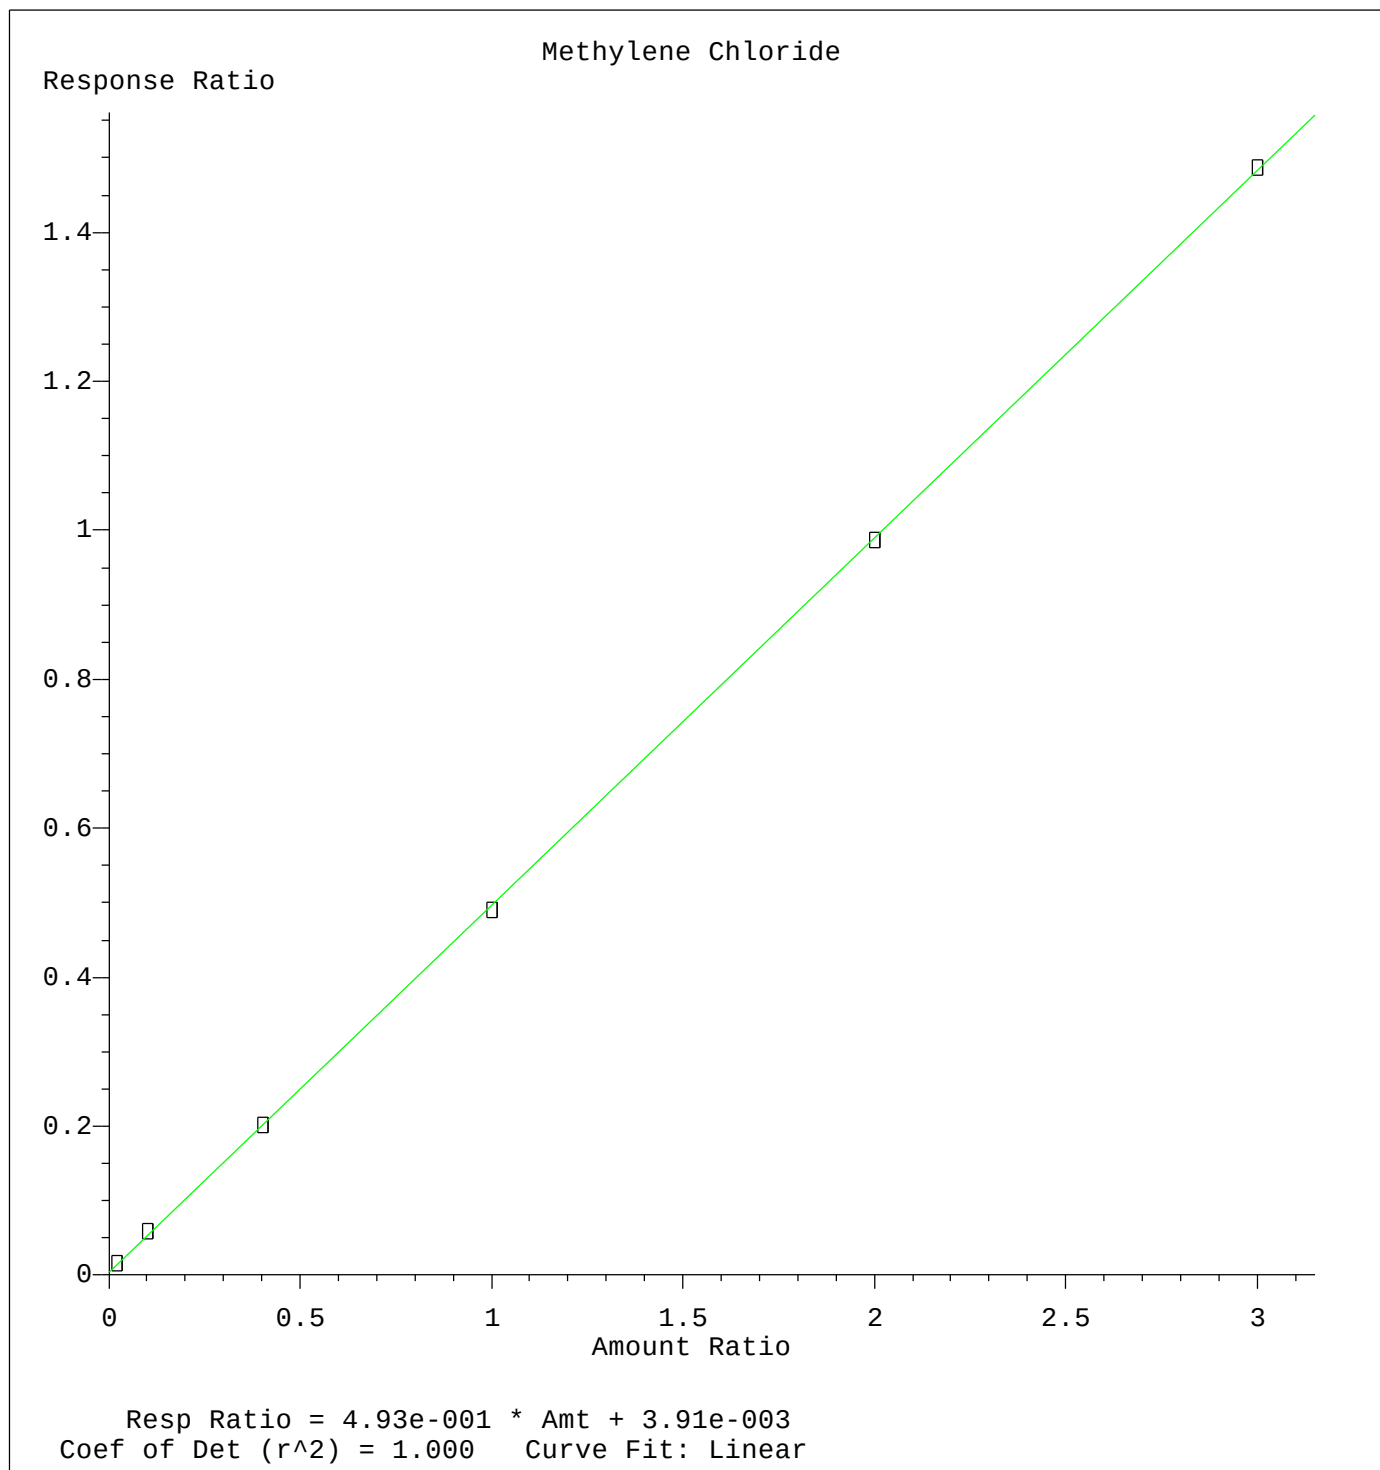

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
Calibration Table Last Updated: Sat Feb 02 01:32:36 2019

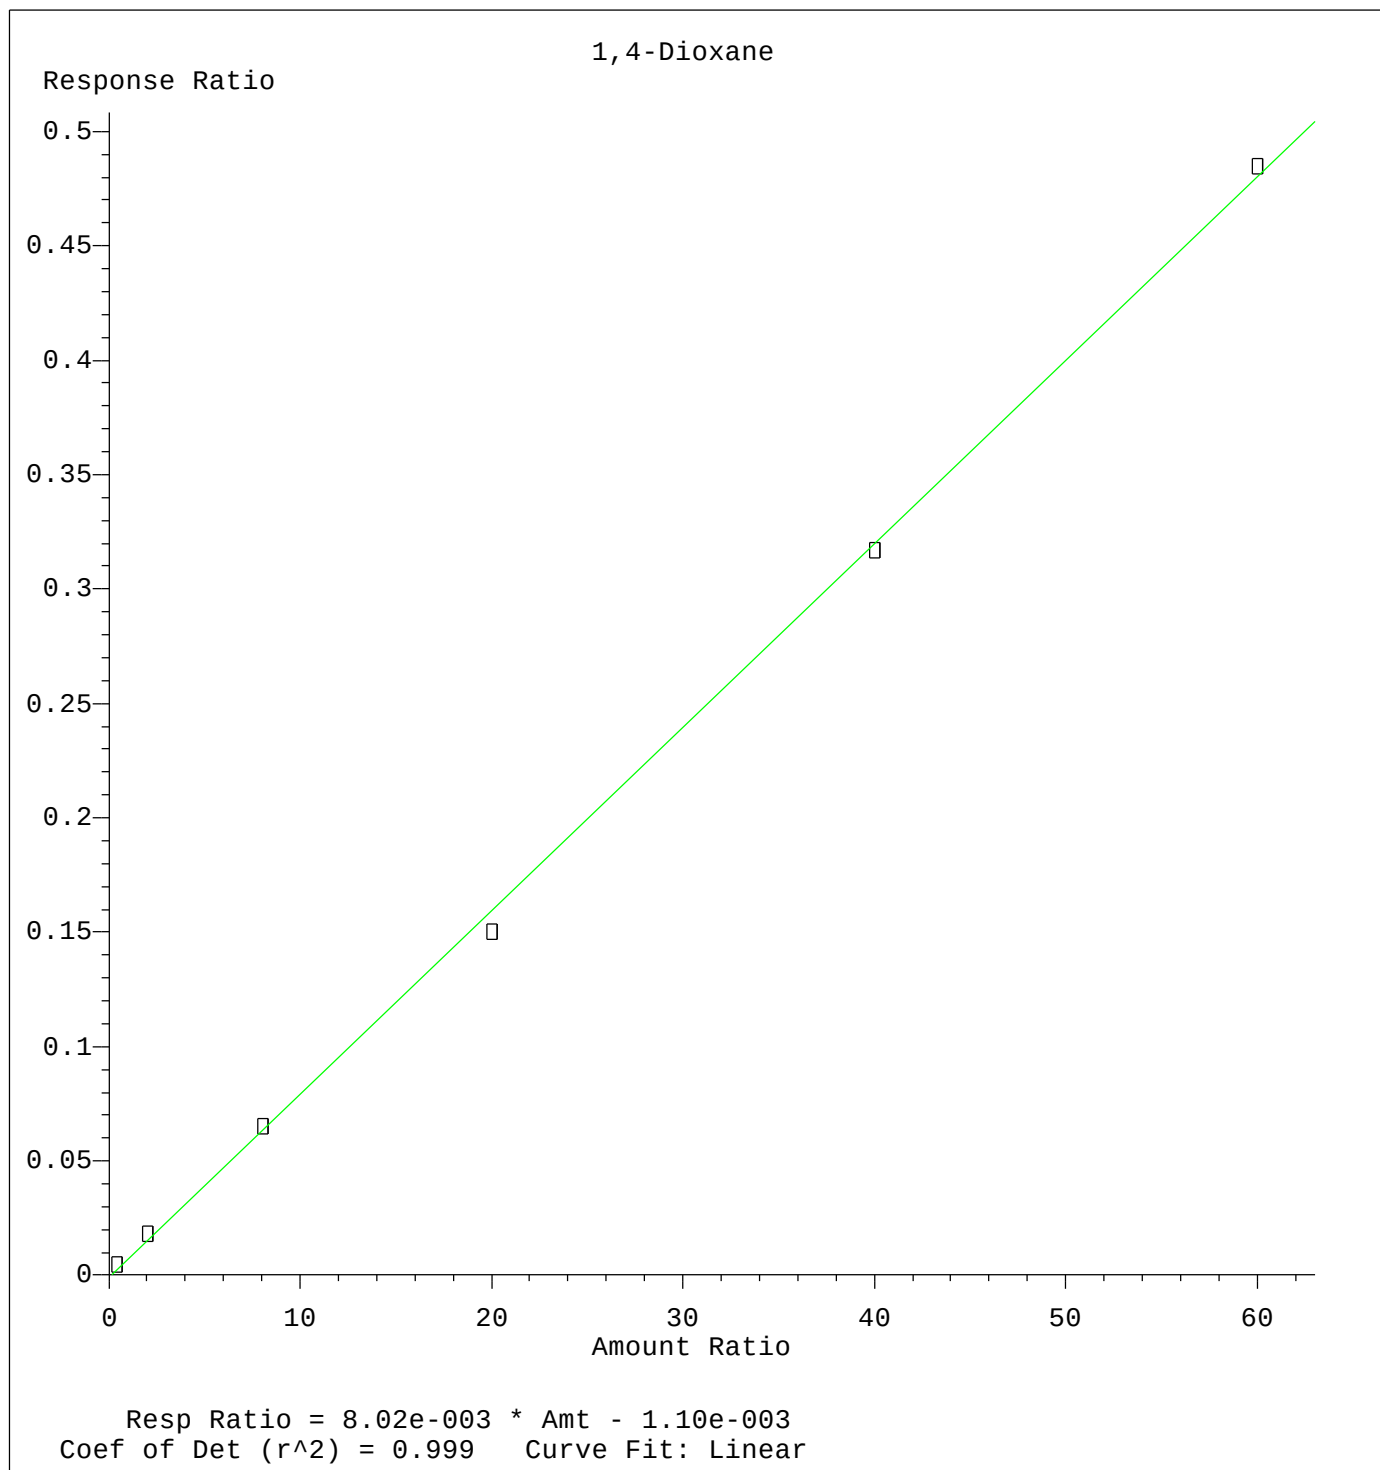


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
Calibration Table Last Updated: Sat Feb 02 01:32:36 2019

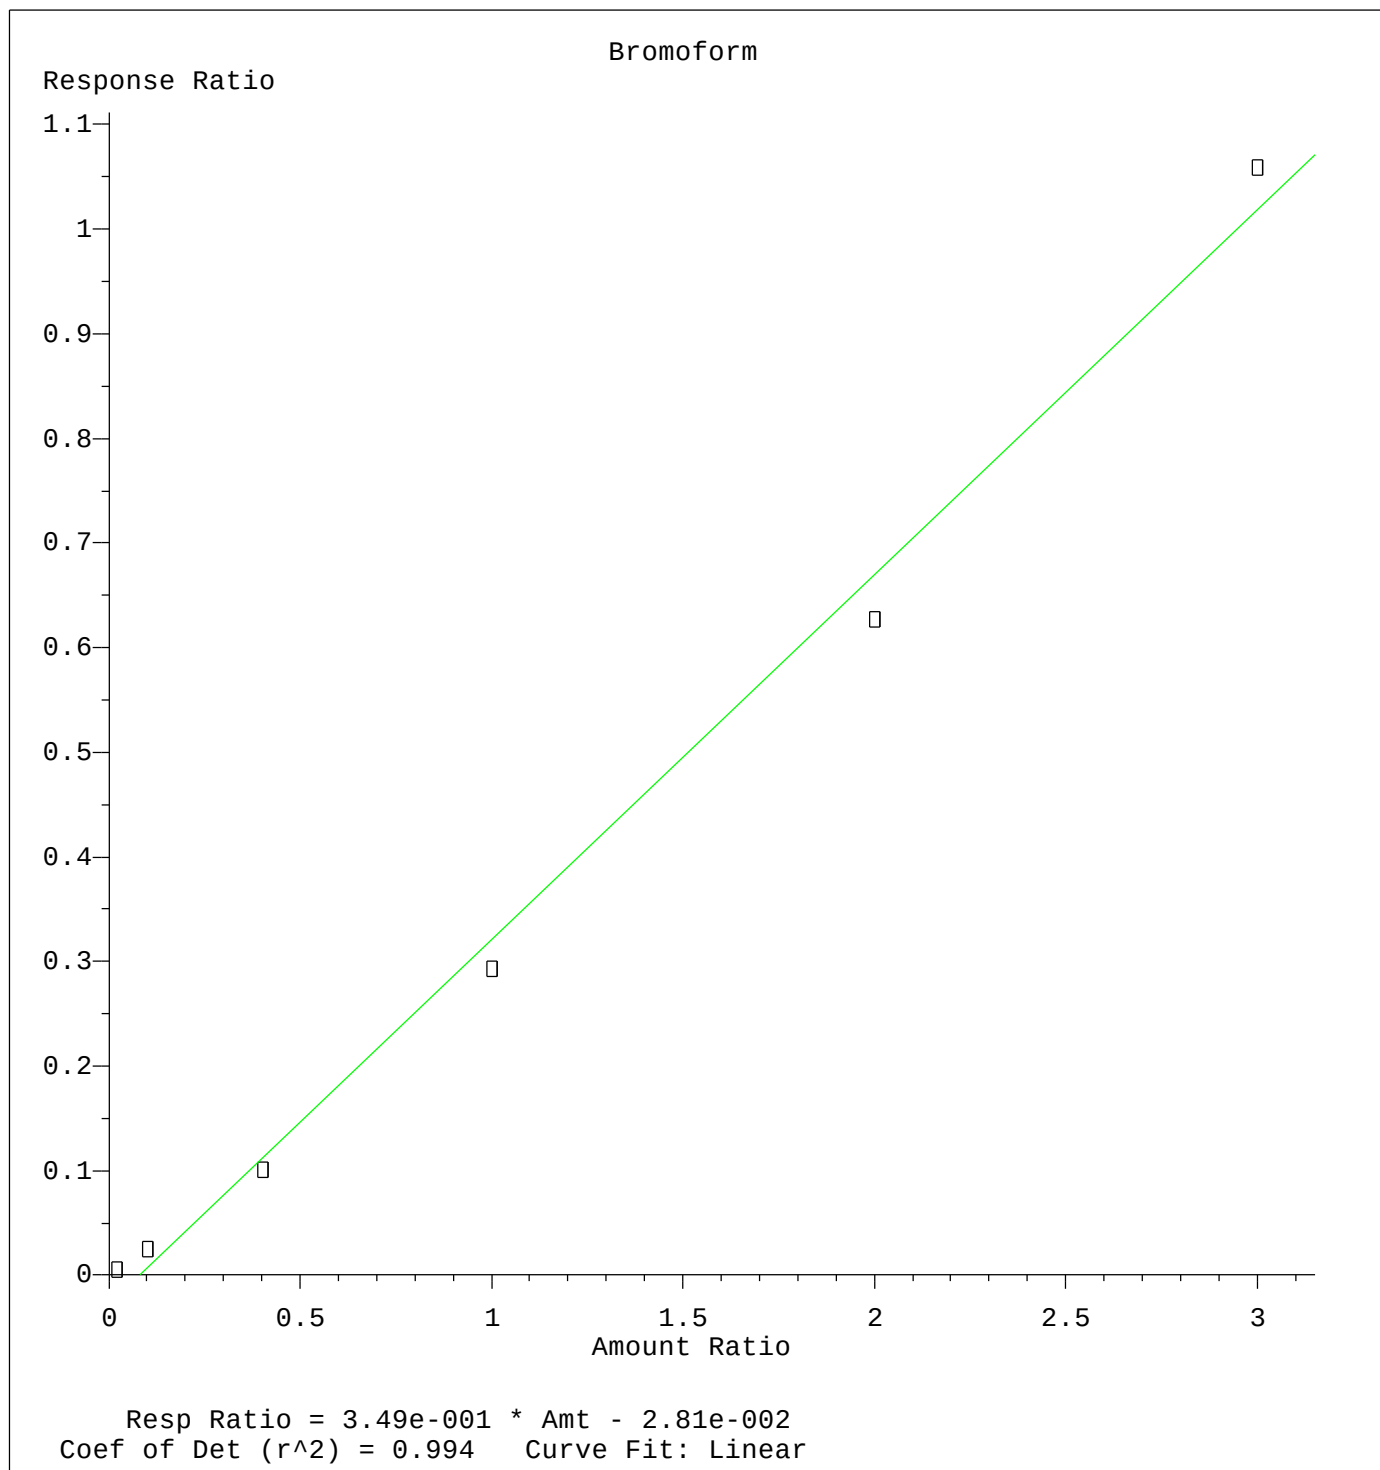

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
Calibration Table Last Updated: Sat Feb 02 01:32:36 2019

trans-1,4-Dichloro-2-butene

Response Ratio

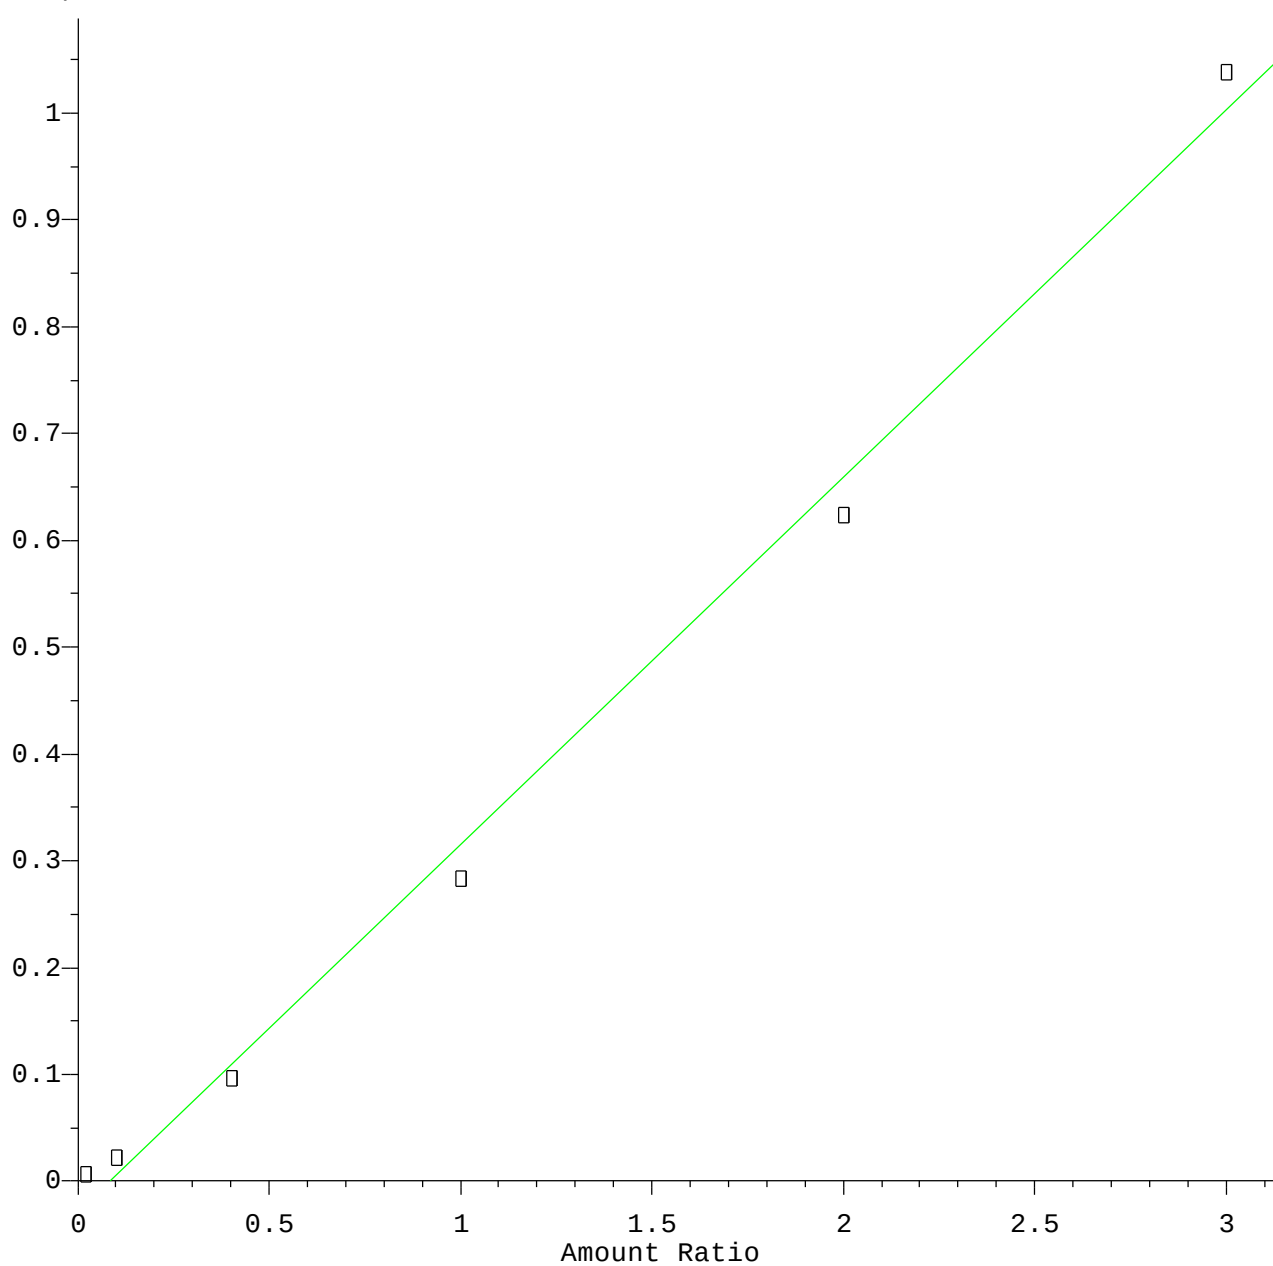

Resp Ratio = $3.44 \times 10^{-1} \times \text{Amt} - 2.91 \times 10^{-2}$
Coef of Det (r^2) = 0.994 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
Calibration Table Last Updated: Sat Feb 02 01:32:36 2019