

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX020119\
 Data File : VX007345.D
 Acq On : 01 Feb 2019 19:06
 Operator : JC/SP
 Sample : K1296-03
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-TT-MW202S-20190129

Quant Time: Feb 04 09:47:03 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
 Quant Title : SW846 8260
 QLast Update : Sat Feb 02 01:32:36 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	490745	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	773895	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	737342	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	363384	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.07	65	267920	51.44	ug/l	0.00
Spiked Amount			Recovery	=	102.88%	
35) Dibromofluoromethane	5.51	113	243390	48.34	ug/l	0.00
Spiked Amount			Recovery	=	96.68%	
50) Toluene-d8	8.71	98	935426	50.07	ug/l	0.00
Spiked Amount			Recovery	=	100.14%	
62) 4-Bromofluorobenzene	11.13	95	337746	49.52	ug/l	0.00
Spiked Amount			Recovery	=	99.04%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX020119\
Data File : VX007345.D
Acq On : 01 Feb 2019 19:06
Operator : JC/SP
Sample : K1296-03
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-MW202S-20190129

Quant Time: Feb 04 09:47:03 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
Quant Title : SW846 8260
QLast Update : Sat Feb 02 01:32:36 2019
Response via : Initial Calibration

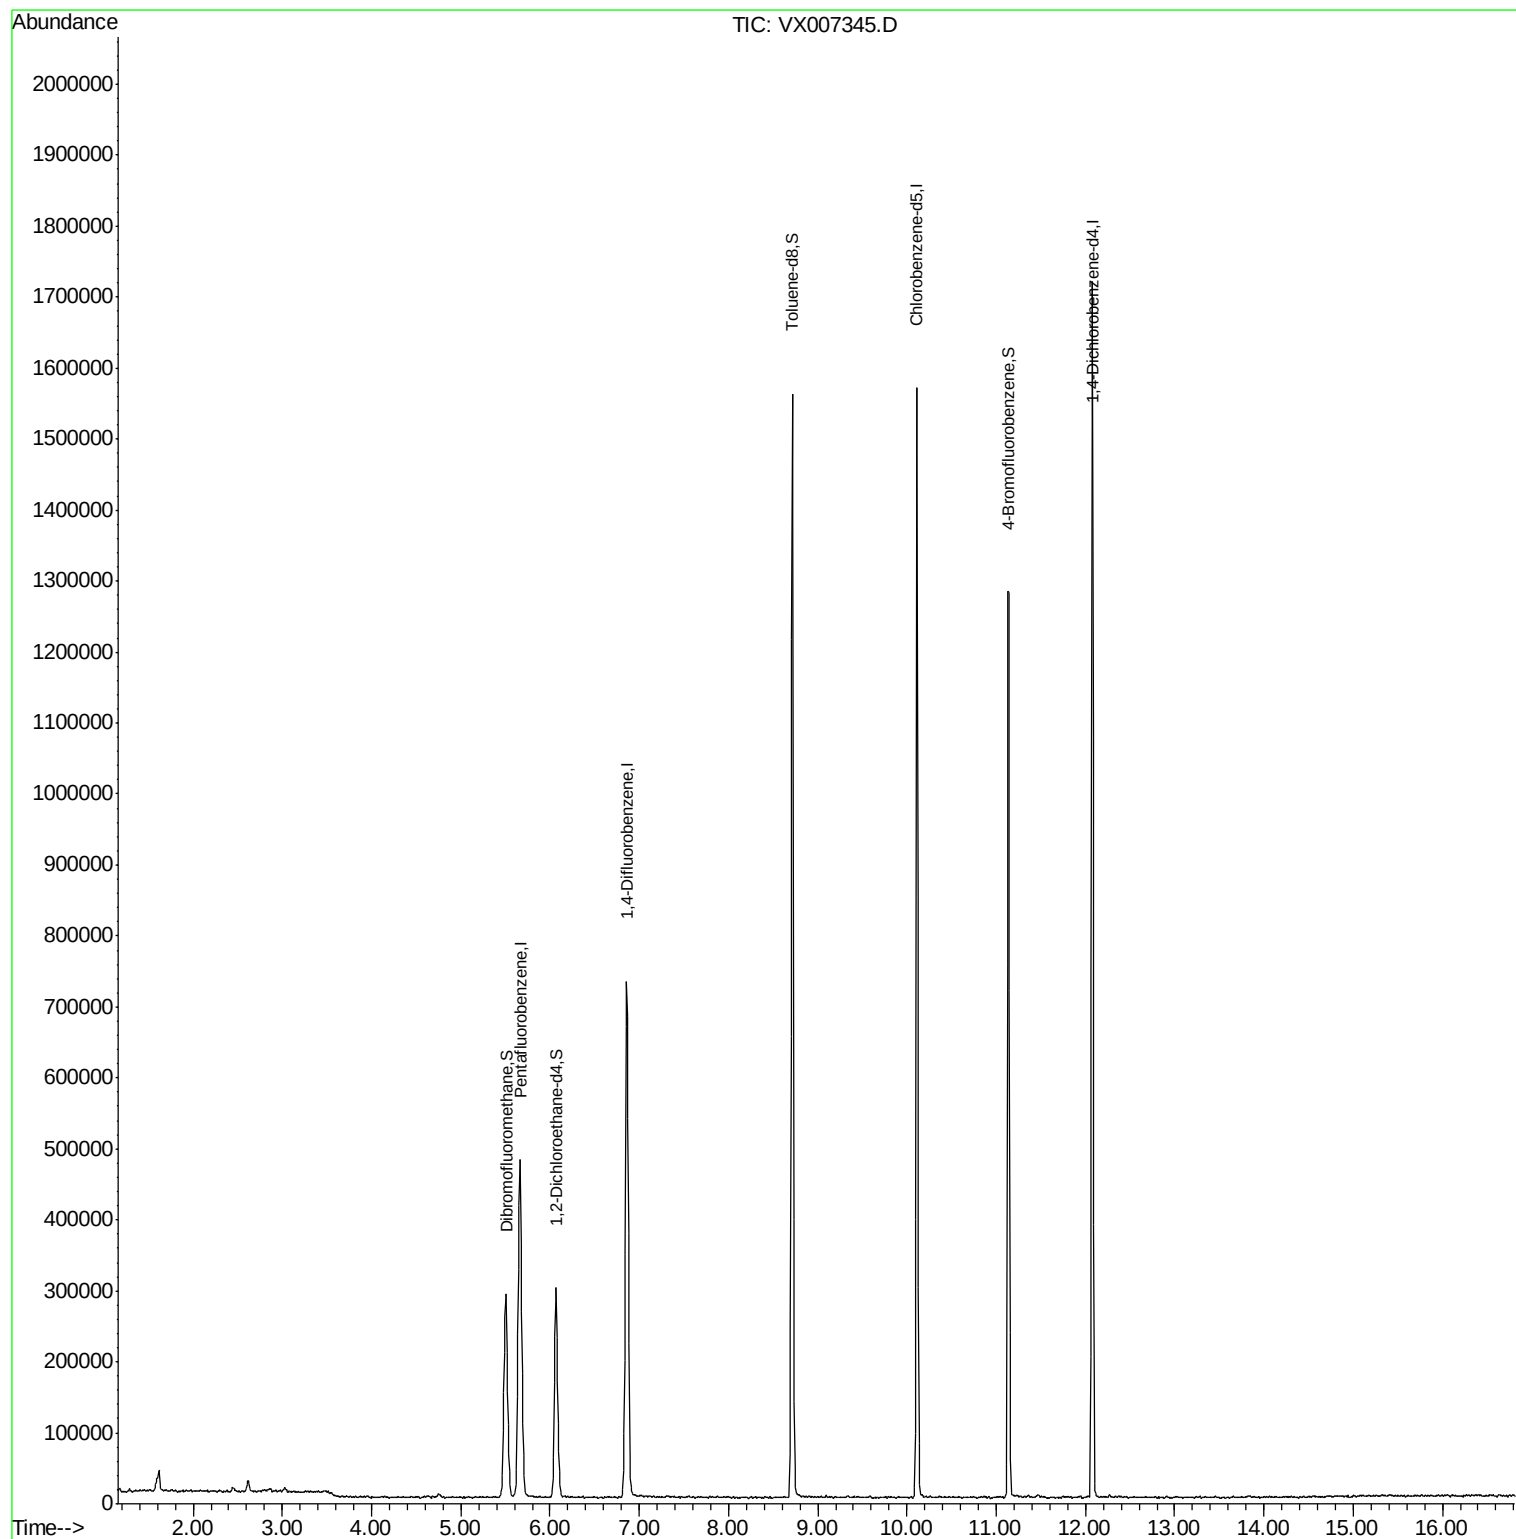

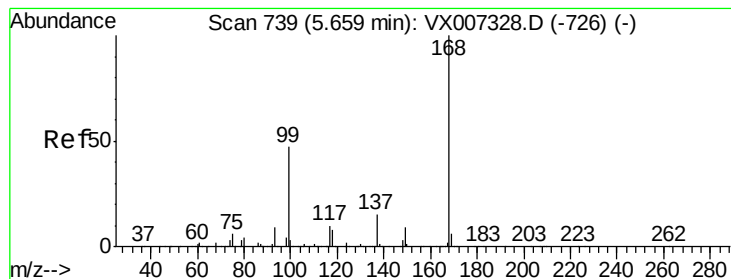

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.01 min

Lab File: VX007345.D

Acq: 01 Feb 2019 19:06

Instrument :

MSVOA_X

ClientSampleId :


BP-TT-MW202S-20190129

Tot Ion:168 Resp: 490745

Ion Ratio Lower Upper

168 100

99 49.2 37.9 56.9

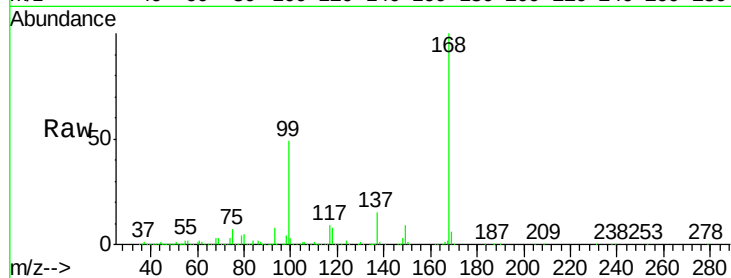

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

200000



150000

100000

50000

0

Time--> 5.50 5.60 5.70 5.80

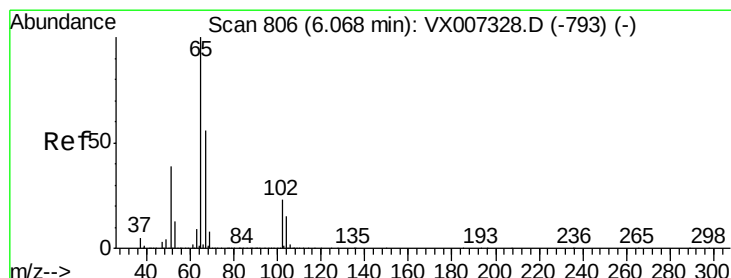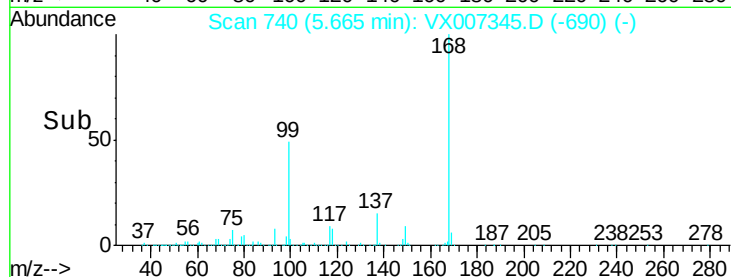

#33

1,2-Dichloroethane-d4

Concen: 51.435 ug/l

RT: 6.07 min Scan# 806

Delta R.T. 0.00 min

Lab File: VX007345.D


Acq: 01 Feb 2019 19:06

Tgt Ion: 65 Resp: 267920

Ion Ratio Lower Upper

65 100

67 54.5 0.0 108.8

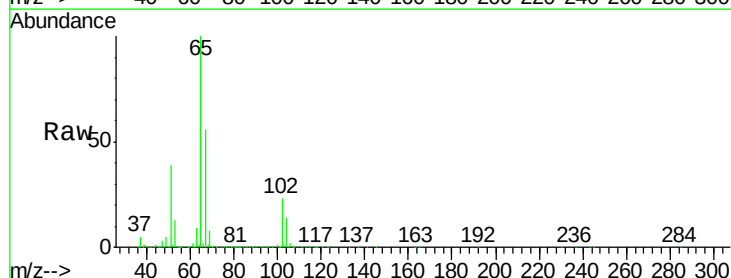

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.07

120000

100000

80000


60000


40000

20000

0

Time--> 6.00 6.10 6.20




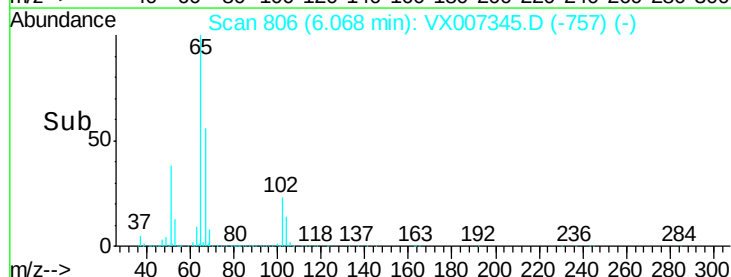


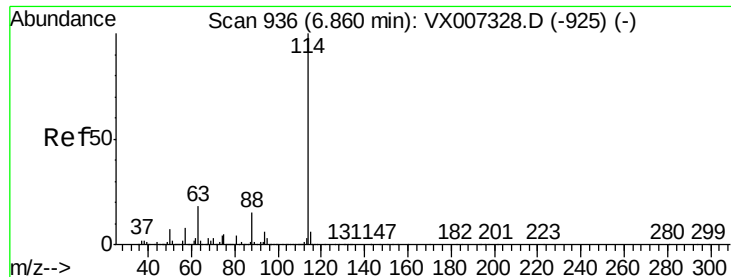

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.86 min Scan# 936
 Delta R.T. 0.00 min
 Lab File: VX007345.D
 Acq: 01 Feb 2019 19:06




Instrument :
 MSVOA_X
 ClientSampleId :
 BP-TT-MW202S-20190129


Tot Ion	Ratio	Lower	Upper
114	100		
63	17.9	0.0	35.6
88	15.1	0.0	29.6

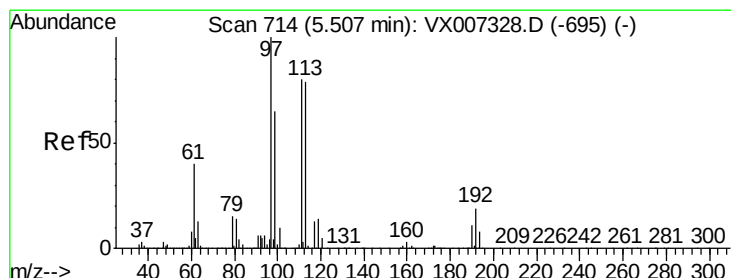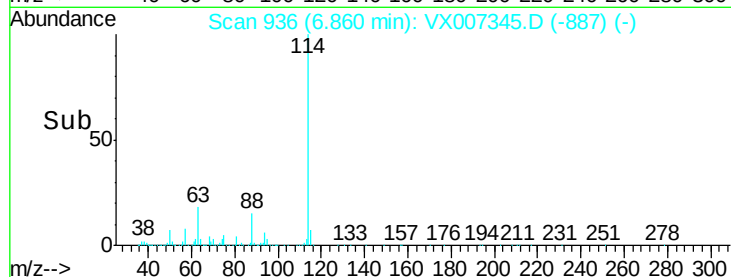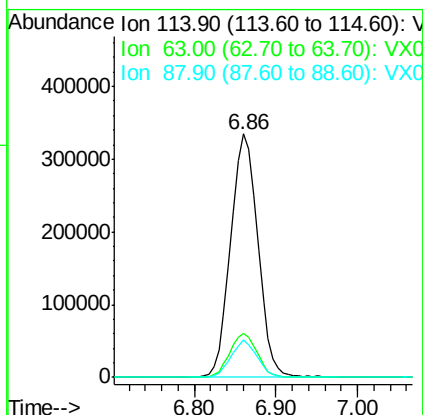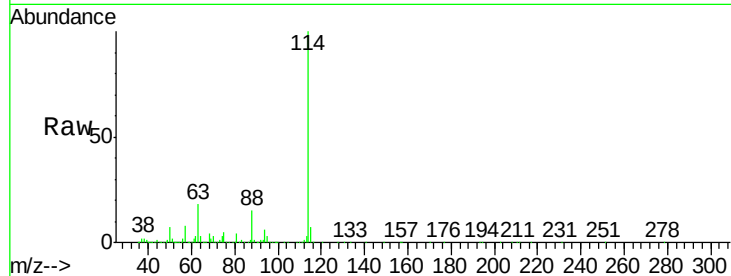

#35
 Dibromofluoromethane
 Concen: 48.335 ug/l
 RT: 5.51 min Scan# 714
 Delta R.T. 0.00 min
 Lab File: VX007345.D
 Acq: 01 Feb 2019 19:06

Tgt Ion	Ratio	Lower	Upper
113	100		
111	102.8	81.8	122.8
192	21.7	18.5	27.7


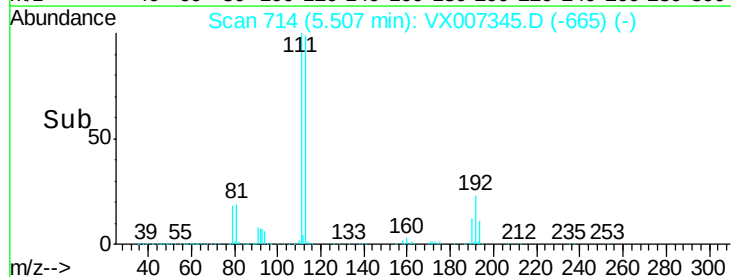
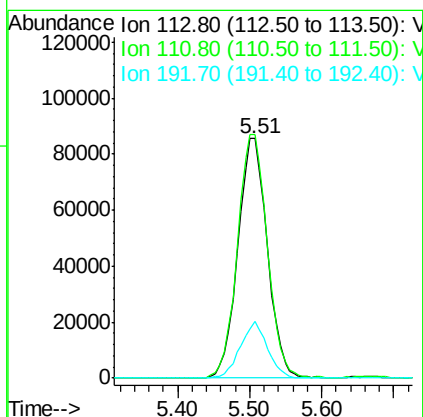
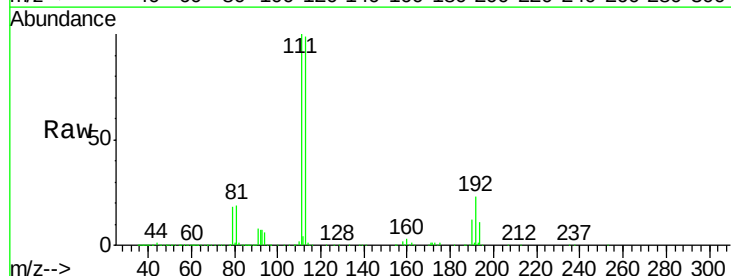


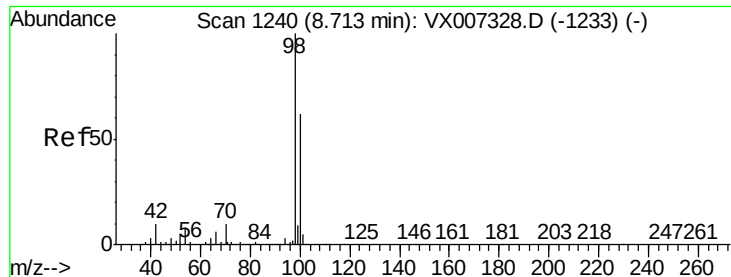

#50
Toluene-d8
Concen: 50.070 ug/l
RT: 8.71 min Scan# 1240
Delta R.T. 0.00 min
Lab File: VX007345.D
Acq: 01 Feb 2019 19:06




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-MW202S-20190129


Tot Ion: 98 Resp: 935426
Ion Ratio Lower Upper
98 100
100 64.4 51.6 77.4

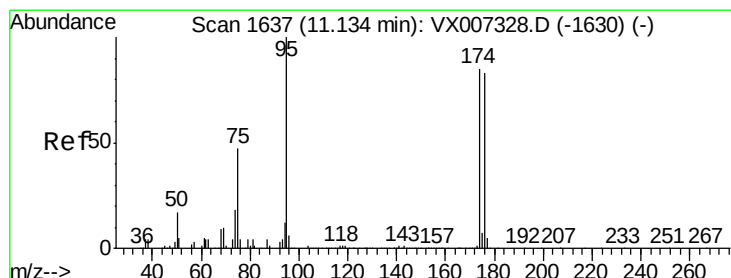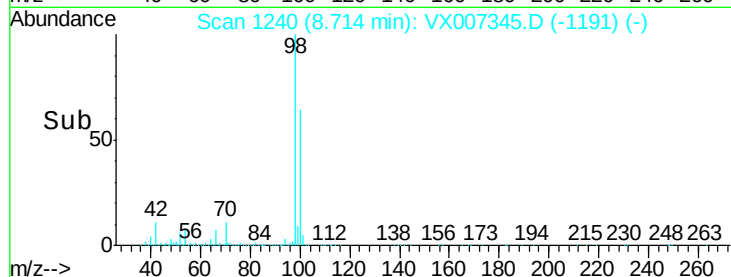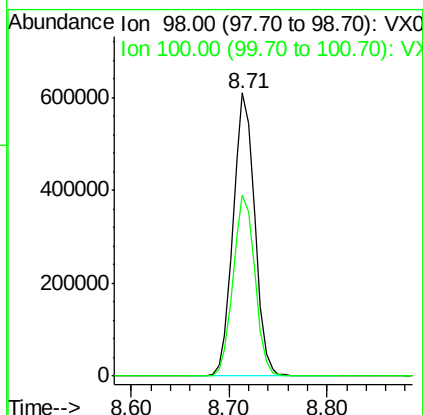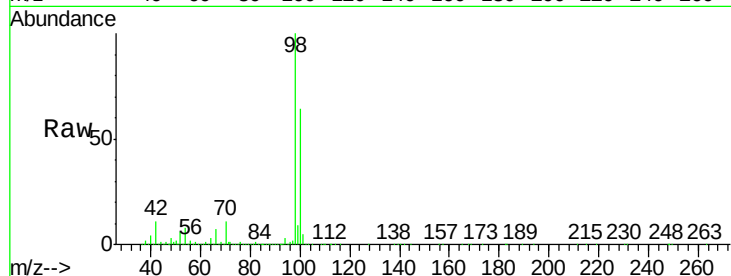

#62
4-Bromofluorobenzene
Concen: 49.516 ug/l
RT: 11.13 min Scan# 1637
Delta R.T. 0.00 min
Lab File: VX007345.D
Acq: 01 Feb 2019 19:06

Tgt Ion: 95 Resp: 337746
Ion Ratio Lower Upper
95 100
174 91.5 0.0 189.2
176 88.4 0.0 186.2


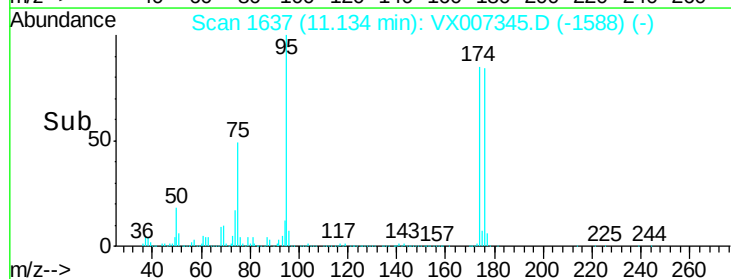
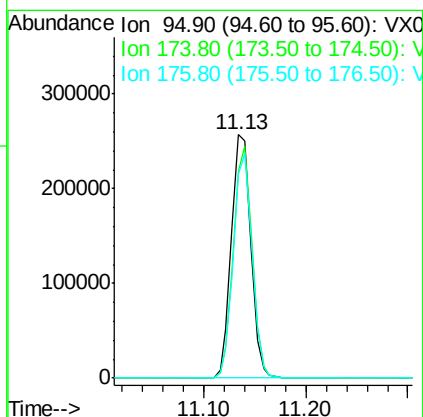
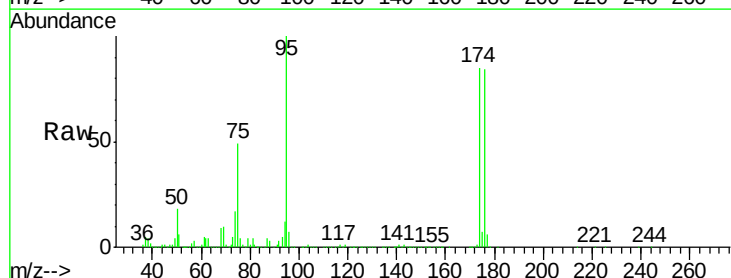


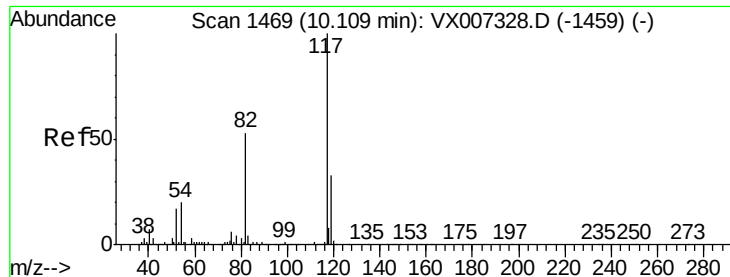

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1469
Delta R.T. 0.00 min
Lab File: VX007345.D
Acq: 01 Feb 2019 19:06

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-MW202S-20190129

Tot Ion:117 Resp: 737342
Ion Ratio Lower Upper
117 100
82 52.9 42.1 63.1
119 32.0 26.5 39.7

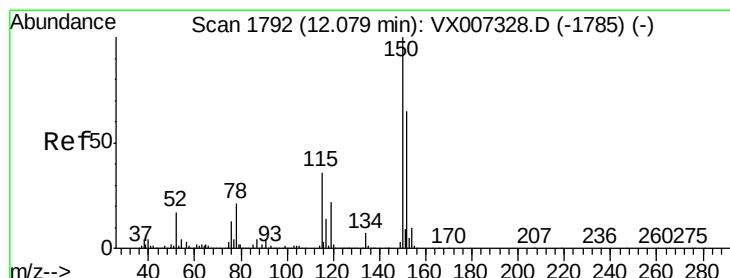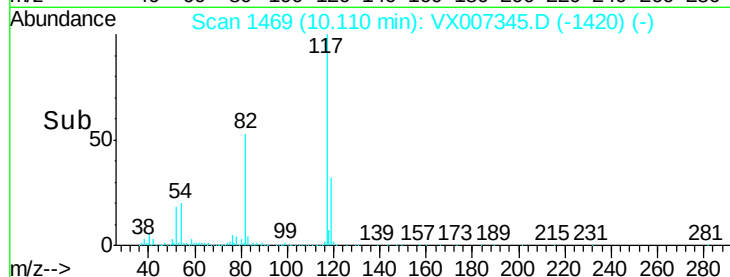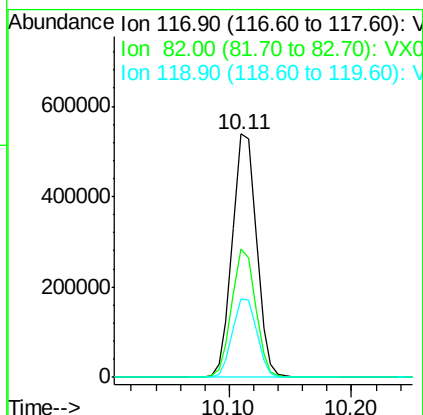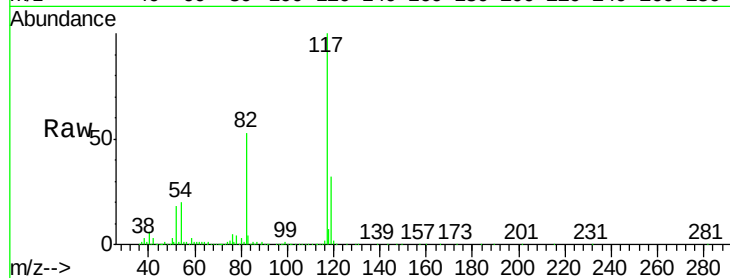

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. 0.00 min
Lab File: VX007345.D
Acq: 01 Feb 2019 19:06

Tgt Ion:152 Resp: 363384
Ion Ratio Lower Upper
152 100
115 55.4 38.0 114.0
150 156.9 0.0 346.4

