

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020122\
 Data File : VX026704.D
 Acq On : 01 Feb 2022 14:11
 Operator : JC/MD
 Sample : N1325-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TEX-3

Quant Time: Feb 02 04:35:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 11 14:45:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	132536	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	222830	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	199334	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	84046	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	84734	45.767	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	91.540%
35) Dibromofluoromethane	5.391	113	68835	47.836	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	95.680%
50) Toluene-d8	8.653	98	260679	50.272	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	100.540%
62) 4-Bromofluorobenzene	11.085	95	92834	50.397	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	100.800%
Target Compounds						
					Qvalue	
16) Acetone	2.386	43	10852	11.494	ug/l	97
20) Methylene Chloride	2.794	84	1749	1.121	ug/l	96
43) Isopropyl Acetate	6.342	43	11509	3.101	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020122\
Data File : VX026704.D
Acq On : 01 Feb 2022 14:11
Operator : JC/MD
Sample : N1325-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TEX-3


Quant Time: Feb 02 04:35:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 11 14:45:13 2022
Response via : Initial Calibration

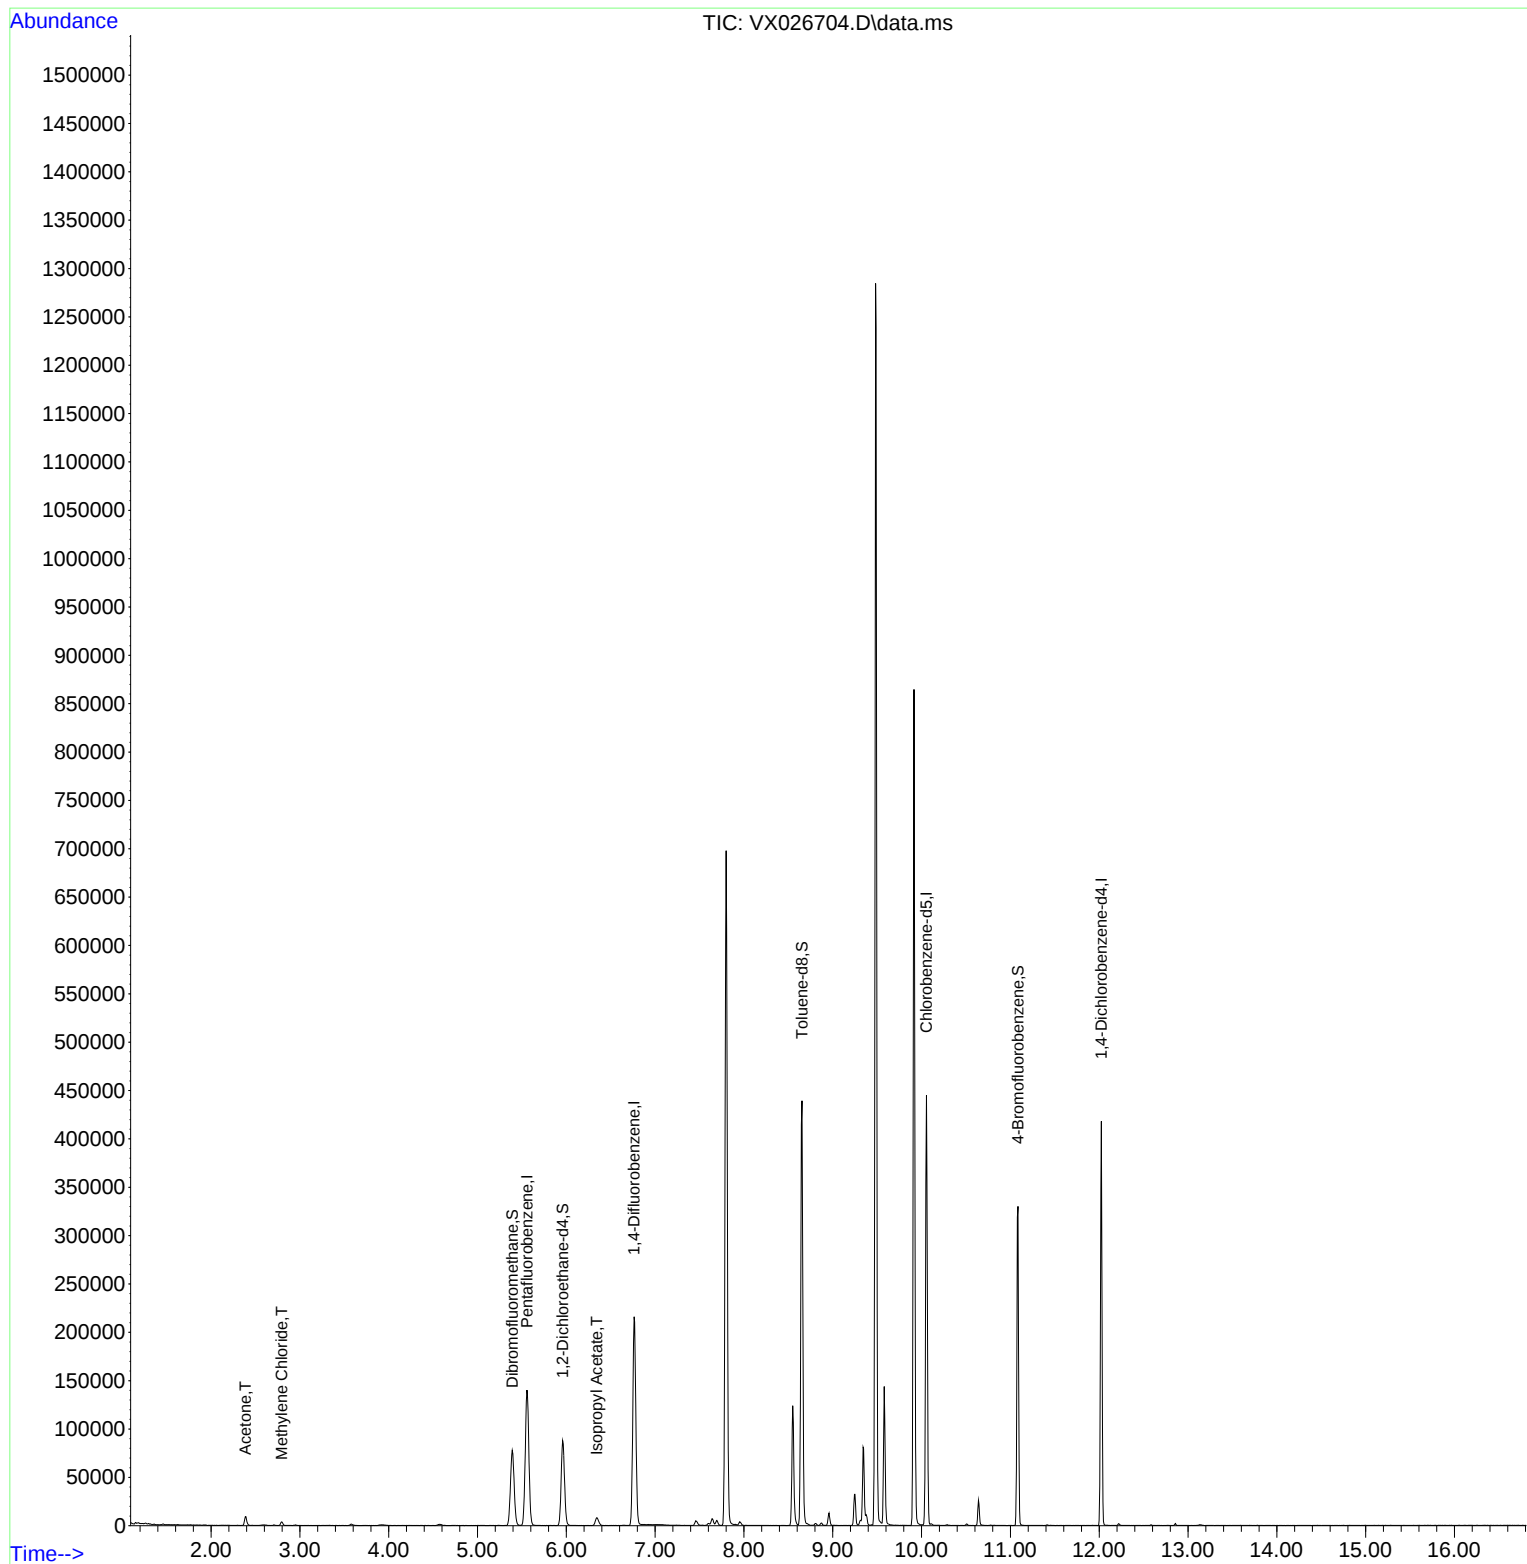






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX026704.D
Acq: 01 Feb 2022 14:11

Instrument :
MSVOA_X
ClientSampleId :
TEX-3



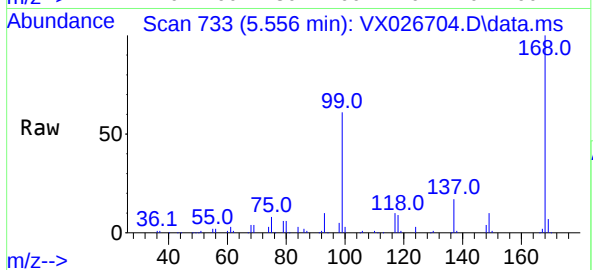



Tgt Ion:168 Resp: 132536
Ion Ratio Lower Upper
168 100
99 61.2 50.3 75.5

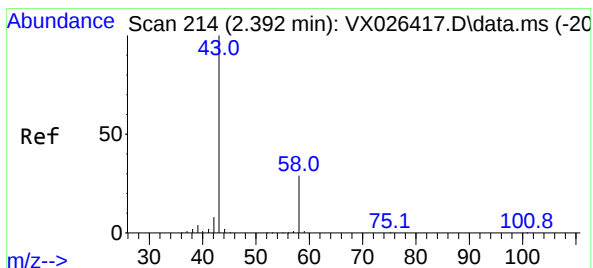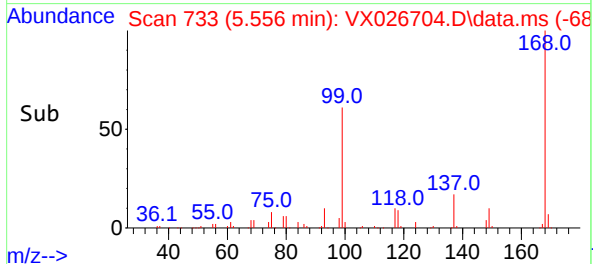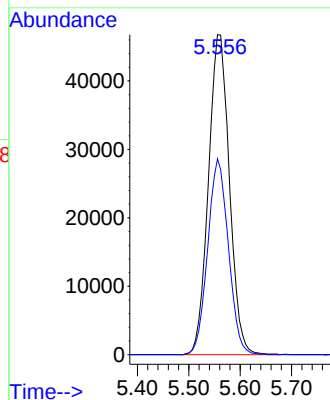

#16
Acetone
Concen: 11.494 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX026704.D
Acq: 01 Feb 2022 14:11

Tgt Ion: 43 Resp: 10852
Ion Ratio Lower Upper
43 100
58 27.1 23.0 34.6

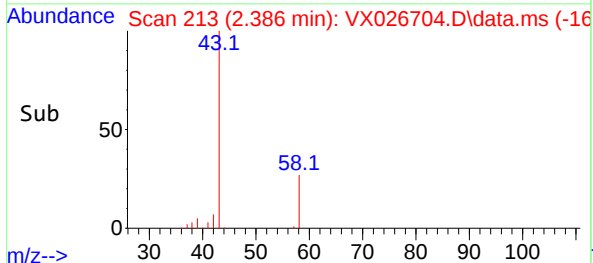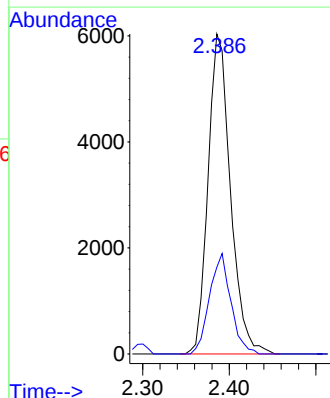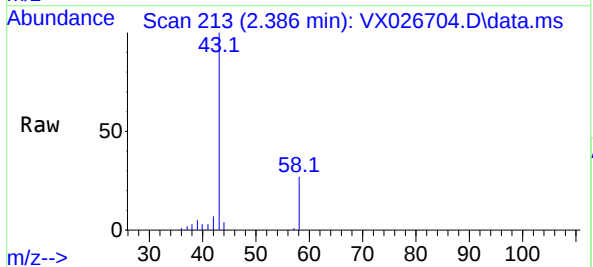




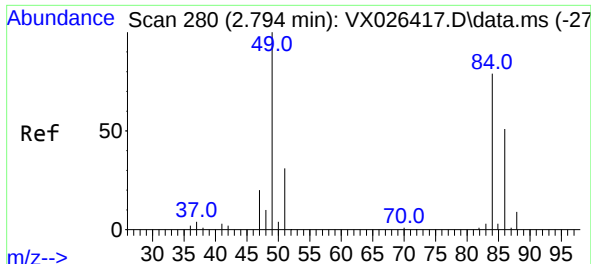


#20
Methylene Chloride
Concen: 1.121 ug/l
RT: 2.794 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX026704.D
Acq: 01 Feb 2022 14:11

Instrument :
MSVOA_X
ClientSampleId :
TEX-3

Tgt Ion: 84 Resp: 1749




Ion	Ratio	Lower	Upper
84	100		
49	123.9	101.5	152.3
51	43.9	31.2	46.8
86	68.9	51.3	76.9

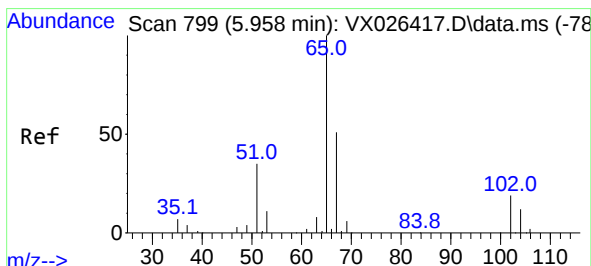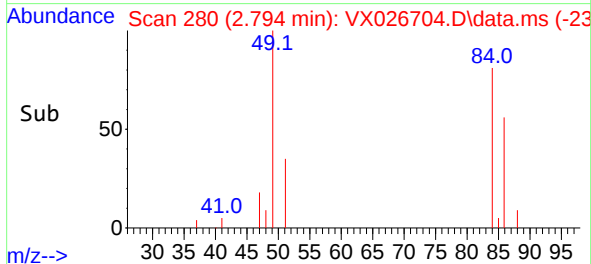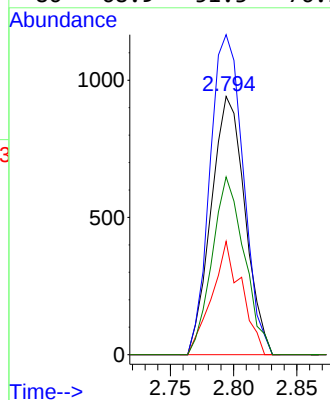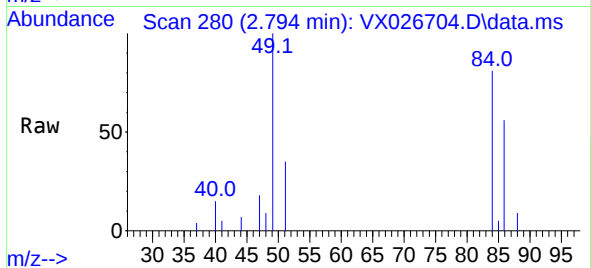


#33
1,2-Dichloroethane-d4
Concen: 45.767 ug/l
RT: 5.958 min Scan# 799
Delta R.T. -0.000 min
Lab File: VX026704.D
Acq: 01 Feb 2022 14:11

Tgt Ion: 65 Resp: 84734

Ion	Ratio	Lower	Upper
65	100		
67	51.5	0.0	100.8


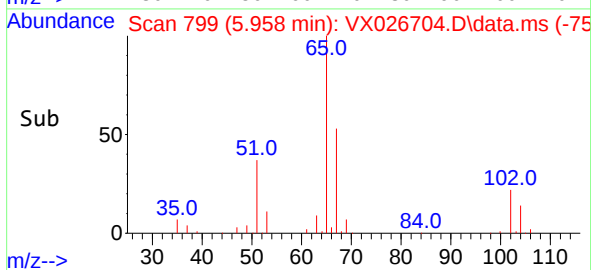
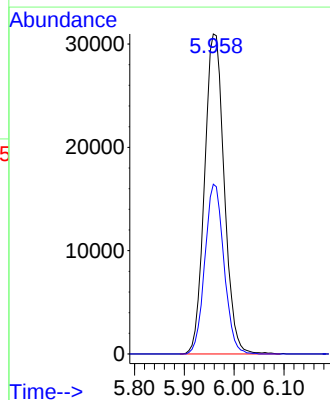
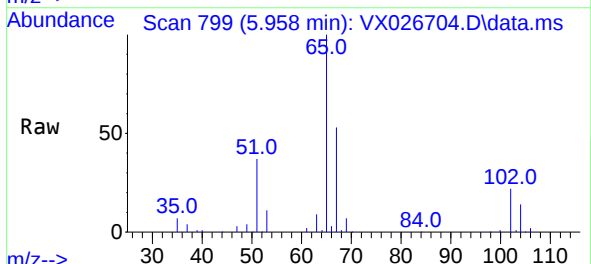


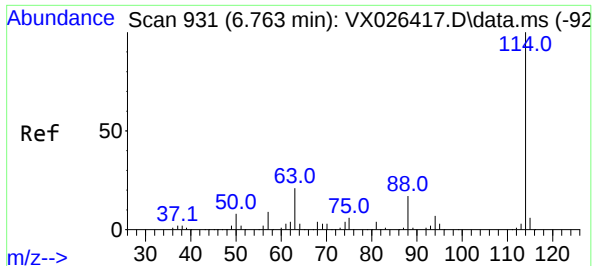

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX026704.D
Acq: 01 Feb 2022 14:11




Instrument :
MSVOA_X
ClientSampleId :
TEX-3


Tgt Ion:114 Resp: 222830
Ion Ratio Lower Upper
114 100
63 21.0 0.0 42.8
88 16.6 0.0 33.0

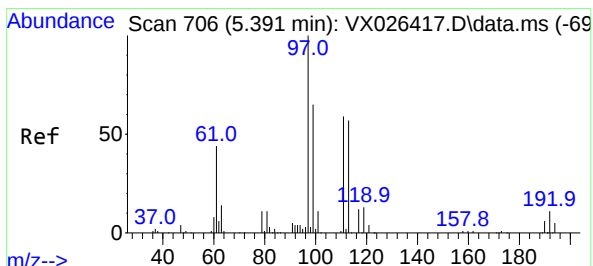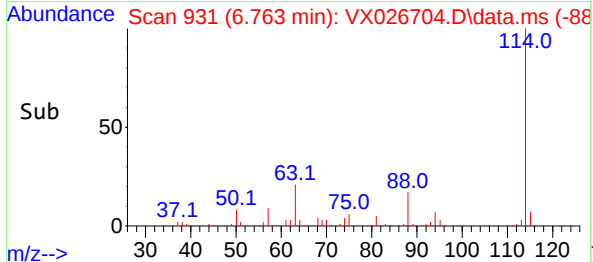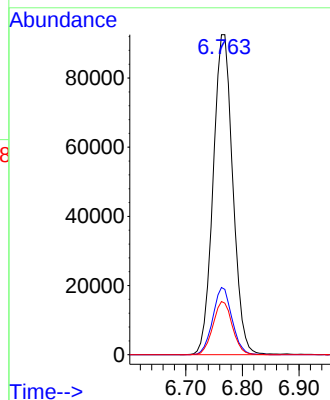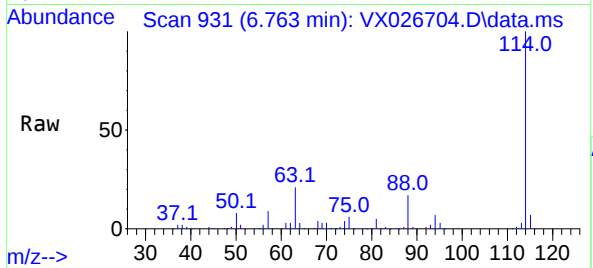

#35
Dibromofluoromethane
Concen: 47.836 ug/l
RT: 5.391 min Scan# 706
Delta R.T. -0.000 min
Lab File: VX026704.D
Acq: 01 Feb 2022 14:11

Tgt Ion:113 Resp: 68835
Ion Ratio Lower Upper
113 100
111 102.4 81.2 121.8
192 19.6 15.0 22.4


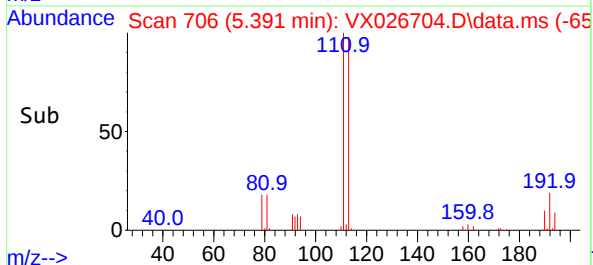
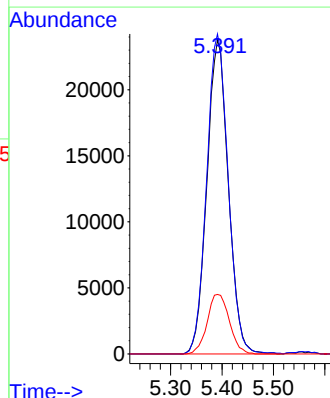
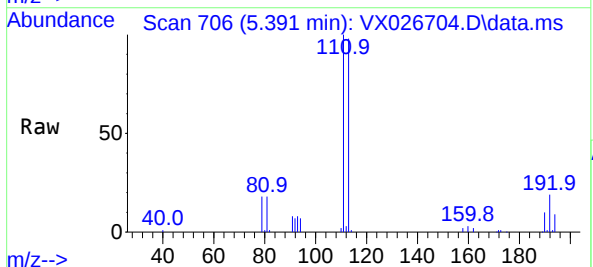


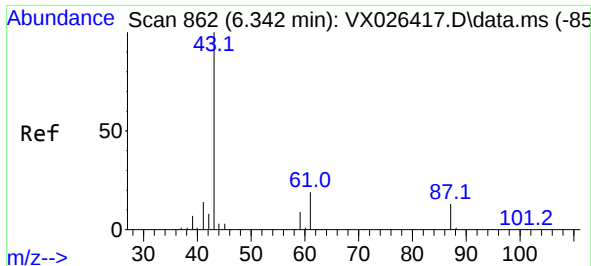

#43
Isopropyl Acetate
Concen: 3.101 ug/l
RT: 6.342 min Scan# 862
Delta R.T. -0.000 min
Lab File: VX026704.D
Acq: 01 Feb 2022 14:11




Instrument :
MSVOA_X
ClientSampleId :
TEX-3


Tgt Ion: 43 Resp: 11509
Ion Ratio Lower Upper
43 100
61 19.0 15.4 23.0
87 13.1 10.2 15.2

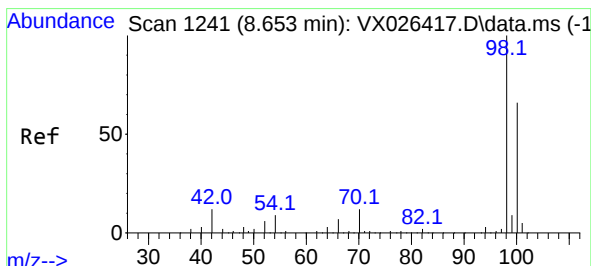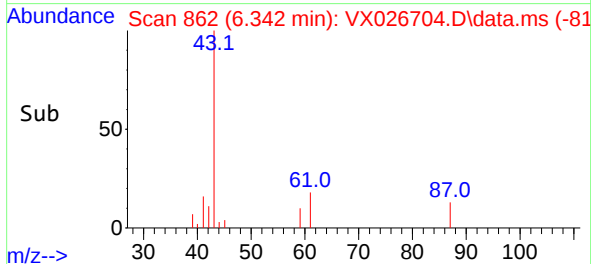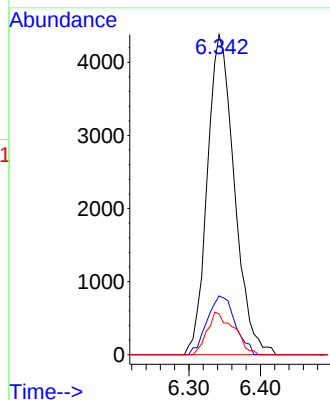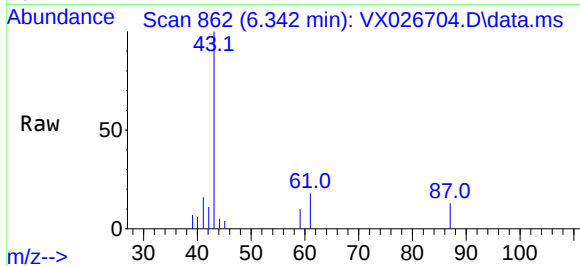

#50
Toluene-d8
Concen: 50.272 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX026704.D
Acq: 01 Feb 2022 14:11

Tgt Ion: 98 Resp: 260679
Ion Ratio Lower Upper
98 100
100 66.9 53.2 79.8


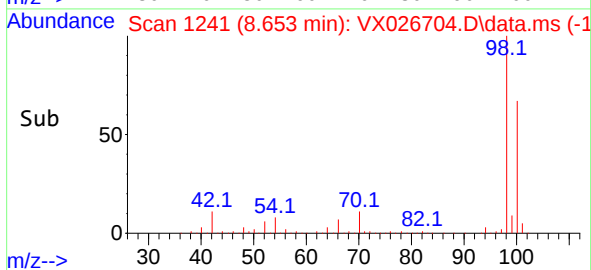
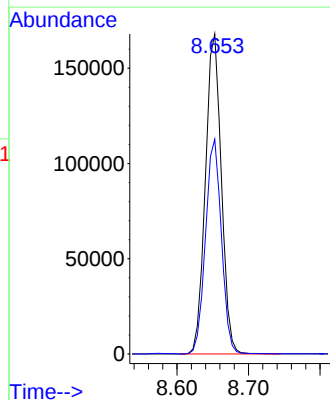
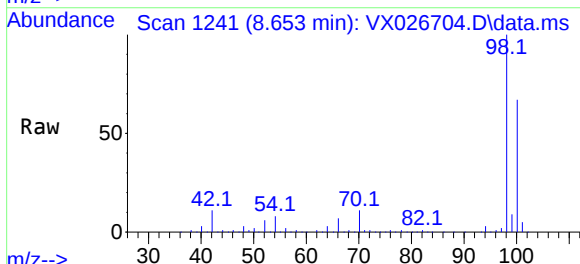


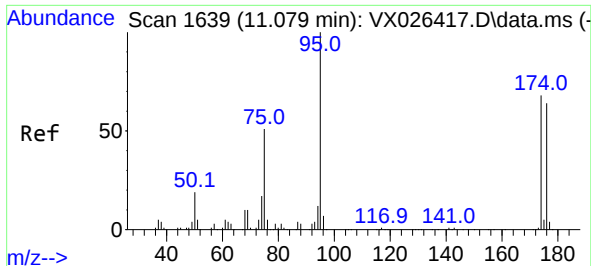

#62
4-Bromofluorobenzene
Concen: 50.397 ug/l
RT: 11.085 min Scan# 1639
Delta R.T. 0.006 min
Lab File: VX026704.D
Acq: 01 Feb 2022 14:11




Instrument :
MSVOA_X
ClientSampleId :
TEX-3


Tgt Ion: 95 Resp: 92834
Ion Ratio Lower Upper
95 100
174 76.9 0.0 148.6
176 72.7 0.0 141.4

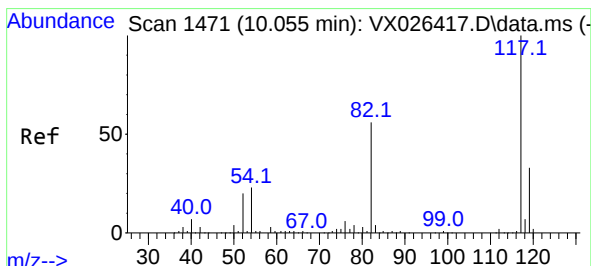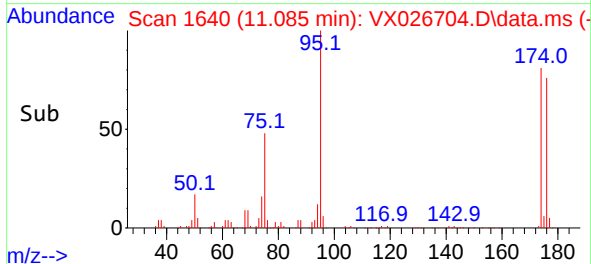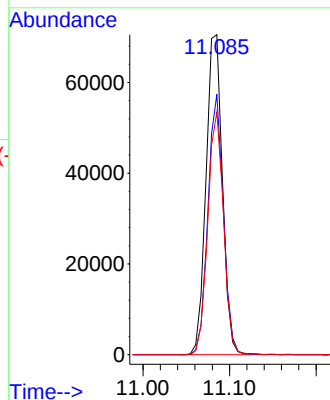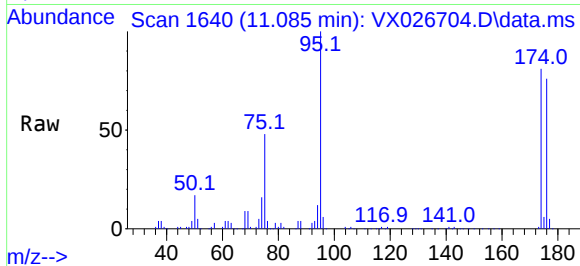

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX026704.D
Acq: 01 Feb 2022 14:11

Tgt Ion: 117 Resp: 199334
Ion Ratio Lower Upper
117 100
82 56.2 45.2 67.8
119 32.4 26.2 39.2

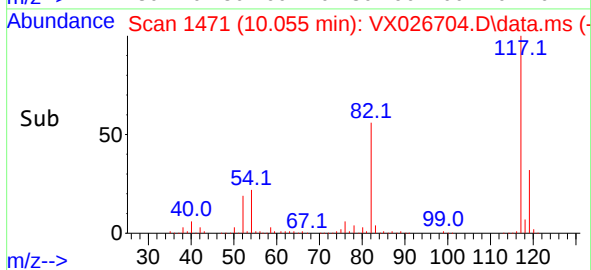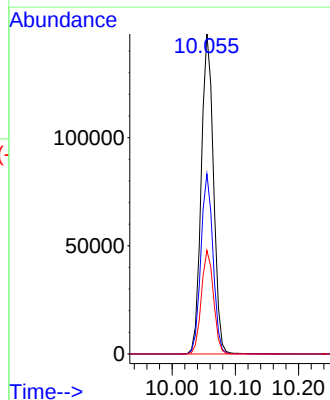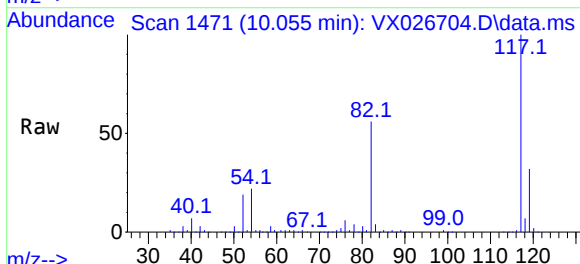

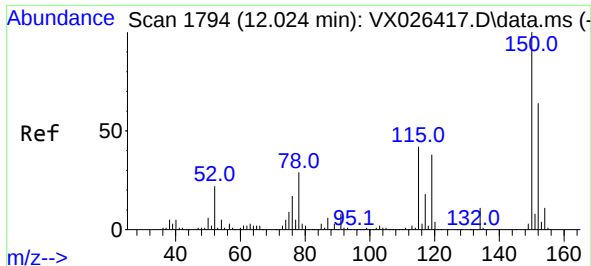

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX026704.D


Acq: 01 Feb 2022 14:11

Instrument :

MSVOA_X

ClientSampleId :

TEX-3

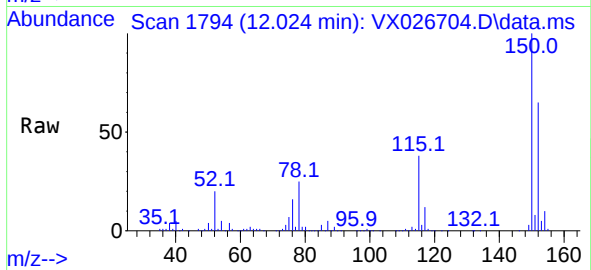

Tgt Ion:152 Resp: 84046

Ion Ratio Lower Upper

152 100

115 59.4 44.2 132.6

150 156.6 0.0 348.2

