
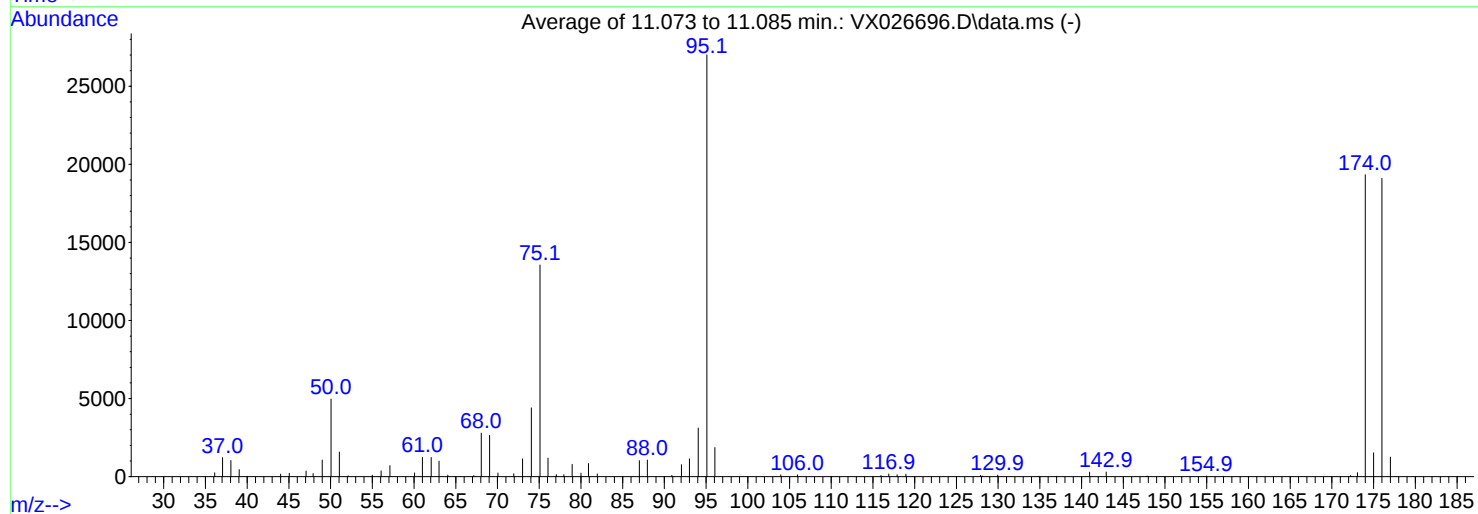


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020122\
 Data File : VX026696.D
 Acq On : 01 Feb 2022 10:01
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
 Title : SW846 8260
 Last Update : Tue Jan 11 14:45:13 2022

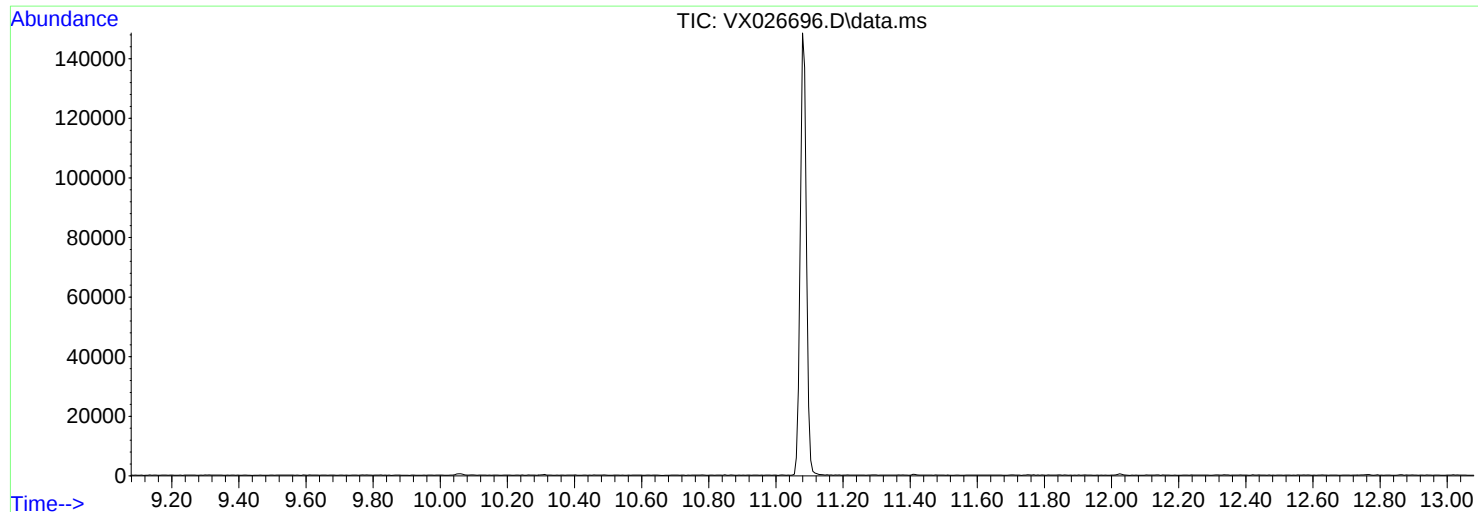

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	4965	PASS
75	95	30	60	50.2	13552	PASS
95	95	100	100	100.0	27011	PASS
96	95	5	9	6.9	1864	PASS
173	174	0.00	2	1.3	260	PASS
174	95	50	100	71.6	19332	PASS
175	174	5	9	7.9	1532	PASS
176	174	95	101	98.8	19108	PASS
177	176	5	9	6.5	1251	PASS