

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020124\
 Data File : VX040069.D
 Acq On : 01 Feb 2024 14:24
 Operator : JC/MD
 Sample : P1312-01 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 NWB-1999

Quant Time: Feb 02 01:41:00 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X013024W.M
 Quant Title : SW846 8260
 QLast Update : Thu Feb 01 05:44:39 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	87940	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	158647	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	153138	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	75698	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	66999	47.340	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	94.680%		
35) Dibromofluoromethane	5.385	113	52609	48.714	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	97.420%		
50) Toluene-d8	8.647	98	187615	46.454	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	92.900%		
62) 4-Bromofluorobenzene	11.079	95	77834	50.050	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	100.100%		
Target Compounds						Qvalue
11) Tert butyl alcohol	2.953	59	282	1.098	ug/l #	78
16) Acetone	2.374	43	4183	6.308	ug/l #	86
18) Methyl Acetate	2.703	43	458	0.292	ug/l #	53
19) Methyl tert-butyl Ether	3.117	73	1308	0.386	ug/l	98
20) Methylene Chloride	2.788	84	264	0.224	ug/l #	65
25) 2-Butanone	4.581	43	999	1.084	ug/l #	51
31) Cyclohexane	5.471	56	386	0.218	ug/l #	78
36) 1,1-Dichloropropene	5.550	75	7739	4.955	ug/l #	50
38) Carbon Tetrachloride	5.550	117	9675	6.474	ug/l #	17
39) Methylcyclohexane	7.379	83	717	0.377	ug/l	92
40) Benzene	6.038	78	12572	2.764	ug/l	93
52) Toluene	8.720	92	47547	16.769	ug/l	96
53) t-1,3-Dichloropropene	8.720	75	593	0.356	ug/l #	1
67) Ethyl Benzene	10.195	91	33823	5.955	ug/l	100
68) m/p-Xylenes	10.299	106	52934	24.775	ug/l	100
69) o-Xylene	10.640	106	24714	12.194	ug/l	96
70) Styrene	10.640	104	1354	0.396	ug/l #	1
73) Isopropylbenzene	10.964	105	3895	0.717	ug/l	98
74) N-amyl acetate	10.842	43	183	0.273	ug/l #	44
76) 1,2,3-Trichloropropane	11.079	75	43592	27.042	ug/l #	39
78) n-propylbenzene	11.305	91	25541	3.818	ug/l	96
79) 2-Chlorotoluene	11.378	91	16260	4.038	ug/l #	42
80) 1,3,5-Trimethylbenzene	11.451	105	38589	8.259	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.079	75	43592	78.930	ug/l #	5
82) 4-Chlorotoluene	11.451	91	4859	1.051	ug/l #	46
83) tert-Butylbenzene	11.750	119	17833	3.988	ug/l #	53
84) 1,2,4-Trimethylbenzene	11.750	105	154948	33.232	ug/l	98
85) sec-Butylbenzene	11.750	105	154948	26.156	ug/l #	57
86) p-Isopropyltoluene	11.969	119	5730	1.185	ug/l	96
89) n-Butylbenzene	12.323	91	12092	2.575	ug/l #	35
90) Hexachloroethane	12.530	117	1843	2.448	ug/l #	17
92) 1,2-Dibromo-3-Chloropr...	12.920	75	197	0.425	ug/l #	9
95) Naphthalene	13.774	128	53385	10.310	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_X
ClientSampleId :
NWB-1999

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020124\
Data File : VX040069.D
Acq On : 01 Feb 2024 14:24
Operator : JC/MD
Sample : P1312-01 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
NWB-1999


Quant Time: Feb 02 01:41:00 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X013024W.M
Quant Title : SW846 8260
QLast Update : Thu Feb 01 05:44:39 2024
Response via : Initial Calibration

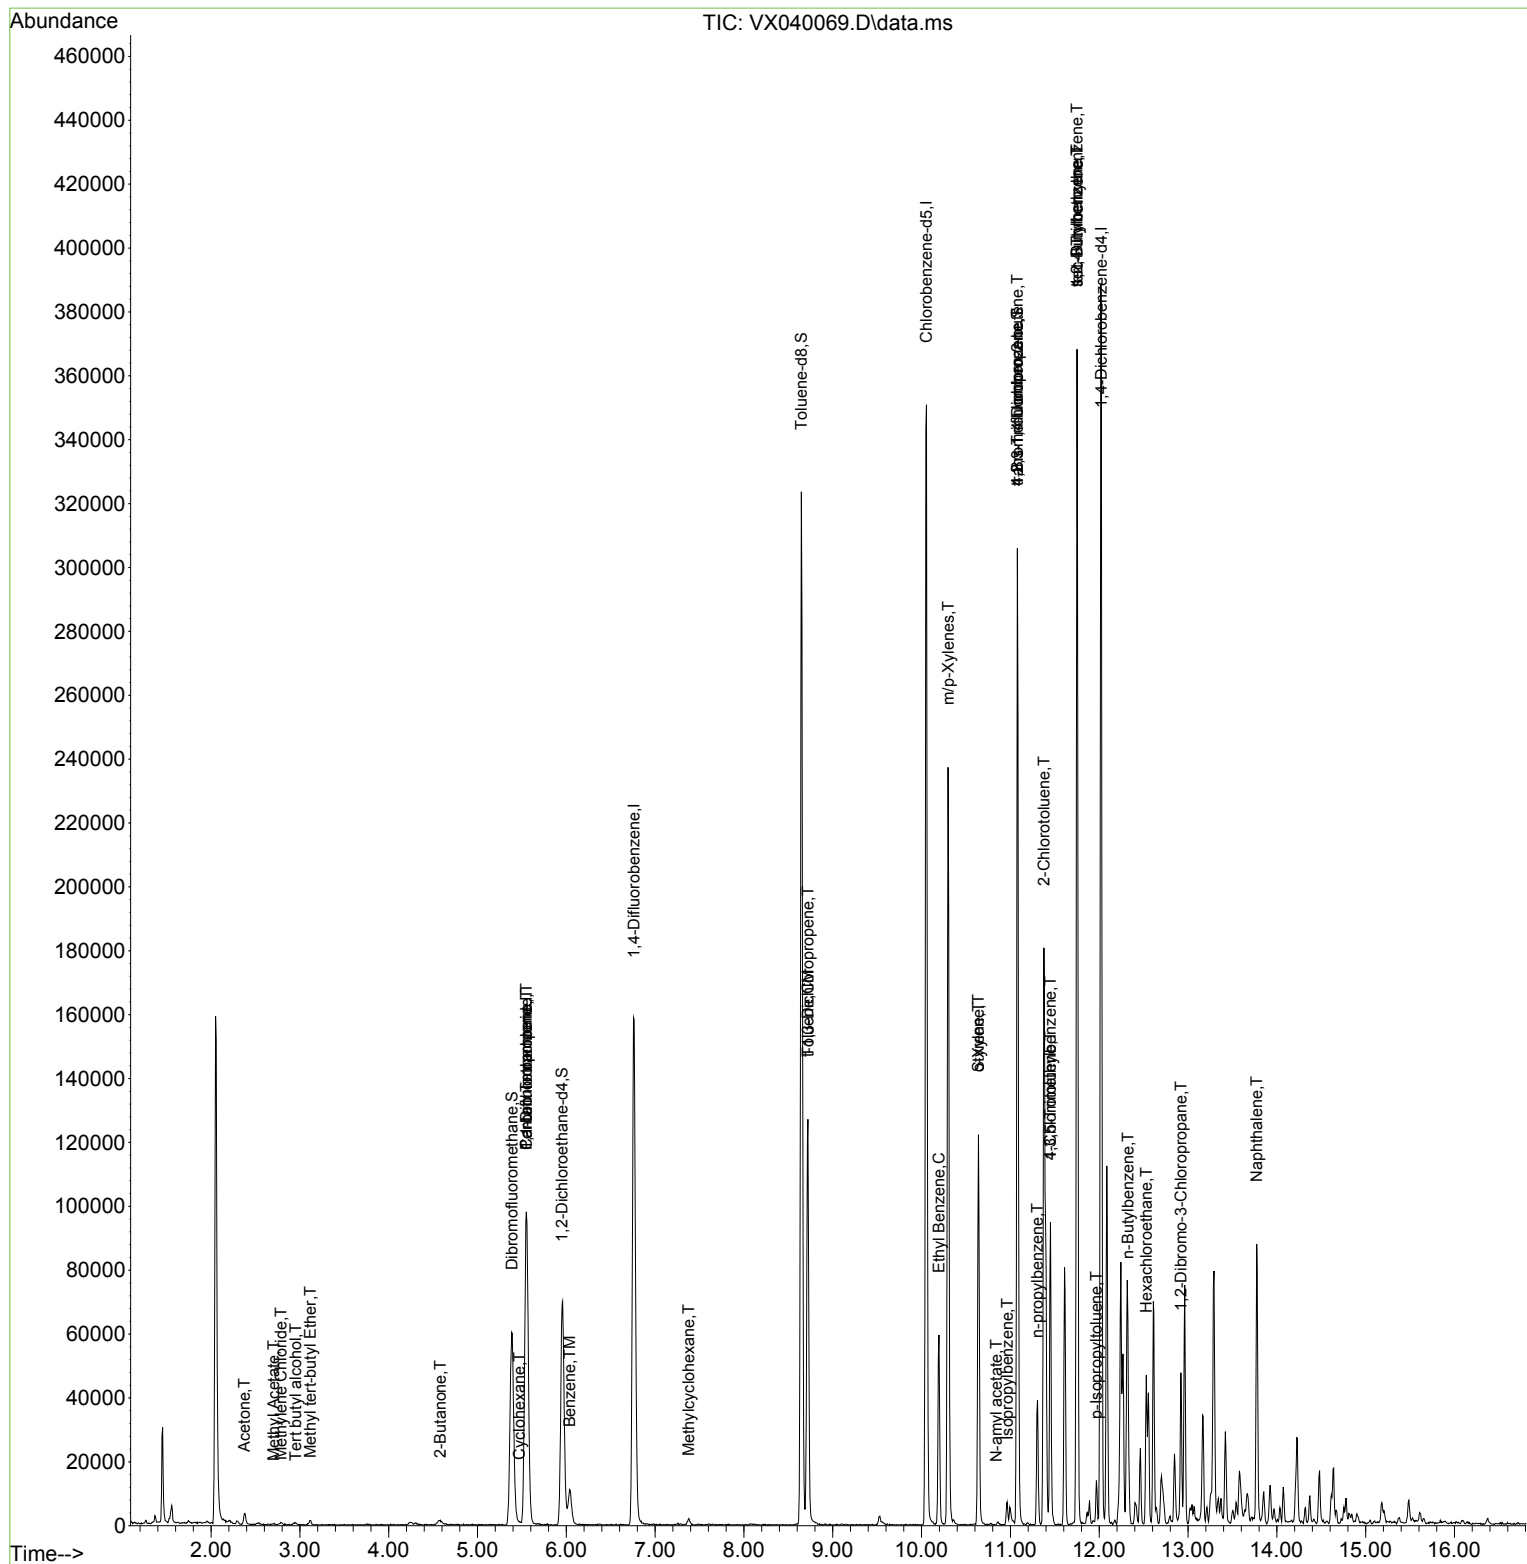



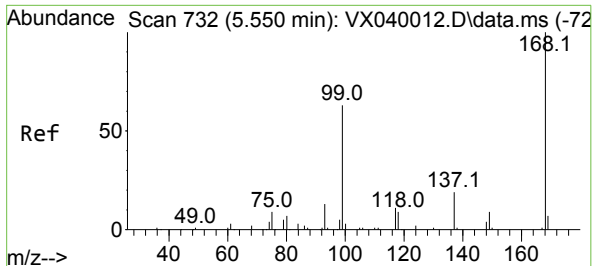


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX040069.D
Acq: 01 Feb 2024 14:24

Instrument :
MSVOA_X
ClientSampleId :
NWB-1999



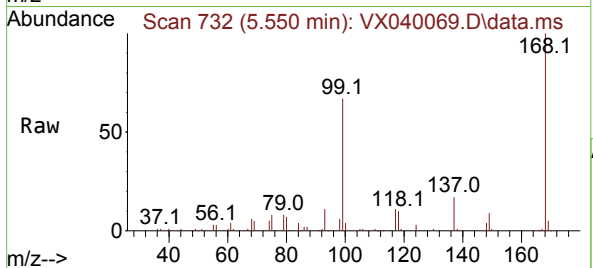



Tgt Ion:168 Resp: 87940
Ion Ratio Lower Upper
168 100
99 66.9 56.6 85.0

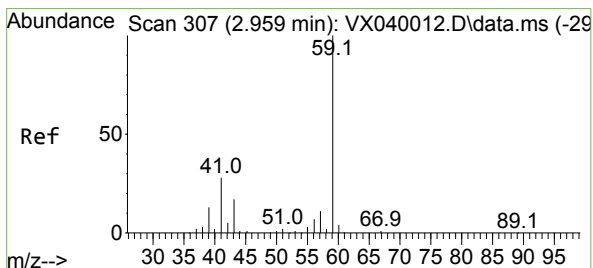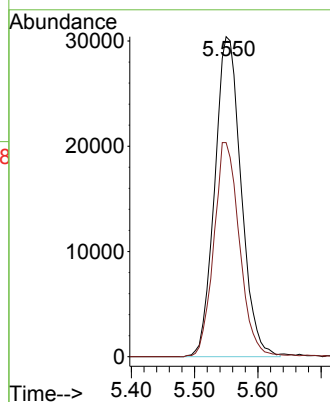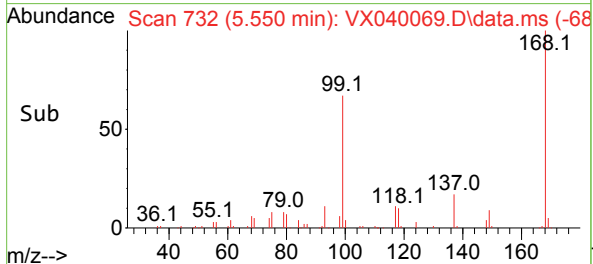

#11
Tert butyl alcohol
Concen: 1.098 ug/l
RT: 2.953 min Scan# 306
Delta R.T. -0.006 min
Lab File: VX040069.D
Acq: 01 Feb 2024 14:24

Tgt Ion: 59 Resp: 282
Ion Ratio Lower Upper
59 100
57 0.0 6.0 9.0#


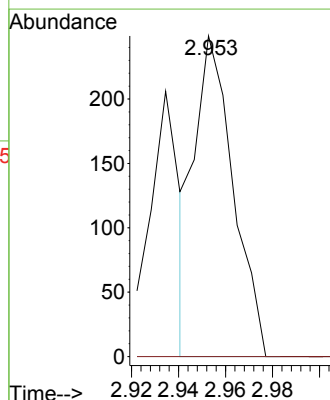
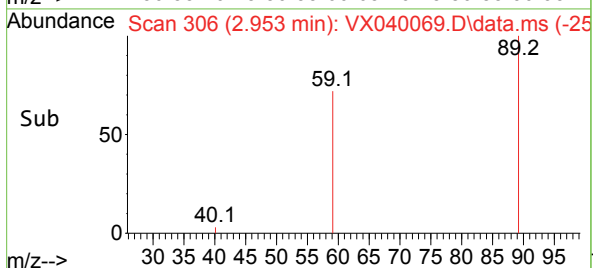
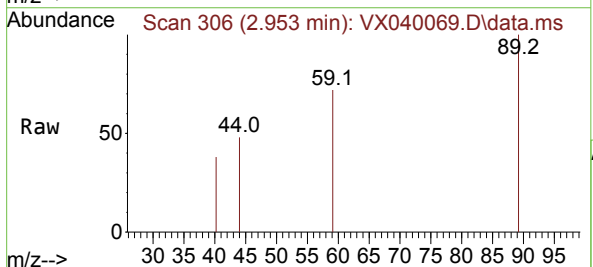




#16
Acetone
Concen: 6.308 ug/l
RT: 2.374 min Scan# 211
Delta R.T. 0.000 min
Lab File: VX040069.D
Acq: 01 Feb 2024 14:24




Instrument :
MSVOA_X
ClientSampleId :
NWB-1999


Tgt Ion: 43 Resp: 4183
Ion Ratio Lower Upper
43 100
58 20.2 21.9 32.9#

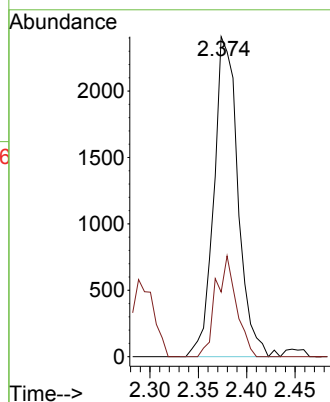

#18
Methyl Acetate
Concen: 0.292 ug/l
RT: 2.703 min Scan# 265
Delta R.T. 0.000 min
Lab File: VX040069.D
Acq: 01 Feb 2024 14:24

Tgt Ion: 43 Resp: 458
Ion Ratio Lower Upper
43 100
74 0.0 17.8 26.8#



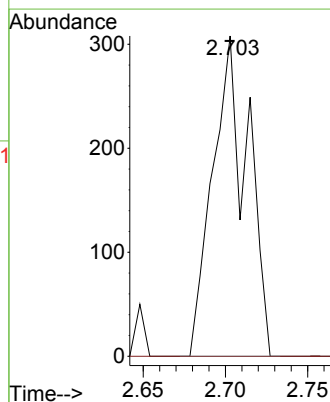





#19
Methyl tert-butyl Ether
Concen: 0.386 ug/l
RT: 3.117 min Scan# 311
Delta R.T. 0.006 min
Lab File: VX040069.D
Acq: 01 Feb 2024 14:24




Instrument :
MSVOA_X
ClientSampleId :
NWB-1999


Tgt Ion: 73 Resp: 1308
Ion Ratio Lower Upper
73 100
57 22.4 17.3 25.9

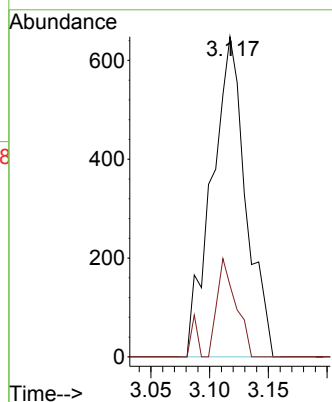

#20
Methylene Chloride
Concen: 0.224 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.000 min
Lab File: VX040069.D
Acq: 01 Feb 2024 14:24

Tgt Ion: 84 Resp: 264
Ion Ratio Lower Upper
84 100
49 78.1 103.6 155.4#
51 42.5 33.8 50.6
86 32.4 49.4 74.0#









#25
2-Butanone
Concen: 1.084 ug/l
RT: 4.581 min Scan# 51
Delta R.T. 0.031 min
Lab File: VX040069.D
Acq: 01 Feb 2024 14:24




Instrument :
MSVOA_X
ClientSampleId :
NWB-1999


Tgt Ion: 43 Resp: 999
Ion Ratio Lower Upper
43 100
72 0.0 19.4 29.2#

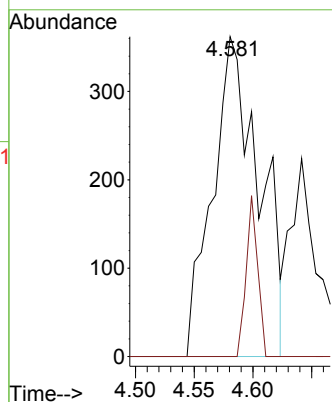

#31
Cyclohexane
Concen: 0.218 ug/l
RT: 5.471 min Scan# 719
Delta R.T. 0.006 min
Lab File: VX040069.D
Acq: 01 Feb 2024 14:24

Tgt Ion: 56 Resp: 386
Ion Ratio Lower Upper
56 100
69 29.6 23.4 35.2
84 56.1 65.9 98.9#



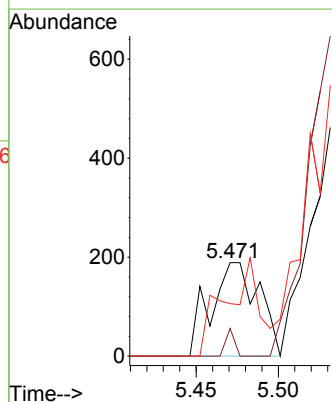
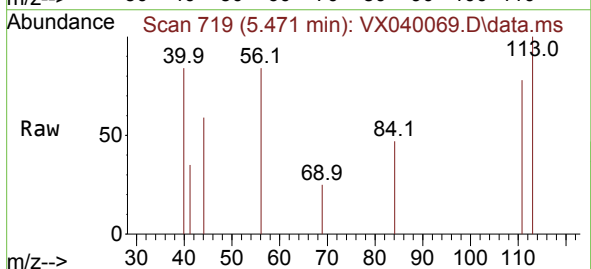




#33
 1,2-Dichloroethane-d4
 Concen: 47.340 ug/l
 RT: 5.952 min Scan# 798
 Delta R.T. 0.000 min
 Lab File: VX040069.D
 Acq: 01 Feb 2024 14:24




Instrument :
 MSVOA_X
 ClientSampleId :
 NWB-1999


Tgt Ion: 65 Resp: 66999
 Ion Ratio Lower Upper
 65 100
 67 52.7 0.0 100.2

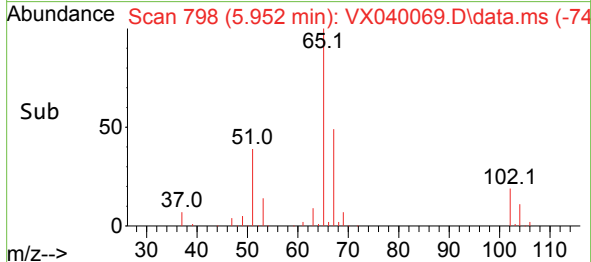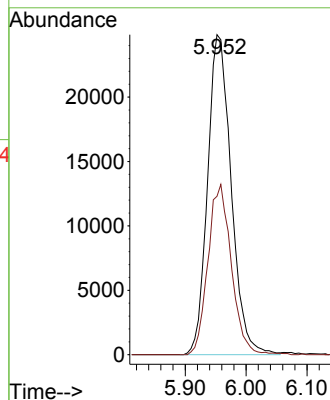

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.763 min Scan# 931
 Delta R.T. 0.000 min
 Lab File: VX040069.D
 Acq: 01 Feb 2024 14:24

Tgt Ion: 114 Resp: 158647
 Ion Ratio Lower Upper
 114 100
 63 21.6 0.0 45.0
 88 16.3 0.0 36.6



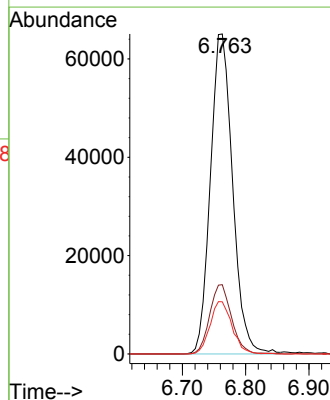



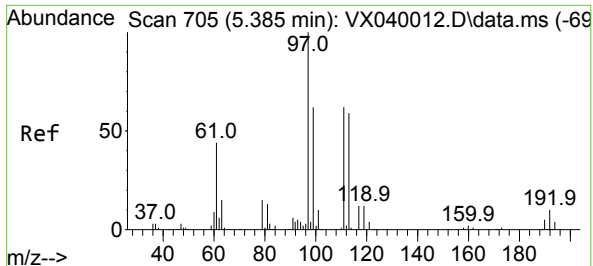

#35
Dibromofluoromethane
Concen: 48.714 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX040069.D
Acq: 01 Feb 2024 14:24




Instrument :
MSVOA_X
ClientSampleId :
NWB-1999


Tgt Ion:113 Resp: 52609
Ion Ratio Lower Upper
113 100
111 103.8 82.9 124.3
192 16.4 13.3 19.9

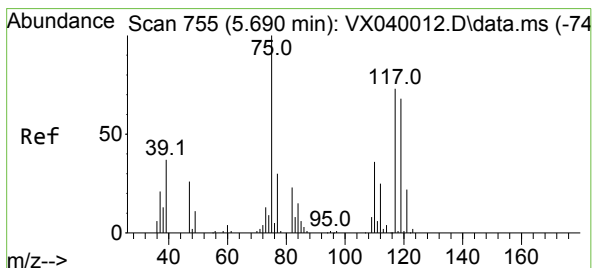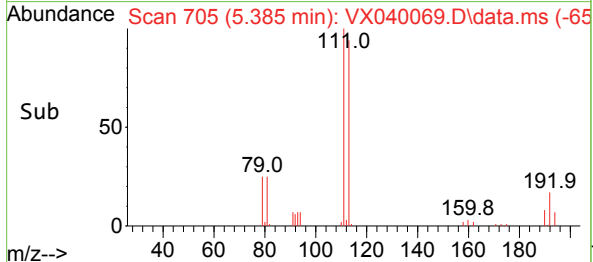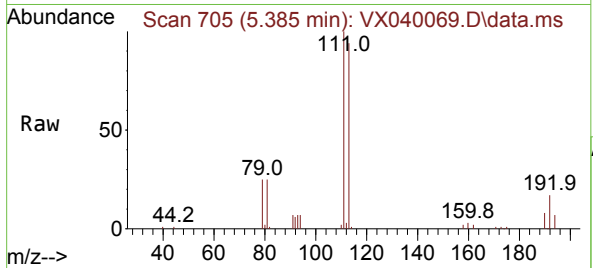

#36
1,1-Dichloropropene
Concen: 4.955 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.140 min
Lab File: VX040069.D
Acq: 01 Feb 2024 14:24


Tgt Ion: 75 Resp: 7739
Ion Ratio Lower Upper
75 100
110 8.2 17.0 50.9#
77 0.0 24.7 37.1#

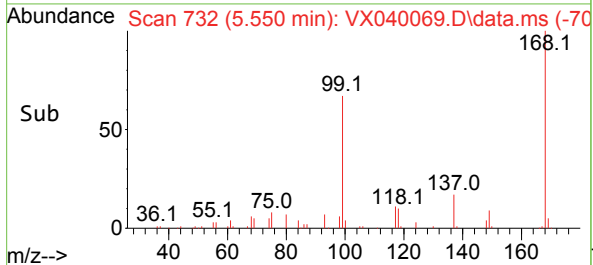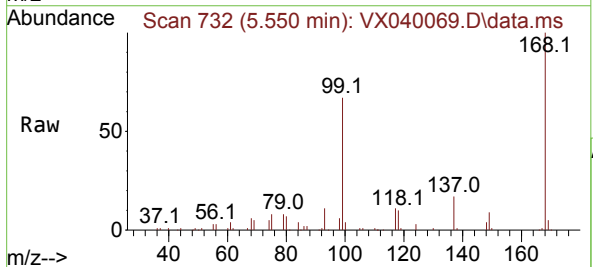






#38
Carbon Tetrachloride
Concen: 6.474 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX040069.D
Acq: 01 Feb 2024 14:24

Instrument :
MSVOA_X
ClientSampleId :
NWB-1999







Tgt Ion:117 Resp: 9675
Ion Ratio Lower Upper
117 100
119 7.2 78.2 117.2#
121 0.0 24.4 36.6#



#39
Methylcyclohexane
Concen: 0.377 ug/l
RT: 7.379 min Scan# 1032
Delta R.T. 0.000 min
Lab File: VX040069.D
Acq: 01 Feb 2024 14:24

Tgt Ion: 83 Resp: 717
Ion Ratio Lower Upper
83 100
55 74.2 64.6 97.0
98 39.4 36.7 55.1





#40

Benzene

Concen: 2.764 ug/l

RT: 6.038 min Scan# 812

Delta R.T. 0.000 min

Lab File: VX040069.D

Acq: 01 Feb 2024 14:24

Instrument :

MSVOA_X

ClientSampleId :





NWB-1999

Tgt Ion: 78 Resp: 12572

Ion Ratio Lower Upper

78 100

77 20.7 19.3 28.9

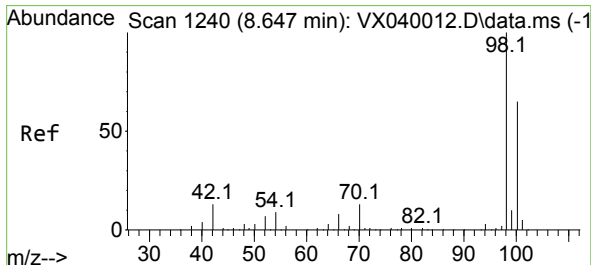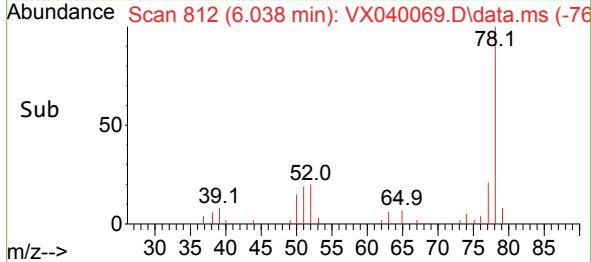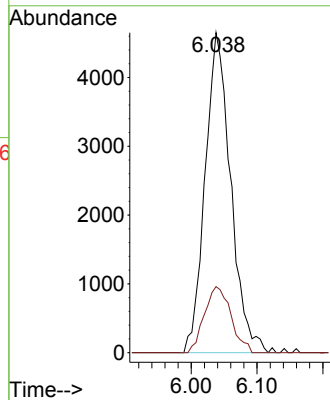

#50

Toluene-d8

Concen: 46.454 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. 0.000 min

Lab File: VX040069.D




Acq: 01 Feb 2024 14:24


Tgt Ion: 98 Resp: 187615

Ion Ratio Lower Upper

98 100

100 64.3 53.1 79.7



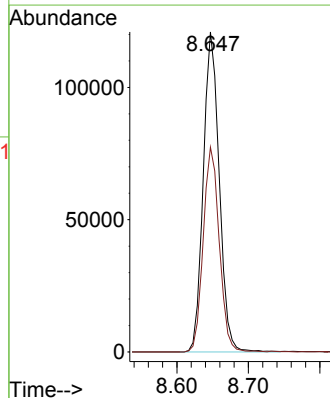
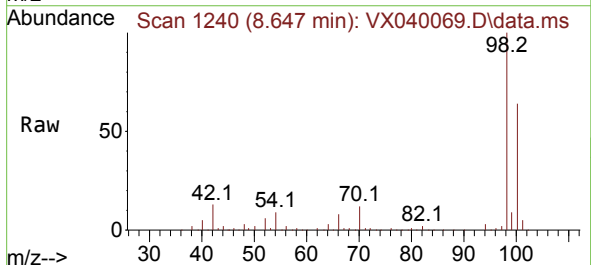




#52
Toluene
Concen: 16.769 ug/l
RT: 8.720 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX040069.D
Acq: 01 Feb 2024 14:24




Instrument :
MSVOA_X
ClientSampleId :
NWB-1999


Tgt Ion: 92 Resp: 47547
Ion Ratio Lower Upper
92 100
91 172.7 134.2 201.2

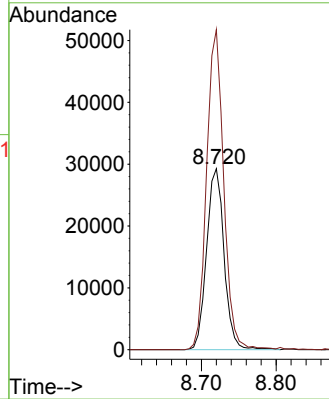

#53
t-1,3-Dichloropropene
Concen: 0.356 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.256 min
Lab File: VX040069.D
Acq: 01 Feb 2024 14:24

Tgt Ion: 75 Resp: 593
Ion Ratio Lower Upper
75 100
77 203.8 25.7 38.5#



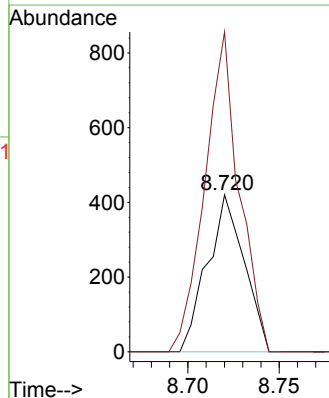





#62
4-Bromofluorobenzene
Concen: 50.050 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX040069.D
Acq: 01 Feb 2024 14:24




Instrument :
MSVOA_X
ClientSampleId :
NWB-1999


Tgt Ion: 95 Resp: 77834
Ion Ratio Lower Upper
95 100
174 71.2 0.0 135.6
176 67.6 0.0 131.0

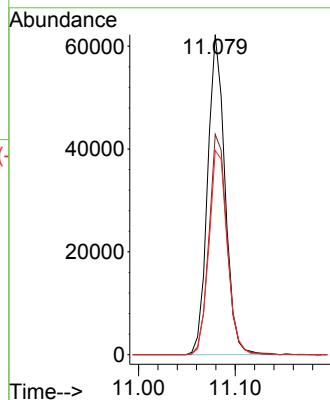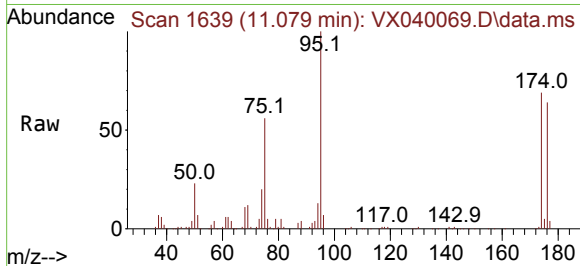

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX040069.D
Acq: 01 Feb 2024 14:24

Tgt Ion: 117 Resp: 153138
Ion Ratio Lower Upper
117 100
82 58.0 46.2 69.4
119 32.2 25.5 38.3

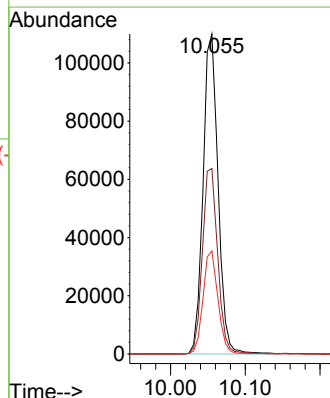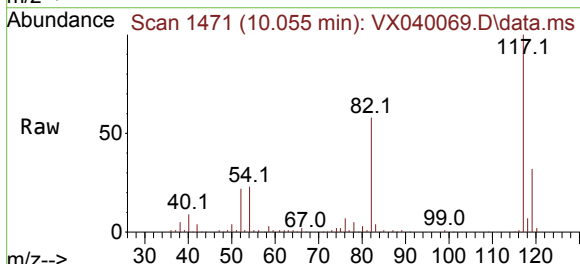



#67

Ethyl Benzene

Concen: 5.955 ug/l

RT: 10.195 min Scan# 1494

Delta R.T. 0.000 min

Lab File: VX040069.D

Acq: 01 Feb 2024 14:24

Instrument :

MSVOA_X

ClientSampleId :





NWB-1999

Tgt Ion: 91 Resp: 33823

Ion Ratio Lower Upper

91 100

106 31.0 24.9 37.3



#68

m/p-Xylenes

Concen: 24.775 ug/l

RT: 10.299 min Scan# 1511

Delta R.T. 0.000 min

Lab File: VX040069.D




Acq: 01 Feb 2024 14:24


Tgt Ion: 106 Resp: 52934

Ion Ratio Lower Upper

106 100

91 206.3 165.5 248.3





#69

o-Xylene

Concen: 12.194 ug/l

RT: 10.640 min Scan# 1567

Delta R.T. 0.000 min

Lab File: VX040069.D

Acq: 01 Feb 2024 14:24

Instrument :

MSVOA_X

ClientSampleId :





NWB-1999

Tgt Ion:106 Resp: 24714

Ion Ratio Lower Upper

106 100

91 224.2 108.9 326.8

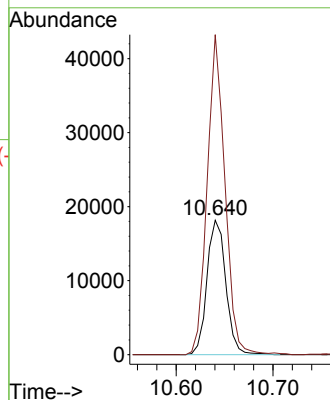

#70

Styrene

Concen: 0.396 ug/l

RT: 10.640 min Scan# 1567

Delta R.T. -0.013 min

Lab File: VX040069.D

Acq: 01 Feb 2024 14:24




Tgt Ion:104 Resp: 1354


Ion Ratio Lower Upper

104 100

78 326.7 43.6 65.4#

103 251.9 43.6 65.4#



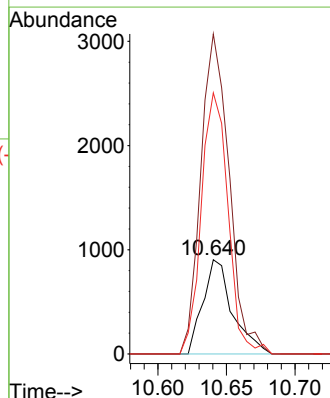





#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1793
Delta R.T. 0.006 min
Lab File: VX040069.D
Acq: 01 Feb 2024 14:24




Instrument :
MSVOA_X
ClientSampleId :
NWB-1999


Tgt Ion:152 Resp: 75698
Ion Ratio Lower Upper
152 100
115 64.4 43.3 129.9
150 159.8 0.0 345.0

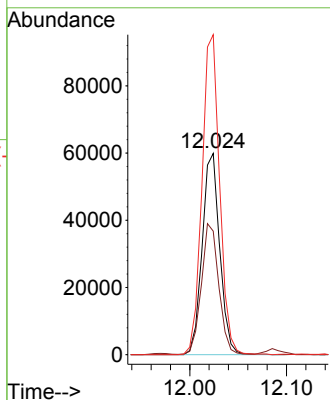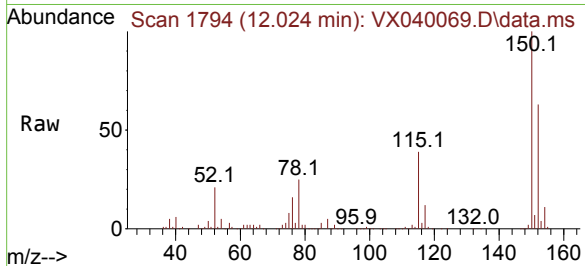

#73
Isopropylbenzene
Concen: 0.717 ug/l
RT: 10.964 min Scan# 1620
Delta R.T. 0.001 min
Lab File: VX040069.D
Acq: 01 Feb 2024 14:24

Tgt Ion:105 Resp: 3895
Ion Ratio Lower Upper
105 100
120 24.6 12.9 38.6



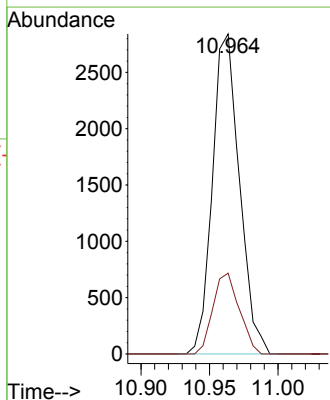
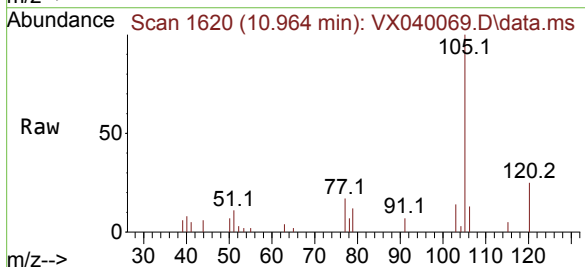




#74
N-amy1 acetate
Concen: 0.273 ug/l
RT: 10.842 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX040069.D
Acq: 01 Feb 2024 14:24




Instrument :
MSVOA_X
ClientSampleId :
NWB-1999


Tgt Ion: 43	Resp:	183	
Ion	Ratio	Lower	Upper
43	100		
70	0.0	32.9	49.3#
55	0.0	19.3	28.9#
61	0.0	18.8	28.2#



#76
1,2,3-Trichloropropane
Concen: 27.042 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.158 min
Lab File: VX040069.D
Acq: 01 Feb 2024 14:24

Tgt Ion: 75	Resp: 43592
Ion Ratio	Lower Upper
75 100	
77 1.2	19.1 57.5#




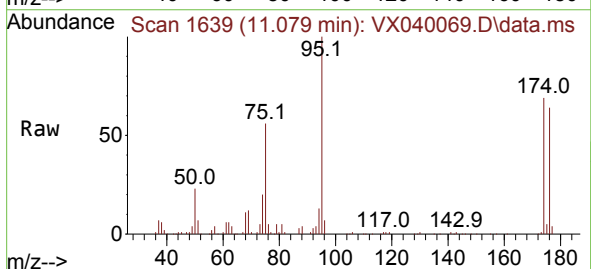




#78
n-propylbenzene
Concen: 3.818 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. 0.000 min
Lab File: VX040069.D
Acq: 01 Feb 2024 14:24




Instrument :
MSVOA_X
ClientSampleId :
NWB-1999


Tgt Ion: 91 Resp: 25541
Ion Ratio Lower Upper
91 100
120 21.1 11.5 34.4

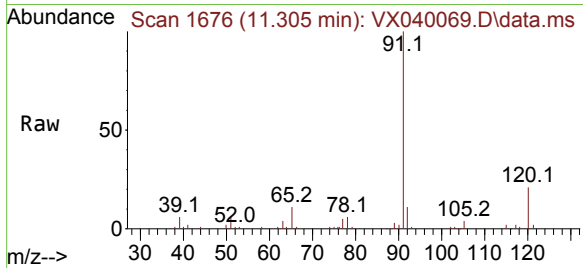

#79
2-Chlorotoluene
Concen: 4.038 ug/l
RT: 11.378 min Scan# 1688
Delta R.T. 0.012 min
Lab File: VX040069.D
Acq: 01 Feb 2024 14:24

Tgt Ion: 91 Resp: 16260
Ion Ratio Lower Upper
91 100
126 0.0 16.3 48.8#

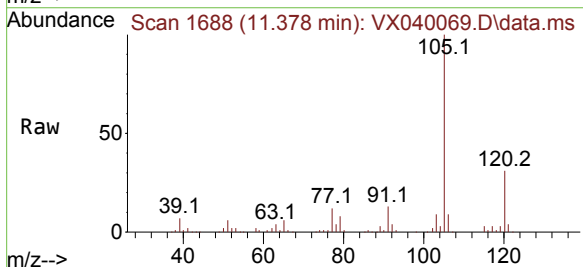



#80

1,3,5-Trimethylbenzene

Concen: 8.259 ug/l

RT: 11.451 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX040069.D

Acq: 01 Feb 2024 14:24

Instrument :

MSVOA_X

ClientSampleId :





NWB-1999

Tgt Ion:105 Resp: 38589

Ion Ratio Lower Upper

105 100

120 47.7 24.1 72.3

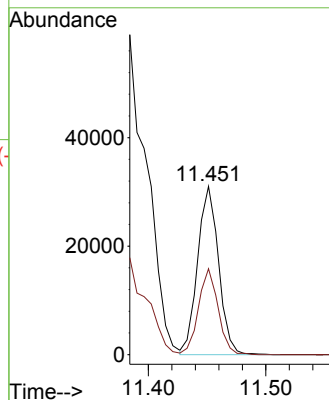

#81

trans-1,4-Dichloro-2-butene

Concen: 78.930 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.061 min

Lab File: VX040069.D

Acq: 01 Feb 2024 14:24




Tgt Ion: 75 Resp: 43592


Ion Ratio Lower Upper

75 100

53 0.0 90.5 135.7#

89 0.0 36.9 55.3#

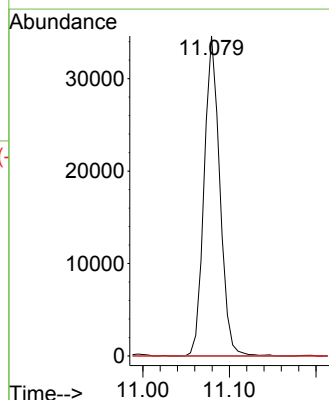



#82

4-Chlorotoluene

Concen: 1.051 ug/l

RT: 11.451 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX040069.D

Acq: 01 Feb 2024 14:24

Instrument :

MSVOA_X

ClientSampleId :





NWB-1999

Tgt Ion: 91 Resp: 4859

Ion Ratio Lower Upper

91 100

126 0.0 14.2 42.6#

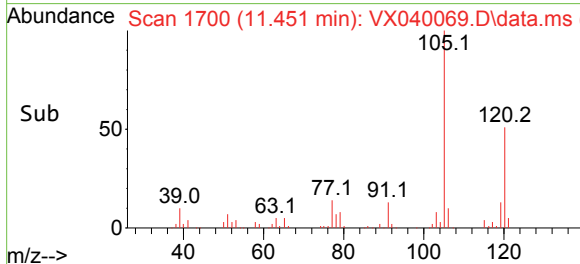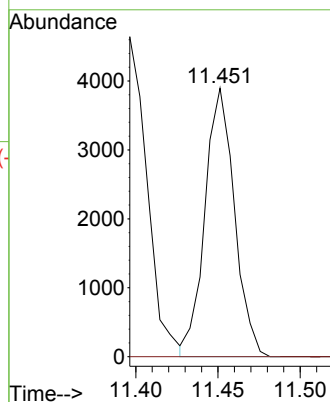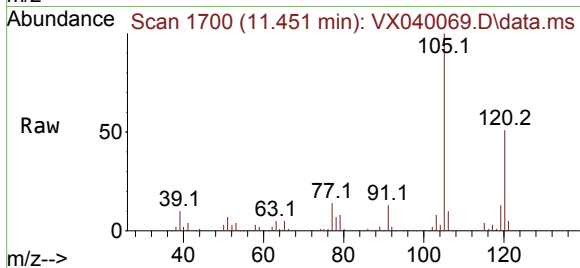

#83

tert-Butylbenzene

Concen: 3.988 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. 0.037 min

Lab File: VX040069.D

Acq: 01 Feb 2024 14:24




Tgt Ion: 119 Resp: 17833


Ion Ratio Lower Upper

119 100

91 98.6 31.2 93.6#

134 0.0 11.7 35.0#


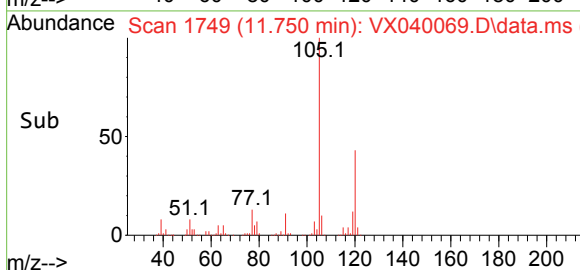
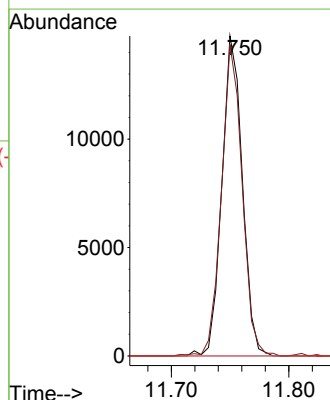
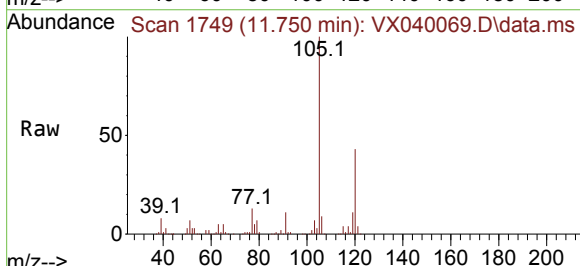




#84
1,2,4-Trimethylbenzene
Concen: 33.232 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VX040069.D
Acq: 01 Feb 2024 14:24




Instrument :
MSVOA_X
ClientSampleId :
NWB-1999


Tgt Ion:105 Resp: 154948
Ion Ratio Lower Upper
105 100
120 43.7 21.2 63.6

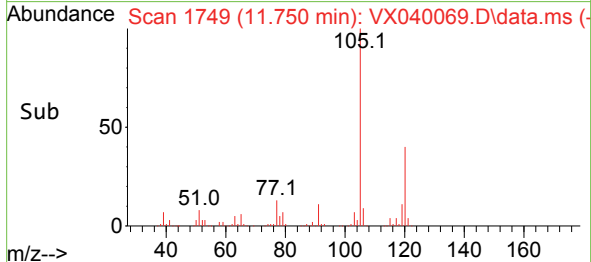

#85
sec-Butylbenzene
Concen: 26.156 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. -0.140 min
Lab File: VX040069.D
Acq: 01 Feb 2024 14:24

Tgt Ion:105 Resp: 154948
Ion Ratio Lower Upper
105 100
134 0.0 9.8 29.4#



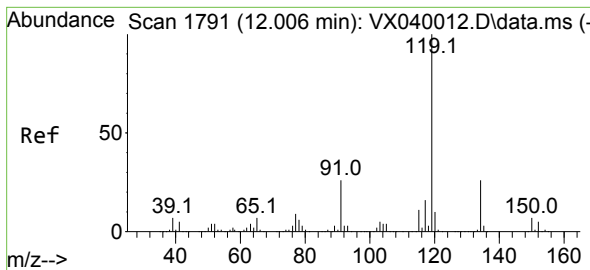

#86

p-Isopropyltoluene

Concen: 1.185 ug/l

RT: 11.969 min Scan# 11

Delta R.T. -0.036 min

Lab File: VX040069.D

Acq: 01 Feb 2024 14:24

Instrument :

MSVOA_X

ClientSampleId :

NWB-1999





Tgt Ion:119 Resp: 5730

Ion Ratio Lower Upper

119 100

134 27.9 12.8 38.3

91 27.8 13.1 39.3

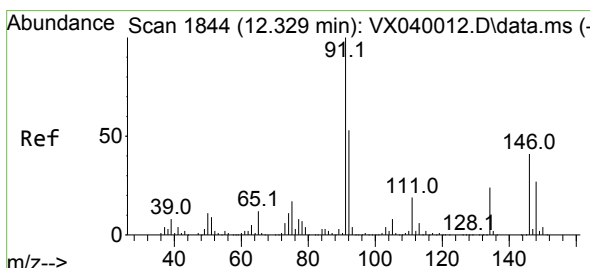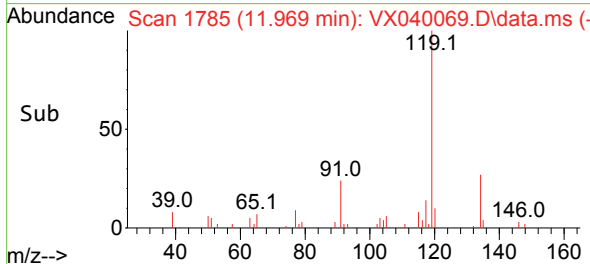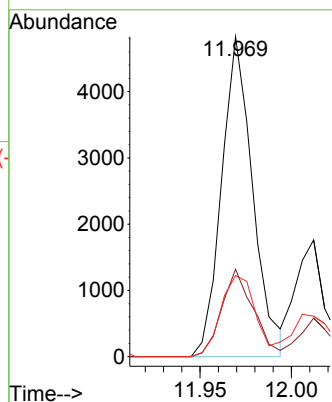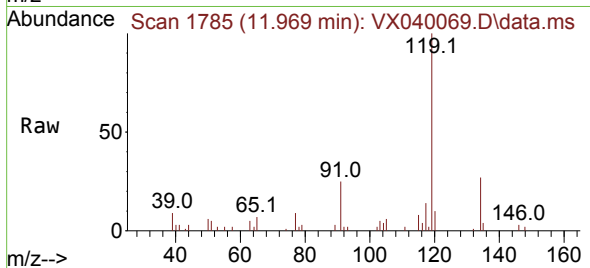

#89

n-Butylbenzene

Concen: 2.575 ug/l

RT: 12.323 min Scan# 1843

Delta R.T. -0.006 min

Lab File: VX040069.D

Acq: 01 Feb 2024 14:24




Tgt Ion: 91 Resp: 12092


Ion Ratio Lower Upper

91 100

92 34.6 27.4 82.0

134 98.5 12.6 37.8#

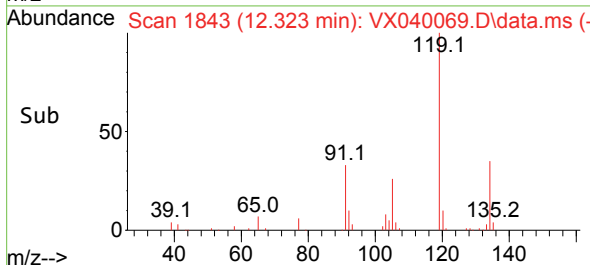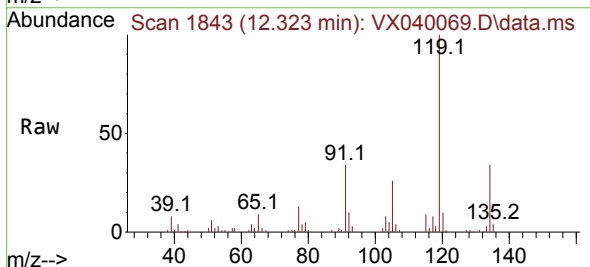



#90

Hexachloroethane

Concen: 2.448 ug/l

RT: 12.530 min Scan# 117

Delta R.T. -0.006 min

Lab File: VX040069.D

Acq: 01 Feb 2024 14:24

Instrument :

MSVOA_X

ClientSampleId :





NWB-1999

Tgt Ion:117 Resp: 1843

Ion Ratio Lower Upper

117 100

201 0.0 32.9 98.6#

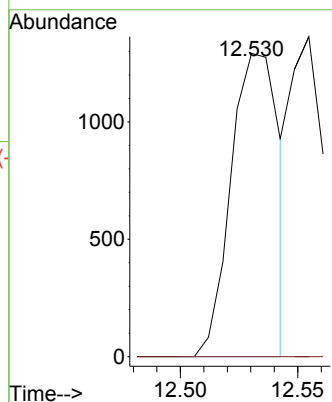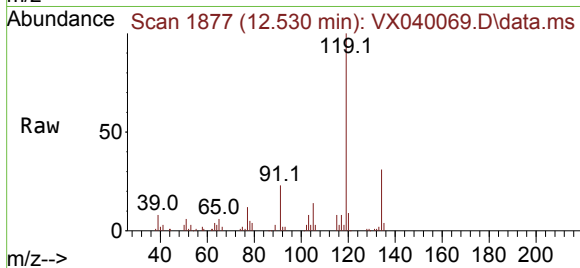

#92

1,2-Dibromo-3-Chloropropane

Concen: 0.425 ug/l

RT: 12.920 min Scan# 1941

Delta R.T. -0.018 min

Lab File: VX040069.D

Acq: 01 Feb 2024 14:24




Tgt Ion: 75 Resp: 197


Ion Ratio Lower Upper

75 100

155 0.0 36.1 108.5#

157 0.0 44.9 134.7#

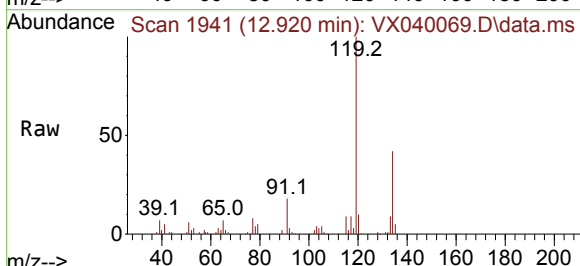



#95

Naphthalene

Concen: 10.310 ug/l

RT: 13.774 min Scan# 20

Delta R.T. 0.000 min

Lab File: VX040069.D


Acq: 01 Feb 2024 14:24

Instrument :

MSVOA_X

ClientSampleId :

NWB-1999

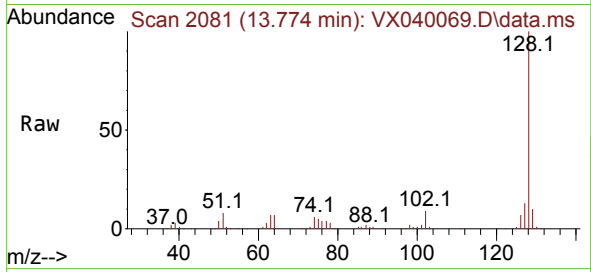

Tgt Ion:128 Resp: 53385

Ion Ratio Lower Upper

128 100

127 13.2 10.3 15.5

129 11.2 8.8 13.2

