

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020124\
 Data File : VX040058.D
 Acq On : 01 Feb 2024 10:10
 Operator : JC/MD
 Sample : VX0201MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0201MBL01

Quant Time: Feb 02 01:35:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X013024W.M
 Quant Title : SW846 8260
 QLast Update : Thu Feb 01 05:44:39 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	97242	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	171959	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	160523	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	74147	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	72735	46.476	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	92.960%
35) Dibromofluoromethane	5.385	113	55482	47.397	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	94.800%
50) Toluene-d8	8.647	98	200285	45.752	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	91.500%#
62) 4-Bromofluorobenzene	11.079	95	72463	42.989	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	85.980%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020124\
Data File : VX040058.D
Acq On : 01 Feb 2024 10:10
Operator : JC/MD
Sample : VX0201MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0201MBL01

Quant Time: Feb 02 01:35:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X013024W.M
Quant Title : SW846 8260
QLast Update : Thu Feb 01 05:44:39 2024
Response via : Initial Calibration




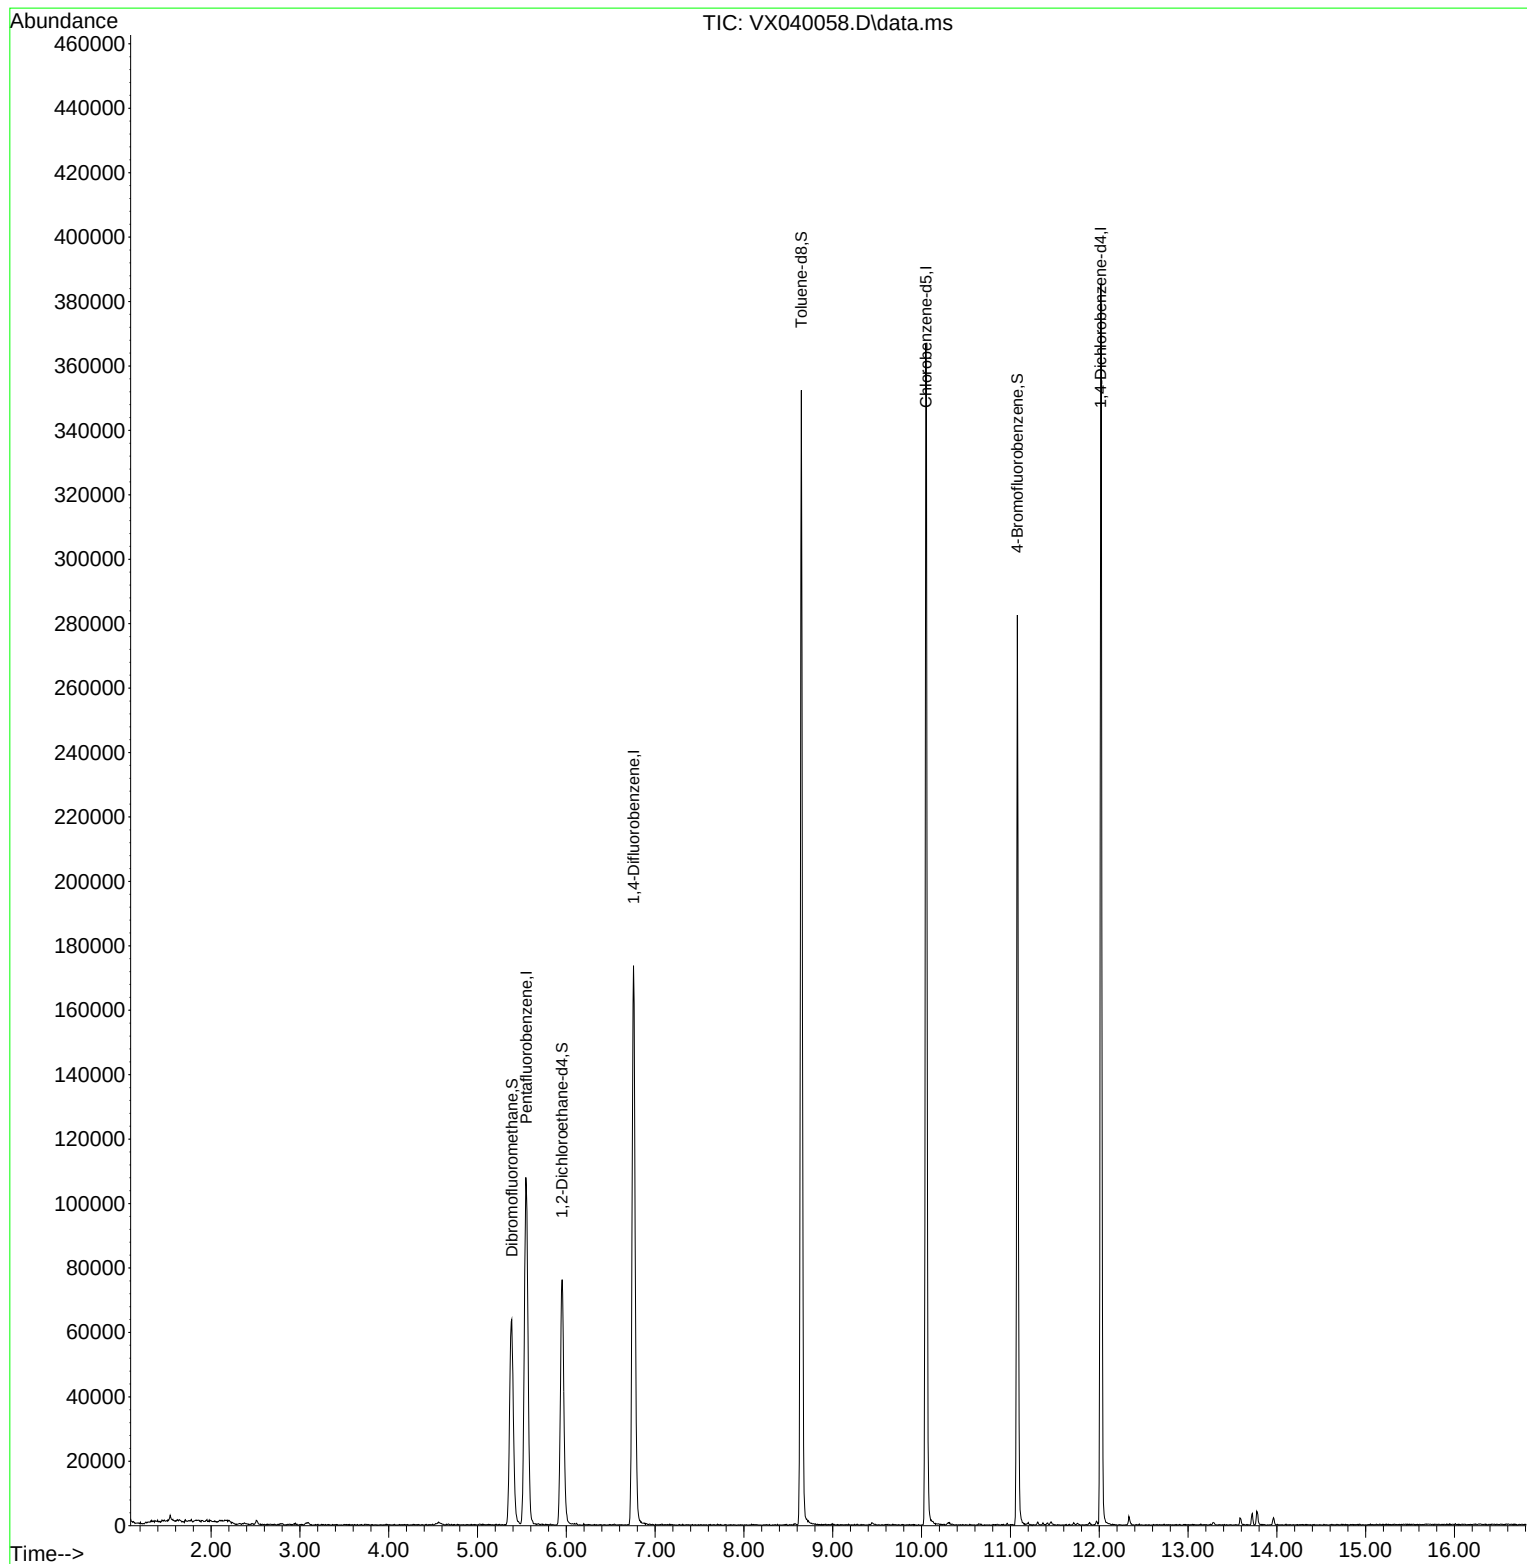




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 712
Delta R.T. -0.000 min
Lab File: VX040058.D
Acq: 01 Feb 2024 10:10




Instrument :
MSVOA_X
ClientSampleId :
VX0201MBL01


Tgt Ion:168 Resp: 97242
Ion Ratio Lower Upper
168 100
99 66.2 56.6 85.0

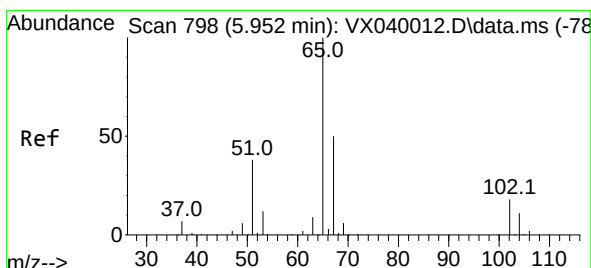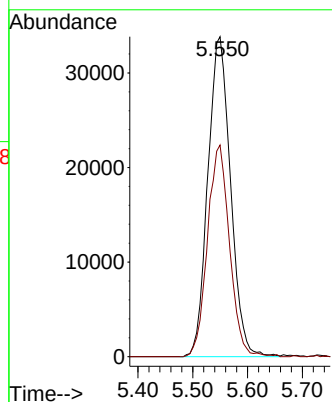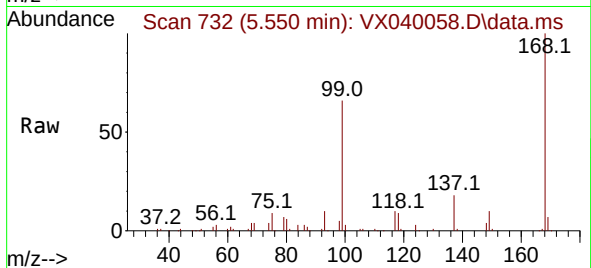

#33
1,2-Dichloroethane-d4
Concen: 46.476 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.000 min
Lab File: VX040058.D
Acq: 01 Feb 2024 10:10

Tgt Ion: 65 Resp: 72735
Ion Ratio Lower Upper
65 100
67 51.6 0.0 100.2


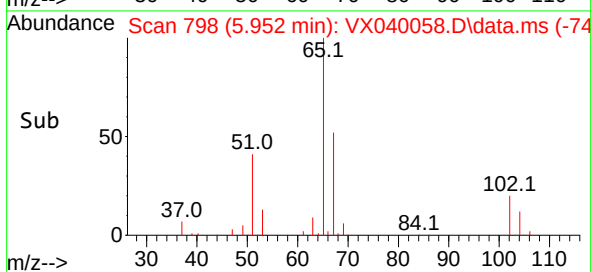
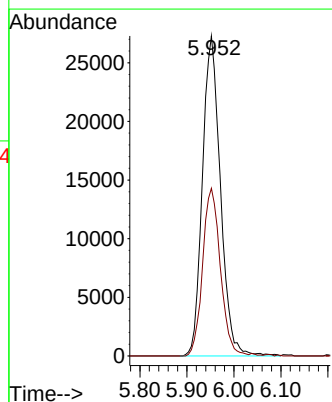





#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX040058.D
Acq: 01 Feb 2024 10:10




Instrument :
MSVOA_X
ClientSampleId :
VX0201MBL01


Tgt Ion:114 Resp: 171959
Ion Ratio Lower Upper
114 100
63 22.3 0.0 45.0
88 15.7 0.0 36.6

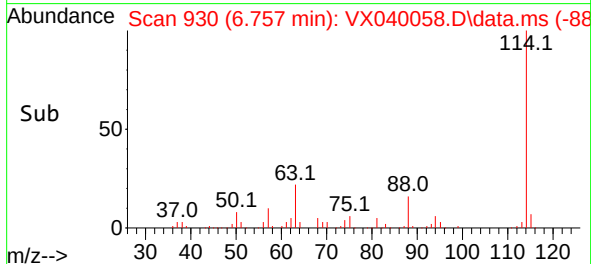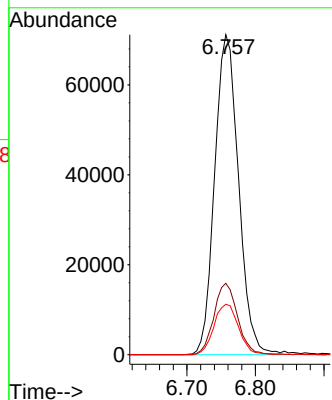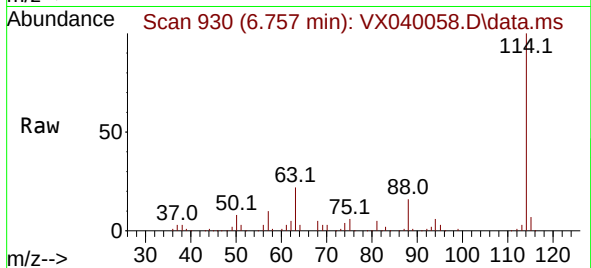

#35
Dibromofluoromethane
Concen: 47.397 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX040058.D
Acq: 01 Feb 2024 10:10

Tgt Ion:113 Resp: 55482
Ion Ratio Lower Upper
113 100
111 105.2 82.9 124.3
192 16.8 13.3 19.9


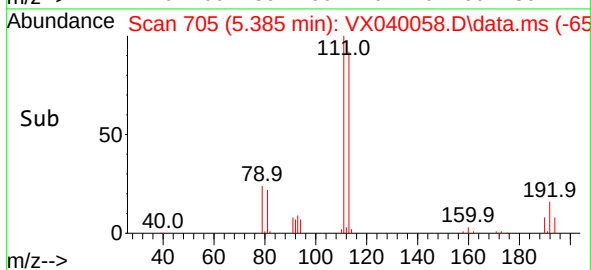
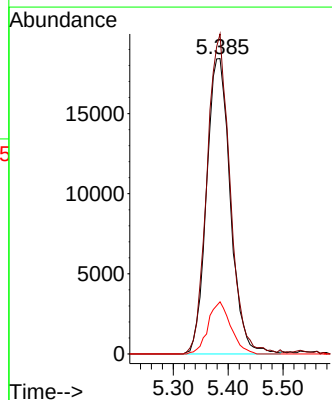
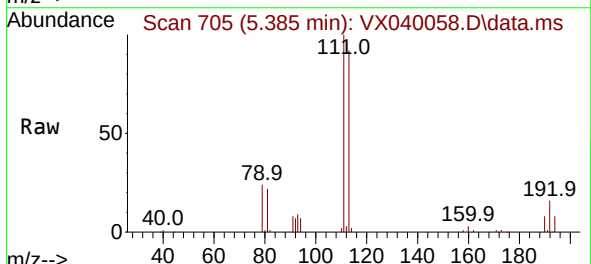




#50
Toluene-d8
Concen: 45.752 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX040058.D
Acq: 01 Feb 2024 10:10




Instrument :
MSVOA_X
ClientSampleId :
VX0201MBL01


Tgt Ion: 98 Resp: 200285
Ion Ratio Lower Upper
98 100
100 64.7 53.1 79.7

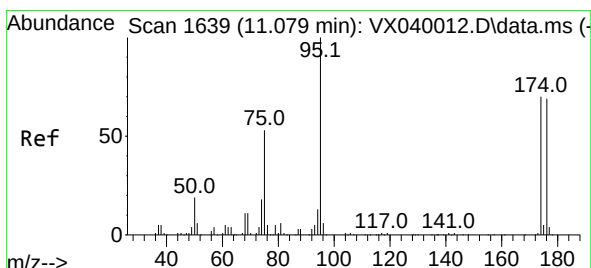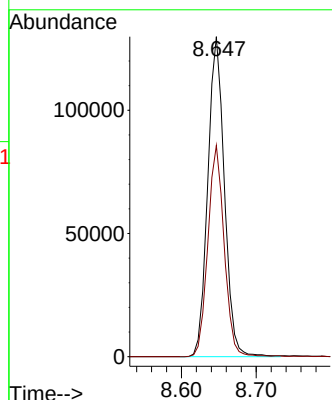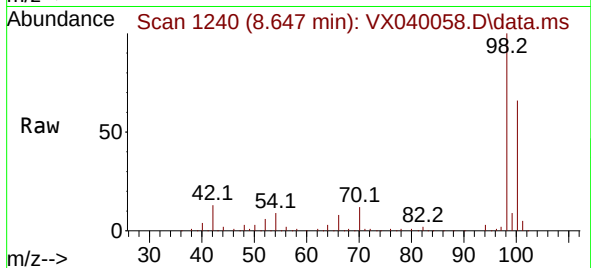

#62
4-Bromofluorobenzene
Concen: 42.989 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX040058.D
Acq: 01 Feb 2024 10:10

Tgt Ion: 95 Resp: 72463
Ion Ratio Lower Upper
95 100
174 68.9 0.0 135.6
176 65.5 0.0 131.0


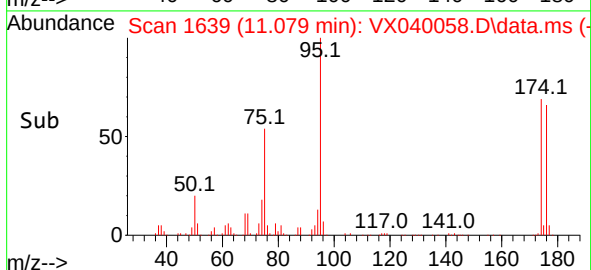
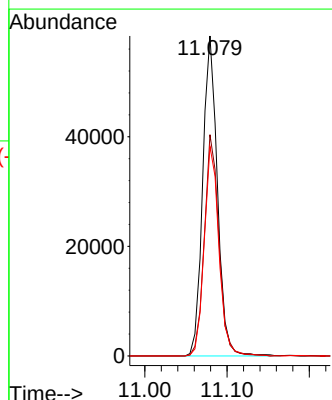





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1471
Delta R.T. -0.006 min
Lab File: VX040058.D
Acq: 01 Feb 2024 10:10

Instrument :
MSVOA_X
ClientSampleId :
VX0201MBL01

Tgt Ion:117 Resp: 160523
Ion Ratio Lower Upper
117 100
82 61.4 46.2 69.4
119 33.6 25.5 38.3

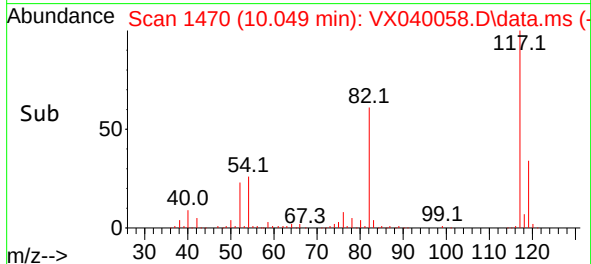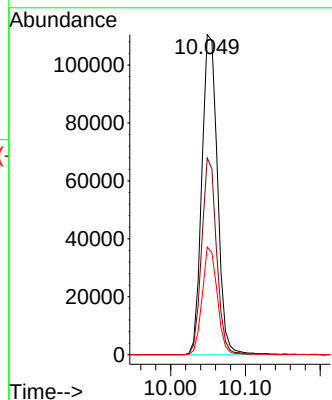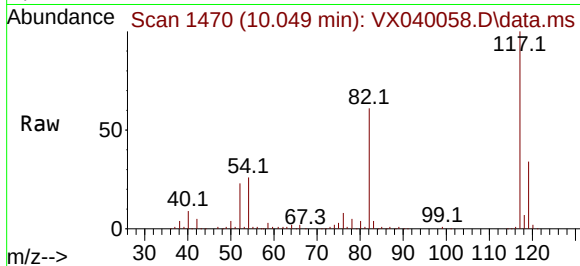

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. -0.000 min
Lab File: VX040058.D
Acq: 01 Feb 2024 10:10

Tgt Ion:152 Resp: 74147
Ion Ratio Lower Upper
152 100
115 64.2 43.3 129.9
150 159.3 0.0 345.0

