
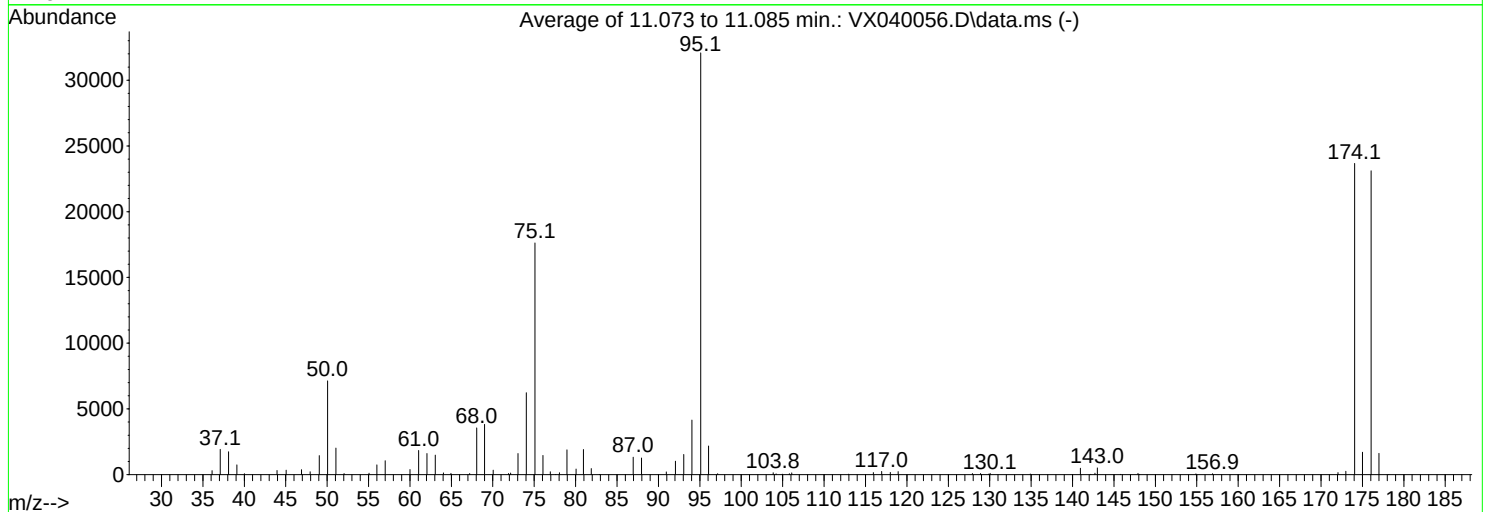


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020124\
Data File : VX040056.D
Acq On : 01 Feb 2024 08:31
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X013024W.M
Title : SW846 8260
Last Update : Thu Feb 01 05:44:39 2024

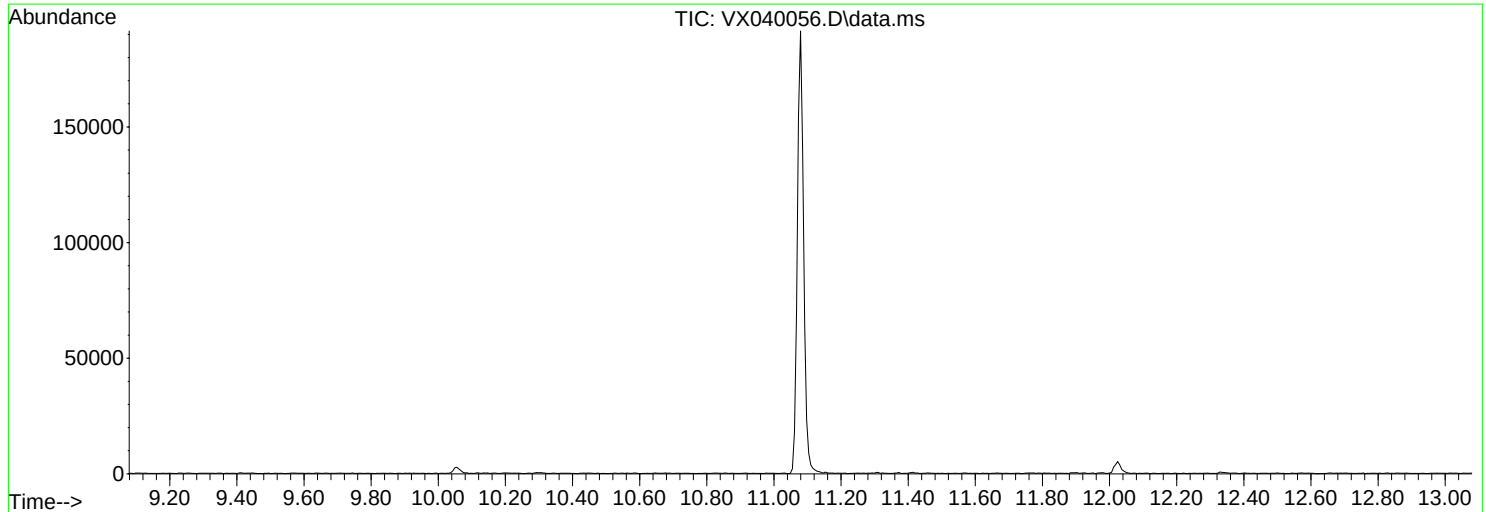

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.2	7129	PASS
75	95	30	60	54.9	17617	PASS
95	95	100	100	100.0	32080	PASS
96	95	5	9	6.8	2183	PASS
173	174	0.00	2	1.1	261	PASS
174	95	50	100	73.8	23664	PASS
175	174	5	9	7.2	1703	PASS
176	174	95	101	97.7	23115	PASS
177	176	5	9	7.0	1616	PASS