


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020222\
 Data File : VX026724.D
 Acq On : 02 Feb 2022 09:19
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
 Title : SW846 8260
 Last Update : Tue Jan 11 14:45:13 2022

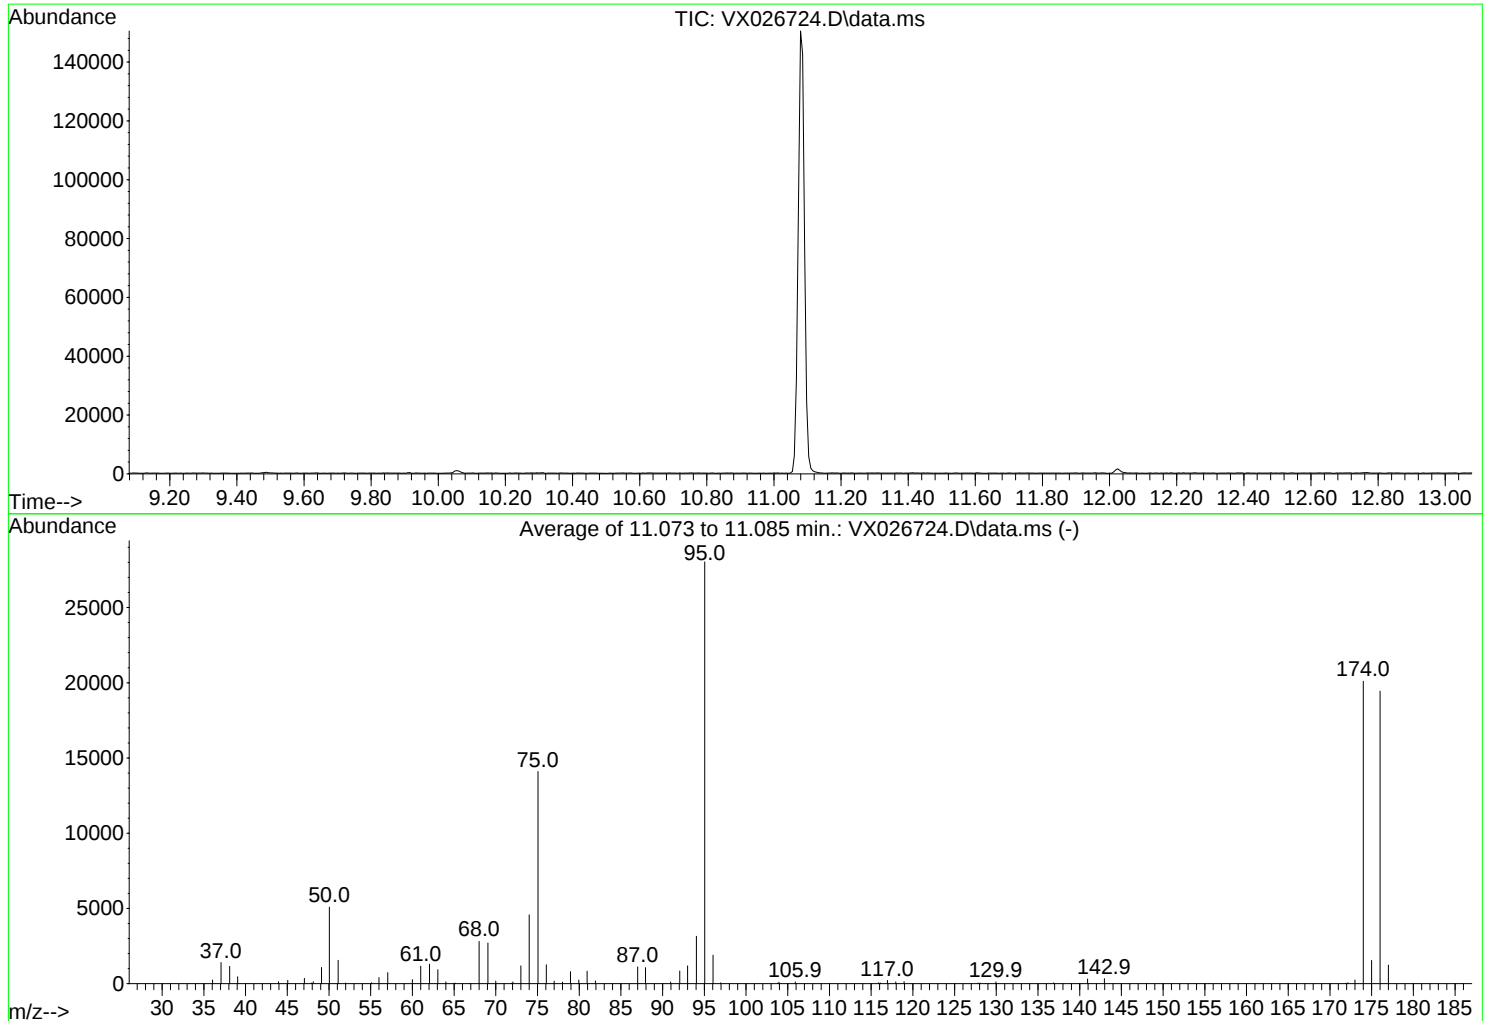

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	5089	PASS
75	95	30	60	50.3	14098	PASS
95	95	100	100	100.0	28037	PASS
96	95	5	9	6.7	1891	PASS
173	174	0.00	2	1.2	244	PASS
174	95	50	100	71.7	20105	PASS
175	174	5	9	7.6	1538	PASS
176	174	95	101	96.7	19444	PASS
177	176	5	9	6.3	1229	PASS