
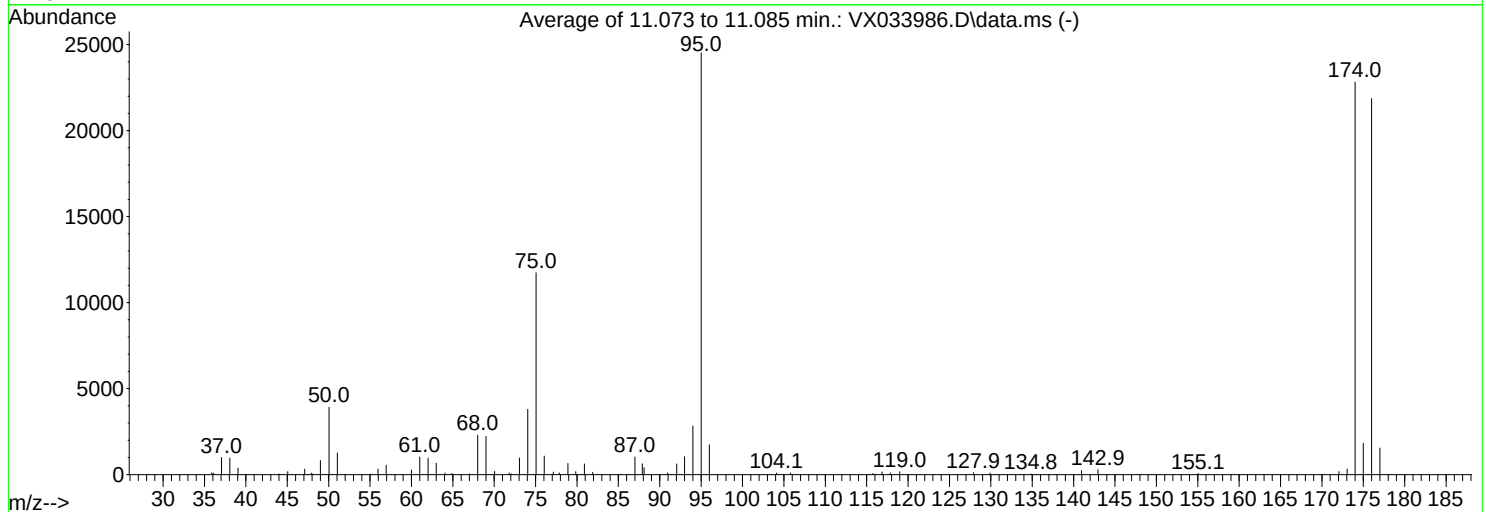


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020223\
Data File : VX033986.D
Acq On : 02 Feb 2023 08:14
Operator : JC/MD
Sample : BFB607
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB607

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM020223WMA.M
Title : VOC Analysis
Last Update : Fri Feb 03 04:22:50 2023

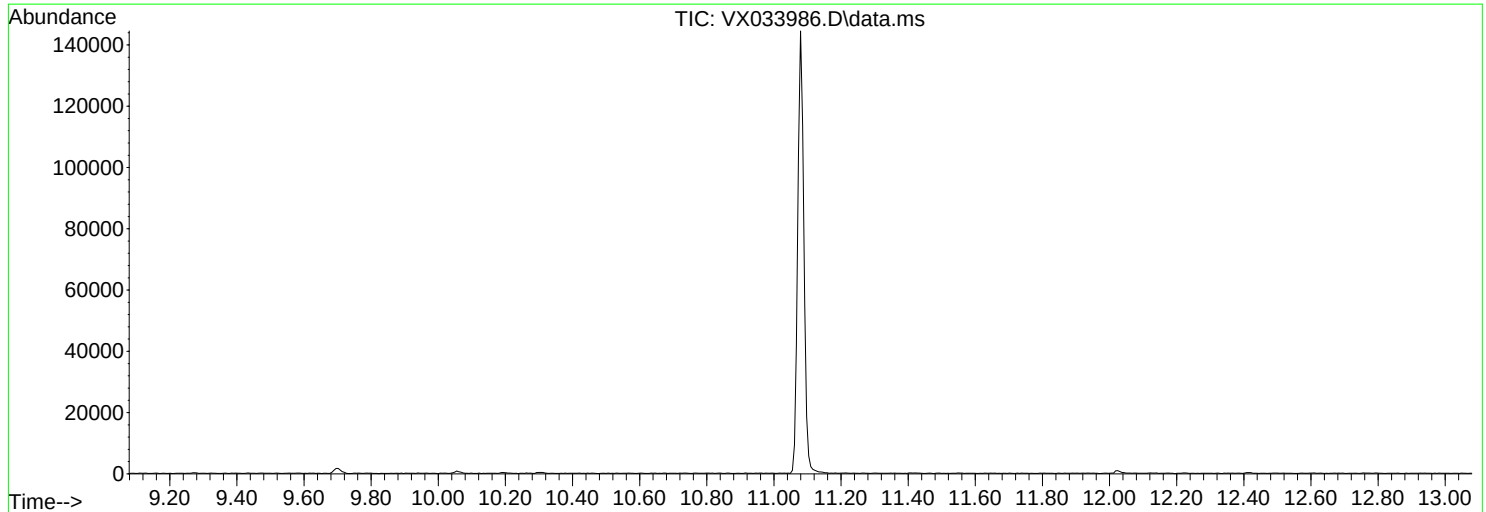

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.0	3916	PASS
75	95	30	80	47.9	11734	PASS
95	95	100	100	100.0	24520	PASS
96	95	5	9	7.1	1739	PASS
173	174	0.00	2	1.4	326	PASS
174	95	50	120	93.1	22816	PASS
175	174	5	9	8.0	1823	PASS
176	174	95	101	95.8	21859	PASS
177	176	5	9	7.1	1543	PASS

m/z	Abundance
40.00	134.0
44.00	150.0

Instrument :
MSVOA_X
ClientSampleId :
BFB607

m/z	Abundance
35.90	235.0
37.10	957.0
38.00	986.0
39.00	363.0
40.00	158.0
44.10	240.0
45.10	185.0
47.00	360.0
47.90	143.0
49.00	795.0
50.00	3695.0
51.00	1332.0
51.90	56.0
56.00	309.0
56.90	558.0
60.00	278.0
61.00	1159.0
62.00	917.0
62.90	555.0
64.10	113.0
64.90	69.0
67.00	67.0
68.00	2260.0
69.00	2111.0
70.10	224.0
71.80	150.0
73.10	1034.0
74.00	3489.0
75.00	11052.0
76.00	1080.0
77.10	141.0
77.80	101.0
78.90	606.0
80.00	159.0
80.90	513.0
81.90	131.0
87.00	889.0
87.90	950.0
90.90	72.0
92.10	496.0
93.00	909.0
94.00	2730.0
95.00	21968.0
96.00	1667.0
104.10	112.0
105.90	59.0
116.00	96.0
116.90	127.0
117.90	66.0
119.00	172.0
127.90	95.0
129.90	83.0
140.90	171.0
143.00	224.0
147.70	53.0
154.80	58.0
159.00	52.0
172.00	105.0
173.10	236.0
174.00	17344.0
175.00	1504.0
176.00	16408.0
177.00	1217.0

Instrument :
MSVOA_X
ClientSampleId :
BFB607

m/z	Abundance
36.10	241.0
37.00	1278.0
38.10	1145.0
39.10	546.0
39.90	151.0
44.00	204.0
45.00	223.0
47.10	306.0
48.10	154.0
49.00	914.0
50.00	4775.0
51.00	1478.0
55.10	60.0
55.90	358.0
57.00	717.0
60.10	293.0
61.00	1126.0
62.00	1174.0
63.00	900.0
64.00	86.0
64.90	78.0
67.10	65.0
68.00	2740.0
69.00	2639.0
70.00	170.0
71.80	131.0
73.00	1077.0
74.00	4621.0
75.00	13854.0
76.10	1273.0
77.10	186.0
77.90	93.0
78.90	752.0
79.80	235.0
80.90	762.0
81.90	183.0
87.00	1266.0
88.10	1191.0
91.00	171.0
92.00	798.0
93.00	1281.0
94.00	3490.0
95.00	29616.0
96.00	2121.0
104.10	85.0
105.80	160.0
115.70	112.0
116.90	202.0
117.80	123.0
118.90	200.0
127.90	119.0
129.90	123.0
134.80	53.0
141.00	293.0
142.90	411.0
155.10	84.0
172.10	196.0
173.00	427.0
174.00	27176.0
175.00	2213.0
176.00	25808.0
177.00	1793.0
178.10	54.0

Instrument :
MSVOA_X
ClientSampleId :
BFB607

m/z	Abundance
35.90	114.0
37.10	756.0
38.10	741.0
39.10	247.0
39.90	108.0
44.10	154.0
45.10	118.0
47.20	308.0
47.90	148.0
49.00	742.0
50.10	3277.0
51.10	969.0
55.10	56.0
56.00	301.0
57.00	368.0
59.90	237.0
61.00	781.0
62.00	792.0
63.10	557.0
64.00	90.0
64.90	86.0
68.00	1870.0
69.00	1930.0
70.00	153.0
72.10	122.0
73.10	789.0
74.10	3264.0
75.10	10297.0
76.00	874.0
77.20	119.0
77.90	122.0
78.90	595.0
79.80	141.0
80.90	596.0
81.90	115.0
87.00	930.0
87.90	946.0
90.90	72.0
92.10	562.0
93.00	924.0
94.00	2271.0
95.00	21976.0
96.00	1428.0
104.10	84.0
105.70	56.0
115.80	70.0
116.80	144.0
117.80	109.0
119.10	130.0
127.90	129.0
129.90	86.0
134.90	58.0
137.00	57.0
140.90	241.0
143.00	236.0
155.00	101.0
172.10	224.0
173.00	314.0
174.00	23928.0
175.00	1753.0
176.00	23360.0
177.00	1619.0

Instrument :
MSVOA_X
ClientSampleId :
BFB607