

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX020224\  
 Data File : VX040084.D  
 Acq On : 02 Feb 2024 14:07  
 Operator : JC/MD  
 Sample : P1342-07  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 MR-323P-GW-20240131-1

Quant Time: Feb 03 02:15:49 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X013024W.M  
 Quant Title : SW846 8260  
 QLast Update : Thu Feb 01 05:44:39 2024  
 Response via : Initial Calibration

### Manual Integrations APPROVED

Reviewed By :John Carlone 02/05/2024  
 Supervised By :Semsettin Yesilyurt 02/05/2024

| Compound                    | R.T.           | QIon | Response   | Conc     | Units  | Dev(Min) |
|-----------------------------|----------------|------|------------|----------|--------|----------|
| -----                       |                |      |            |          |        |          |
| Internal Standards          |                |      |            |          |        |          |
| 1) Pentafluorobenzene       | 5.556          | 168  | 86779      | 50.000   | ug/l   | 0.00     |
| 34) 1,4-Difluorobenzene     | 6.763          | 114  | 156755     | 50.000   | ug/l   | 0.00     |
| 63) Chlorobenzene-d5        | 10.055         | 117  | 150271     | 50.000   | ug/l   | 0.00     |
| 72) 1,4-Dichlorobenzene-d4  | 12.024         | 152  | 79957      | 50.000   | ug/l   | 0.00     |
|                             |                |      |            |          |        |          |
| System Monitoring Compounds |                |      |            |          |        |          |
| 33) 1,2-Dichloroethane-d4   | 5.952          | 65   | 63624      | 45.556   | ug/l   | 0.00     |
| Spiked Amount 50.000        | Range 78 - 117 |      | Recovery = | 91.120%  |        |          |
| 35) Dibromofluoromethane    | 5.391          | 113  | 49312      | 46.212   | ug/l   | 0.00     |
| Spiked Amount 50.000        | Range 75 - 124 |      | Recovery = | 92.420%  |        |          |
| 50) Toluene-d8              | 8.647          | 98   | 194695     | 48.788   | ug/l   | 0.00     |
| Spiked Amount 50.000        | Range 92 - 112 |      | Recovery = | 97.580%  |        |          |
| 62) 4-Bromofluorobenzene    | 11.079         | 95   | 80656      | 52.490   | ug/l   | 0.00     |
| Spiked Amount 50.000        | Range 83 - 123 |      | Recovery = | 104.980% |        |          |
|                             |                |      |            |          |        |          |
| Target Compounds            |                |      |            |          | Qvalue |          |
| 11) Tert butyl alcohol      | 2.959          | 59   | 61008      | 240.747  | ug/l # | 91       |
| 16) Acetone                 | 2.380          | 43   | 4691       | 7.169    | ug/l   | 99       |
| 19) Methyl tert-butyl Ether | 3.117          | 73   | 50339      | 15.056   | ug/l   | 91       |
| 20) Methylene Chloride      | 2.788          | 84   | 1384       | 1.190    | ug/l # | 86       |
| 25) 2-Butanone              | 4.586          | 43   | 2292       | 2.520    | ug/l   | 93       |
| 30) Chloroform              | 5.099          | 83   | 2078       | 0.991    | ug/l   | 96       |
| 31) Cyclohexane             | 5.470          | 56   | 12521      | 7.157    | ug/l # | 87       |
| 39) Methylcyclohexane       | 7.379          | 83   | 29938      | 15.944   | ug/l   | 99       |
| 40) Benzene                 | 6.037          | 78   | 32889      | 7.317    | ug/l   | 94       |
| 52) Toluene                 | 8.720          | 92   | 6005       | 2.143    | ug/l   | 79       |
| 65) Chlorobenzene           | 10.079         | 112  | 4304       | 1.386    | ug/l   | 94       |
| 67) Ethyl Benzene           | 10.195         | 91   | 3119420    | 559.742  | ug/l   | 100      |
| 68) m/p-Xylenes             | 10.299         | 106  | 23906m     | 11.402   | ug/l   |          |
| 69) o-Xylene                | 10.640         | 106  | 5390       | 2.710    | ug/l   | 89       |
| 73) Isopropylbenzene        | 10.963         | 105  | 742688     | 129.354  | ug/l   | 100      |
| 78) n-propylbenzene         | 11.305         | 91   | 2555173    | 361.647  | ug/l   | 98       |
| 80) 1,3,5-Trimethylbenzene  | 11.451         | 105  | 899716     | 182.294  | ug/l   | 97       |
| 84) 1,2,4-Trimethylbenzene  | 11.756         | 105  | 5460770    | 1108.793 | ug/l   | 95       |
| 85) sec-Butylbenzene        | 11.890         | 105  | 103392m    | 16.524   | ug/l   |          |
| 86) p-Isopropyltoluene      | 12.012         | 119  | 44395m     | 8.689    | ug/l   |          |
| 89) n-Butylbenzene          | 12.329         | 91   | 244150     | 49.230   | ug/l # | 47       |
| 91) 1,2-Dichlorobenzene     | 12.341         | 146  | 1725       | 0.670    | ug/l # | 78       |
| -----                       |                |      |            |          |        |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX020224\  
Data File : VX040084.D  
Acq On : 02 Feb 2024 14:07  
Operator : JC/MD  
Sample : P1342-07  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 12 Sample Multiplier: 1


Instrument :  
MSVOA\_X  
ClientSampleId :  
MR-323P-GW-20240131-1

Quant Time: Feb 03 02:15:49 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X013024W.M  
Quant Title : SW846 8260  
QLast Update : Thu Feb 01 05:44:39 2024  
Response via : Initial Calibration

Manual Integrations  
APPROVED

Reviewed By :John Carlone 02/05/2024  
Supervised By :Semsettin Yesilyurt 02/05/2024

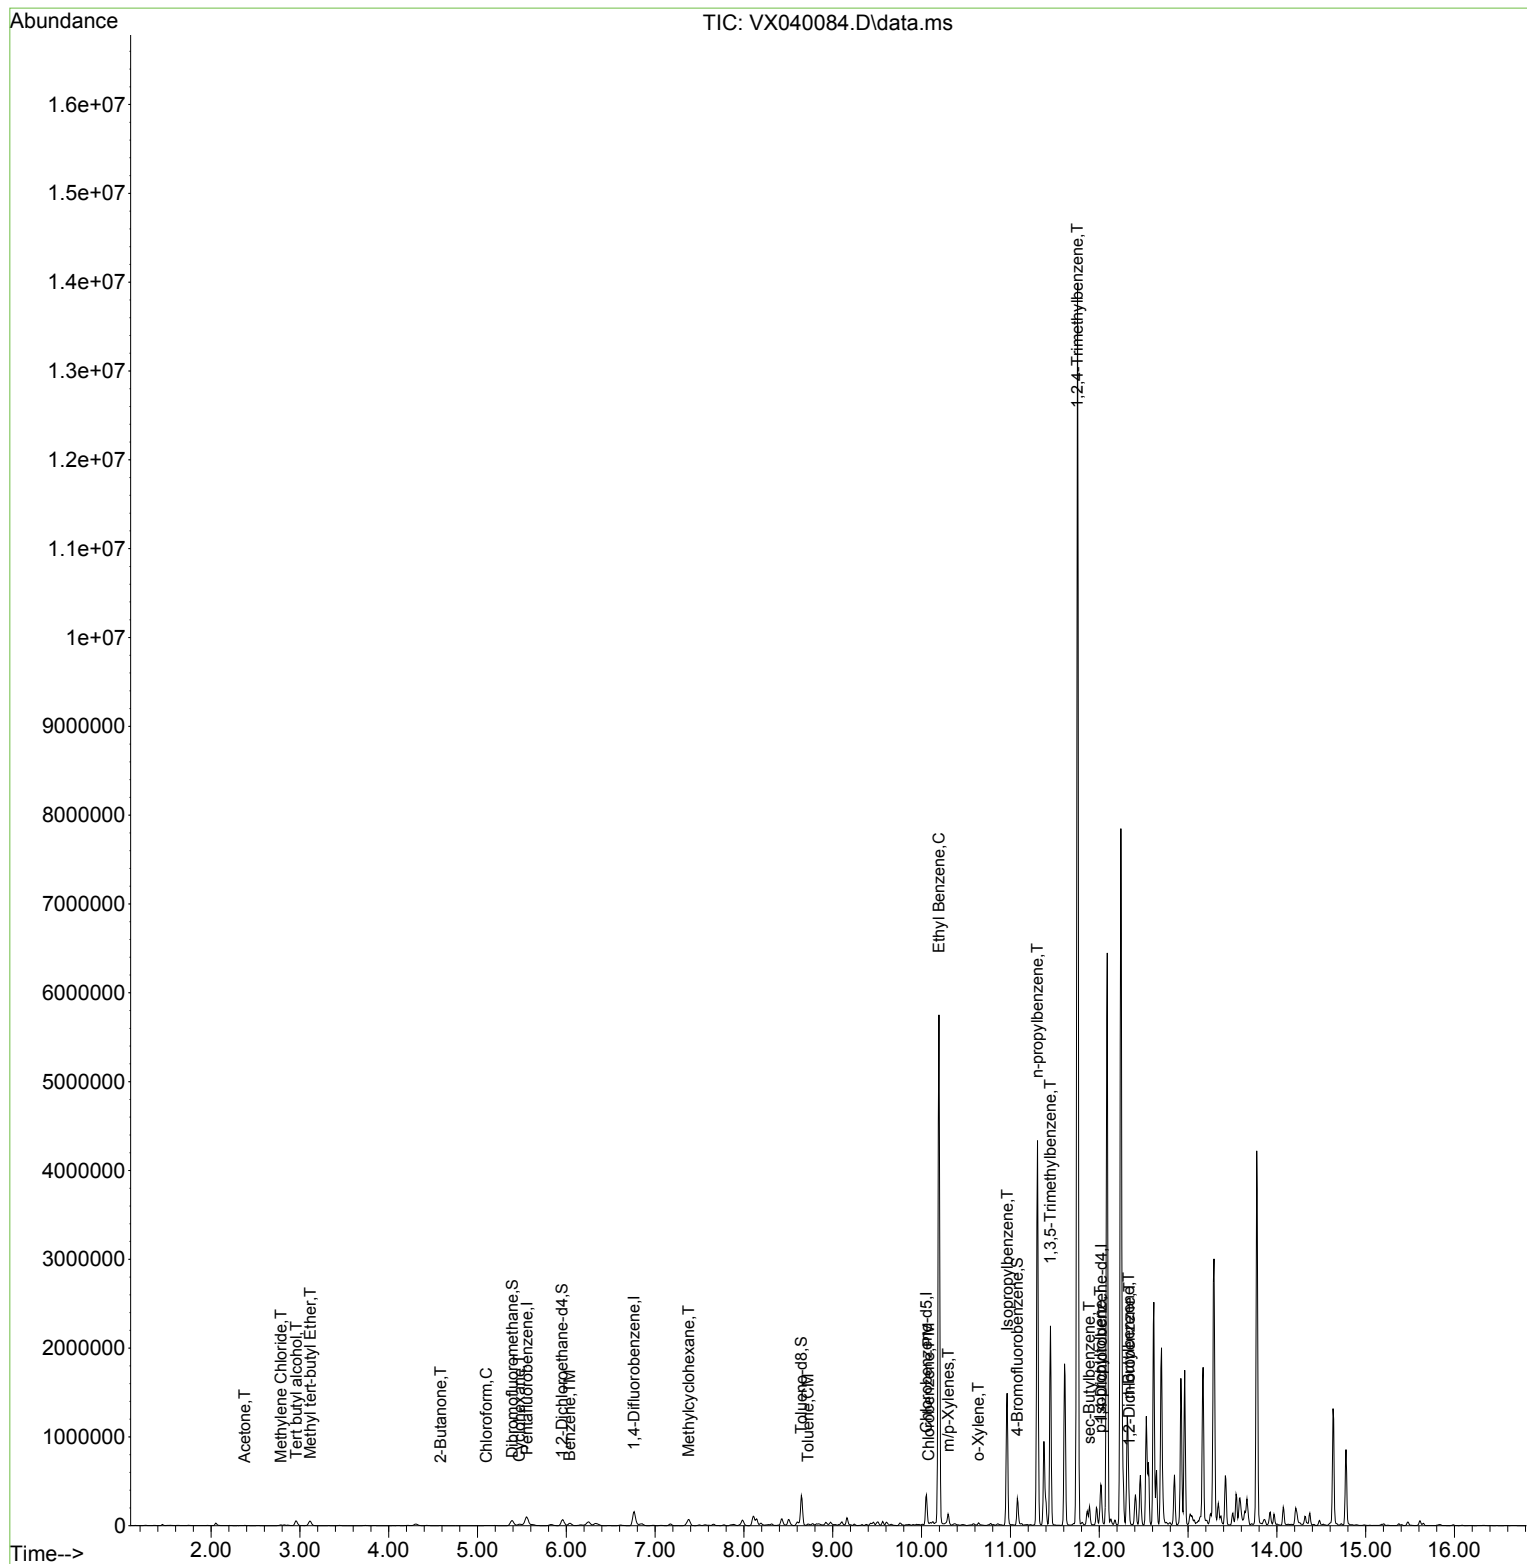

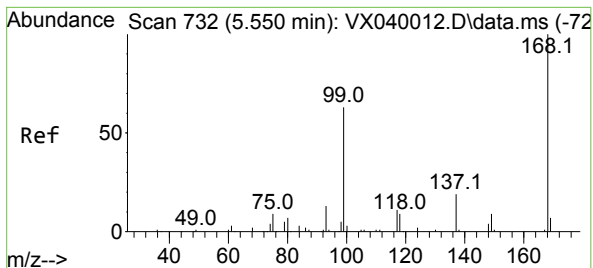

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.556 min Scan# 732

Delta R.T. 0.006 min

Lab File: VX040084.D

Acq: 02 Feb 2024 14:07

Instrument :

MSVOA\_X

ClientSampleId :

MR-323P-GW-20240131-1

Tgt Ion:168 Resp: 86779

Ion Ratio Lower Upper

168 100





99 62.1 56.6 85.0

Manual Integrations

APPROVED

Reviewed By :John Carlone 02/05/2024

Supervised By :Semsettin Yesilyurt 02/05/2024

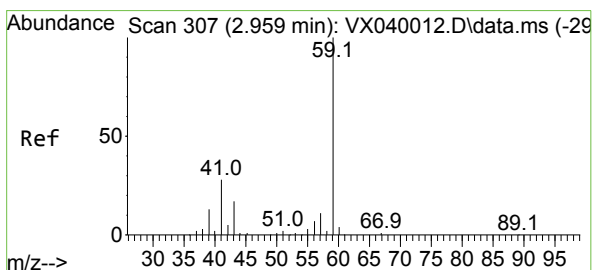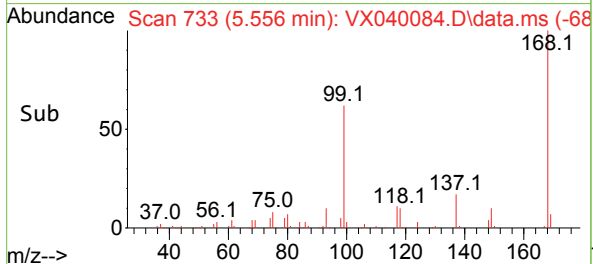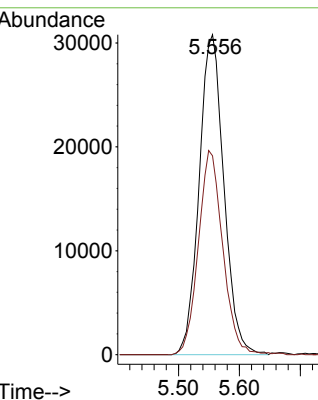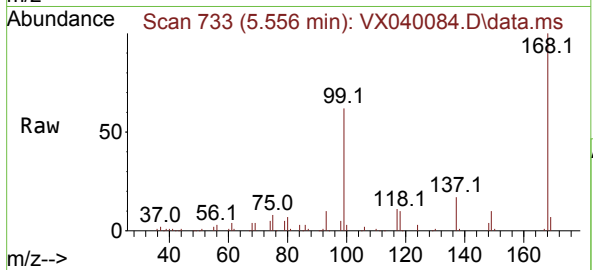

#11

Tert butyl alcohol

Concen: 240.747 ug/l

RT: 2.959 min Scan# 307

Delta R.T. -0.000 min

Lab File: VX040084.D




Acq: 02 Feb 2024 14:07


Tgt Ion: 59 Resp: 61008

Ion Ratio Lower Upper

59 100

57 10.5 6.0 9.0#

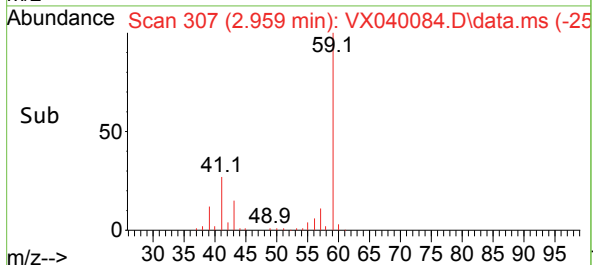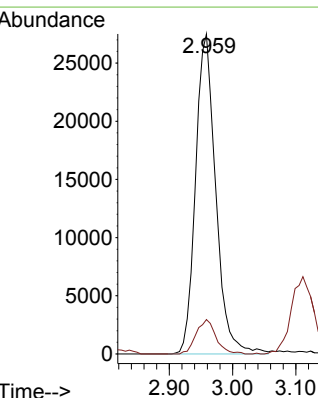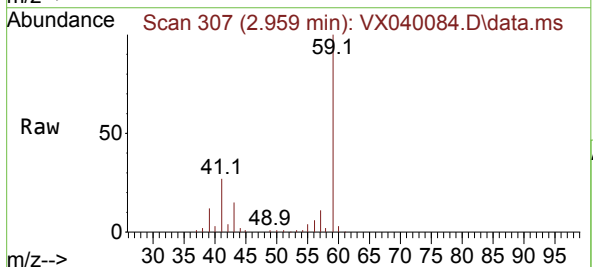



#16

Acetone

Concen: 7.169 ug/l

RT: 2.380 min Scan# 211

Delta R.T. 0.006 min

Lab File: VX040084.D

Acq: 02 Feb 2024 14:07

Instrument :

MSVOA\_X

ClientSampleId :

MR-323P-GW-20240131-1

Tgt Ion: 43 Resp: 469

Ion Ratio Lower Upper

43 100





58 27.9 21.9 32.9

Manual Integrations

APPROVED

Reviewed By :John Carlone 02/05/2024

Supervised By :Semsettin Yesilyurt 02/05/2024

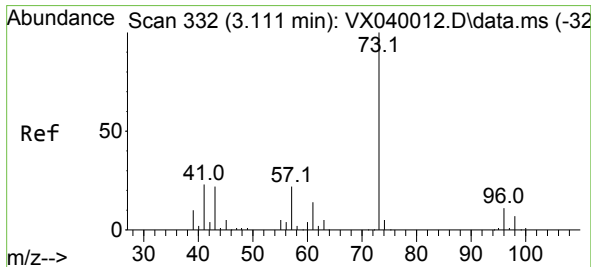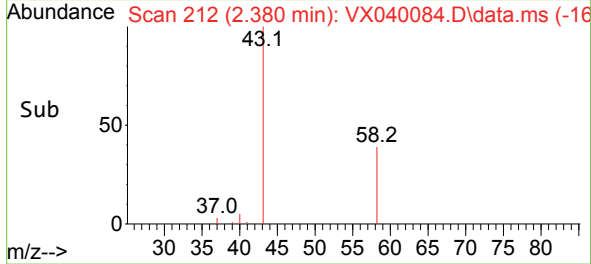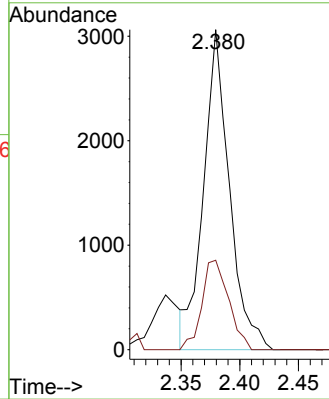

#19

Methyl tert-butyl Ether

Concen: 15.056 ug/l

RT: 3.117 min Scan# 333

Delta R.T. 0.006 min

Lab File: VX040084.D




Acq: 02 Feb 2024 14:07


Tgt Ion: 73 Resp: 50339

Ion Ratio Lower Upper

73 100


57 25.9 17.3 25.9

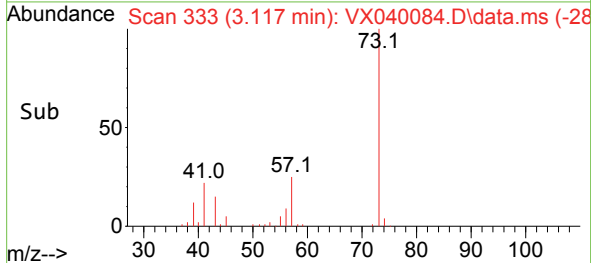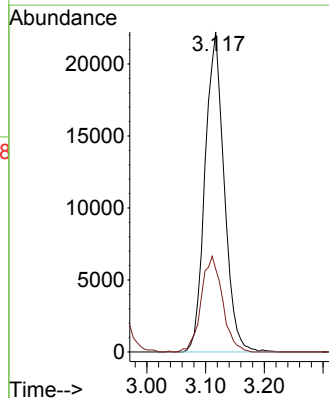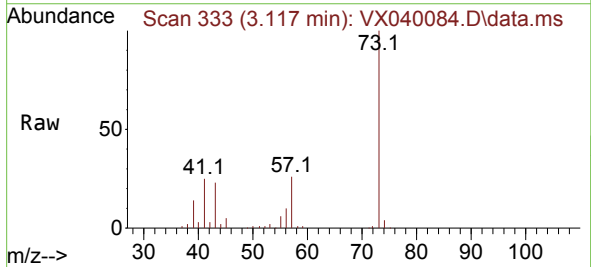



#20  
Methylene Chloride  
Concen: 1.190 ug/l  
RT: 2.788 min Scan# 21  
Delta R.T. -0.000 min  
Lab File: VX040084.D  
Acq: 02 Feb 2024 14:07




Instrument :  
MSVOA\_X  
ClientSampleId :  
MR-323P-GW-20240131-1



Tgt Ion: 84 Resp: 1384  
Ion Ratio Lower Upper  
84 100  
49 130.4 103.6 155.4  
51 35.0 33.8 50.6  
86 95.0 49.4 74.0#




Manual Integrations  
APPROVED


Reviewed By :John Carlone 02/05/2024  
Supervised By :Semsettin Yesilyurt 02/05/2024

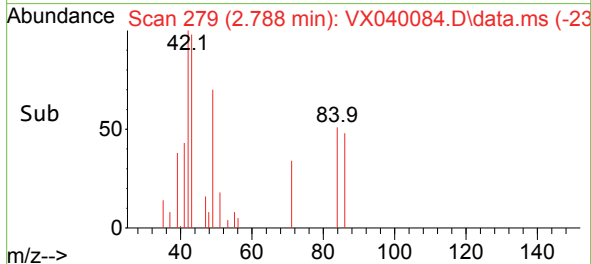

#25  
2-Butanone  
Concen: 2.520 ug/l  
RT: 4.586 min Scan# 574  
Delta R.T. 0.036 min  
Lab File: VX040084.D  
Acq: 02 Feb 2024 14:07

Tgt Ion: 43 Resp: 2292  
Ion Ratio Lower Upper  
43 100  
72 27.7 19.4 29.2

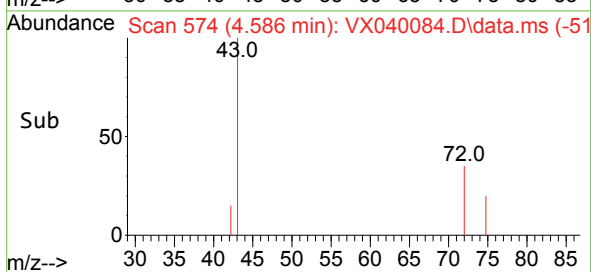



#30

Chloroform

Concen: 0.991 ug/l

RT: 5.099 min Scan# 61

Delta R.T. 0.006 min

Lab File: VX040084.D


Acq: 02 Feb 2024 14:07

Instrument :

MSVOA\_X

ClientSampleId :

MR-323P-GW-20240131-1



Tgt Ion: 83 Resp: 2078

Ion Ratio Lower Upper

83 100




85 66.1 50.3 75.5

Manual Integrations

APPROVED

Reviewed By :John Carlone 02/05/2024

Supervised By :Semsettin Yesilyurt 02/05/2024

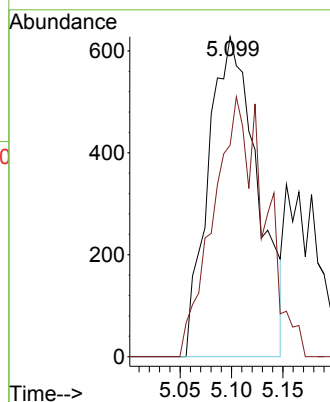

#31

Cyclohexane

Concen: 7.157 ug/l

RT: 5.470 min Scan# 719

Delta R.T. 0.006 min

Lab File: VX040084.D

Acq: 02 Feb 2024 14:07




Tgt Ion: 56 Resp: 12521


Ion Ratio Lower Upper

56 100

69 20.6 23.4 35.2#

84 71.7 65.9 98.9

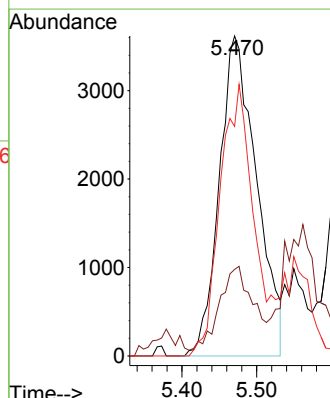



#33

1,2-Dichloroethane-d4

Concen: 45.556 ug/l

RT: 5.952 min Scan# 798

Delta R.T. -0.000 min

Lab File: VX040084.D

Acq: 02 Feb 2024 14:07

Instrument :

MSVOA\_X

ClientSampleId :

MR-323P-GW-20240131-1





Tgt Ion: 65 Resp: 63624  
 Ion Ratio Lower Upper  
 65 100  
 67 51.2 0.0 100.2

Manual Integrations

APPROVED

Reviewed By :John Carlone 02/05/2024

Supervised By :Semsettin Yesilyurt 02/05/2024

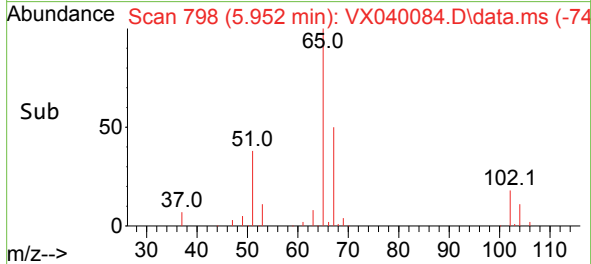

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l




RT: 6.763 min Scan# 931


Delta R.T. -0.000 min

Lab File: VX040084.D

Acq: 02 Feb 2024 14:07

Tgt Ion:114 Resp: 156755  
 Ion Ratio Lower Upper  
 114 100  
 63 21.7 0.0 45.0  
 88 16.3 0.0 36.6

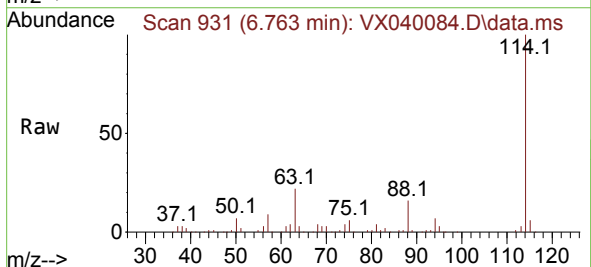



#35

Dibromofluoromethane

Concen: 46.212 ug/l

RT: 5.391 min Scan# 705

Delta R.T. 0.006 min

Lab File: VX040084.D


Acq: 02 Feb 2024 14:07

Instrument :

MSVOA\_X

ClientSampleId :

MR-323P-GW-20240131-1



Tgt Ion:113 Resp: 4931

Ion Ratio Lower Upper

113 100

111 104.6 82.9 124.3




192 17.2 13.3 19.9

Manual Integrations

APPROVED

Reviewed By :John Carlone 02/05/2024

Supervised By :Semsettin Yesilyurt 02/05/2024

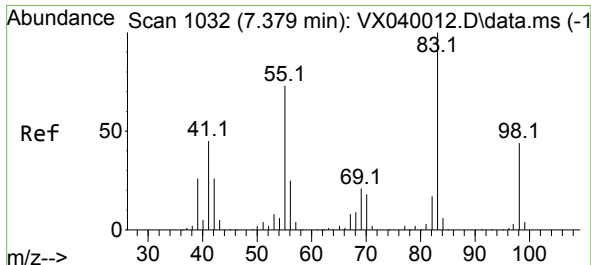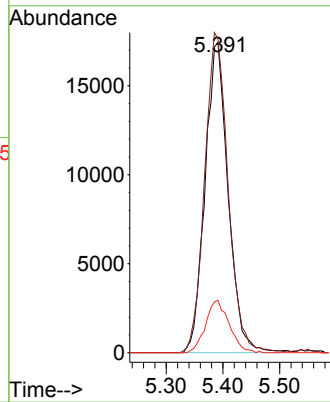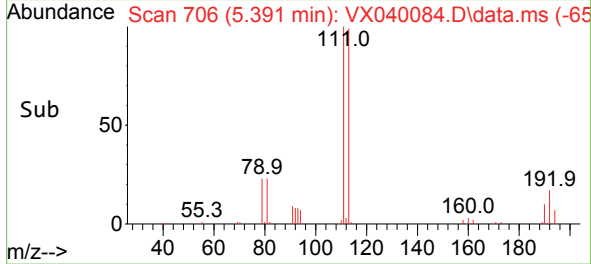

#39

Methylcyclohexane

Concen: 15.944 ug/l

RT: 7.379 min Scan# 1032

Delta R.T. -0.000 min

Lab File: VX040084.D

Acq: 02 Feb 2024 14:07




Tgt Ion: 83 Resp: 29938


Ion Ratio Lower Upper

83 100

55 79.8 64.6 97.0


98 47.3 36.7 55.1

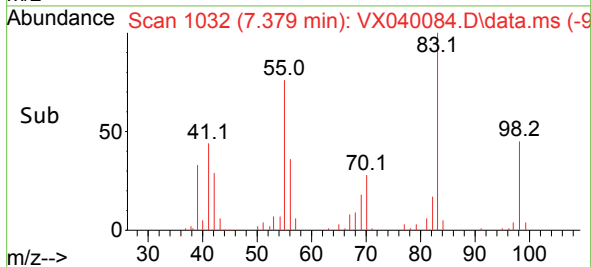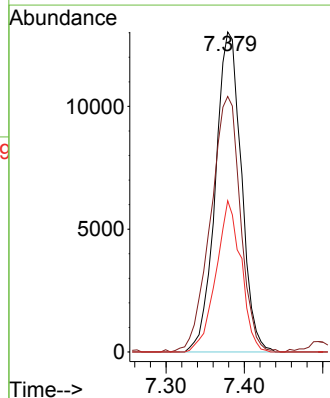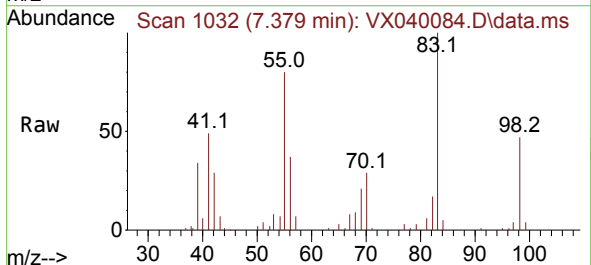

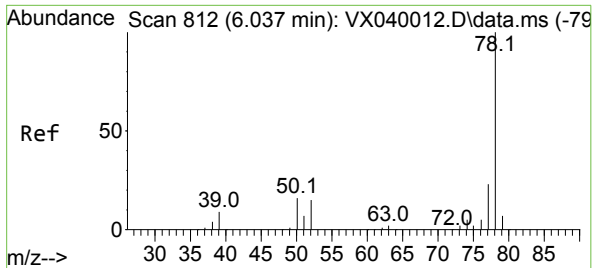

#40  
Benzene  
Concen: 7.317 ug/l  
RT: 6.037 min Scan# 812  
Delta R.T. -0.000 min  
Lab File: VX040084.D  
Acq: 02 Feb 2024 14:07




Instrument :  
MSVOA\_X  
ClientSampleId :  
MR-323P-GW-20240131-1

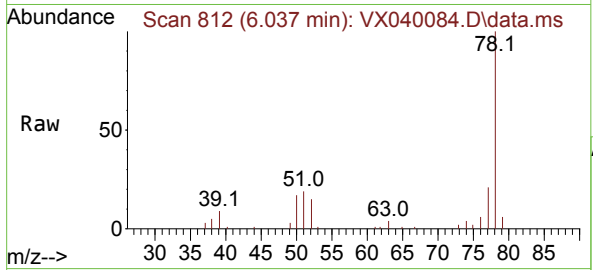

Tgt Ion: 78 Resp: 32889  
Ion Ratio Lower Upper  
78 100  
77 21.4 19.3 28.9




Manual Integrations  
APPROVED


Reviewed By :John Carlone 02/05/2024  
Supervised By :Semsettin Yesilyurt 02/05/2024

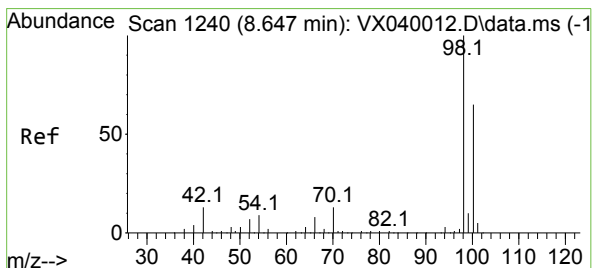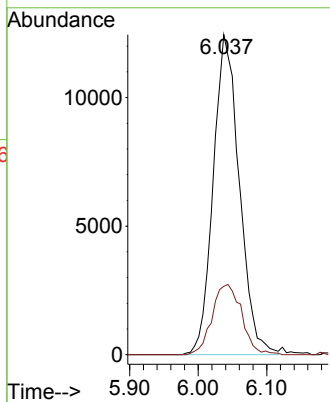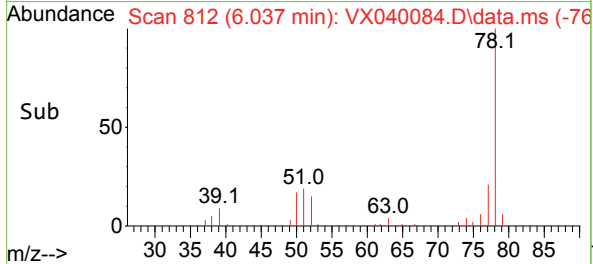

#50  
Toluene-d8  
Concen: 48.788 ug/l  
RT: 8.647 min Scan# 1240  
Delta R.T. -0.000 min  
Lab File: VX040084.D  
Acq: 02 Feb 2024 14:07

Tgt Ion: 98 Resp: 194695  
Ion Ratio Lower Upper  
98 100  
100 63.3 53.1 79.7

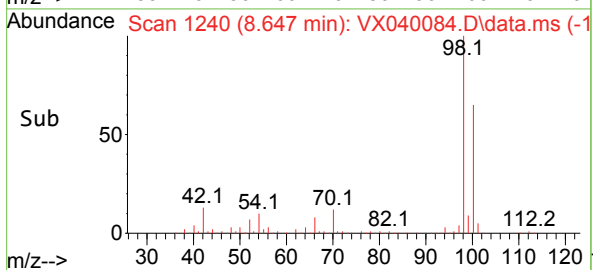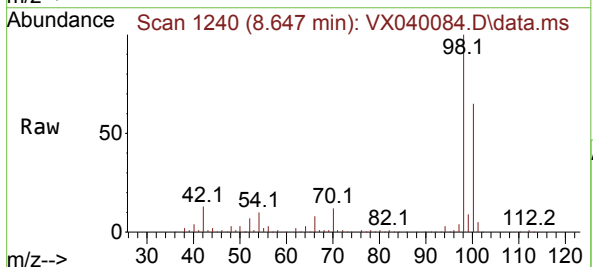



#52

Toluene

Concen: 2.143 ug/l

RT: 8.720 min Scan# 1251

Delta R.T. 0.006 min

Lab File: VX040084.D

Acq: 02 Feb 2024 14:07

Instrument :

MSVOA\_X

ClientSampleId :

MR-323P-GW-20240131-1

Tgt Ion: 92 Resp: 600

Ion Ratio Lower Upper

92 100





91 196.5 134.2 201.2

Manual Integrations

APPROVED

Reviewed By :John Carlone 02/05/2024

Supervised By :Semsettin Yesilyurt 02/05/2024

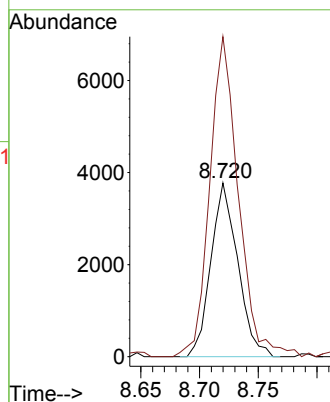

#62

4-Bromofluorobenzene

Concen: 52.490 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.000 min

Lab File: VX040084.D

Acq: 02 Feb 2024 14:07




Tgt Ion: 95 Resp: 80656


Ion Ratio Lower Upper

95 100

174 68.6 0.0 135.6

176 65.3 0.0 131.0









#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.055 min Scan# 1471  
Delta R.T. -0.000 min  
Lab File: VX040084.D  
Acq: 02 Feb 2024 14:07

Instrument :  
MSVOA\_X  
ClientSampleId :  
MR-323P-GW-20240131-1

Tgt Ion:117 Resp: 15027  
Ion Ratio Lower Upper  
117 100  
82 59.5 46.2 69.4  
119 31.8 25.5 38.3




Manual Integrations  
APPROVED


Reviewed By :John Carlone 02/05/2024  
Supervised By :Semsettin Yesilyurt 02/05/2024



#65  
Chlorobenzene  
Concen: 1.386 ug/l  
RT: 10.079 min Scan# 1475  
Delta R.T. -0.000 min  
Lab File: VX040084.D  
Acq: 02 Feb 2024 14:07


Tgt Ion:112 Resp: 4304  
Ion Ratio Lower Upper  
112 100  
114 28.6 25.7 38.5



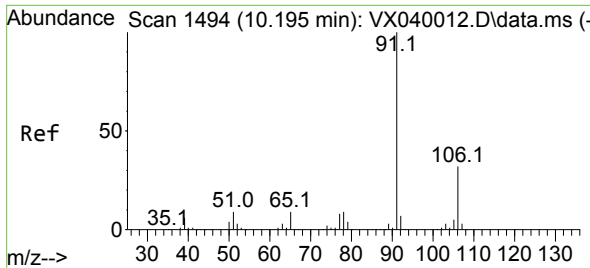

#67  
Ethyl Benzene  
Concen: 559.742 ug/l  
RT: 10.195 min Scan# 1494  
Delta R.T. -0.000 min  
Lab File: VX040084.D  
Acq: 02 Feb 2024 14:07




Instrument :  
MSVOA\_X  
ClientSampleId :  
MR-323P-GW-20240131-1

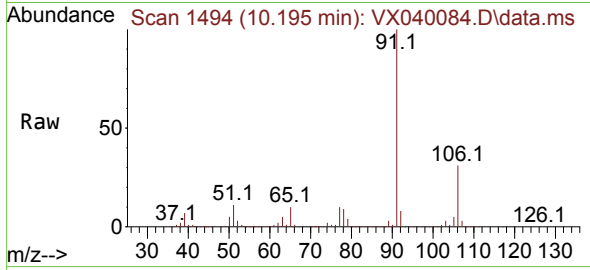


Tgt Ion: 91 Resp: 3119420  
Ion Ratio Lower Upper  
91 100  
106 31.2 24.9 37.3

Manual Integrations  
APPROVED



Reviewed By :John Carlone 02/05/2024  
Supervised By :Semsettin Yesilyurt 02/05/2024

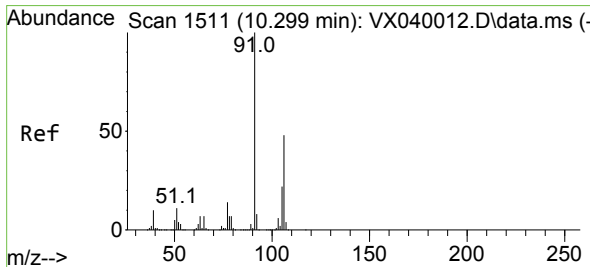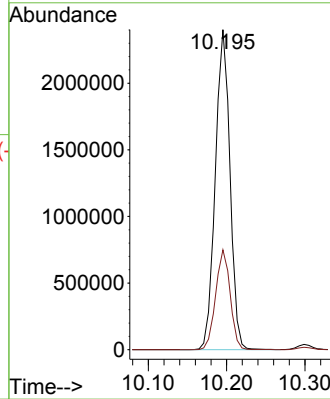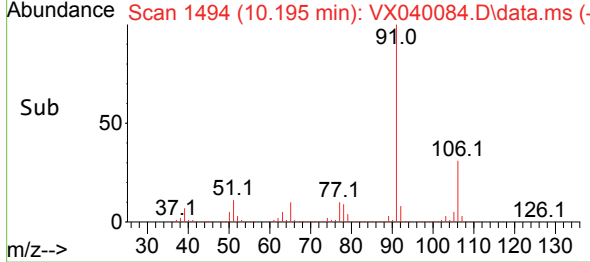


#68  
m/p-Xylenes  
Concen: 11.402 ug/l m  
RT: 10.299 min Scan# 1511  
Delta R.T. -0.000 min  
Lab File: VX040084.D  
Acq: 02 Feb 2024 14:07

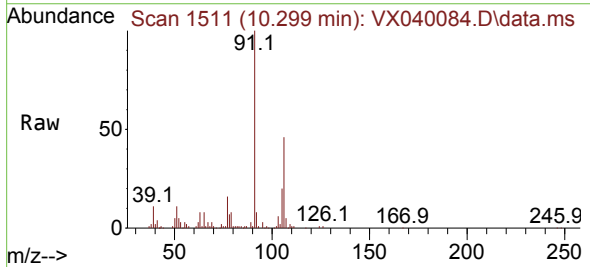

Tgt Ion:106 Resp: 23906  
Ion Ratio Lower Upper  
106 100  
91 13048.7 165.5 248.3#

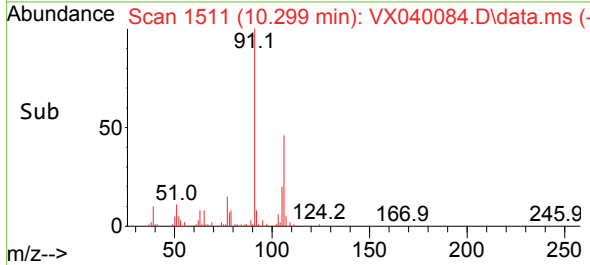



#69

o-Xylene

Concen: 2.710 ug/l

RT: 10.640 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX040084.D

Acq: 02 Feb 2024 14:07

Instrument :

MSVOA\_X

ClientSampleId :

MR-323P-GW-20240131-1

Tgt Ion:106 Resp: 5390

Ion Ratio Lower Upper

106 100





91 235.3 108.9 326.8

Manual Integrations

APPROVED

Reviewed By :John Carlone 02/05/2024

Supervised By :Semsettin Yesilyurt 02/05/2024

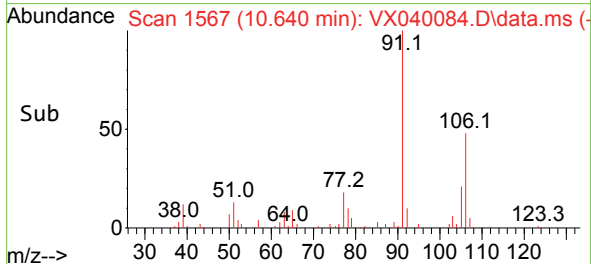

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. 0.006 min

Lab File: VX040084.D

Acq: 02 Feb 2024 14:07




Tgt Ion:152 Resp: 79957


Ion Ratio Lower Upper

152 100

115 67.7 43.3 129.9

150 156.5 0.0 345.0





#73

Isopropylbenzene

Concen: 129.354 ug/l

RT: 10.963 min Scan# 1620

Delta R.T. 0.000 min

Lab File: VX040084.D

Acq: 02 Feb 2024 14:07

Instrument :

MSVOA\_X

ClientSampleId :

MR-323P-GW-20240131-1

Tgt Ion:105 Resp: 742688

Ion Ratio Lower Upper

105 100





120 25.9 12.9 38.6

Manual Integrations

APPROVED

Reviewed By :John Carlone 02/05/2024

Supervised By :Semsettin Yesilyurt 02/05/2024

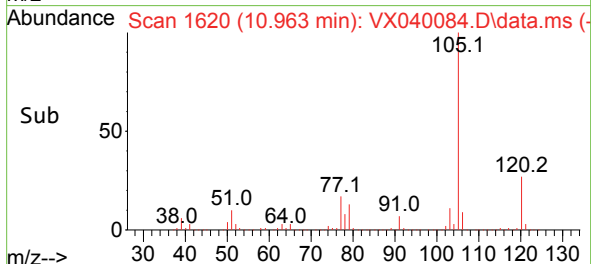

#78

n-propylbenzene

Concen: 361.647 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. -0.000 min

Lab File: VX040084.D




Acq: 02 Feb 2024 14:07


Tgt Ion: 91 Resp: 2555173

Ion Ratio Lower Upper

91 100


120 21.8 11.5 34.4

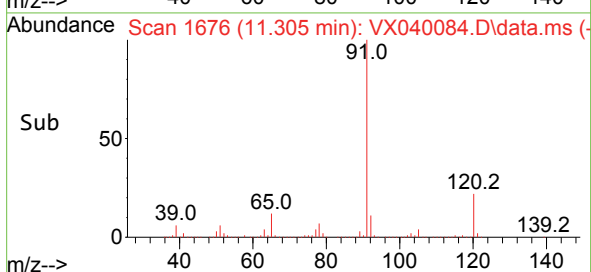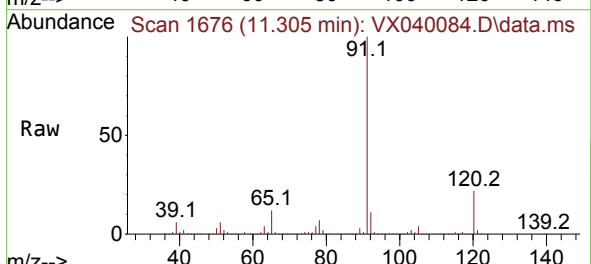



#80  
1,3,5-Trimethylbenzene  
Concen: 182.294 ug/l  
RT: 11.451 min Scan# 1700  
Delta R.T. -0.000 min  
Lab File: VX040084.D  
Acq: 02 Feb 2024 14:07




Instrument :  
MSVOA\_X  
ClientSampleId :  
MR-323P-GW-20240131-1




Tgt Ion:105 Resp: 899710  
Ion Ratio Lower Upper  
105 100  
120 46.0 24.1 72.3

Manual Integrations  
APPROVED



Reviewed By :John Carlone 02/05/2024  
Supervised By :Semsettin Yesilyurt 02/05/2024

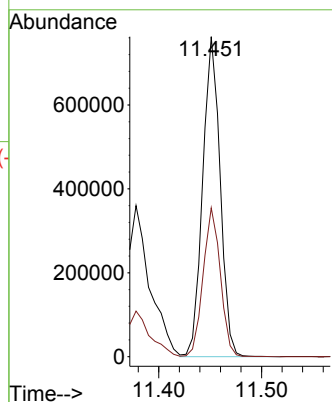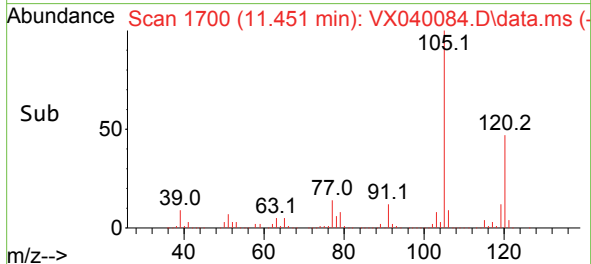


#84  
1,2,4-Trimethylbenzene  
Concen: 1108.793 ug/l  
RT: 11.756 min Scan# 1750  
Delta R.T. 0.006 min  
Lab File: VX040084.D  
Acq: 02 Feb 2024 14:07



Tgt Ion:105 Resp: 5460770  
Ion Ratio Lower Upper  
105 100  
120 45.4 21.2 63.6

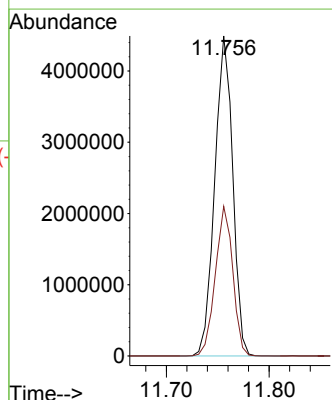



#85

sec-Butylbenzene

Concen: 16.524 ug/l m

RT: 11.890 min Scan# 1772

Delta R.T. -0.000 min

Lab File: VX040084.D

Acq: 02 Feb 2024 14:07

Instrument :

MSVOA\_X

ClientSampleId :

MR-323P-GW-20240131-1

Tgt Ion:105 Resp: 103392

Ion Ratio Lower Upper

105 100





134 0.0 9.8 29.4#

Manual Integrations

APPROVED

Reviewed By :John Carlone 02/05/2024

Supervised By :Semsettin Yesilyurt 02/05/2024

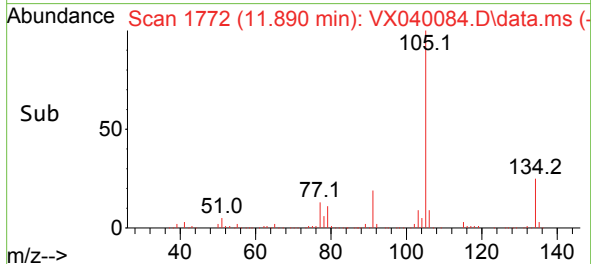

#86

p-Isopropyltoluene

Concen: 8.689 ug/l m

RT: 12.012 min Scan# 1792

Delta R.T. 0.006 min

Lab File: VX040084.D

Acq: 02 Feb 2024 14:07




Tgt Ion:119 Resp: 44395


Ion Ratio Lower Upper

119 100

134 50.7 12.8 38.3#


91 51.5 13.1 39.3#

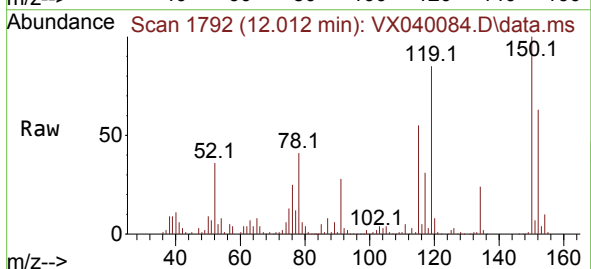

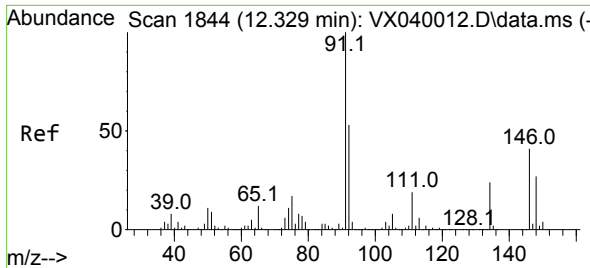

#89  
n-Butylbenzene  
Concen: 49.230 ug/l  
RT: 12.329 min Scan# 1844  
Delta R.T. -0.000 min  
Lab File: VX040084.D  
Acq: 02 Feb 2024 14:07




Instrument : MSVOA\_X  
ClientSampleId : MR-323P-GW-20240131-1

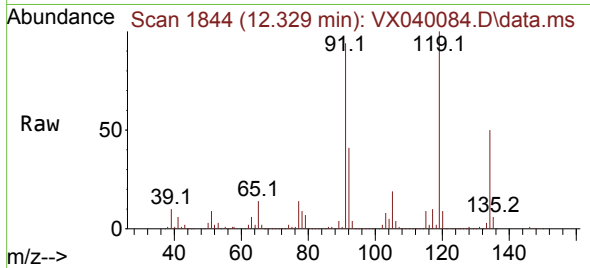


Tgt Ion: 91 Resp: 244150  
Ion Ratio Lower Upper  
91 100  
92 33.8 27.4 82.0  
134 77.5 12.6 37.8

Manual Integrations  
APPROVED

Reviewed By :John Carlone 02/05/2024  
Supervised By :Semsettin Yesilyurt 02/05/2024

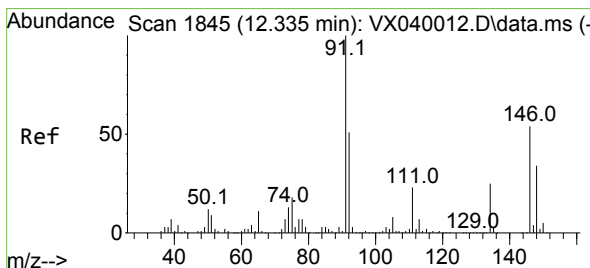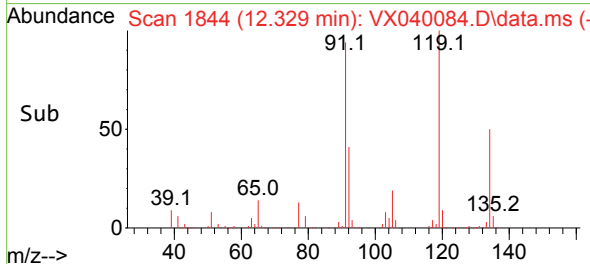

#91  
1,2-Dichlorobenzene  
Concen: 0.670 ug/l  
RT: 12.341 min Scan# 1846  
Delta R.T. 0.006 min  
Lab File: VX040084.D  
Acq: 02 Feb 2024 14:07

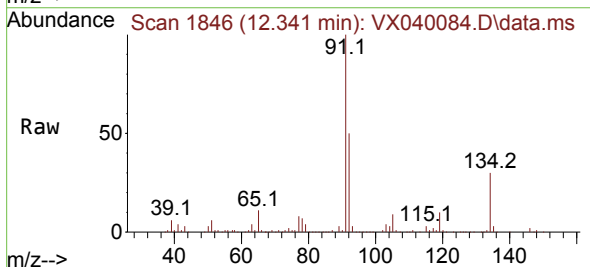

Tgt Ion:146 Resp: 1725  
Ion Ratio Lower Upper  
146 100  
111 73.3 22.4 67.0#  
148 57.7 31.6 95.0

