



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020321\
Data File : VX020826.D
Acq On : 03 Feb 2021 09:00
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012521W.M
Title : SW846 8260
Last Update : Mon Jan 25 13:38:15 2021

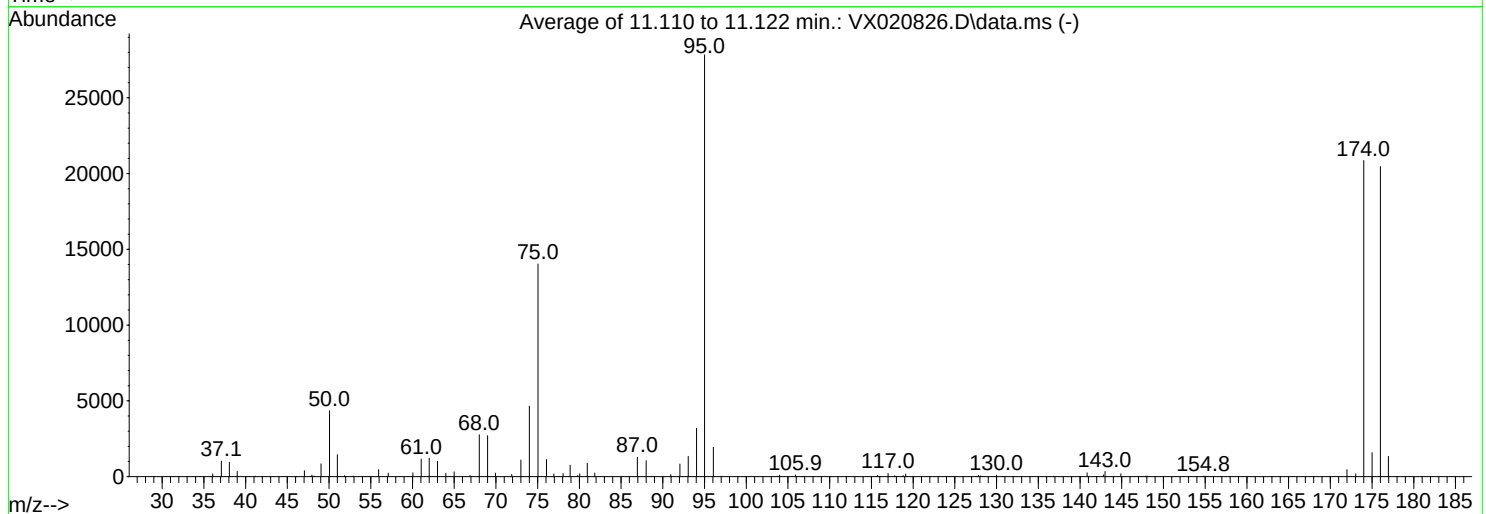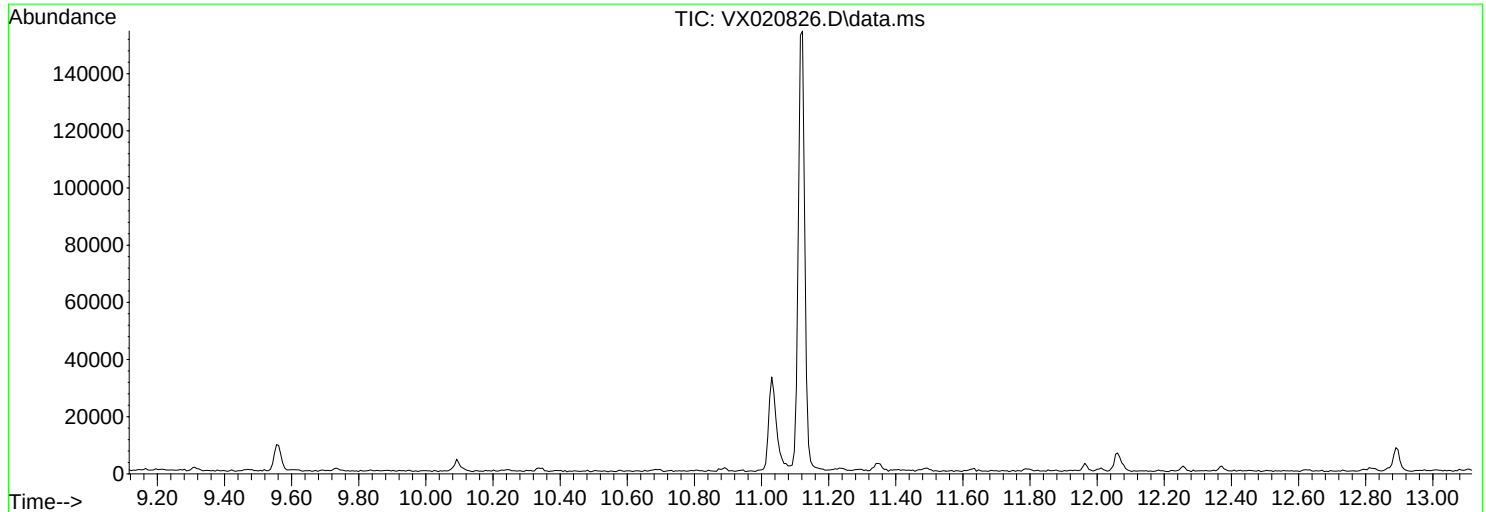

AutoFind: Scans 1644, 1645, 1646; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	4353	PASS
75	95	30	60	50.4	14038	PASS
95	95	100	100	100.0	27835	PASS
96	95	5	9	7.0	1941	PASS
173	174	0.00	2	0.9	190	PASS
174	95	50	100	75.0	20868	PASS
175	174	5	9	7.6	1580	PASS
176	174	95	101	98.0	20460	PASS
177	176	5	9	6.6	1341	PASS