

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020322\
 Data File : VX026768.D
 Acq On : 03 Feb 2022 19:08
 Operator : JC/MD
 Sample : N1345-02 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 34025

Quant Time: Feb 04 02:35:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 11 14:45:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	124136	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	206602	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	177723	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	73953	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	77828	44.881	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	89.760%
35) Dibromofluoromethane	5.391	113	64185	48.108	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	96.220%
50) Toluene-d8	8.659	98	232450	48.349	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	96.700%
62) 4-Bromofluorobenzene	11.085	95	83030	48.615	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	97.240%


Target Compounds					Qvalue	
8) Diethyl Ether	2.136	74	182	0.231	ug/l #	1
11) Tert butyl alcohol	2.965	59	4210	17.452	ug/l	97
16) Acetone	2.380	43	8600	9.725	ug/l	97
18) Methyl Acetate	2.709	43	1318	0.750	ug/l #	85
22) Diisopropyl ether	3.702	45	988	0.204	ug/l #	1
25) 2-Butanone	4.562	43	21708	18.876	ug/l	96
29) Tetrahydrofuran	5.025	42	221	0.324	ug/l #	34
31) Cyclohexane	5.556	56	2455	0.960	ug/l #	1
36) 1,1-Dichloropropene	5.562	75	9400	4.463	ug/l #	50
37) Ethyl Acetate	4.562	43	21708	10.189	ug/l #	69
38) Carbon Tetrachloride	5.562	117	12686	5.856	ug/l #	16
40) Benzene	6.050	78	7379	1.268	ug/l	100
43) Isopropyl Acetate	6.123	43	134959	39.214	ug/l #	62
49) 1,4-Dioxane	7.671	88	6045	215.972	ug/l	96
51) 4-Methyl-2-Pentanone	8.586	43	3155322	1545.721	ug/l	96
52) Toluene	8.726	92	4603	1.289	ug/l	99
53) t-1,3-Dichloropropene	8.903	75	903	2.272	ug/l #	43
54) cis-1,3-Dichloropropene	8.586	75	463	0.208	ug/l #	1
56) Ethyl methacrylate	9.183	69	742	0.348	ug/l #	22
59) 2-Hexanone	9.433	43	1417	0.907	ug/l	64
67) Ethyl Benzene	10.195	91	2499	0.367	ug/l	97
68) m/p-Xylenes	10.305	106	4436	1.743	ug/l	96
69) o-Xylene	10.646	106	2415	0.983	ug/l	98
74) N-amyl acetate	10.756	43	40730	17.404	ug/l #	1
75) 1,1,2,2-Tetrachloroethane	11.280	83	20094	12.350	ug/l #	26
76) 1,2,3-Trichloropropane	11.085	75	41161	25.279	ug/l #	40
81) trans-1,4-Dichloro-2-b...	11.085	75	41161	76.782	ug/l #	3
84) 1,2,4-Trimethylbenzene	11.750	105	71444	14.293	ug/l #	35
85) sec-Butylbenzene	11.750	105	71444	11.839	ug/l #	56
89) n-Butylbenzene	12.305	91	996	0.229	ug/l #	37
90) Hexachloroethane	12.609	117	116	2.309	ug/l #	14
95) Naphthalene	13.780	128	3540	0.673	ug/l	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020322\
Data File : VX026768.D
Acq On : 03 Feb 2022 19:08
Operator : JC/MD
Sample : N1345-02 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
34025

Quant Time: Feb 04 02:35:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 11 14:45:13 2022
Response via : Initial Calibration




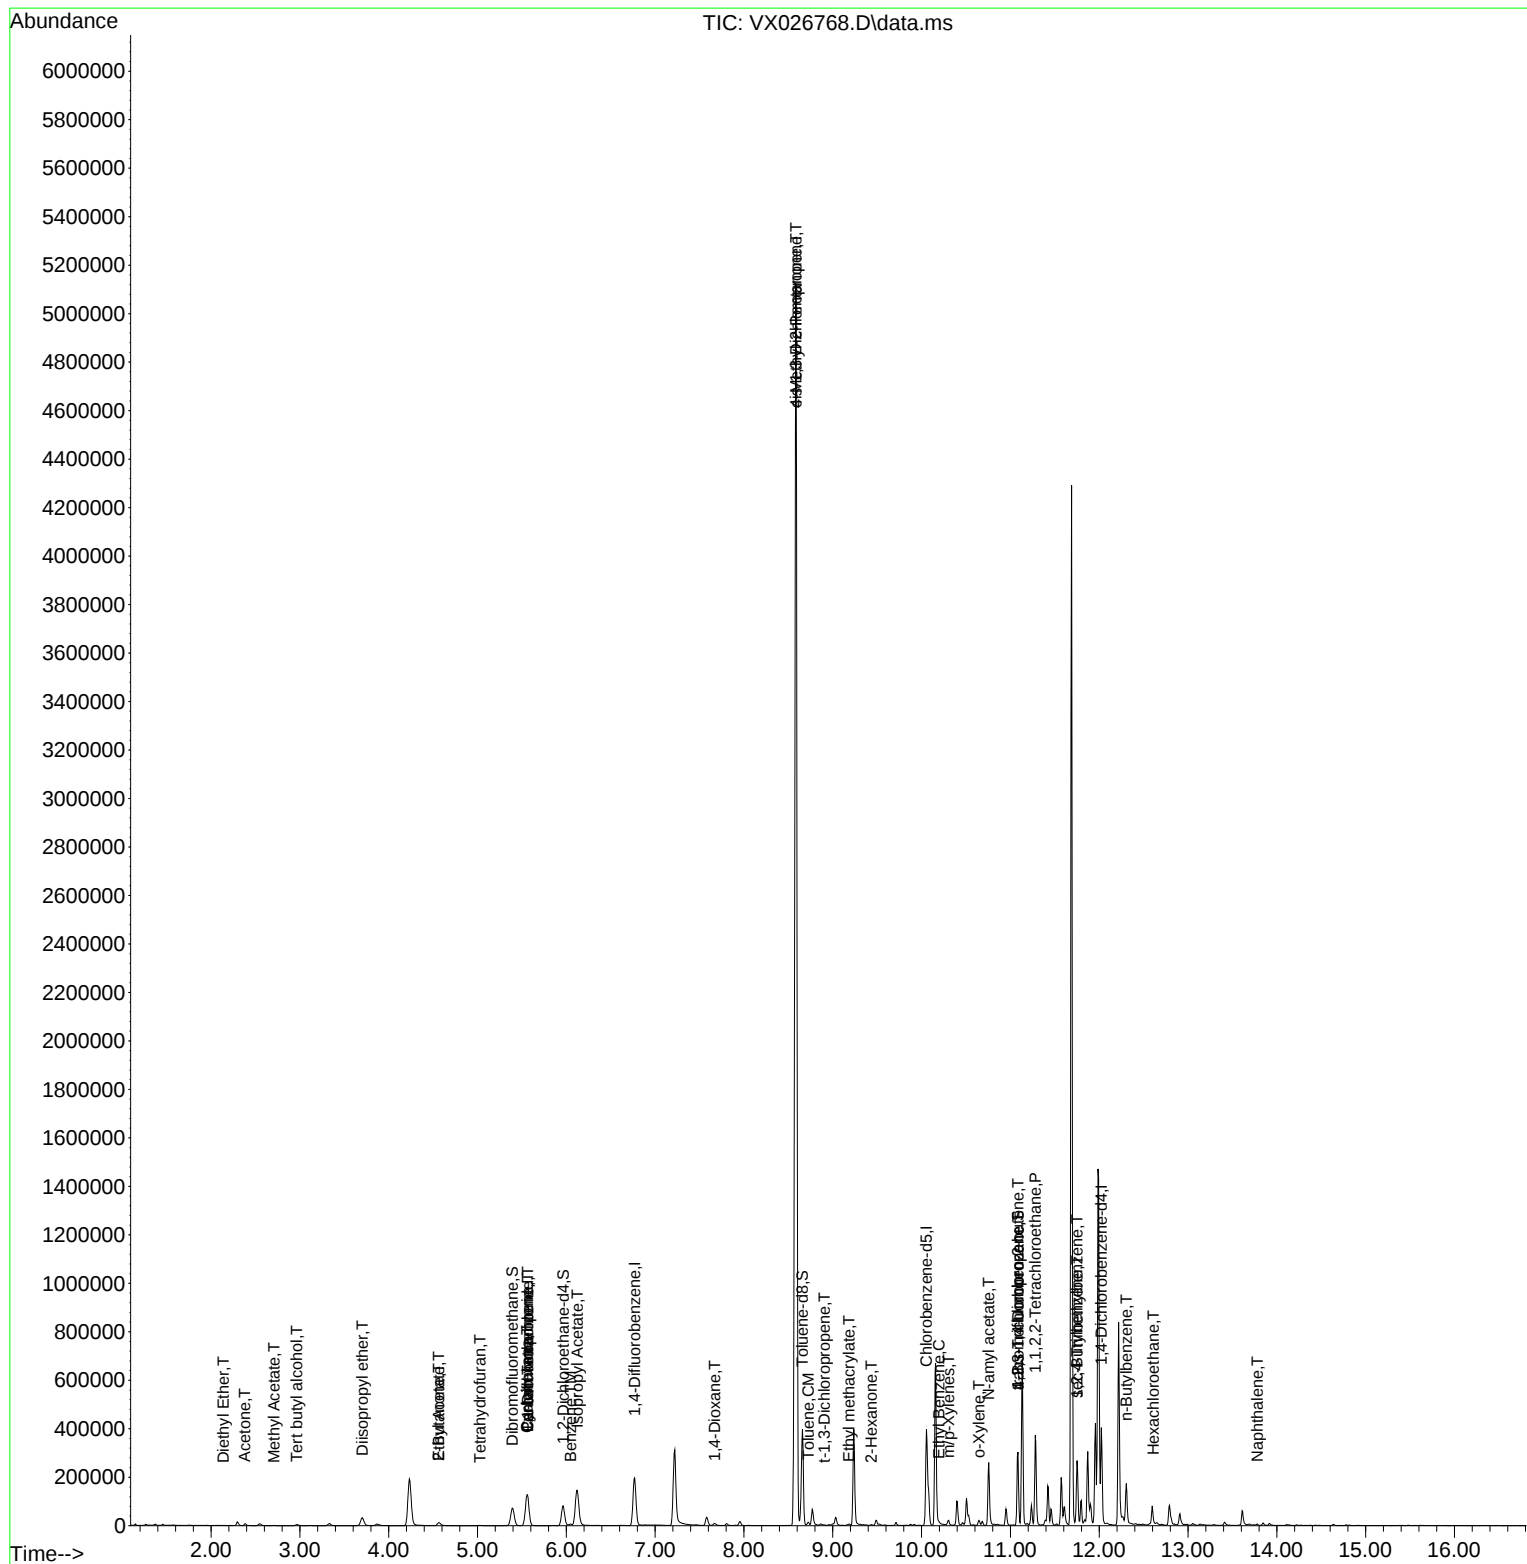


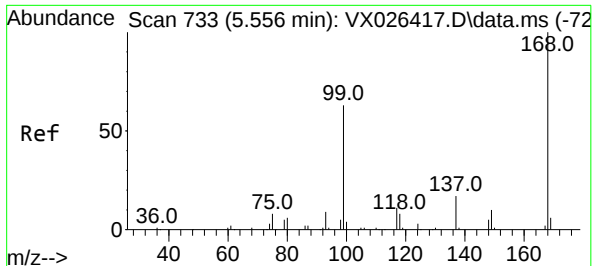

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX026768.D
Acq: 03 Feb 2022 19:08




Instrument :
MSVOA_X
ClientSampleId :
34025


Tgt Ion:168 Resp: 124136
Ion Ratio Lower Upper
168 100
99 59.0 50.3 75.5

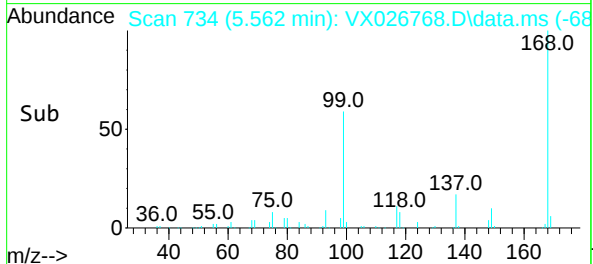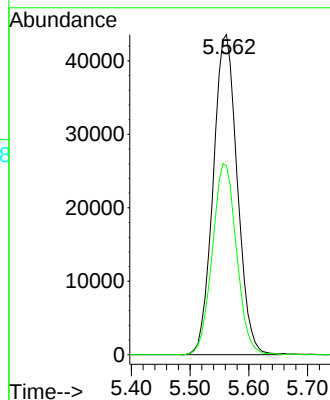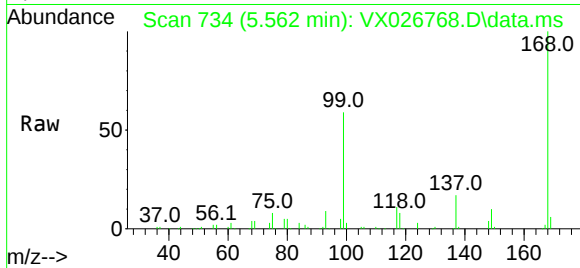

#8
Diethyl Ether
Concen: 0.231 ug/l
RT: 2.136 min Scan# 172
Delta R.T. -0.000 min
Lab File: VX026768.D
Acq: 03 Feb 2022 19:08

Tgt Ion: 74 Resp: 182
Ion Ratio Lower Upper
74 100
45 228.6 50.7 152.1#


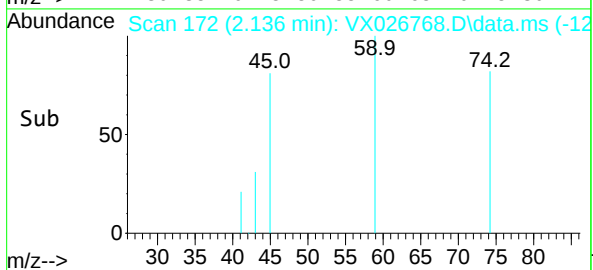
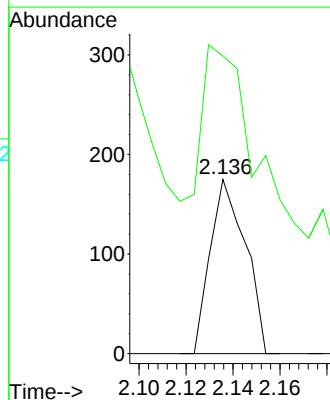
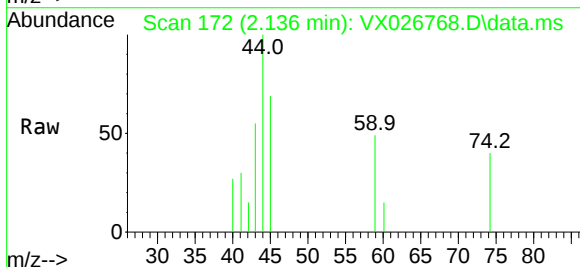




#11
Tert butyl alcohol
Concen: 17.452 ug/l
RT: 2.965 min Scan# 308
Delta R.T. -0.042 min
Lab File: VX026768.D
Acq: 03 Feb 2022 19:08




Instrument :
MSVOA_X
ClientSampleId :
34025


Tgt Ion: 59 Resp: 4210
Ion Ratio Lower Upper
59 100
57 10.2 7.2 10.8

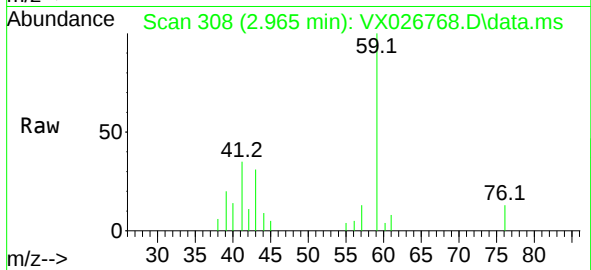

#16
Acetone
Concen: 9.725 ug/l
RT: 2.380 min Scan# 212
Delta R.T. -0.012 min
Lab File: VX026768.D
Acq: 03 Feb 2022 19:08

Tgt Ion: 43 Resp: 8600
Ion Ratio Lower Upper
43 100
58 30.3 23.0 34.6

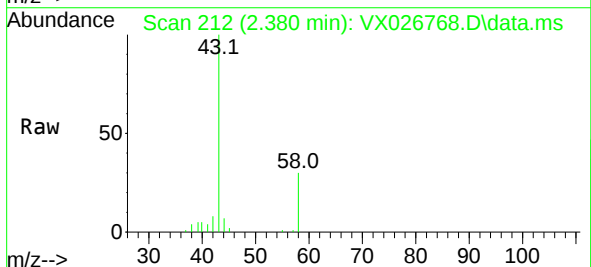



#18

Methyl Acetate

Concen: 0.750 ug/l

RT: 2.709 min Scan# 2

Delta R.T. -0.000 min

Lab File: VX026768.D

Acq: 03 Feb 2022 19:08

Instrument :

MSVOA_X

ClientSampleId :





34025

Tgt Ion: 43 Resp: 1318

Ion Ratio Lower Upper

43 100

74 15.6 18.3 27.5#

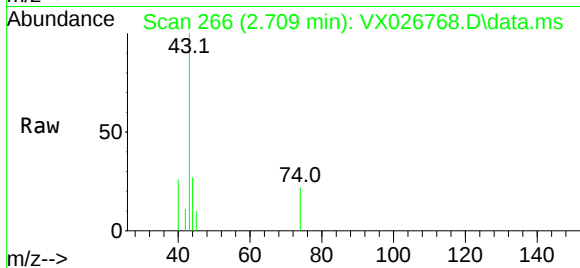

#22

Diisopropyl ether

Concen: 0.204 ug/l

RT: 3.702 min Scan# 429

Delta R.T. -0.061 min

Lab File: VX026768.D

Acq: 03 Feb 2022 19:08

Tgt Ion: 45 Resp: 988




Ion Ratio Lower Upper


45 100

43 0.0 60.6 91.0#

87 0.0 22.0 33.0#

59 204.4 9.0 13.4#


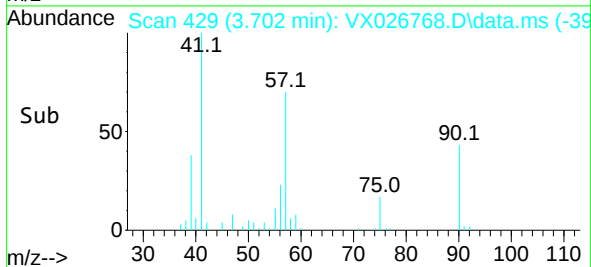

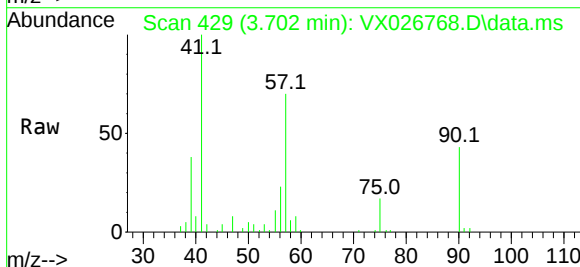




#25
2-Butanone
Concen: 18.876 ug/l
RT: 4.562 min Scan# 51
Delta R.T. -0.000 min
Lab File: VX026768.D
Acq: 03 Feb 2022 19:08




Instrument :
MSVOA_X
ClientSampleId :
34025


Tgt Ion: 43 Resp: 21708
Ion Ratio Lower Upper
43 100
72 27.3 20.4 30.6

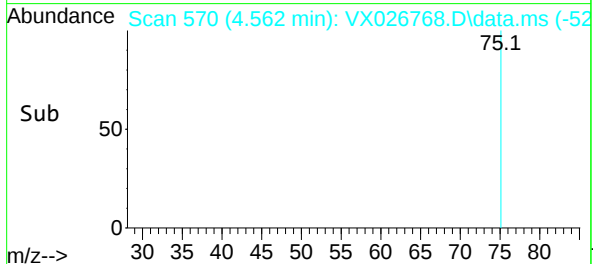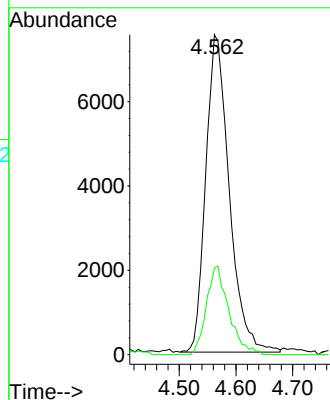

#29
Tetrahydrofuran
Concen: 0.324 ug/l
RT: 5.025 min Scan# 646
Delta R.T. 0.012 min
Lab File: VX026768.D
Acq: 03 Feb 2022 19:08

Tgt Ion: 42 Resp: 221
Ion Ratio Lower Upper
42 100
72 0.0 34.6 52.0#
71 0.0 31.8 47.8#


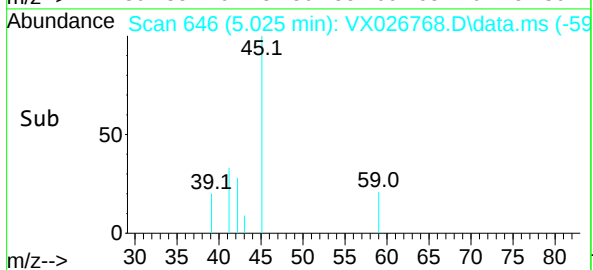
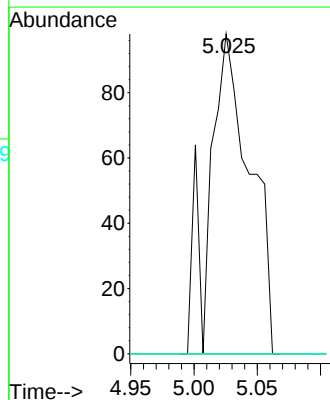
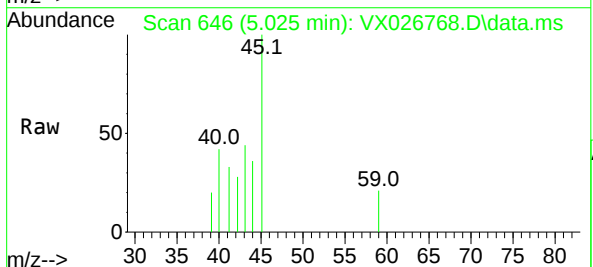


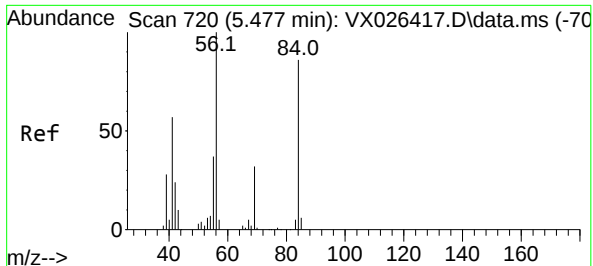

#31
Cyclohexane
Concen: 0.960 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.079 min
Lab File: VX026768.D
Acq: 03 Feb 2022 19:08




Instrument :
MSVOA_X
ClientSampleId :
34025


Tgt Ion: 56 Resp: 2455
Ion Ratio Lower Upper
56 100
69 176.3 25.8 38.6#
84 145.6 68.9 103.3#

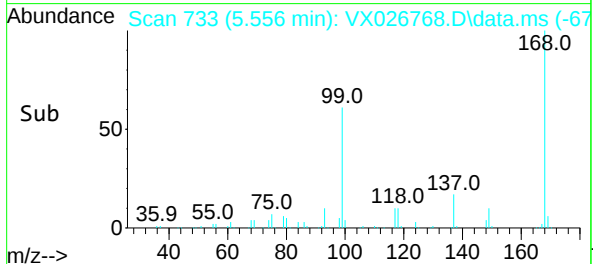

#33
1,2-Dichloroethane-d4
Concen: 44.881 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.006 min
Lab File: VX026768.D
Acq: 03 Feb 2022 19:08

Tgt Ion: 65 Resp: 77828
Ion Ratio Lower Upper
65 100
67 52.0 0.0 100.8




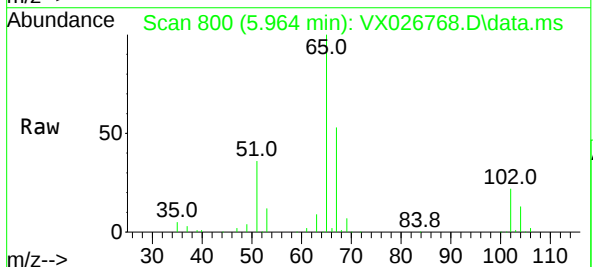




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 911
Delta R.T. 0.006 min
Lab File: VX026768.D
Acq: 03 Feb 2022 19:08




Instrument :
MSVOA_X
ClientSampleId :
34025


Tgt Ion:114 Resp: 206602
Ion Ratio Lower Upper
114 100
63 19.9 0.0 42.8
88 16.2 0.0 33.0



#35
Dibromofluoromethane
Concen: 48.108 ug/l
RT: 5.391 min Scan# 706
Delta R.T. -0.000 min
Lab File: VX026768.D
Acq: 03 Feb 2022 19:08

Tgt Ion:113 Resp: 64185
Ion Ratio Lower Upper
113 100
111 102.5 81.2 121.8
192 20.0 15.0 22.4

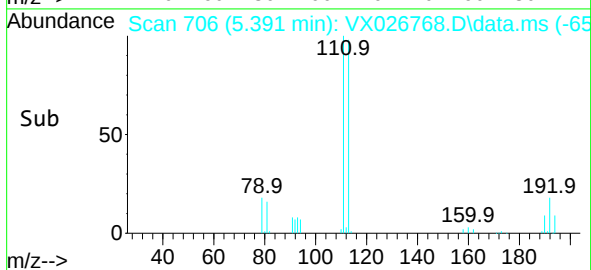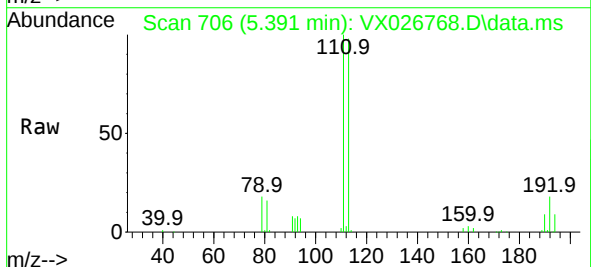



#36

1,1-Dichloropropene

Concen: 4.463 ug/l

RT: 5.562 min Scan# 71

Delta R.T. -0.134 min

Lab File: VX026768.D


Acq: 03 Feb 2022 19:08

Instrument :




MSVOA_X

ClientSampleId :

34025

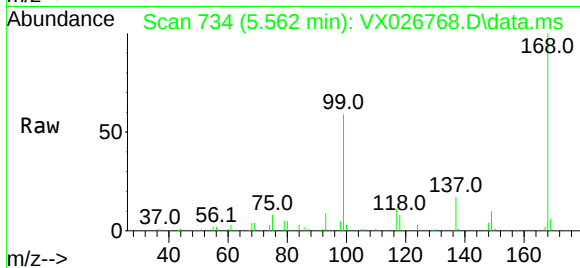

Tgt Ion:	75	Resp:	9400
Ion	Ratio	Lower	Upper
75	100		
110	8.7	17.2	51.6#
77	0.0	24.6	36.8#

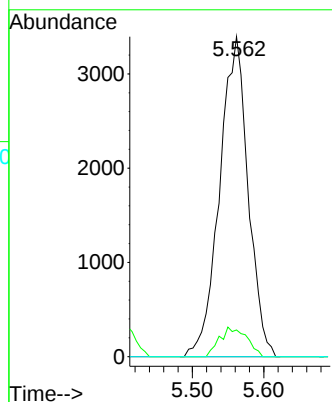

#37

Ethyl Acetate

Concen: 10.189 ug/l




RT: 4.562 min Scan# 570


Delta R.T. -0.159 min

Lab File: VX026768.D

Acq: 03 Feb 2022 19:08


Tgt Ion:	43	Resp:	21708
Ion	Ratio	Lower	Upper
43	100		
61	0.1	10.6	16.0#
70	0.0	8.5	12.7#

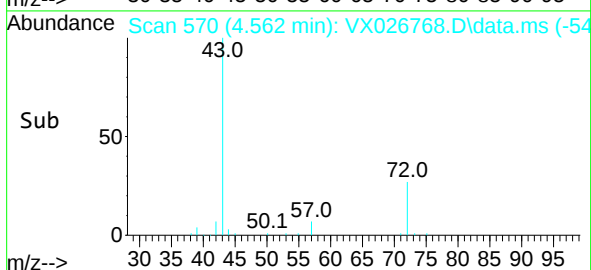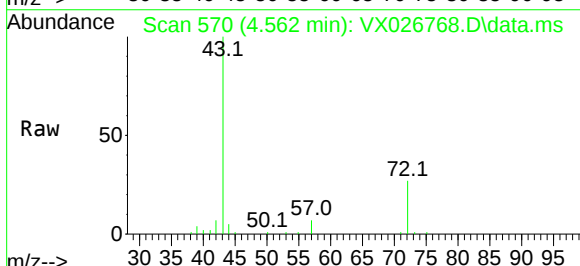



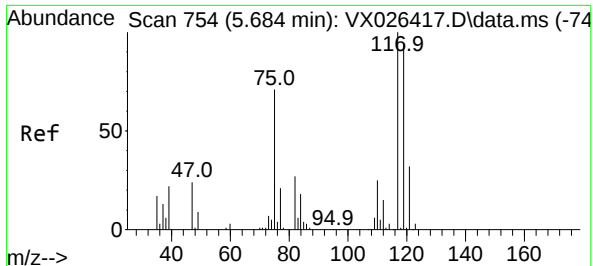


#38
Carbon Tetrachloride
Concen: 5.856 ug/l
RT: 5.562 min Scan# 71
Delta R.T. -0.122 min
Lab File: VX026768.D
Acq: 03 Feb 2022 19:08

Instrument :
MSVOA_X
ClientSampleId :
34025



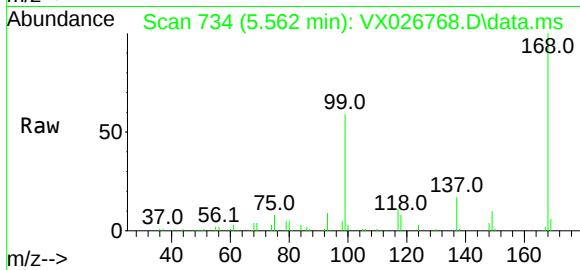



Tgt Ion:117 Resp: 12686
Ion Ratio Lower Upper
117 100
119 4.0 74.7 112.1#
121 0.0 25.4 38.0#

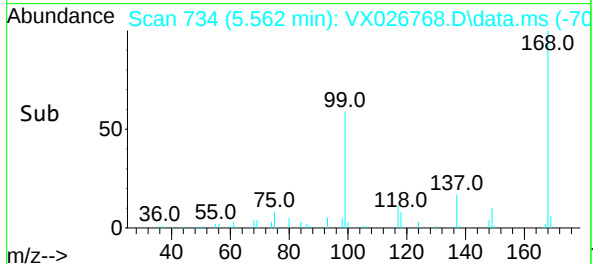

#40
Benzene
Concen: 1.268 ug/l
RT: 6.050 min Scan# 814
Delta R.T. 0.006 min
Lab File: VX026768.D
Acq: 03 Feb 2022 19:08

Tgt Ion: 78 Resp: 7379
Ion Ratio Lower Upper
78 100
77 23.8 18.9 28.3


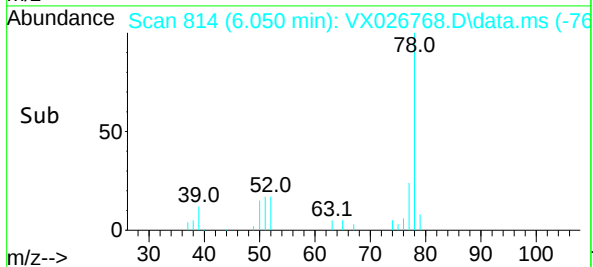

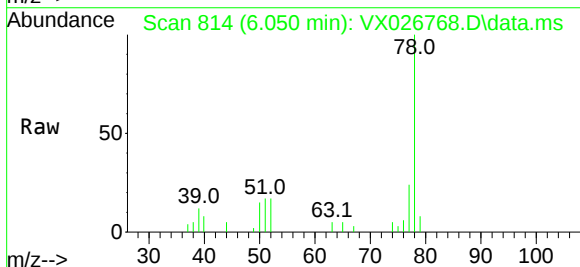




#43
Isopropyl Acetate
Concen: 39.214 ug/l
RT: 6.123 min Scan# 81
Delta R.T. -0.220 min
Lab File: VX026768.D
Acq: 03 Feb 2022 19:08




Instrument :
MSVOA_X
ClientSampleId :
34025


Tgt Ion: 43 Resp: 134959
Ion Ratio Lower Upper
43 100
61 0.0 15.4 23.0#
87 0.0 10.2 15.2#

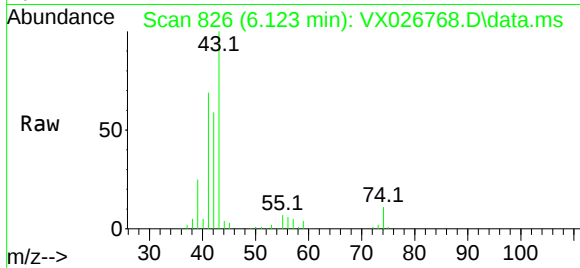

#49
1,4-Dioxane
Concen: 215.972 ug/l
RT: 7.671 min Scan# 1080
Delta R.T. -0.024 min
Lab File: VX026768.D
Acq: 03 Feb 2022 19:08

Tgt Ion: 88 Resp: 6045
Ion Ratio Lower Upper
88 100
43 31.0 29.9 44.9
58 71.1 57.8 86.6




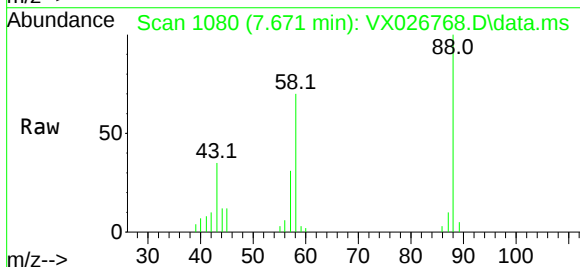


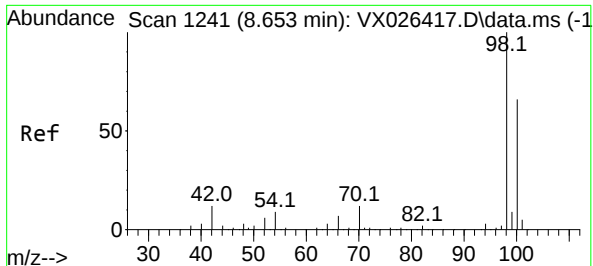

#50
Toluene-d8
Concen: 48.349 ug/l
RT: 8.659 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX026768.D
Acq: 03 Feb 2022 19:08




Instrument :
MSVOA_X
ClientSampleId :
34025


Tgt Ion: 98 Resp: 232450
Ion Ratio Lower Upper
98 100
100 66.8 53.2 79.8

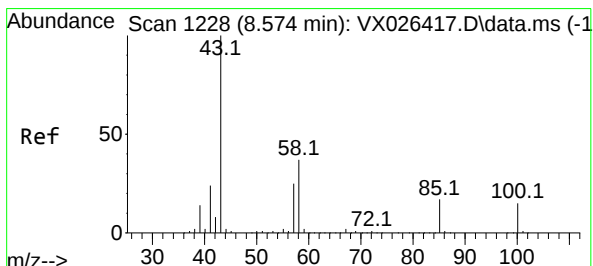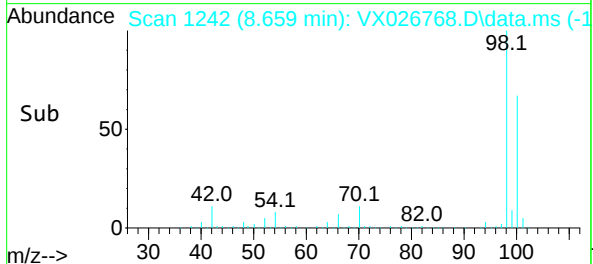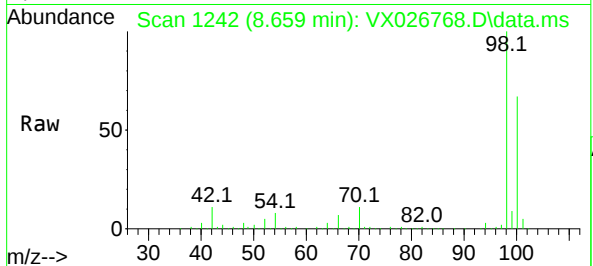

#51
4-Methyl-2-Pentanone
Concen: 1545.721 ug/l
RT: 8.586 min Scan# 1230
Delta R.T. 0.012 min
Lab File: VX026768.D
Acq: 03 Feb 2022 19:08

Tgt Ion: 43 Resp: 3155322
Ion Ratio Lower Upper
43 100
58 40.3 30.5 45.7




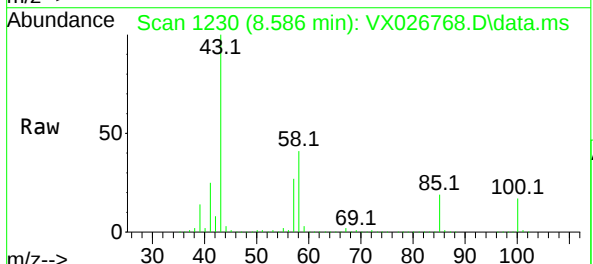


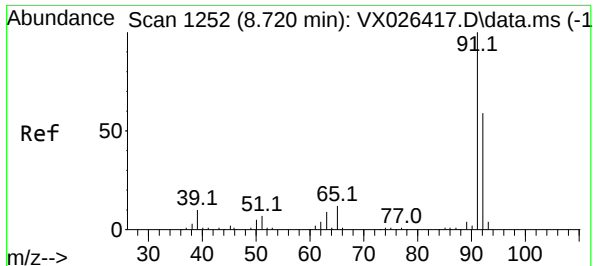

#52
Toluene
Concen: 1.289 ug/l
RT: 8.726 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX026768.D
Acq: 03 Feb 2022 19:08




Instrument :
MSVOA_X
ClientSampleId :
34025


Tgt Ion: 92 Resp: 4603
Ion Ratio Lower Upper
92 100
91 170.7 135.7 203.5

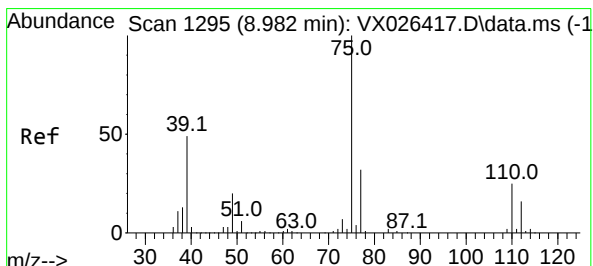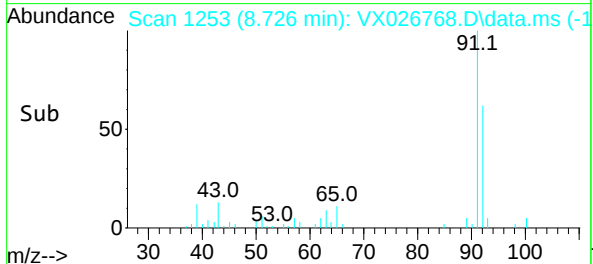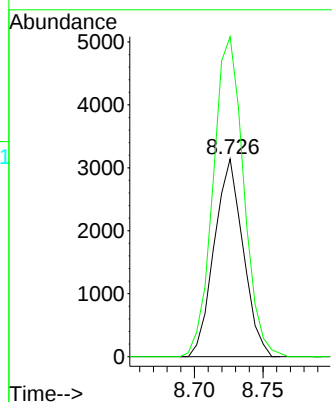

#53
t-1,3-Dichloropropene
Concen: 2.272 ug/l
RT: 8.903 min Scan# 1282
Delta R.T. -0.079 min
Lab File: VX026768.D
Acq: 03 Feb 2022 19:08

Tgt Ion: 75 Resp: 903
Ion Ratio Lower Upper
75 100
77 0.0 25.7 38.5#


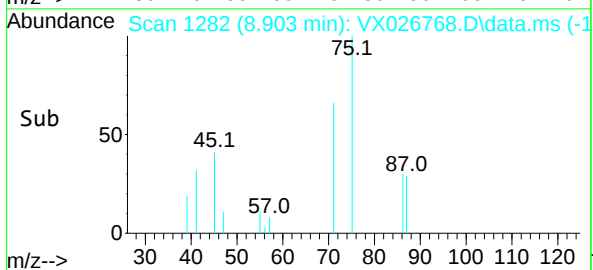
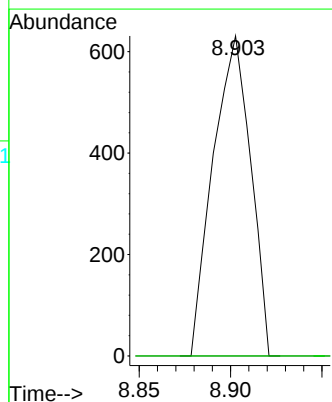
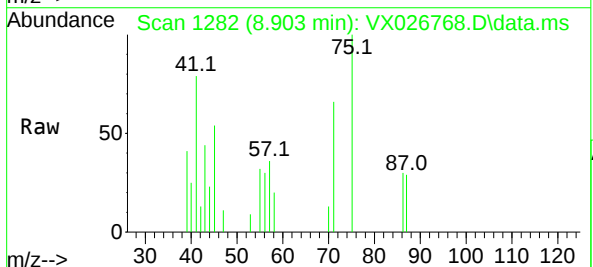




#54
 cis-1,3-Dichloropropene
 Concen: 0.208 ug/l
 RT: 8.586 min Scan# 1194
 Delta R.T. 0.219 min
 Lab File: VX026768.D
 Acq: 03 Feb 2022 19:08




Instrument :
 MSVOA_X
 ClientSampleId :
 34025


Tgt Ion: 75 Resp: 463
 Ion Ratio Lower Upper
 75 100
 77 454.4 26.2 39.2#
 39 137558.5 43.5 65.3#

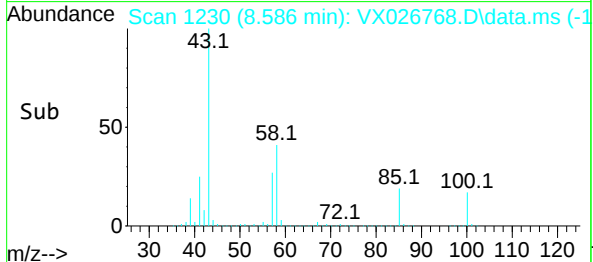

#56
 Ethyl methacrylate
 Concen: 0.348 ug/l
 RT: 9.183 min Scan# 1328
 Delta R.T. 0.067 min
 Lab File: VX026768.D
 Acq: 03 Feb 2022 19:08

Tgt Ion: 69 Resp: 742
 Ion Ratio Lower Upper
 69 100
 41 0.0 57.2 85.8#
 39 0.0 30.9 46.3#


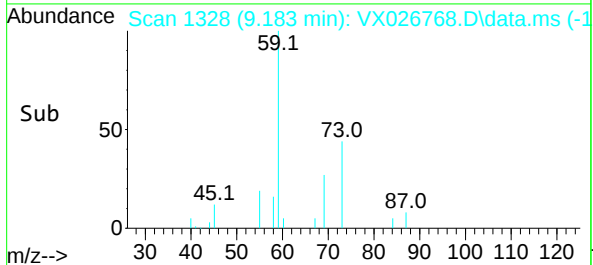

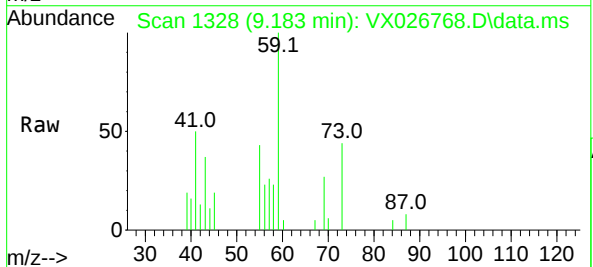


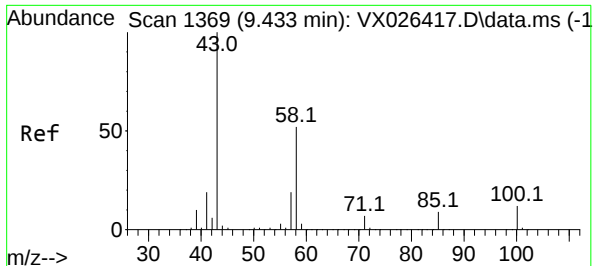

#59
2-Hexanone
Concen: 0.907 ug/l
RT: 9.433 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX026768.D
Acq: 03 Feb 2022 19:08




Instrument :
MSVOA_X
ClientSampleId :
34025


Tgt Ion: 43 Resp: 1417
Ion Ratio Lower Upper
43 100
58 78.1 26.4 79.2

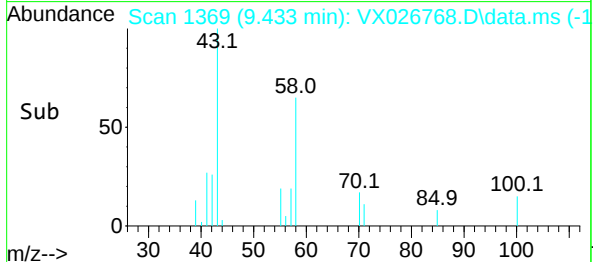

#62
4-Bromofluorobenzene
Concen: 48.615 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.006 min
Lab File: VX026768.D
Acq: 03 Feb 2022 19:08

Tgt Ion: 95 Resp: 83030
Ion Ratio Lower Upper
95 100
174 75.9 0.0 148.6
176 74.0 0.0 141.4


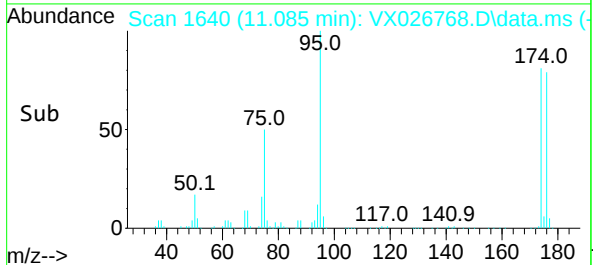

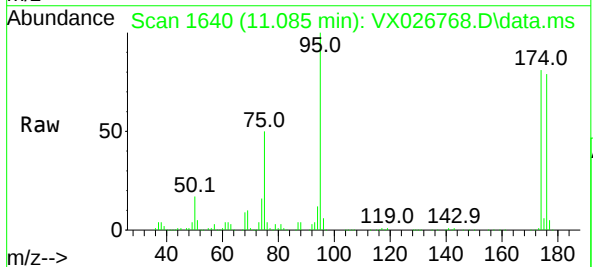




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX026768.D
Acq: 03 Feb 2022 19:08




Instrument :
MSVOA_X
ClientSampleId :
34025


Tgt Ion:117 Resp: 177723
Ion Ratio Lower Upper
117 100
82 55.1 45.2 67.8
119 31.7 26.2 39.2

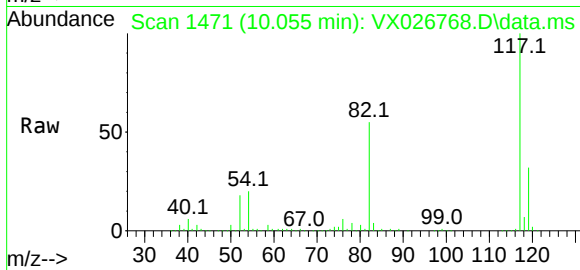

#67
Ethyl Benzene
Concen: 0.367 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. -0.000 min
Lab File: VX026768.D
Acq: 03 Feb 2022 19:08

Tgt Ion: 91 Resp: 2499
Ion Ratio Lower Upper
91 100
106 29.2 24.7 37.1




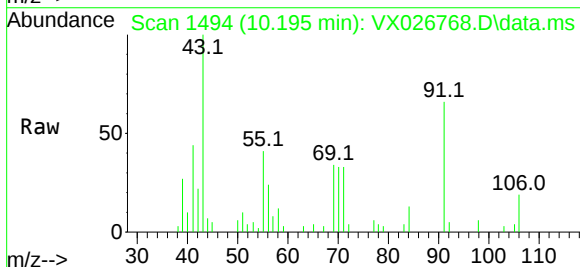




#68
m/p-Xylenes
Concen: 1.743 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX026768.D
Acq: 03 Feb 2022 19:08




Instrument :
MSVOA_X
ClientSampleId :
34025


Tgt Ion:106 Resp: 4436
Ion Ratio Lower Upper
106 100
91 212.6 165.3 247.9



#69
o-Xylene
Concen: 0.983 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. 0.006 min
Lab File: VX026768.D
Acq: 03 Feb 2022 19:08

Tgt Ion:106 Resp: 2415
Ion Ratio Lower Upper
106 100
91 222.4 109.7 329.0


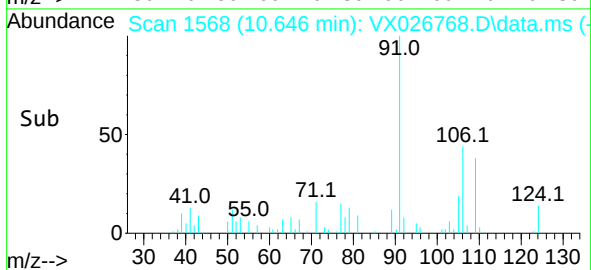






#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: VX026768.D
 Acq: 03 Feb 2022 19:08




Instrument :
 MSVOA_X
 ClientSampleId :
 34025


Tgt Ion:152 Resp: 73953
 Ion Ratio Lower Upper
 152 100
 115 60.1 44.2 132.6
 150 158.2 0.0 348.2

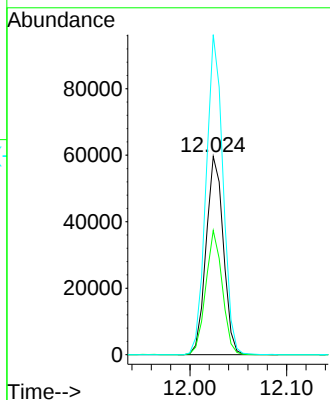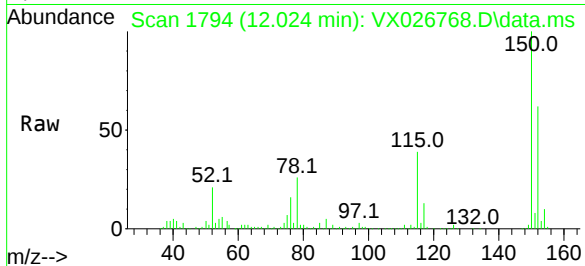

#74
 N-ethyl acetate
 Concen: 17.404 ug/l
 RT: 10.756 min Scan# 1586
 Delta R.T. -0.085 min
 Lab File: VX026768.D
 Acq: 03 Feb 2022 19:08

Tgt Ion: 43 Resp: 40730
 Ion Ratio Lower Upper
 43 100
 70 5.6 32.9 49.3#
 55 236.9 18.3 27.5#
 61 0.0 18.9 28.3#


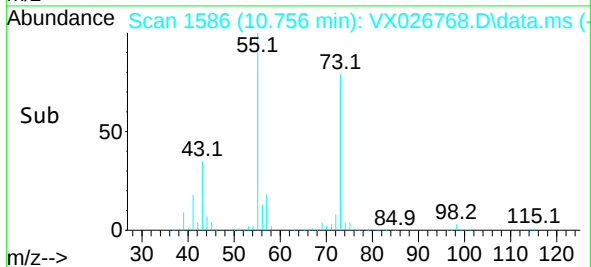
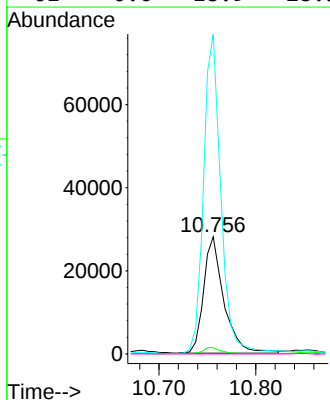
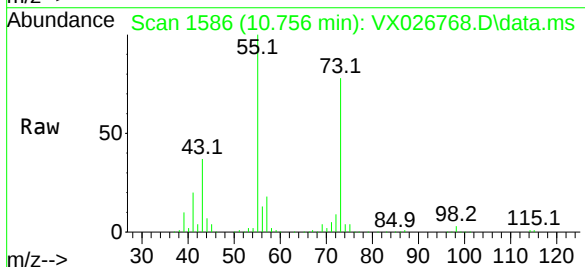




#75
 1,1,2,2-Tetrachloroethane
 Concen: 12.350 ug/l
 RT: 11.280 min Scan# 1
 Delta R.T. 0.067 min
 Lab File: VX026768.D
 Acq: 03 Feb 2022 19:08




Instrument :
 MSVOA_X
 ClientSampleId :
 34025


Tgt Ion: 83 Resp: 20094
 Ion Ratio Lower Upper
 83 100
 131 0.0 5.3 15.9#
 85 0.0 32.0 96.2#

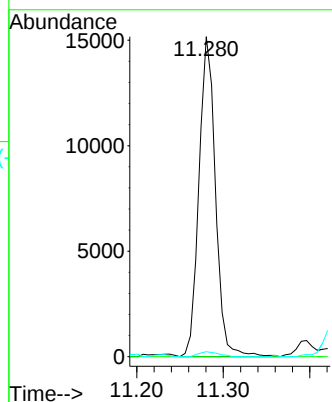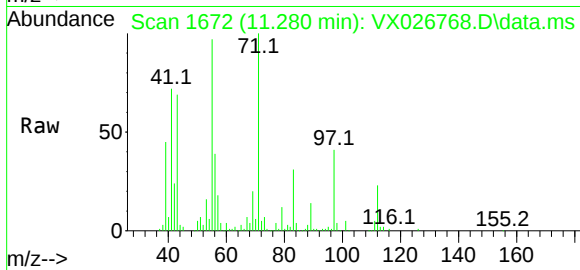

#76
 1,2,3-Trichloropropane
 Concen: 25.279 ug/l
 RT: 11.085 min Scan# 1640
 Delta R.T. -0.159 min
 Lab File: VX026768.D
 Acq: 03 Feb 2022 19:08

Tgt Ion: 75 Resp: 41161
 Ion Ratio Lower Upper
 75 100
 77 1.2 18.3 54.8#


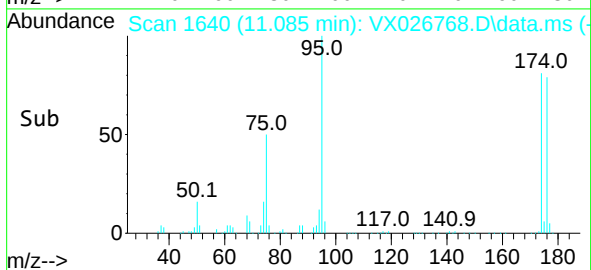
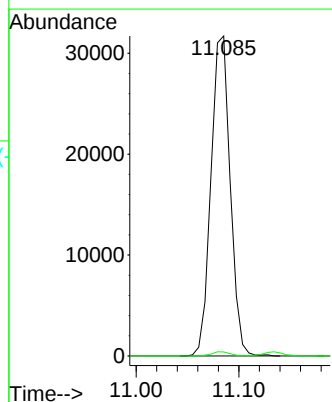
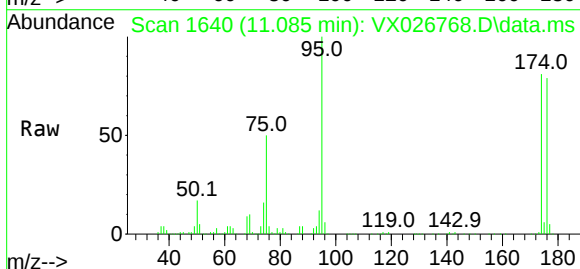




#81
 trans-1,4-Dichloro-2-butene
 Concen: 76.782 ug/l
 RT: 11.085 min Scan# 11085
 Delta R.T. 0.067 min
 Lab File: VX026768.D
 Acq: 03 Feb 2022 19:08




Instrument :
 MSVOA_X
 ClientSampleId :
 34025


Tgt Ion: 75 Resp: 41161
 Ion Ratio Lower Upper
 75 100
 53 0.0 94.0 141.0#
 89 0.0 37.0 55.4#

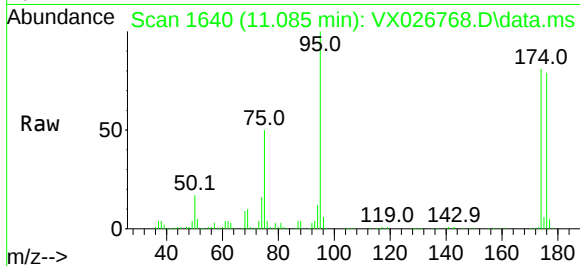

#84
 1,2,4-Trimethylbenzene
 Concen: 14.293 ug/l
 RT: 11.750 min Scan# 1749
 Delta R.T. -0.000 min
 Lab File: VX026768.D
 Acq: 03 Feb 2022 19:08

Tgt Ion: 105 Resp: 71444
 Ion Ratio Lower Upper
 105 100
 120 2.0 21.9 65.5#


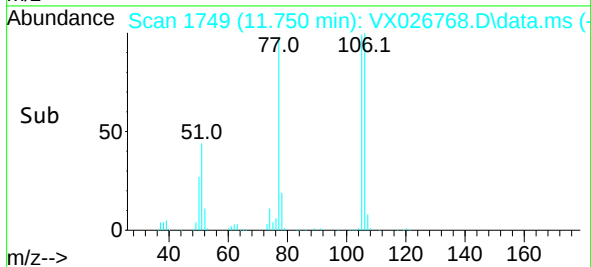

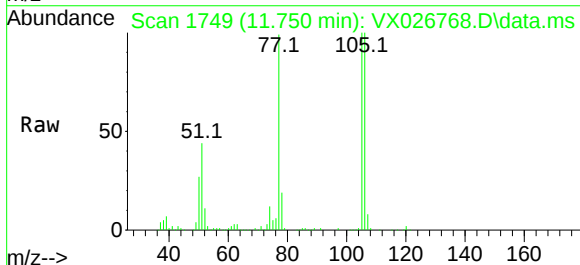




#85
 sec-Butylbenzene
 Concen: 11.839 ug/l
 RT: 11.750 min Scan# 11
 Delta R.T. -0.140 min
 Lab File: VX026768.D
 Acq: 03 Feb 2022 19:08




Instrument :
 MSVOA_X
 ClientSampleId :
 34025


Tgt Ion:105 Resp: 71444
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.1 30.1#

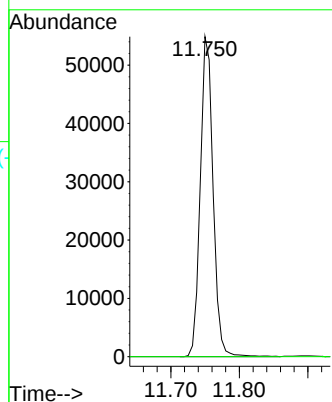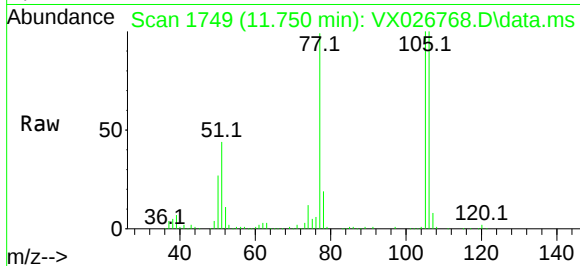

#89
 n-Butylbenzene
 Concen: 0.229 ug/l
 RT: 12.305 min Scan# 1840
 Delta R.T. -0.031 min
 Lab File: VX026768.D
 Acq: 03 Feb 2022 19:08

Tgt Ion: 91 Resp: 996
 Ion Ratio Lower Upper
 91 100
 92 0.0 27.2 81.6#
 134 7.6 13.1 39.1#


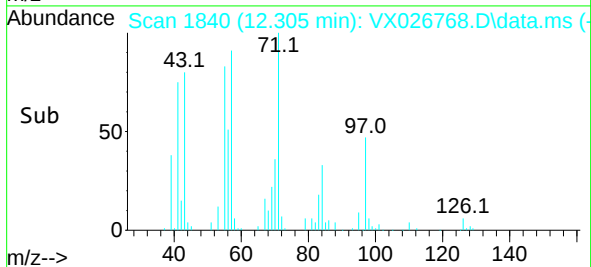

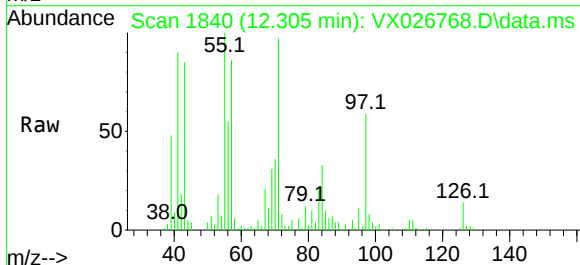




#90
Hexachloroethane
Concen: 2.309 ug/l
RT: 12.609 min Scan# 117
Delta R.T. 0.067 min
Lab File: VX026768.D
Acq: 03 Feb 2022 19:08

Instrument :
MSVOA_X
ClientSampleId :
34025

Tgt Ion:117 Resp: 116
Ion Ratio Lower Upper
117 100
201 0.0 35.6 106.8#

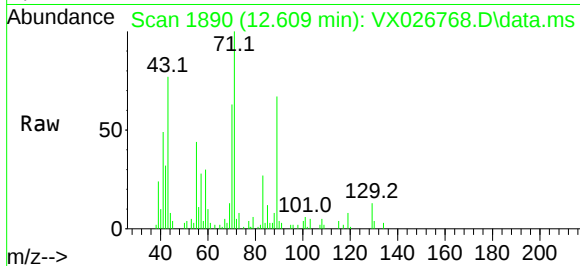

#95
Naphthalene
Concen: 0.673 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX026768.D
Acq: 03 Feb 2022 19:08

Tgt Ion:128 Resp: 3540
Ion Ratio Lower Upper
128 100
127 15.1 10.3 15.5
129 12.2 8.7 13.1

