

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020323\
 Data File : VX034001.D
 Acq On : 03 Feb 2023 09:42
 Operator : JC/MD
 Sample : VX0203WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK610

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
 Title : VOC Analysis

Signal : TIC: VX034001.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	60	rBV	79477	100356	12.87%	1.724%
2	1.672	91	96	119	rVB	47039	76133	9.76%	1.308%
3	2.185	178	180	181	rBV	220	143	0.02%	0.002%
4	2.307	194	200	211	rBV	179403	278430	35.70%	4.782%
5	2.514	230	234	240	rVB2	742	1293	0.17%	0.022%
6	2.691	260	263	264	rBV	195	213	0.03%	0.004%
7	2.788	274	279	285	rBV	1146	1836	0.24%	0.032%
8	2.941	297	304	313	rBV	2307	5638	0.72%	0.097%
9	3.020	316	317	319	rBV	167	168	0.02%	0.003%
10	3.087	326	328	332	rVB3	266	292	0.04%	0.005%
11	3.178	342	343	346	rVB	138	118	0.02%	0.002%
12	3.209	346	348	350	rBV	88	108	0.01%	0.002%
13	3.367	370	374	375	rBV	126	151	0.02%	0.003%
14	3.398	378	379	382	rBB	134	109	0.01%	0.002%
15	3.489	393	394	396	rBV	138	145	0.02%	0.002%
16	3.587	406	410	413	rBV2	108	173	0.02%	0.003%
17	3.623	413	416	417	rBV2	122	118	0.02%	0.002%
18	3.776	438	441	444	rVB	176	202	0.03%	0.003%
19	3.800	444	445	447	rBV	92	91	0.01%	0.002%
20	3.818	447	448	452	rVB	161	165	0.02%	0.003%
21	3.855	452	454	455	rVB	179	112	0.01%	0.002%
22	3.867	455	456	458	rBV	126	90	0.01%	0.002%
23	3.904	458	462	464	rBV	142	181	0.02%	0.003%
24	3.928	464	466	469	rVB2	260	229	0.03%	0.004%
25	3.977	469	474	476	rBV2	180	377	0.05%	0.006%
26	4.044	484	485	489	rBV2	148	202	0.03%	0.003%
27	4.105	494	495	497	rBV	148	145	0.02%	0.002%
28	4.178	505	507	510	rBV	107	115	0.01%	0.002%
29	4.215	511	513	515	rBV2	106	108	0.01%	0.002%
30	4.270	519	522	526	rBV2	199	328	0.04%	0.006%
31	4.452	543	552	566	rBV	46396	135721	17.40%	2.331%
32	4.855	614	618	619	rVB	138	147	0.02%	0.003%
33	4.867	619	620	623	rBV	118	118	0.02%	0.002%
34	4.891	623	624	626	rBV	122	106	0.01%	0.002%
35	5.050	638	650	666	rBV2	98741	305820	39.21%	5.252%
36	5.397	699	707	709	rVV3	422	964	0.12%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020323\
 Data File : VX034001.D
 Acq On : 03 Feb 2023 09:42
 Operator : JC/MD
 Sample : VX0203WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK610

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
 Title : VOC Analysis

37	5.556	724	733	739	rBV2	1006	2398	0.31%	0.041%
38	5.605	739	741	742	rBV	159	108	0.01%	0.002%
39	5.757	763	766	768	rBV2	128	137	0.02%	0.002%
40	5.964	788	800	818	rBV2	262280	779946	100.00%	13.395%
41	6.269	848	850	852	rVB2	152	135	0.02%	0.002%
42	6.330	859	860	862	rBV	158	104	0.01%	0.002%
43	6.428	874	876	880	rBV	73	97	0.01%	0.002%
44	6.464	880	882	883	rBV	105	105	0.01%	0.002%
45	6.544	891	895	896	rBV2	168	237	0.03%	0.004%
46	6.580	900	901	906	rBV	79	127	0.02%	0.002%
47	6.617	906	907	910	rBV	126	146	0.02%	0.003%
48	6.757	920	930	944	rBV	213741	514187	65.93%	8.831%
49	7.037	974	976	978	rVB	116	103	0.01%	0.002%
50	7.111	982	988	996	rVB5	1333	2932	0.38%	0.050%
51	7.202	1000	1003	1004	rBV	103	108	0.01%	0.002%
52	7.306	1011	1020	1032	rBV	156581	346865	44.47%	5.957%
53	7.556	1059	1061	1062	rBV	113	93	0.01%	0.002%
54	7.708	1082	1086	1087	rBV2	159	177	0.02%	0.003%
55	7.757	1090	1094	1097	rBV2	147	244	0.03%	0.004%
56	7.885	1113	1115	1117	rBV2	111	111	0.01%	0.002%
57	7.946	1124	1125	1128	rBV2	165	157	0.02%	0.003%
58	8.202	1165	1167	1169	rBV	140	153	0.02%	0.003%
59	8.318	1180	1186	1208	rVV	102897	174637	22.39%	2.999%
60	8.488	1211	1214	1216	rBV	161	167	0.02%	0.003%
61	8.647	1233	1240	1250	rBV	408751	653458	83.78%	11.223%
62	8.946	1284	1289	1301	rBV	73180	108688	13.94%	1.867%
63	9.068	1307	1309	1311	rVB	255	193	0.02%	0.003%
64	9.275	1340	1343	1347	rVB3	364	481	0.06%	0.008%
65	9.385	1355	1361	1380	rBV	183461	291702	37.40%	5.010%
66	9.677	1407	1409	1412	rBV2	110	109	0.01%	0.002%
67	9.744	1418	1420	1422	rBV	126	107	0.01%	0.002%
68	10.049	1465	1470	1483	rBV	405733	560919	71.92%	9.634%
69	10.305	1509	1512	1517	rVB3	434	702	0.09%	0.012%
70	10.342	1517	1518	1521	rBV	167	154	0.02%	0.003%
71	10.531	1546	1549	1552	rBV	170	196	0.03%	0.003%
72	10.646	1565	1568	1570	rBV2	360	512	0.07%	0.009%
73	10.768	1586	1588	1589	rBV	185	125	0.02%	0.002%
74	11.043	1631	1633	1636	rVB2	139	142	0.02%	0.002%
75	11.189	1652	1657	1666	rBV	264531	343144	44.00%	5.893%
76	11.311	1675	1677	1681	rVB3	329	414	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020323\
 Data File : VX034001.D
 Acq On : 03 Feb 2023 09:42
 Operator : JC/MD
 Sample : VX0203WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK610

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
 Title : VOC Analysis

77	11.341	1681	1682	1684	rBV	158	159	0.02%	0.003%
78	11.457	1696	1701	1706	rVB3	495	743	0.10%	0.013%
79	11.506	1706	1709	1710	rVB3	136	108	0.01%	0.002%
80	11.524	1710	1712	1713	rBV	180	117	0.02%	0.002%
81	11.713	1741	1743	1746	rVB2	255	230	0.03%	0.004%
82	11.750	1746	1749	1754	rBV2	567	832	0.11%	0.014%
83	11.969	1782	1785	1788	rBV2	592	739	0.09%	0.013%
84	12.018	1788	1793	1807	rVV	419149	551205	70.67%	9.467%
85	12.225	1824	1827	1828	rBV2	121	127	0.02%	0.002%
86	12.317	1837	1842	1855	rBV	438120	564181	72.34%	9.690%
87	12.579	1881	1885	1886	rBV2	187	262	0.03%	0.004%
88	12.689	1901	1903	1904	rBV2	157	142	0.02%	0.002%
89	12.762	1911	1915	1919	rBV2	707	1121	0.14%	0.019%
90	12.939	1942	1944	1945	rBV	172	146	0.02%	0.003%
91	13.116	1969	1973	1977	rBV2	810	998	0.13%	0.017%
92	13.591	2047	2051	2056	rVB3	1357	1822	0.23%	0.031%
93	13.640	2056	2059	2060	rBV2	143	148	0.02%	0.003%
94	13.780	2079	2082	2086	rVB	828	1123	0.14%	0.019%
95	13.963	2109	2112	2116	rVB2	1154	1355	0.17%	0.023%
96	14.128	2136	2139	2143	rBV3	930	1043	0.13%	0.018%
97	14.378	2178	2180	2182	rBV	154	127	0.02%	0.002%
98	14.445	2190	2191	2193	rBV	119	90	0.01%	0.002%
99	14.603	2215	2217	2219	rBV2	197	213	0.03%	0.004%
100	14.627	2219	2221	2223	rVV2	342	253	0.03%	0.004%




Sum of corrected areas: 5822449

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020323\
Data File : VX034001.D
Acq On : 03 Feb 2023 09:42
Operator : JC/MD
Sample : VX0203WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK610

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

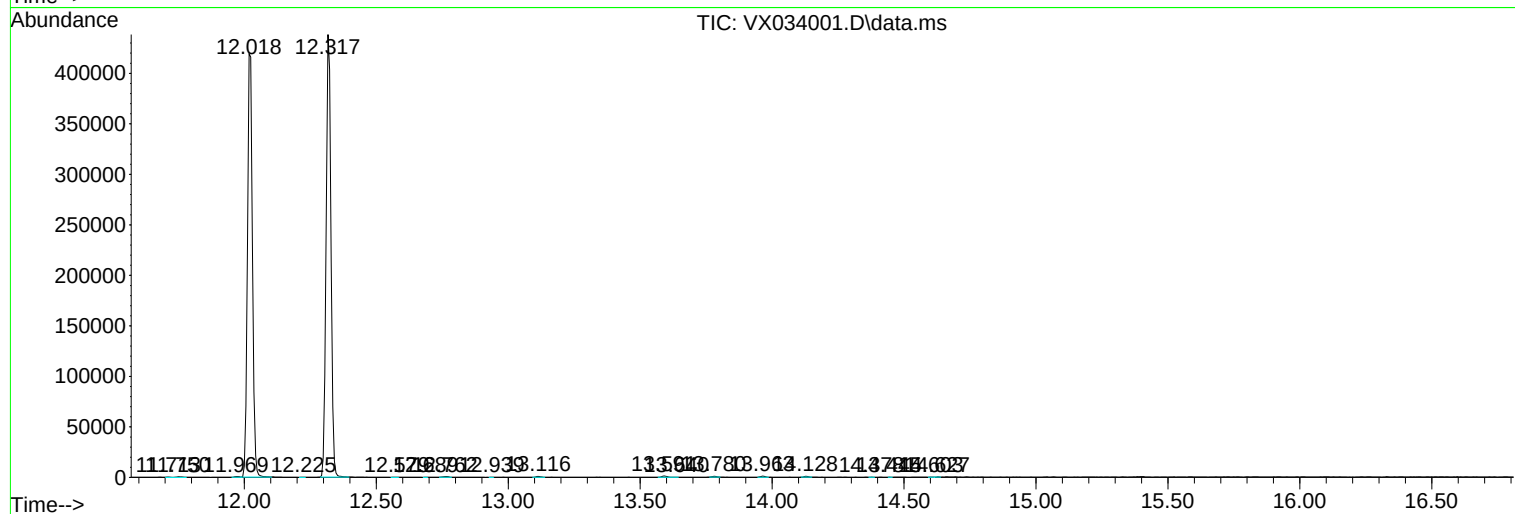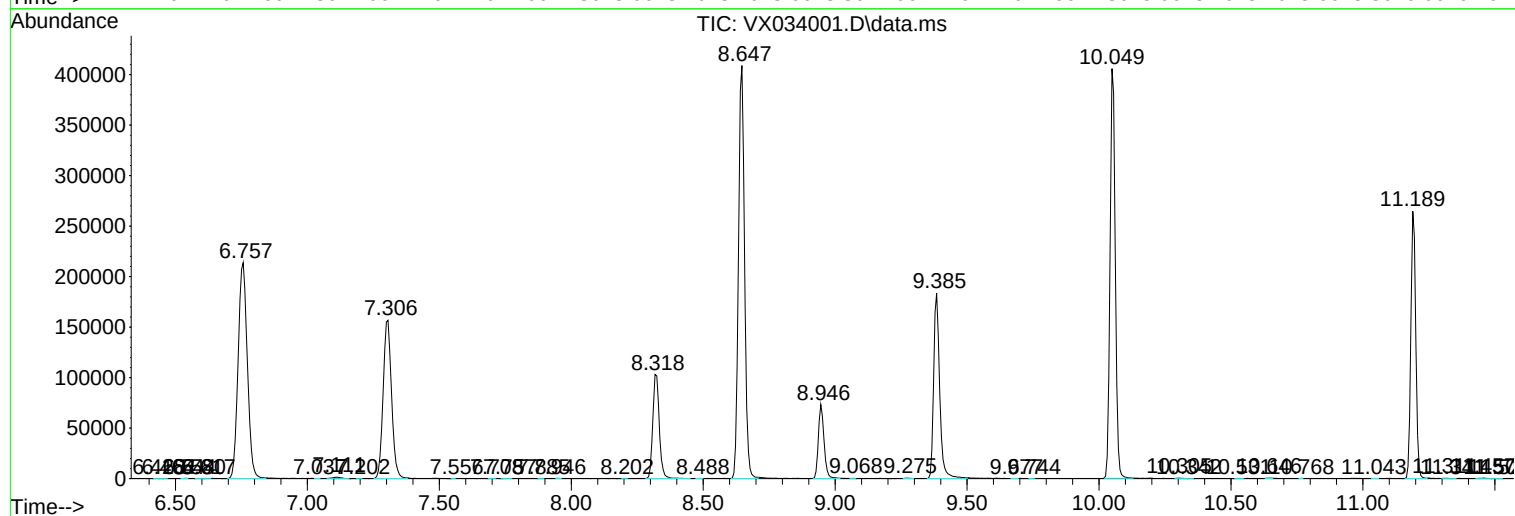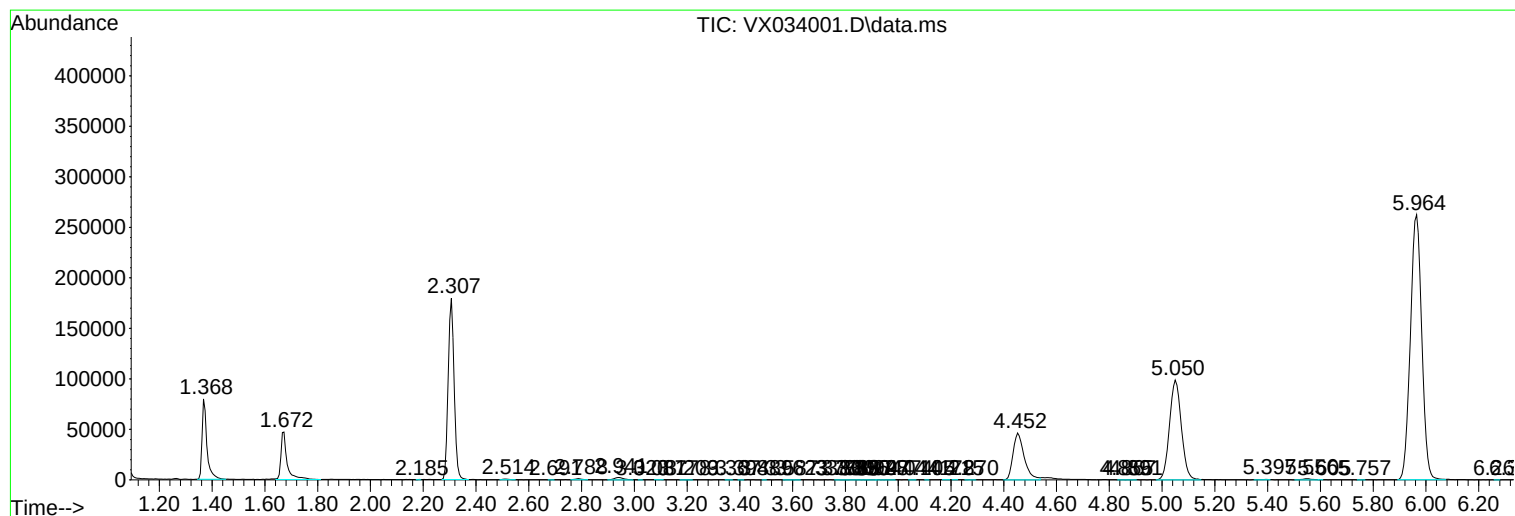

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020323\
Data File : VX034001.D
Acq On : 03 Feb 2023 09:42
Operator : JC/MD
Sample : VX0203WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK610

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020323\
Data File : VX034001.D
Acq On : 03 Feb 2023 09:42
Operator : JC/MD
Sample : VX0203WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK610

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc