

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020323\
 Data File : VX034002.D
 Acq On : 03 Feb 2023 10:05
 Operator : JC/MD
 Sample : VX0203MBL01
 Misc : 5.00g/5.0mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK611

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
 Title : VOC Analysis

Signal : TIC: VX034002.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	27	29	32	rVB3	983	926	0.12%	0.016%
2	1.367	42	46	58	rBV	86174	100927	13.10%	1.743%
3	1.672	92	96	110	rVB	53060	75431	9.79%	1.303%
4	1.953	140	142	143	rBV	209	178	0.02%	0.003%
5	2.245	188	190	191	rBV	203	102	0.01%	0.002%
6	2.306	194	200	210	rBV	169378	273395	35.49%	4.722%
7	2.471	224	227	229	rBV	147	180	0.02%	0.003%
8	2.514	229	234	239	rVV3	608	1169	0.15%	0.020%
9	2.739	270	271	274	rBV2	198	245	0.03%	0.004%
10	2.788	275	279	284	rVB2	972	1598	0.21%	0.028%
11	2.867	290	292	295	rBV	129	161	0.02%	0.003%
12	2.940	300	304	314	rVB3	636	1563	0.20%	0.027%
13	3.020	314	317	319	rBV	185	218	0.03%	0.004%
14	3.105	329	331	332	rBV	278	151	0.02%	0.003%
15	3.123	332	334	336	rVB	192	168	0.02%	0.003%
16	3.142	336	337	339	rBV	174	142	0.02%	0.002%
17	3.166	339	341	344	rBV	125	138	0.02%	0.002%
18	3.270	356	358	361	rVB2	170	168	0.02%	0.003%
19	3.300	361	363	364	rBV	187	160	0.02%	0.003%
20	3.379	373	376	378	rVV	122	119	0.02%	0.002%
21	3.404	378	380	383	rVV	124	133	0.02%	0.002%
22	3.513	395	398	399	rBV	140	137	0.02%	0.002%
23	3.562	401	406	407	rVV2	114	192	0.02%	0.003%
24	3.617	411	415	417	rVB	132	153	0.02%	0.003%
25	3.684	425	426	427	rBV	126	79	0.01%	0.001%
26	3.849	451	453	454	rBV	156	126	0.02%	0.002%
27	3.952	468	470	471	rBV	172	121	0.02%	0.002%
28	3.977	471	474	477	rBV2	183	270	0.04%	0.005%
29	4.111	494	496	499	rBV	118	120	0.02%	0.002%
30	4.361	534	537	542	rBV2	225	470	0.06%	0.008%
31	4.452	542	552	567	rBV2	48574	141099	18.32%	2.437%
32	4.751	600	601	603	rBV	124	92	0.01%	0.002%
33	4.806	608	610	611	rBV	157	107	0.01%	0.002%
34	5.056	639	651	673	rBV	98262	305226	39.63%	5.272%
35	5.367	699	702	703	rBV2	356	365	0.05%	0.006%
36	5.452	713	716	719	rBV2	182	267	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020323\
 Data File : VX034002.D
 Acq On : 03 Feb 2023 10:05
 Operator : JC/MD
 Sample : VX0203MBL01
 Misc : 5.00g/5.0mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK611

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
 Title : VOC Analysis

37	5.556	727	733	741	rVB4	1131	3003	0.39%	0.052%
38	5.653	748	749	750	rBV4	187	133	0.02%	0.002%
39	5.970	788	801	819	rBV2	254517	770280	100.00%	13.305%
40	6.293	850	854	856	rBV2	121	187	0.02%	0.003%
41	6.348	860	863	866	rBV	160	163	0.02%	0.003%
42	6.470	880	883	886	rVB3	190	225	0.03%	0.004%
43	6.507	886	889	890	rBV	121	82	0.01%	0.001%
44	6.592	902	903	906	rBV2	73	78	0.01%	0.001%
45	6.635	909	910	915	rVB2	103	137	0.02%	0.002%
46	6.757	921	930	947	rBV	210657	503097	65.31%	8.690%
47	7.013	970	972	975	rVB2	155	131	0.02%	0.002%
48	7.110	983	988	995	rBV2	1339	3077	0.40%	0.053%
49	7.208	1002	1004	1006	rBV	133	159	0.02%	0.003%
50	7.305	1011	1020	1037	rBV	157607	344158	44.68%	5.945%
51	7.415	1037	1038	1040	rBV	112	87	0.01%	0.002%
52	7.446	1040	1043	1045	rBV	176	250	0.03%	0.004%
53	7.885	1113	1115	1118	rBV	118	119	0.02%	0.002%
54	8.043	1137	1141	1143	rBV2	120	224	0.03%	0.004%
55	8.122	1153	1154	1157	rBV2	110	108	0.01%	0.002%
56	8.324	1181	1187	1197	rBV	104183	171512	22.27%	2.963%
57	8.470	1209	1211	1213	rBV	152	134	0.02%	0.002%
58	8.494	1213	1215	1217	rBV	156	106	0.01%	0.002%
59	8.647	1233	1240	1250	rBV	412943	652303	84.68%	11.267%
60	8.897	1279	1281	1283	rBV	126	113	0.01%	0.002%
61	8.951	1284	1290	1301	rVV	70182	108140	14.04%	1.868%
62	9.214	1331	1333	1335	rBV	127	114	0.01%	0.002%
63	9.275	1339	1343	1348	rVV3	511	735	0.10%	0.013%
64	9.384	1355	1361	1375	rBV	205455	304495	39.53%	5.260%
65	9.653	1401	1405	1406	rVB2	192	219	0.03%	0.004%
66	9.707	1412	1414	1415	rVB2	253	174	0.02%	0.003%
67	10.055	1465	1471	1486	rBV	393771	556498	72.25%	9.612%
68	10.311	1509	1513	1514	rBV2	335	324	0.04%	0.006%
69	10.409	1527	1529	1531	rBV2	166	218	0.03%	0.004%
70	10.469	1537	1539	1540	rBV	110	107	0.01%	0.002%
71	10.622	1562	1564	1565	rVB	166	96	0.01%	0.002%
72	10.658	1565	1570	1571	rBV2	363	509	0.07%	0.009%
73	10.787	1590	1591	1594	rBV	88	81	0.01%	0.001%
74	10.963	1617	1620	1624	rBV3	355	530	0.07%	0.009%
75	11.036	1630	1632	1633	rBV	115	92	0.01%	0.002%
76	11.189	1652	1657	1672	rVB	265092	344078	44.67%	5.943%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020323\
 Data File : VX034002.D
 Acq On : 03 Feb 2023 10:05
 Operator : JC/MD
 Sample : VX0203MBL01
 Misc : 5.00g/5.0mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK611

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
 Title : VOC Analysis

77	11.317	1675	1678	1680	rBV	172	230	0.03%	0.004%
78	11.457	1698	1701	1703	rBV3	296	393	0.05%	0.007%
79	11.567	1717	1719	1721	rBV	111	113	0.01%	0.002%
80	11.707	1740	1742	1746	rVB2	151	177	0.02%	0.003%
81	11.750	1746	1749	1753	rBV2	433	548	0.07%	0.009%
82	11.823	1759	1761	1762	rBV	149	120	0.02%	0.002%
83	11.975	1782	1786	1788	rBV	453	489	0.06%	0.008%
84	12.018	1788	1793	1803	rBV	415980	544630	70.71%	9.407%
85	12.201	1822	1823	1826	rBV	163	180	0.02%	0.003%
86	12.244	1826	1830	1832	rBV2	148	264	0.03%	0.005%
87	12.317	1837	1842	1859	rVV	437193	564274	73.26%	9.747%
88	12.506	1870	1873	1874	rBV2	249	225	0.03%	0.004%
89	12.768	1912	1916	1923	rVB2	617	1001	0.13%	0.017%
90	13.115	1970	1973	1975	rBV	341	336	0.04%	0.006%
91	13.310	2003	2005	2006	rBV	174	91	0.01%	0.002%
92	13.493	2030	2035	2036	rBV2	176	266	0.03%	0.005%
93	13.591	2048	2051	2056	rBV2	524	739	0.10%	0.013%
94	13.780	2080	2082	2086	rVB2	447	507	0.07%	0.009%
95	13.969	2110	2113	2116	rVB4	341	437	0.06%	0.008%
96	14.133	2135	2140	2145	rVB	1061	1321	0.17%	0.023%
97	14.335	2171	2173	2174	rVB	217	98	0.01%	0.002%
98	14.475	2194	2196	2197	rBV2	230	208	0.03%	0.004%
99	15.036	2286	2288	2289	rBV	250	150	0.02%	0.003%
100	16.462	2521	2522	2523	rBV	413	228	0.03%	0.004%


Sum of corrected areas: 5789397

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020323\
Data File : VX034002.D
Acq On : 03 Feb 2023 10:05
Operator : JC/MD
Sample : VX0203MBL01
Misc : 5.00g/5.0mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK611

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

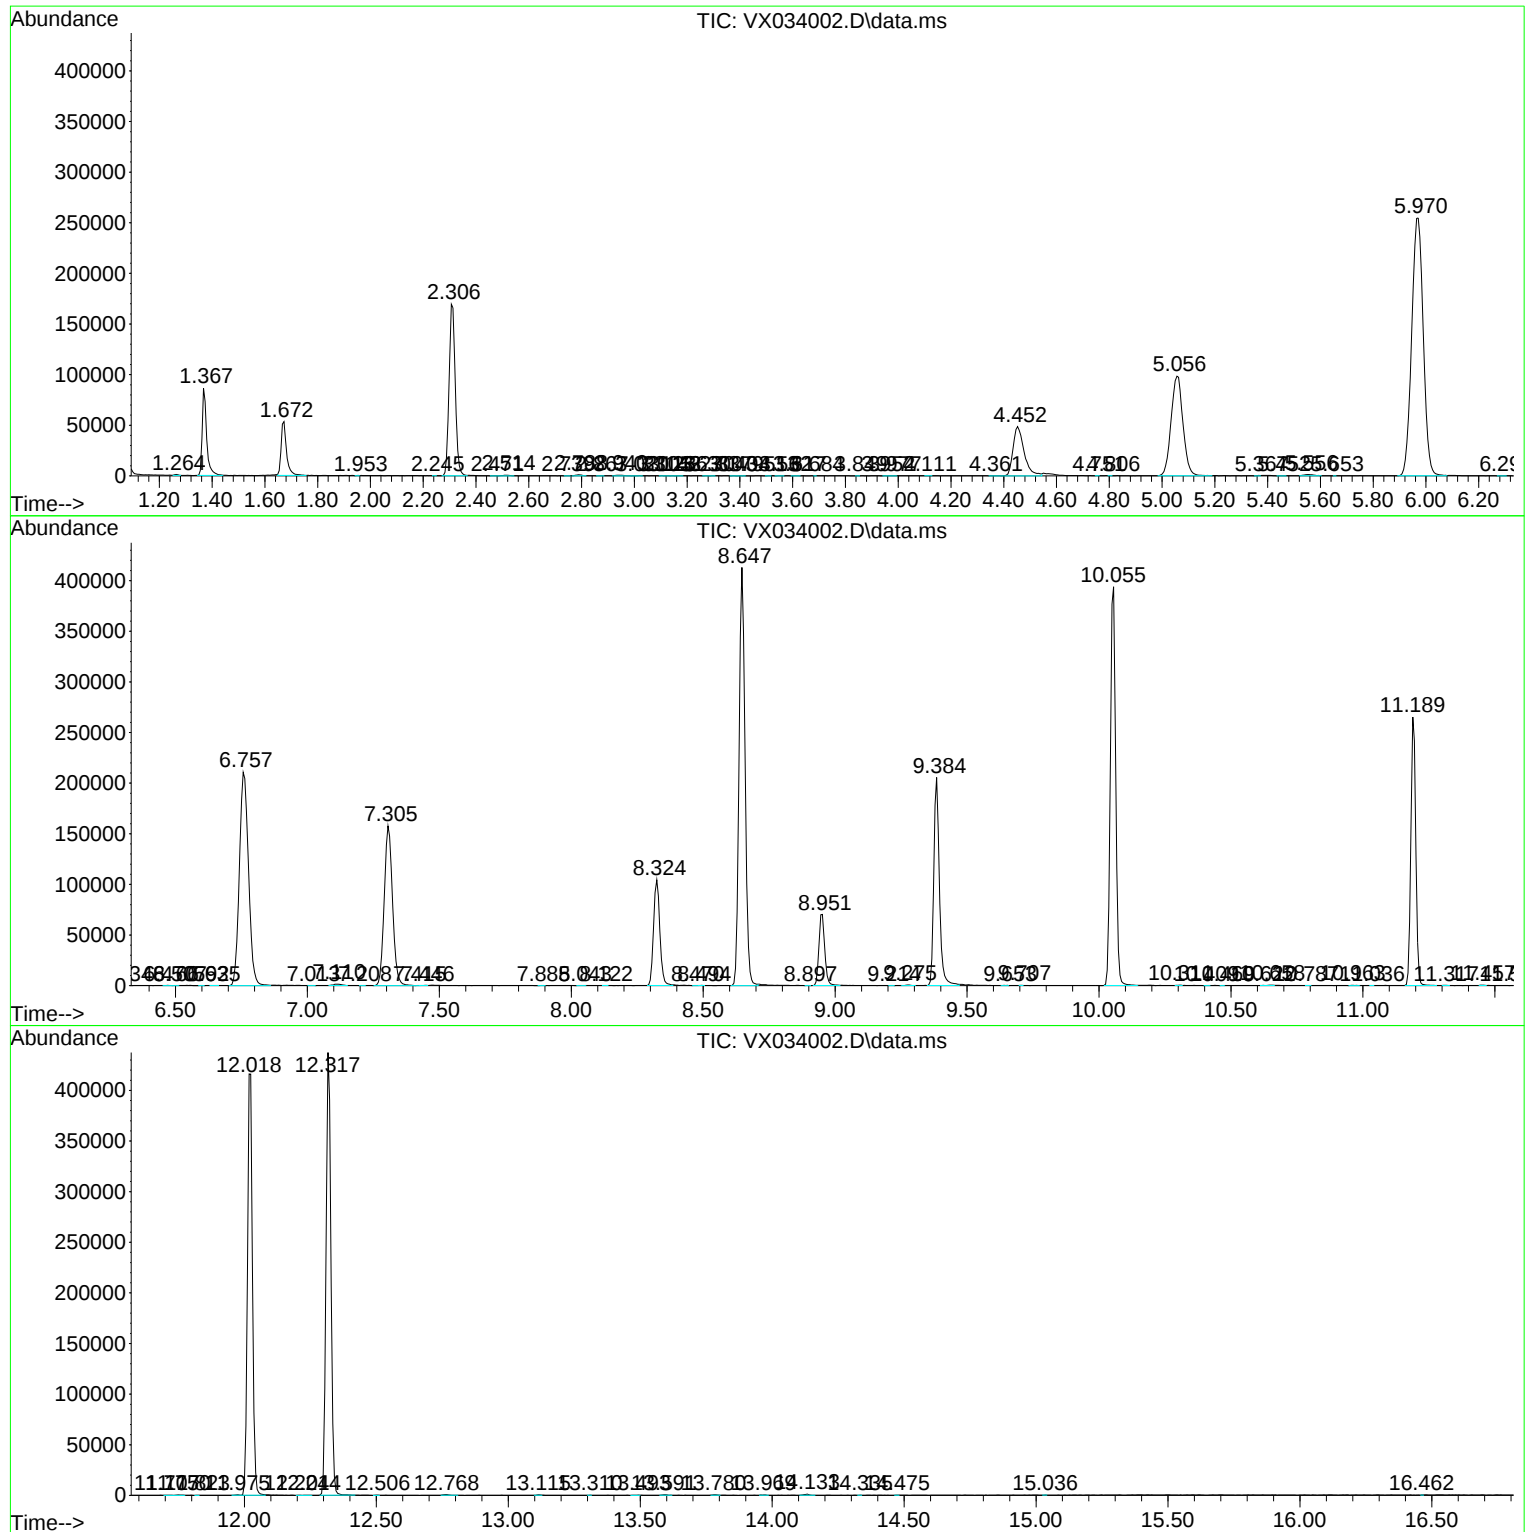

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020323\
Data File : VX034002.D
Acq On : 03 Feb 2023 10:05
Operator : JC/MD
Sample : VX0203MBL01
Misc : 5.00g/5.0mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK611

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020323\
Data File : VX034002.D
Acq On : 03 Feb 2023 10:05
Operator : JC/MD
Sample : VX0203MBL01
Misc : 5.00g/5.0mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK611

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc