
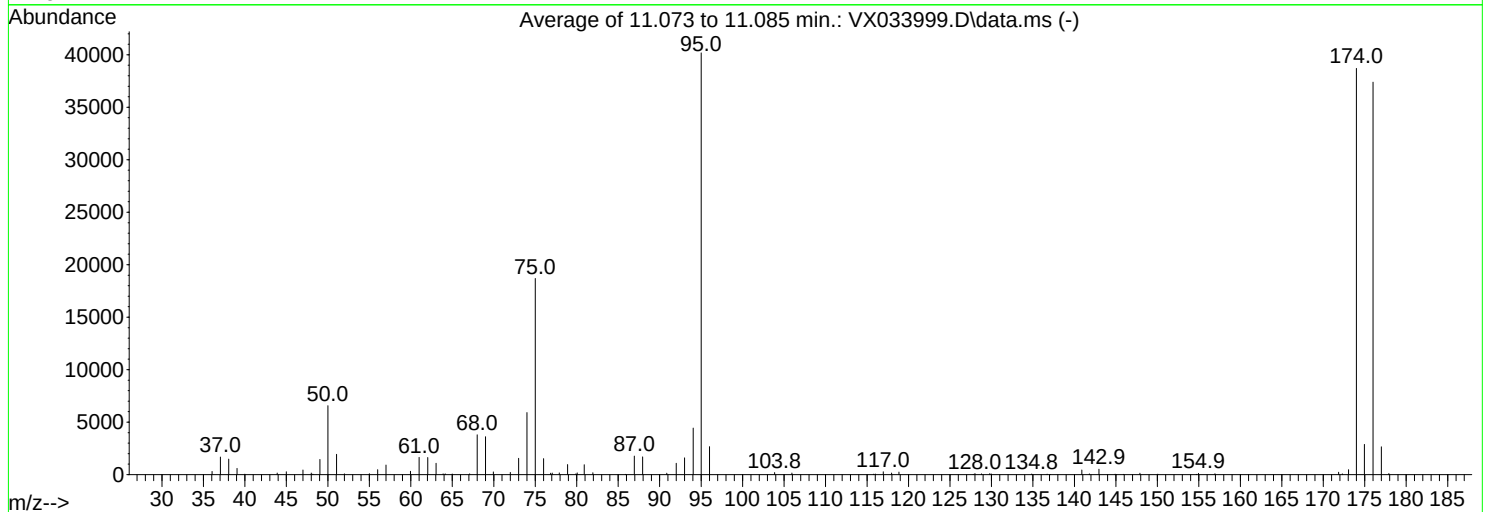


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020323\
Data File : VX033999.D
Acq On : 03 Feb 2023 08:08
Operator : JC/MD
Sample : BFB608
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB608

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM020223WMA.M
Title : VOC Analysis
Last Update : Sat Feb 04 03:17:09 2023

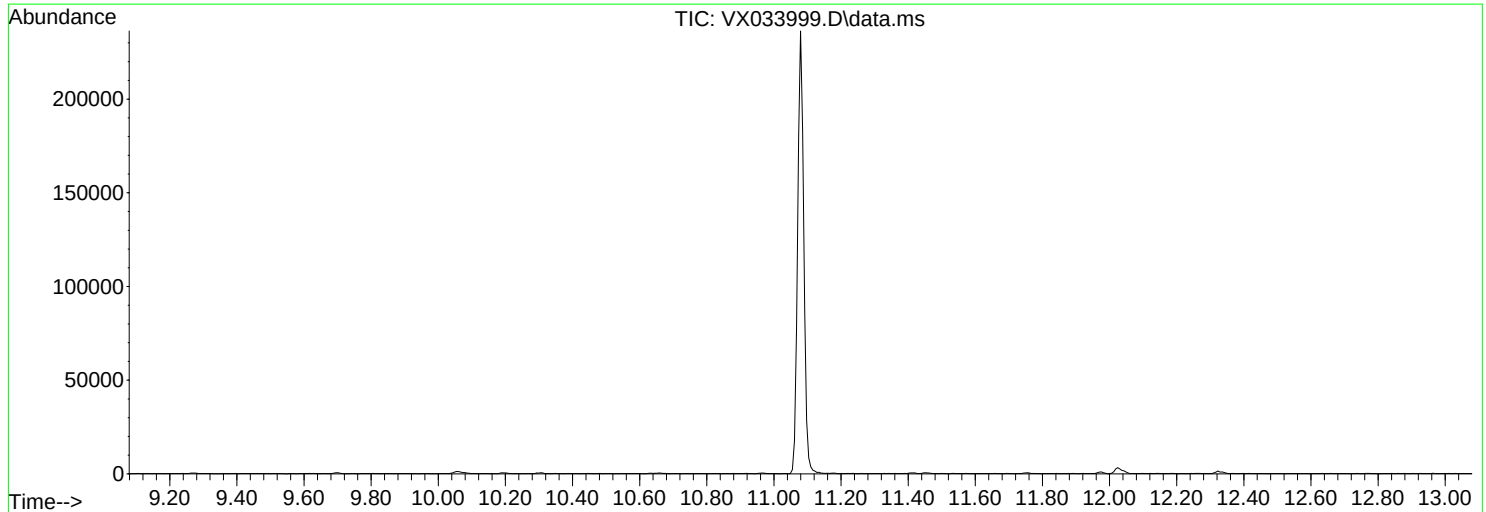

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.3	6567	PASS
75	95	30	80	46.5	18693	PASS
95	95	100	100	100.0	40184	PASS
96	95	5	9	6.6	2668	PASS
173	174	0.00	2	1.2	471	PASS
174	95	50	120	96.3	38707	PASS
175	174	5	9	7.5	2888	PASS
176	174	95	101	96.6	37397	PASS
177	176	5	9	7.1	2647	PASS

m/z	Abundance
40.00	59.0
43.90	65.0

Instrument :
MSVOA_X
ClientSampleId :
BFB608

m/z	Abundance
36.10	317.0
37.00	1537.0
38.00	1494.0
39.10	530.0
40.00	109.0
43.90	191.0
45.10	342.0
47.10	398.0
48.00	174.0
49.10	1437.0
50.00	6388.0
51.00	1944.0
52.00	123.0
55.00	60.0
56.00	539.0
57.00	857.0
59.90	339.0
61.00	1767.0
62.10	1519.0
63.10	1063.0
63.90	138.0
65.00	102.0
67.10	92.0
68.00	3735.0
69.00	3551.0
69.90	243.0
72.00	194.0
73.00	1440.0
74.00	5686.0
75.00	18352.0
76.00	1554.0
76.90	204.0
78.00	200.0
78.90	880.0
79.90	238.0
80.90	897.0
81.90	184.0
86.90	1641.0
87.90	1534.0
90.90	107.0
92.00	980.0
93.00	1439.0
94.00	4073.0
95.00	37744.0
96.00	2637.0
103.80	228.0
105.90	145.0
115.80	138.0
117.00	245.0
118.00	136.0
118.90	177.0
127.80	116.0
128.80	75.0
129.80	157.0
134.90	70.0
136.70	77.0
140.90	353.0
141.70	63.0
143.00	362.0
147.90	110.0
150.00	76.0
154.70	74.0
155.00	69.0
157.10	62.0
171.80	184.0
173.10	385.0
174.00	31936.0
175.00	2551.0
176.00	30280.0
177.00	2217.0
177.90	54.0

Instrument :
MSVOA_X
ClientSampleId :
BFB608

m/z	Abundance
36.00	348.0
37.10	2084.0
38.10	1814.0
39.00	696.0
40.00	112.0
43.90	243.0
45.00	284.0
46.90	533.0
48.00	302.0
49.00	1635.0
50.00	7573.0
51.00	2363.0
52.00	94.0
55.00	111.0
56.00	584.0
57.00	1038.0
60.00	402.0
61.00	1759.0
62.10	2023.0
63.00	1288.0
64.10	150.0
65.00	96.0
67.10	125.0
68.00	4415.0
69.00	4463.0
70.00	318.0
72.10	248.0
73.00	1769.0
74.00	6990.0
75.00	21888.0
76.00	1823.0
76.80	221.0
77.10	202.0
77.80	173.0
78.90	1158.0
80.10	264.0
80.90	1177.0
82.00	189.0
87.00	2209.0
88.00	2043.0
90.80	147.0
92.00	1306.0
93.00	1848.0
94.10	5160.0
95.00	48104.0
96.00	3238.0
103.80	162.0
105.00	57.0
105.90	164.0
116.00	101.0
116.90	287.0
117.80	154.0
118.80	275.0
128.00	216.0
128.80	73.0
130.00	174.0
134.80	112.0
136.70	75.0
140.90	484.0
141.80	86.0
143.00	687.0
144.90	133.0
145.90	87.0
147.80	154.0
150.10	68.0
154.90	145.0
156.90	115.0
161.00	54.0
171.80	284.0
172.30	224.0
173.00	514.0
174.00	45520.0
175.00	3434.0
176.00	44408.0
177.00	2986.0
177.90	103.0

Instrument :
MSVOA_X
ClientSampleId :
BFB608

m/z	Abundance
36.10	263.0
37.10	1399.0
38.10	1116.0
39.10	573.0
40.00	115.0
44.00	206.0
44.90	211.0
47.00	410.0
48.20	137.0
49.10	1288.0
50.00	5740.0
51.10	1489.0
55.00	92.0
56.00	293.0
57.00	828.0
60.00	222.0
61.00	1394.0
62.00	1371.0
63.10	903.0
63.90	110.0
64.20	86.0
68.00	3259.0
69.00	2846.0
70.00	214.0
71.90	218.0
73.00	1458.0
74.00	5078.0
75.00	15838.0
76.00	1180.0
77.00	257.0
77.90	129.0
78.90	823.0
80.00	230.0
80.90	747.0
81.90	168.0
85.90	85.0
87.00	1441.0
88.00	1526.0
90.90	148.0
92.00	971.0
93.00	1517.0
94.00	4072.0
95.00	34704.0
96.00	2128.0
103.90	195.0
106.00	148.0
116.00	107.0
116.90	287.0
118.00	173.0
118.80	266.0
128.00	118.0
128.80	83.0
129.80	172.0
137.10	51.0
140.90	477.0
141.90	74.0
142.90	490.0
145.10	58.0
148.00	141.0
154.90	171.0
156.90	87.0
171.90	237.0
173.10	514.0
174.00	38664.0
174.90	2679.0
176.00	37504.0
177.00	2739.0
177.90	147.0

Instrument :
MSVOA_X
ClientSampleId :
BFB608