

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020325\
 Data File : VX044819.D
 Acq On : 03 Feb 2025 16:55
 Operator : JC/MD
 Sample : Q1232-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 JPP-51.1-012925

Quant Time: Feb 04 02:11:35 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011525W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jan 16 01:16:09 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	115498	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	232958	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	204621	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	85623	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	82379	47.253	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	94.500%
35) Dibromofluoromethane	5.379	113	72678	49.109	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.220%
50) Toluene-d8	8.647	98	276609	53.604	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	107.200%
62) 4-Bromofluorobenzene	11.079	95	94005	48.867	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	97.740%
Target Compounds						
					Qvalue	
16) Acetone	2.380	43	36115	52.360	ug/l	96
18) Methyl Acetate	2.703	43	2850	1.339	ug/l	92
20) Methylene Chloride	2.782	84	4724	2.941	ug/l #	79
43) Isopropyl Acetate	6.336	43	112520	27.880	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020325\
Data File : VX044819.D
Acq On : 03 Feb 2025 16:55
Operator : JC/MD
Sample : Q1232-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
JPP-51.1-012925

Quant Time: Feb 04 02:11:35 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011525W.M
Quant Title : SW846 8260
QLast Update : Thu Jan 16 01:16:09 2025
Response via : Initial Calibration




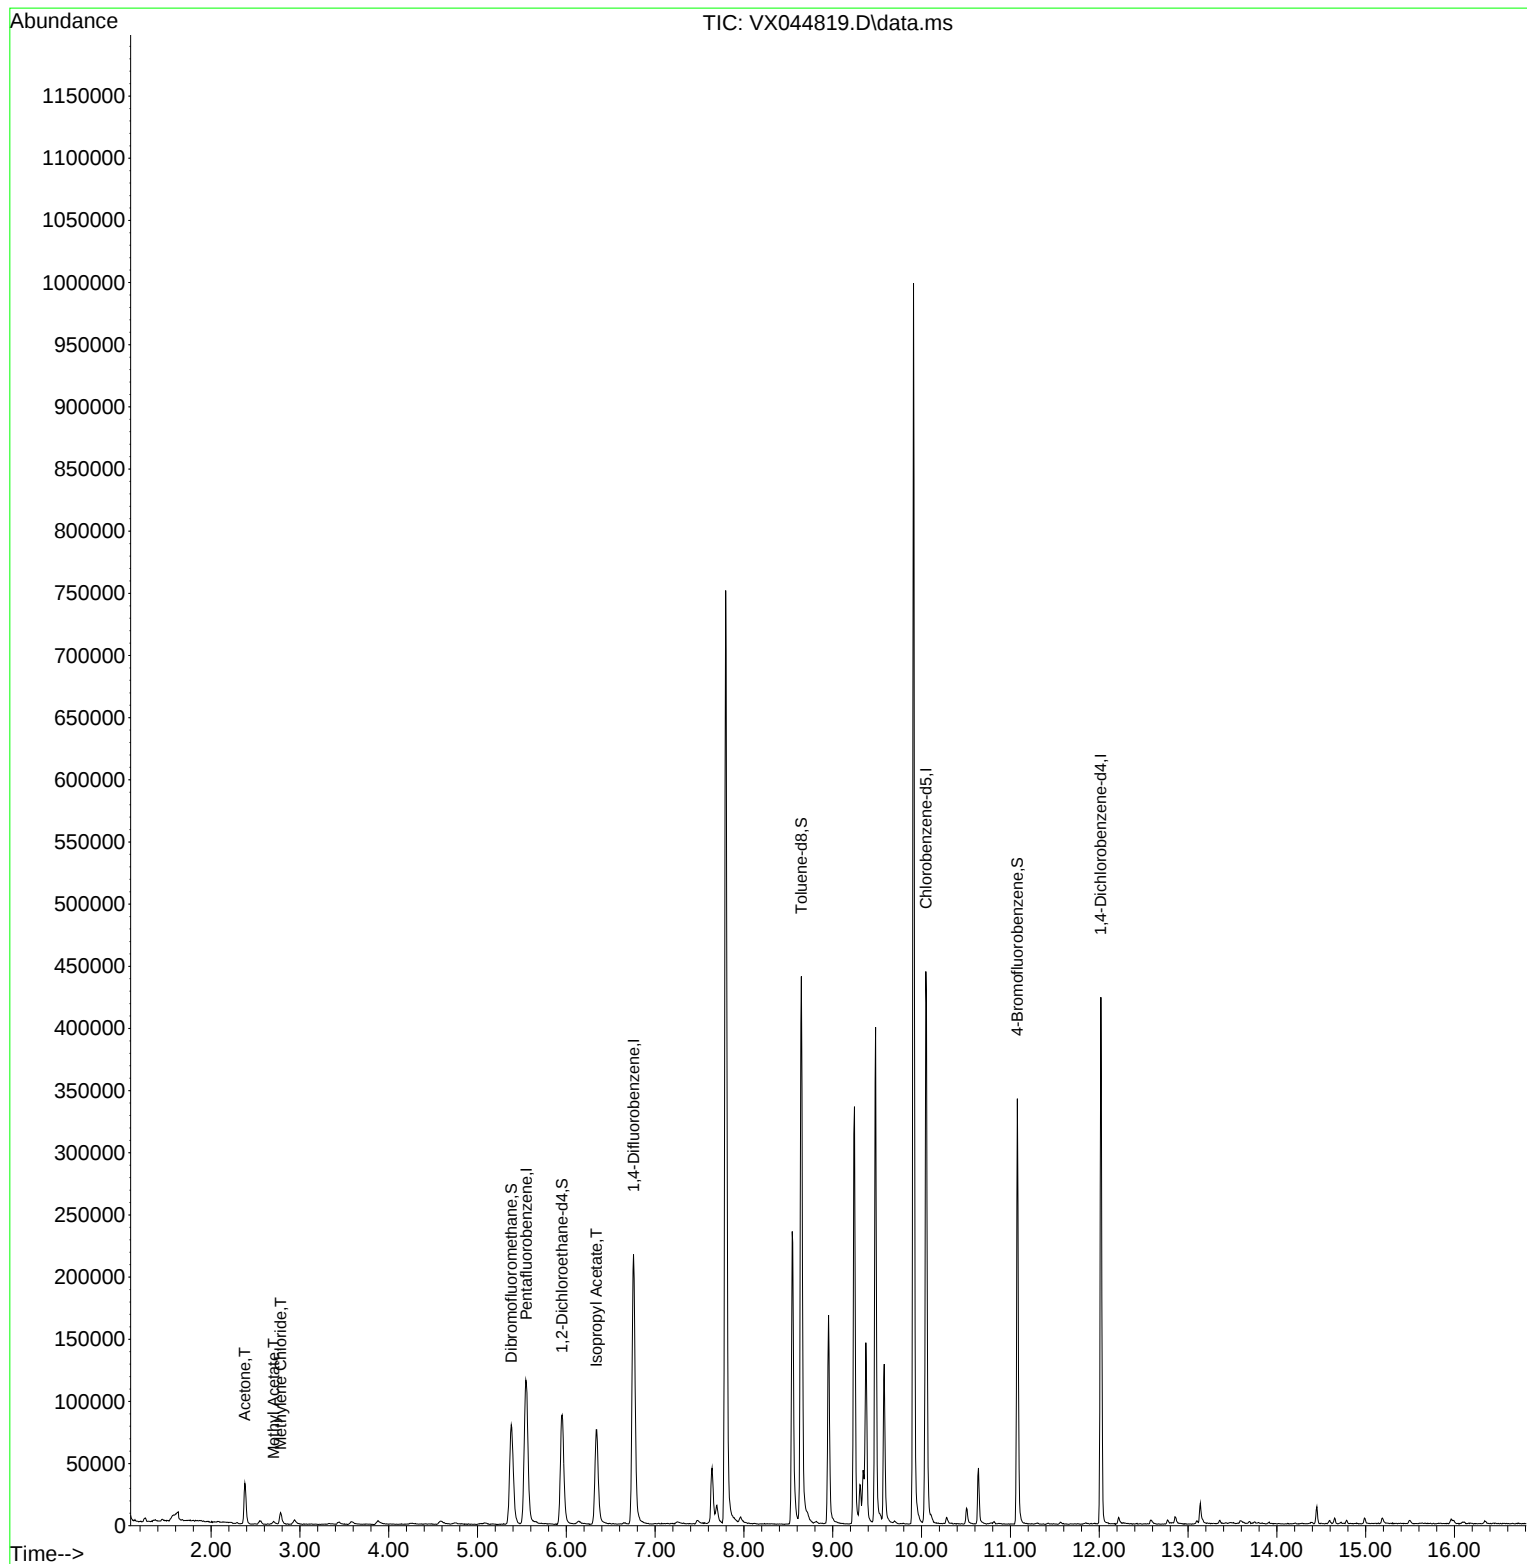




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX044819.D
Acq: 03 Feb 2025 16:55




Instrument :
MSVOA_X
ClientSampleId :
JPP-51.1-012925


Tgt Ion:168 Resp: 115498
Ion Ratio Lower Upper
168 100
99 59.7 51.1 76.7

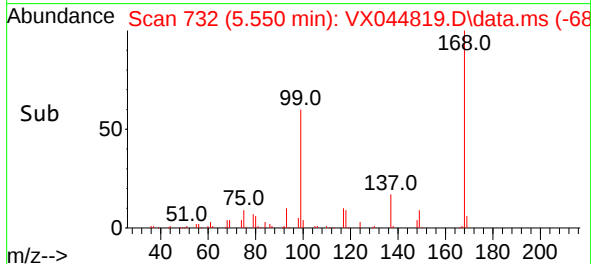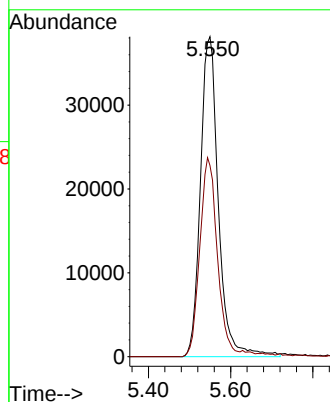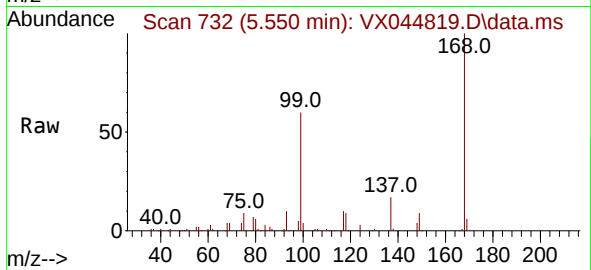

#16
Acetone
Concen: 52.360 ug/l
RT: 2.380 min Scan# 212
Delta R.T. -0.006 min
Lab File: VX044819.D
Acq: 03 Feb 2025 16:55

Tgt Ion: 43 Resp: 36115
Ion Ratio Lower Upper
43 100
58 28.4 24.6 37.0



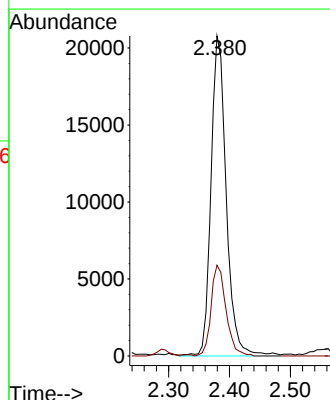
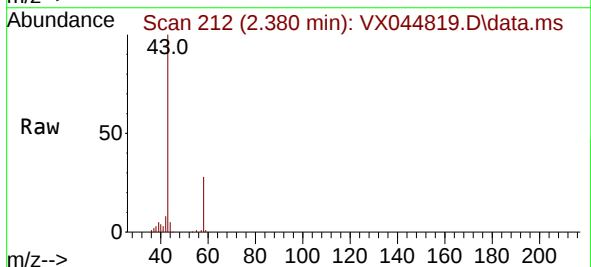


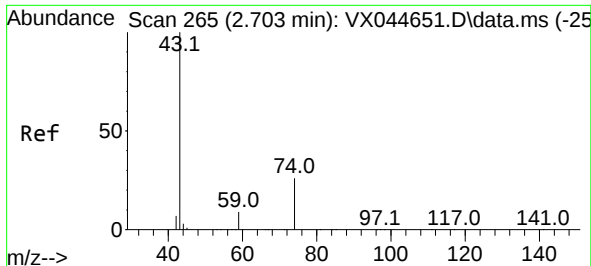

#18
Methyl Acetate
Concen: 1.339 ug/l
RT: 2.703 min Scan# 265
Delta R.T. 0.000 min
Lab File: VX044819.D
Acq: 03 Feb 2025 16:55




Instrument :
MSVOA_X
ClientSampleId :
JPP-51.1-012925


Tgt Ion: 43 Resp: 2850
Ion Ratio Lower Upper
43 100
74 21.0 19.8 29.8

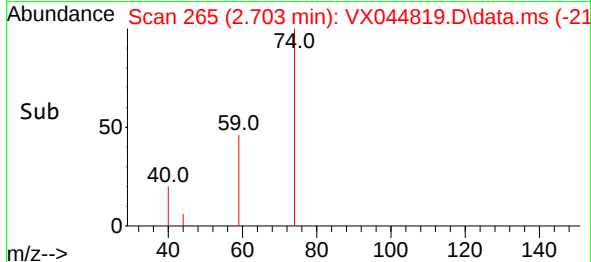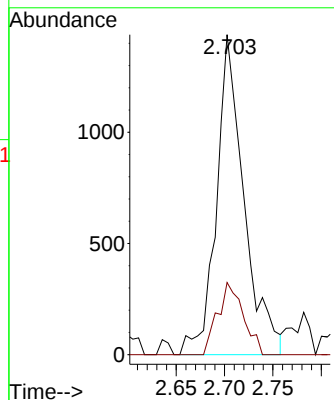

#20
Methylene Chloride
Concen: 2.941 ug/l
RT: 2.782 min Scan# 278
Delta R.T. 0.000 min
Lab File: VX044819.D
Acq: 03 Feb 2025 16:55

Tgt Ion: 84 Resp: 4724
Ion Ratio Lower Upper
84 100
49 88.6 94.2 141.4#
51 27.6 28.8 43.2#
86 52.4 50.3 75.5


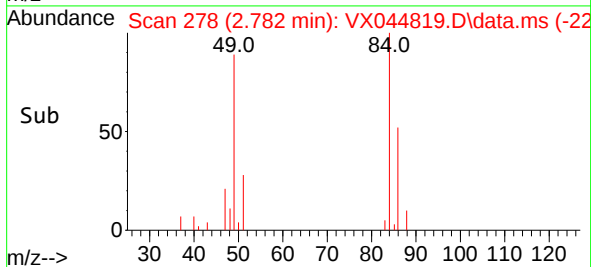
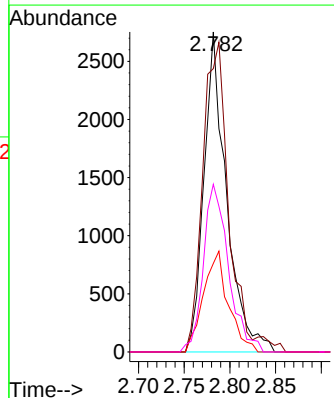
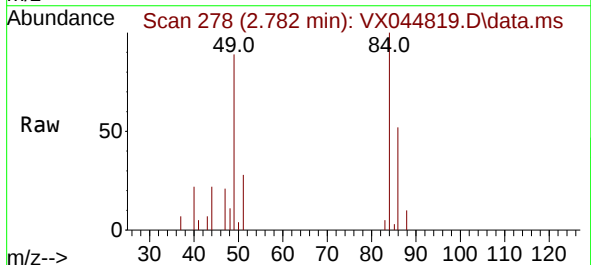


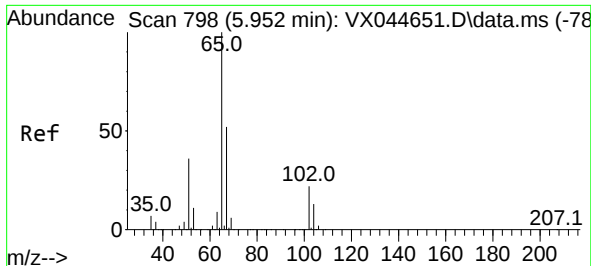

#33
 1,2-Dichloroethane-d4
 Concen: 47.253 ug/l
 RT: 5.952 min Scan# 798
 Delta R.T. 0.000 min
 Lab File: VX044819.D
 Acq: 03 Feb 2025 16:55




Instrument :
 MSVOA_X
 ClientSampleId :
 JPP-51.1-012925


Tgt Ion: 65 Resp: 82379
 Ion Ratio Lower Upper
 65 100
 67 55.1 0.0 103.4

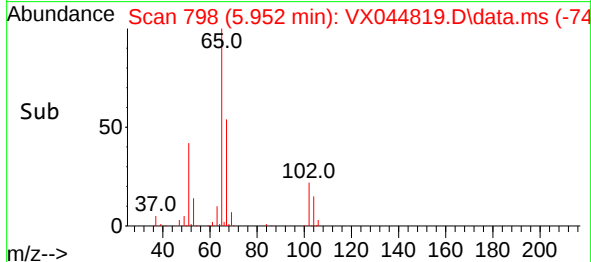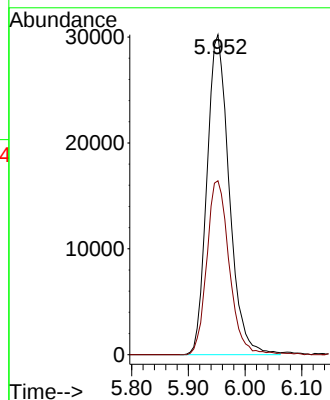

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.757 min Scan# 930
 Delta R.T. 0.000 min
 Lab File: VX044819.D
 Acq: 03 Feb 2025 16:55

Tgt Ion: 114 Resp: 232958
 Ion Ratio Lower Upper
 114 100
 63 20.3 0.0 43.0
 88 16.3 0.0 35.4


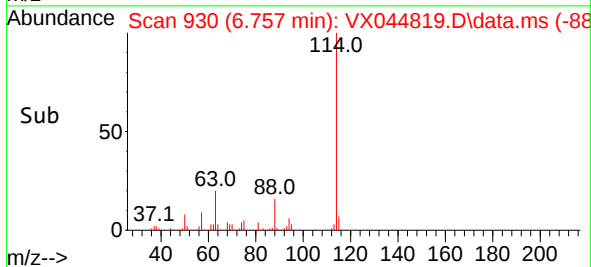
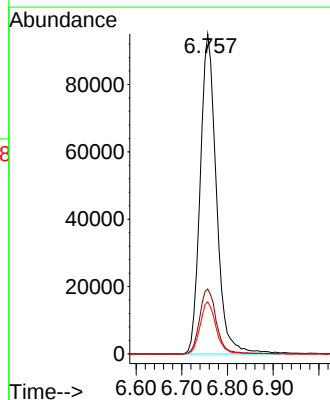
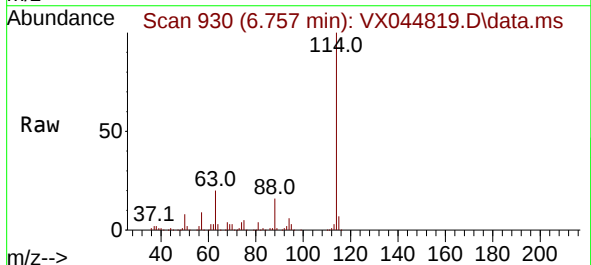


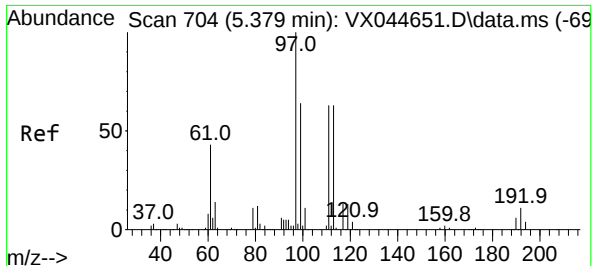

#35
Dibromofluoromethane
Concen: 49.109 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.000 min
Lab File: VX044819.D
Acq: 03 Feb 2025 16:55




Instrument :
MSVOA_X
ClientSampleId :
JPP-51.1-012925


Tgt Ion:113 Resp: 72678
Ion Ratio Lower Upper
113 100
111 102.7 81.6 122.4
192 17.3 14.4 21.6

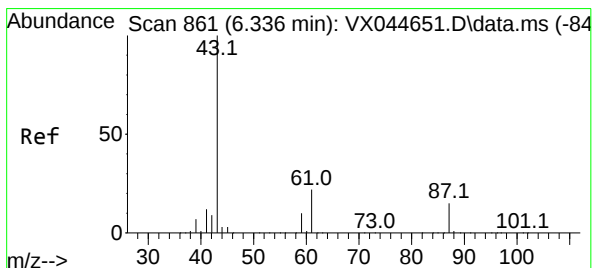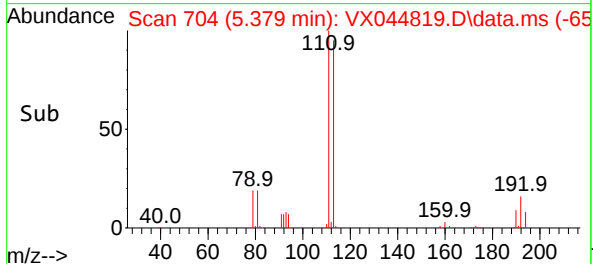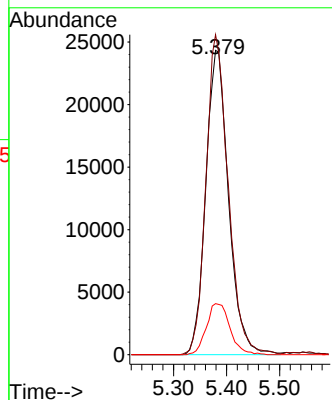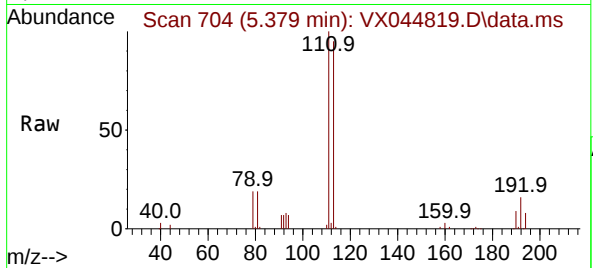

#43
Isopropyl Acetate
Concen: 27.880 ug/l
RT: 6.336 min Scan# 861
Delta R.T. -0.000 min
Lab File: VX044819.D
Acq: 03 Feb 2025 16:55

Tgt Ion: 43 Resp: 112520
Ion Ratio Lower Upper
43 100
61 20.5 16.6 24.8
87 13.0 11.0 16.6


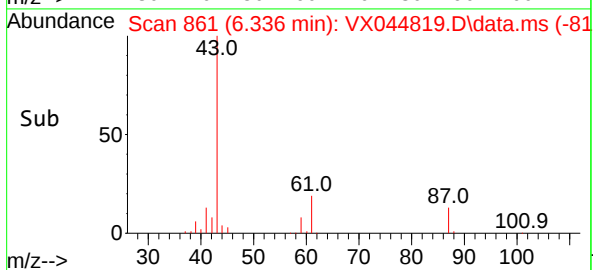
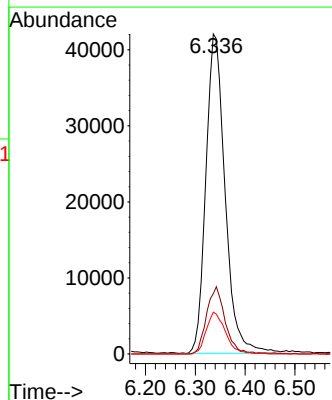
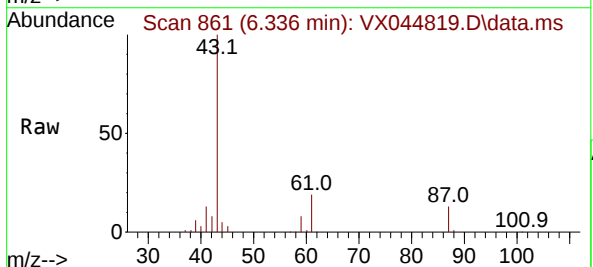


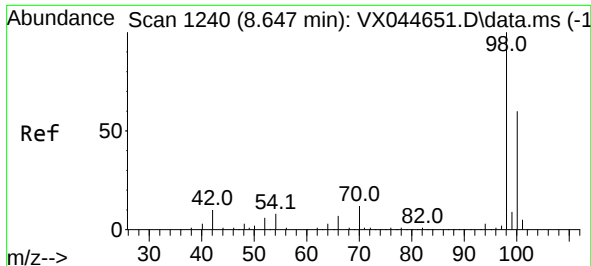

#50
Toluene-d8
Concen: 53.604 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX044819.D
Acq: 03 Feb 2025 16:55




Instrument :
MSVOA_X
ClientSampleId :
JPP-51.1-012925


Tgt Ion: 98 Resp: 276609
Ion Ratio Lower Upper
98 100
100 65.3 53.2 79.8

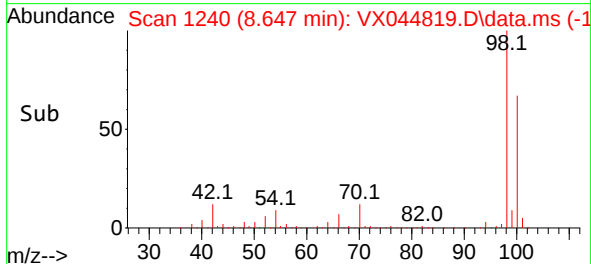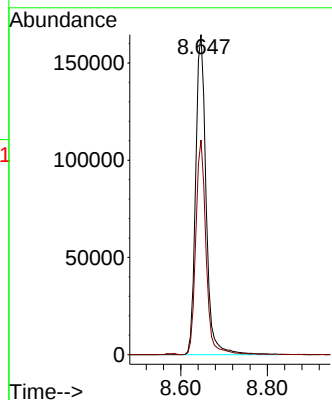

#62
4-Bromofluorobenzene
Concen: 48.867 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX044819.D
Acq: 03 Feb 2025 16:55

Tgt Ion: 95 Resp: 94005
Ion Ratio Lower Upper
95 100
174 71.5 0.0 133.0
176 69.1 0.0 129.4


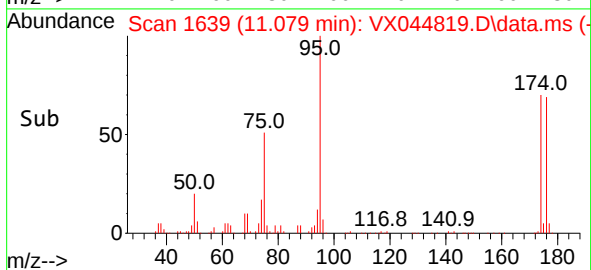
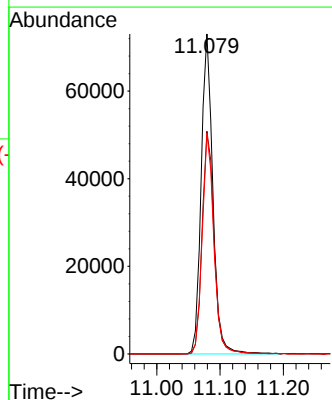
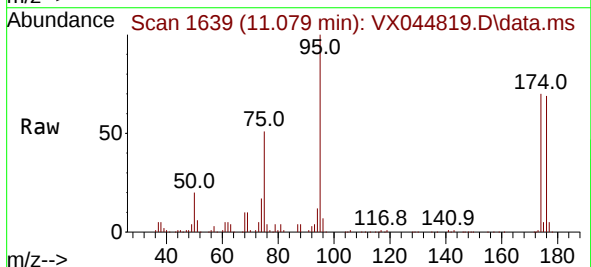


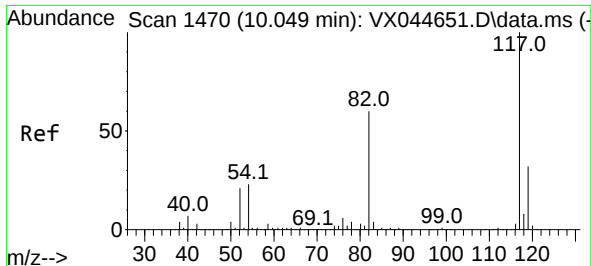

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. -0.000 min
Lab File: VX044819.D
Acq: 03 Feb 2025 16:55

Instrument :
MSVOA_X
ClientSampleId :
JPP-51.1-012925

Tgt Ion:117 Resp: 204621
Ion Ratio Lower Upper
117 100
82 57.0 47.6 71.4
119 31.9 25.4 38.2

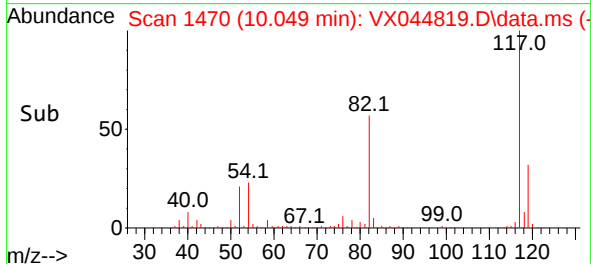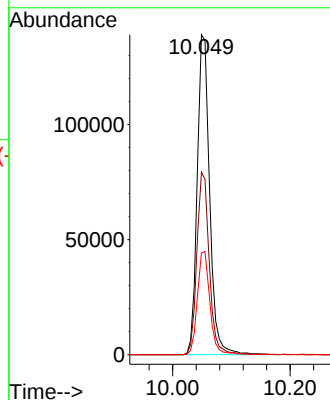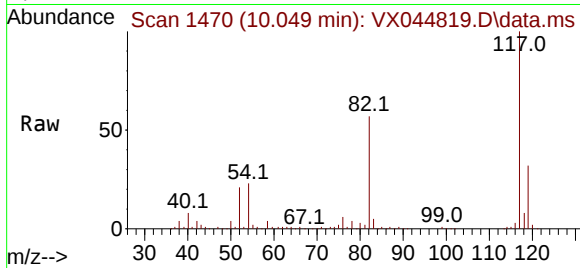

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. 0.000 min
Lab File: VX044819.D
Acq: 03 Feb 2025 16:55

Tgt Ion:152 Resp: 85623
Ion Ratio Lower Upper
152 100
115 60.9 43.8 131.4
150 155.7 0.0 347.8

