


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX020419\
 Data File : VX007349.D
 Acq On : 04 Feb 2019 10:08
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
 Title : SW846 8260
 Last Update : Sat Feb 02 01:32:36 2019

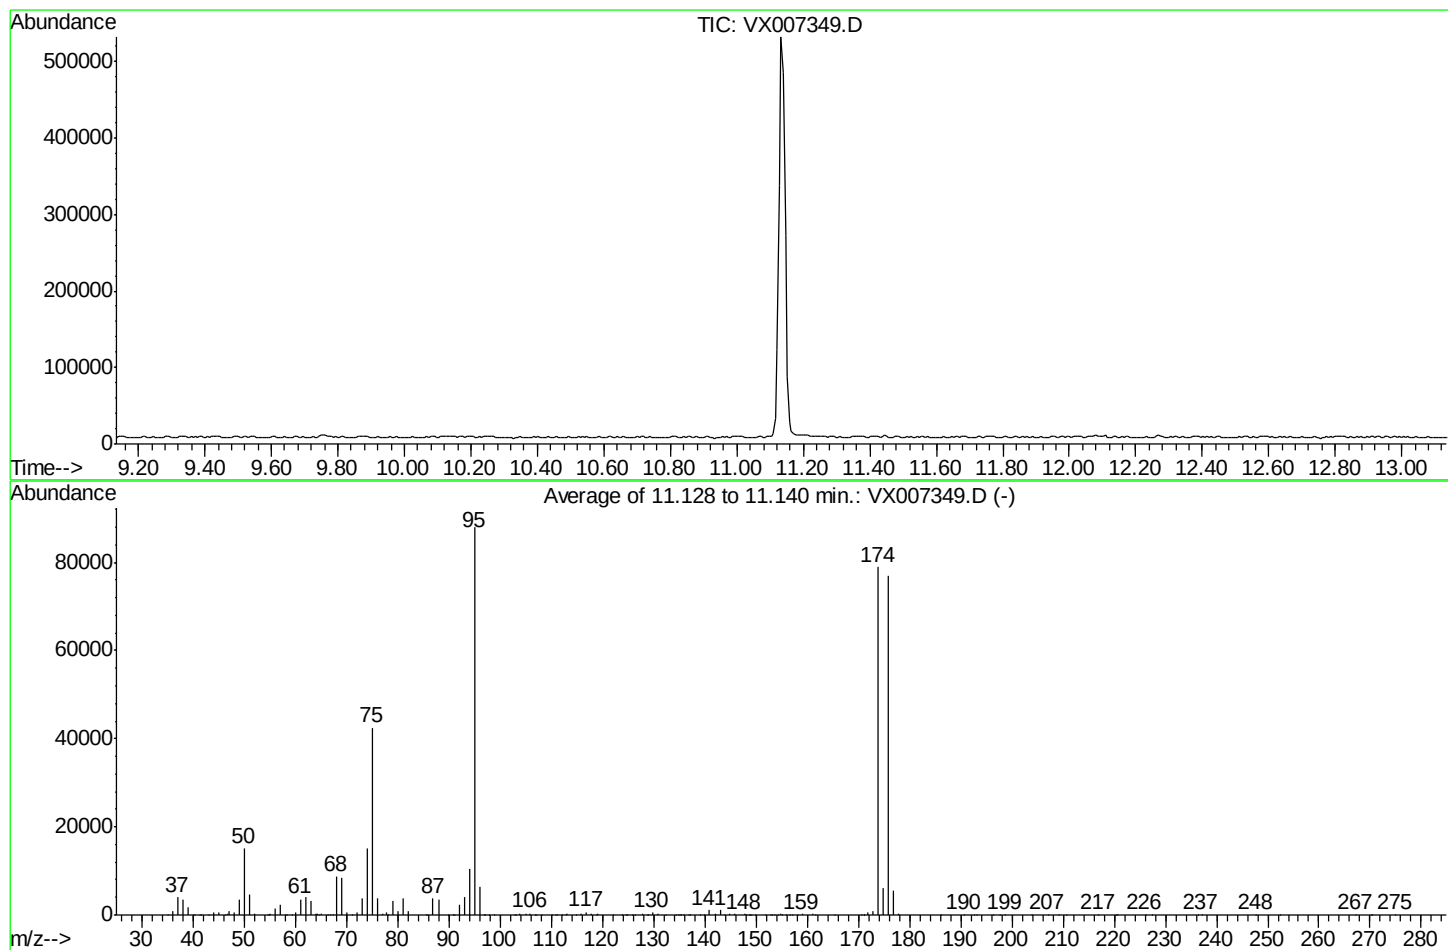

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	15010	PASS
75	95	30	60	48.3	42448	PASS
95	95	100	100	100.0	87954	PASS
96	95	5	9	7.2	6291	PASS
173	174	0.00	2	1.2	978	PASS
174	95	50	100	89.8	78962	PASS
175	174	5	9	7.6	6008	PASS
176	174	95	101	97.5	76970	PASS
177	176	5	9	7.2	5561	PASS