
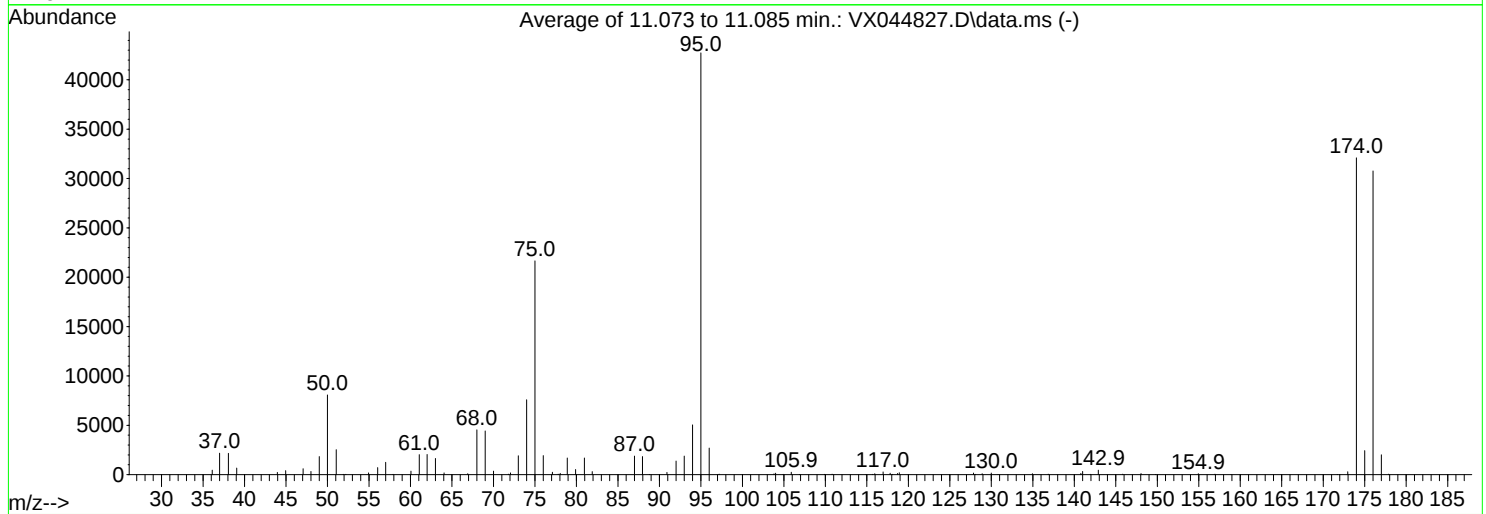


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020425\
Data File : VX044827.D
Acq On : 04 Feb 2025 07:53
Operator : JC/MD
Sample : BFB717
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB717

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
Title : VOC Analysis
Last Update : Mon Feb 03 07:31:09 2025

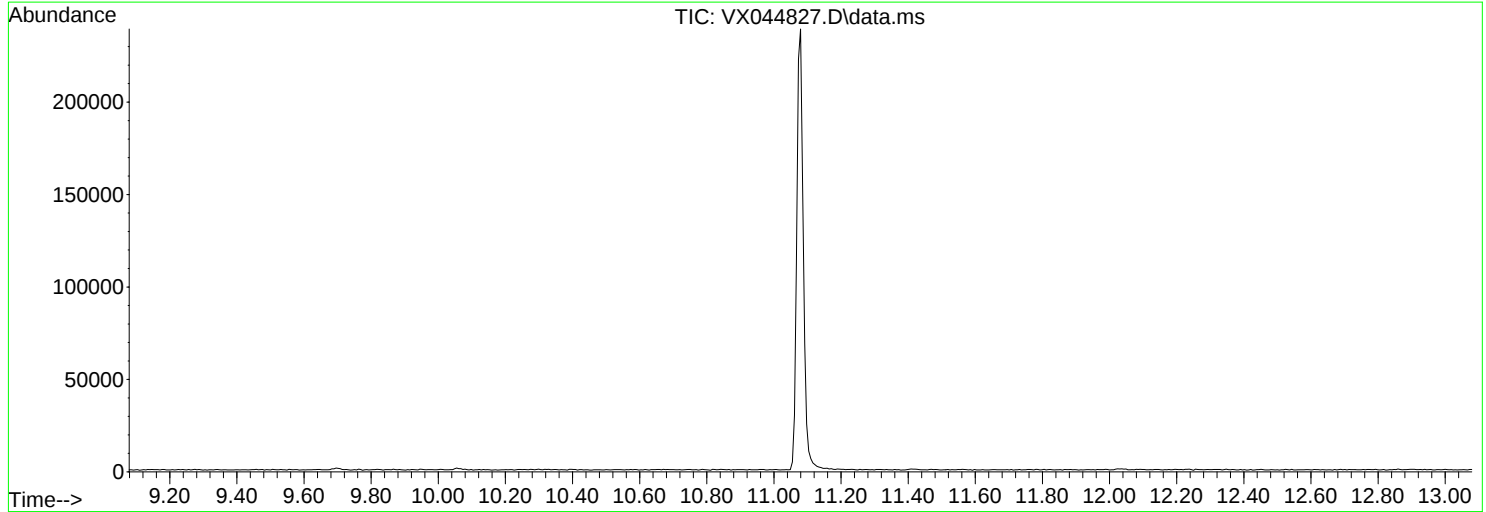

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.9	8067	PASS
75	95	30	80	50.7	21654	PASS
95	95	100	100	100.0	42731	PASS
96	95	5	9	6.3	2696	PASS
173	174	0.00	2	0.9	294	PASS
174	95	50	120	75.1	32096	PASS
175	174	5	9	7.6	2431	PASS
176	174	95	101	95.9	30768	PASS
177	176	5	9	6.6	2016	PASS

m/z	Abundance
39.10	62.0
40.00	725.0
43.90	460.0

Instrument :
MSVOA_X
ClientSampleId :
BFB717

m/z	Abundance
36.10	565.0
37.00	2594.0
38.10	2791.0
39.00	1010.0
40.00	788.0
44.10	831.0
44.90	405.0
47.00	767.0
48.10	291.0
49.00	2209.0
50.00	9488.0
51.00	3149.0
52.20	77.0
54.90	292.0
56.00	799.0
57.00	1340.0
60.10	448.0
61.10	2541.0
62.00	2557.0
63.00	1929.0
64.10	250.0
67.00	150.0
68.00	5281.0
69.00	5104.0
70.00	396.0
72.10	243.0
73.00	2153.0
74.00	9166.0
75.00	24264.0
76.00	2033.0
77.10	258.0
78.00	231.0
78.90	1997.0
80.00	667.0
80.90	1857.0
81.90	372.0
87.00	2108.0
87.90	2030.0
90.90	329.0
92.00	1451.0
93.00	2267.0
94.00	5500.0
95.00	48136.0
96.00	3110.0
97.20	63.0
103.80	259.0
104.90	99.0
105.90	247.0
106.90	57.0
110.80	53.0
114.90	55.0
115.70	113.0
116.90	292.0
117.80	130.0
118.70	343.0
127.90	147.0
128.90	94.0
130.00	162.0
130.80	74.0
135.00	110.0
136.80	80.0
140.80	376.0
141.90	52.0
142.90	436.0
145.80	83.0
148.10	116.0
155.00	87.0
157.00	57.0
172.00	56.0
173.00	244.0
174.00	30640.0
175.00	2570.0
176.00	29728.0
177.00	2031.0
177.90	97.0

Instrument :
MSVOA_X
ClientSampleId :
BFB717

m/z	Abundance
36.10	466.0
37.00	2421.0
38.00	2344.0
39.10	757.0
40.00	705.0
44.10	689.0
45.00	474.0
47.10	620.0
47.90	439.0
49.00	2089.0
50.00	9359.0
51.10	2817.0
51.90	92.0
55.00	99.0
56.10	841.0
57.00	1533.0
57.90	82.0
60.00	382.0
61.00	1931.0
62.00	2446.0
63.00	1765.0
64.00	199.0
66.80	103.0
68.00	5320.0
69.00	5257.0
70.00	432.0
72.00	278.0
73.00	2208.0
74.00	8407.0
75.00	25128.0
76.00	2437.0
77.10	357.0
78.10	156.0
78.90	2005.0
79.80	557.0
81.00	1884.0
81.90	388.0
87.00	2095.0
88.00	2220.0
90.80	234.0
92.00	1642.0
93.00	2048.0
94.00	5853.0
95.00	49344.0
96.00	3254.0
97.20	77.0
104.00	277.0
105.80	307.0
109.90	78.0
110.80	111.0
116.00	168.0
117.00	263.0
117.80	307.0
118.90	376.0
127.90	231.0
128.80	110.0
130.00	153.0
134.90	106.0
136.90	75.0
141.00	638.0
142.00	56.0
142.90	531.0
145.90	63.0
148.00	73.0
149.80	76.0
154.90	184.0
156.90	68.0
158.90	68.0
173.00	337.0
174.00	38504.0
175.00	2774.0
176.00	36680.0
177.00	2639.0
177.90	52.0

Instrument :
MSVOA_X
ClientSampleId :
BFB717

m/z	Abundance
36.10	325.0
37.00	1523.0
38.10	1325.0
39.10	436.0
40.00	756.0
44.00	540.0
44.90	317.0
47.00	418.0
47.90	241.0
49.00	1207.0
50.00	5353.0
51.00	1616.0
55.00	130.0
56.10	522.0
57.00	864.0
60.10	260.0
61.00	1610.0
62.00	1130.0
63.00	1198.0
64.10	68.0
66.90	62.0
68.00	3030.0
69.00	2896.0
70.00	234.0
71.80	156.0
73.00	1359.0
74.00	5188.0
75.00	15569.0
76.00	1318.0
77.10	124.0
77.80	149.0
78.90	1068.0
80.00	349.0
80.90	1302.0
81.80	167.0
87.00	1435.0
88.00	1264.0
88.80	68.0
91.00	129.0
92.00	1036.0
93.00	1341.0
94.00	3762.0
95.00	30712.0
96.00	1725.0
104.00	186.0
106.00	193.0
115.90	135.0
117.00	256.0
118.10	122.0
118.90	218.0
127.70	90.0
128.10	103.0
129.00	65.0
130.00	167.0
135.00	55.0
141.00	349.0
142.90	385.0
148.00	138.0
171.70	58.0
172.90	302.0
174.00	27144.0
175.00	1948.0
176.00	25896.0
177.00	1378.0

Instrument :
MSVOA_X
ClientSampleId :
BFB717