

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX020519\
Data File : VX007386.D
Acq On : 05 Feb 2019 19:24
Operator : JC/SP
Sample : K1380-04
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
KY038PS036-190204

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.288	19	22	32	rVB2	22288	41478	1.92%	0.344%
2	1.684	65	87	88	rBV3	69610	350787	16.27%	2.906%
3	2.800	268	270	276	rVB2	17435	25105	1.16%	0.208%
4	4.586	554	563	573	rBV	57964	159489	7.40%	1.321%
5	5.501	703	713	724	rBV	258161	725442	33.65%	6.010%
6	5.659	727	739	752	rVV2	439742	1223010	56.73%	10.132%
7	6.068	795	806	816	rBV	266343	696584	32.31%	5.771%
8	6.860	926	936	946	rBV	653843	1524352	70.70%	12.628%
9	8.713	1232	1240	1253	rBV	1380920	2155956	100.00%	17.861%
10	10.116	1464	1470	1482	rVB	1293292	1830446	84.90%	15.164%
11	11.140	1631	1638	1648	rBV	1160005	1477293	68.52%	12.238%
12	12.079	1784	1792	1801	rBV	1514010	1861096	86.32%	15.418%


Sum of corrected areas: 12071038

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX020519\
Data File : VX007386.D
Acq On : 05 Feb 2019 19:24
Operator : JC/SP
Sample : K1380-04
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
KY038PS036-190204

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

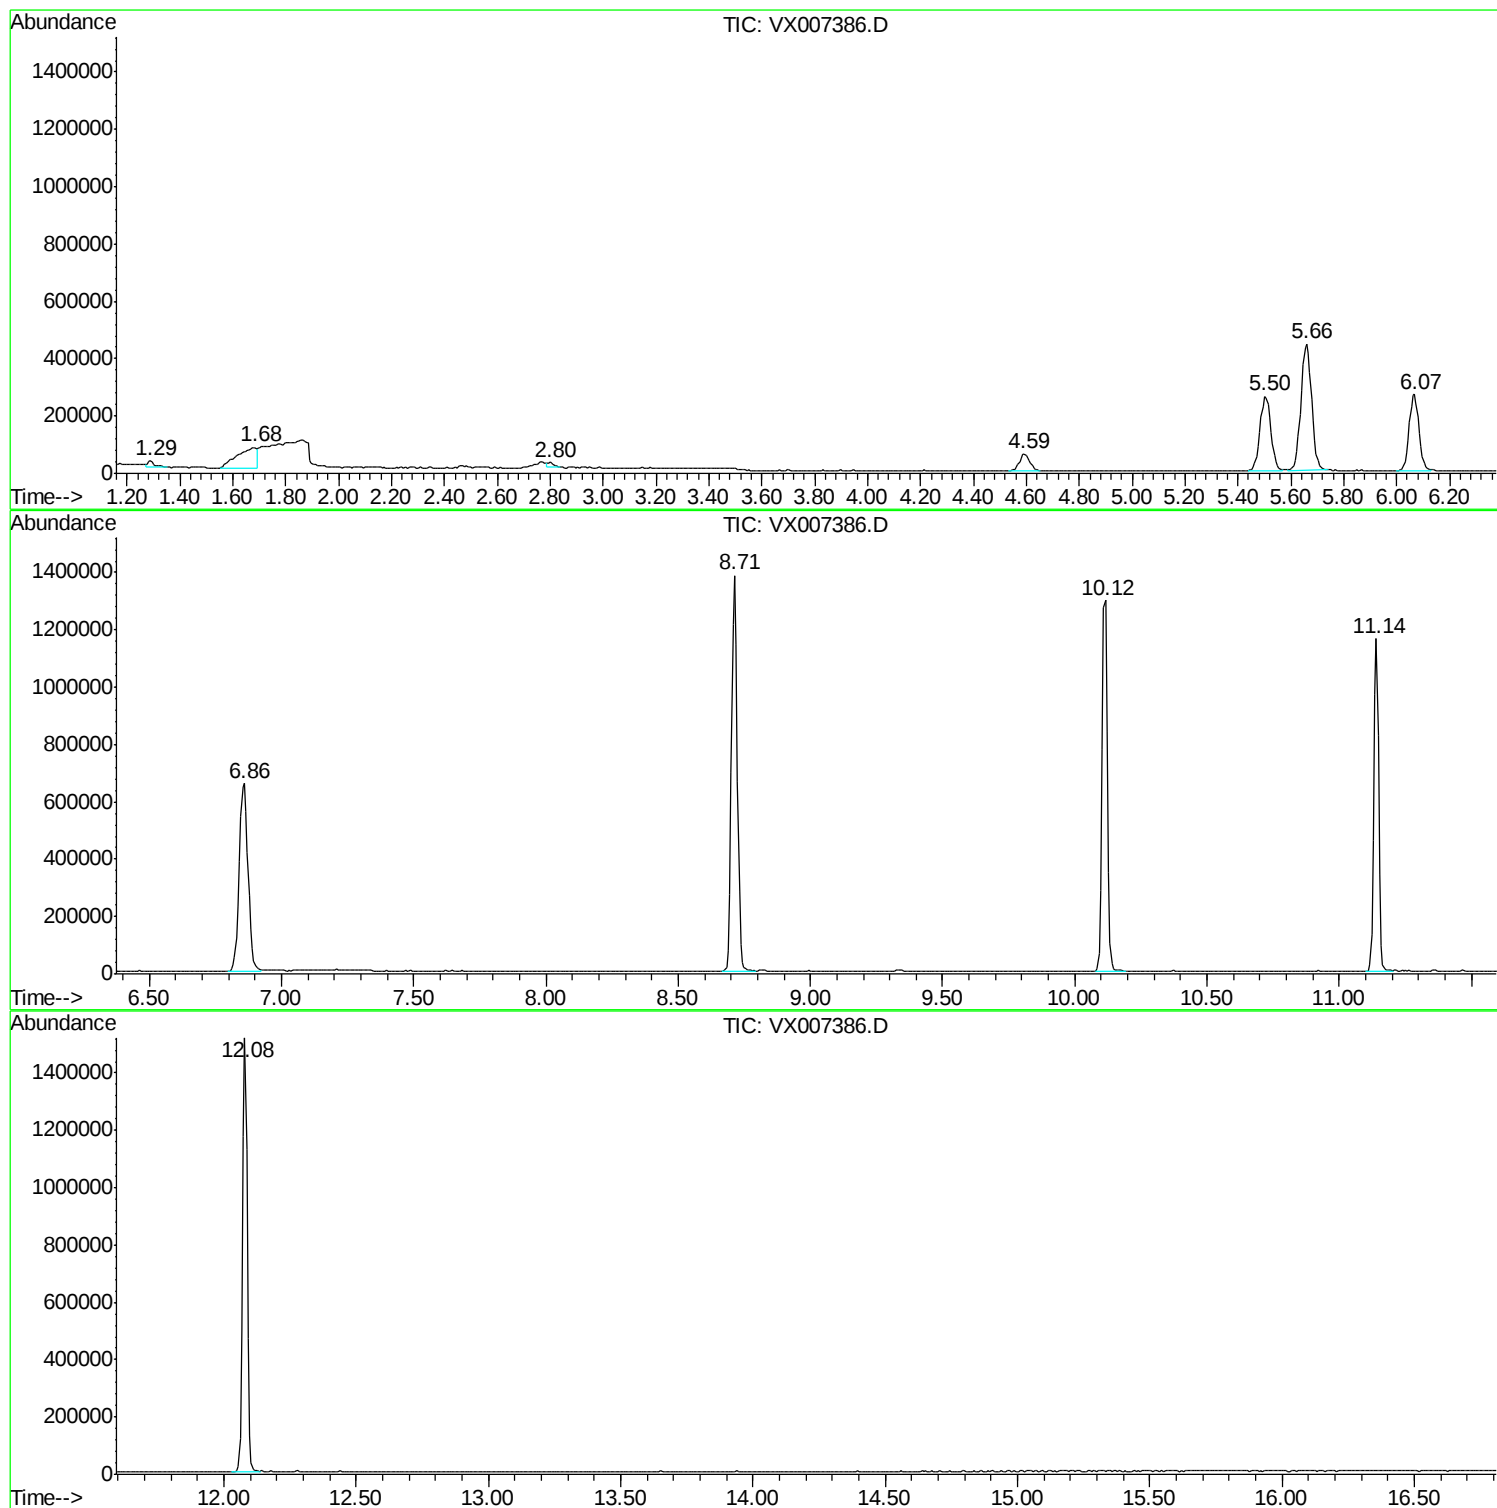

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX020519\
Data File : VX007386.D
Acq On : 05 Feb 2019 19:24
Operator : JC/SP
Sample : K1380-04
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
KY038PS036-190204










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown1.68 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.68	14.34 ug/l	350787	Pentafluorobenzene	5.66

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Oxalyl chloride	126	C2Cl2O2	000079-37-8	17
2		Ethane, 1,1-dichloro-	98	C2H4Cl2	000075-34-3	12
3		Bis(2-chloroethyl) sulfone	190	C4H8Cl2O2S	000471-03-4	12
4		1,3-Dioxonane, 5,5,6,6,7,7,8,8-o...	274	C7H6F8O2	036301-47-0	12
5		Silane, bis(fluoromethyl)dimethyl-	124	C4H10F2Si	065864-63-3	9

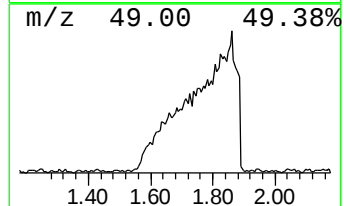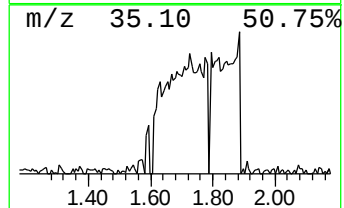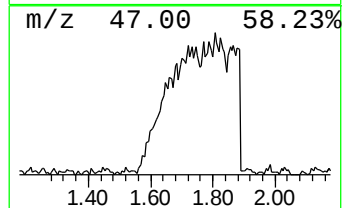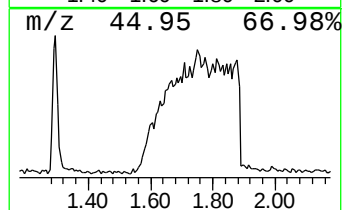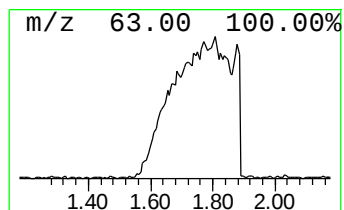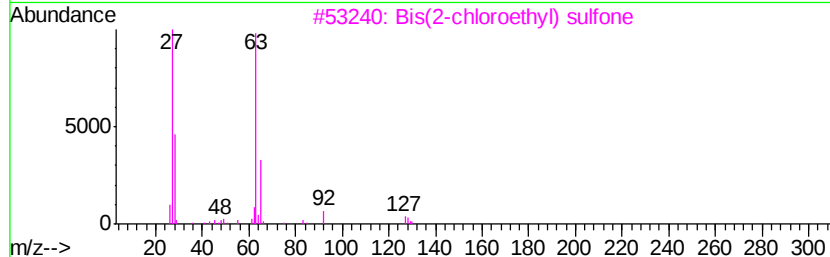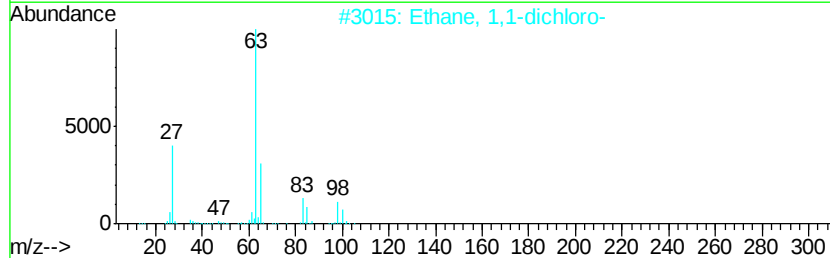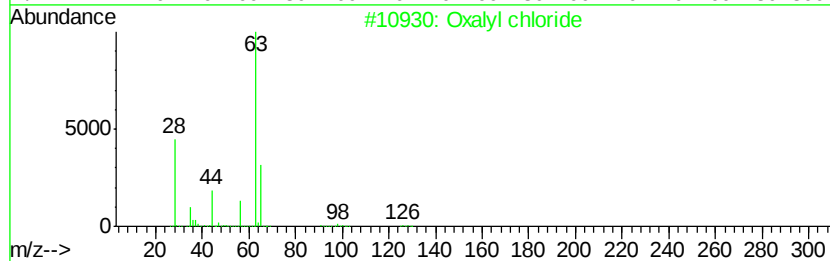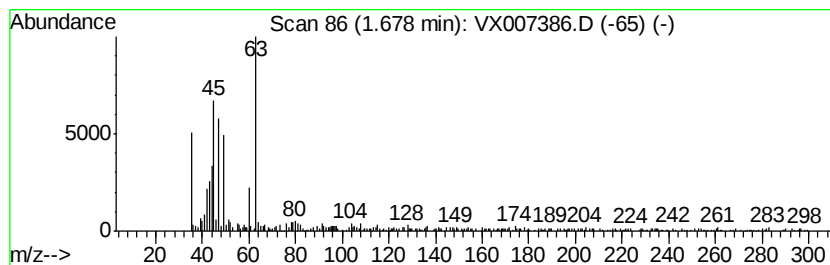

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX020519\
Data File : VX007386.D
Acq On : 05 Feb 2019 19:24
Operator : JC/SP
Sample : K1380-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
KY038PS036-190204

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown1.68	1.68	14.3	ug/l	350787	1	5.66	1223010	50.0