

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX020519\
 Data File : VX007387.D
 Acq On : 05 Feb 2019 19:51
 Operator : JC/SP
 Sample : K1380-05
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 KY038PS038-190204

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.678	64	86	87	rBV5	71735	342588	15.98%	2.892%
2	2.763	254	264	268	rBV	19858	53821	2.51%	0.454%
3	5.501	699	713	726	rBV	254418	723812	33.76%	6.110%
4	5.659	728	739	754	rVB	441600	1226636	57.22%	10.355%
5	6.068	795	806	820	rVB	268282	701782	32.73%	5.924%
6	6.854	925	935	947	rBV	658107	1547856	72.20%	13.067%
7	8.713	1233	1240	1252	rBV	1404948	2143904	100.00%	18.099%
8	10.116	1464	1470	1480	rBV	1304330	1817880	84.79%	15.347%
9	11.140	1630	1638	1645	rBV	1119969	1456905	67.96%	12.299%
10	12.079	1785	1792	1798	rBV	1471933	1830347	85.37%	15.452%


Sum of corrected areas: 11845531

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX020519\
Data File : VX007387.D
Acq On : 05 Feb 2019 19:51
Operator : JC/SP
Sample : K1380-05
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
KY038PS038-190204

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

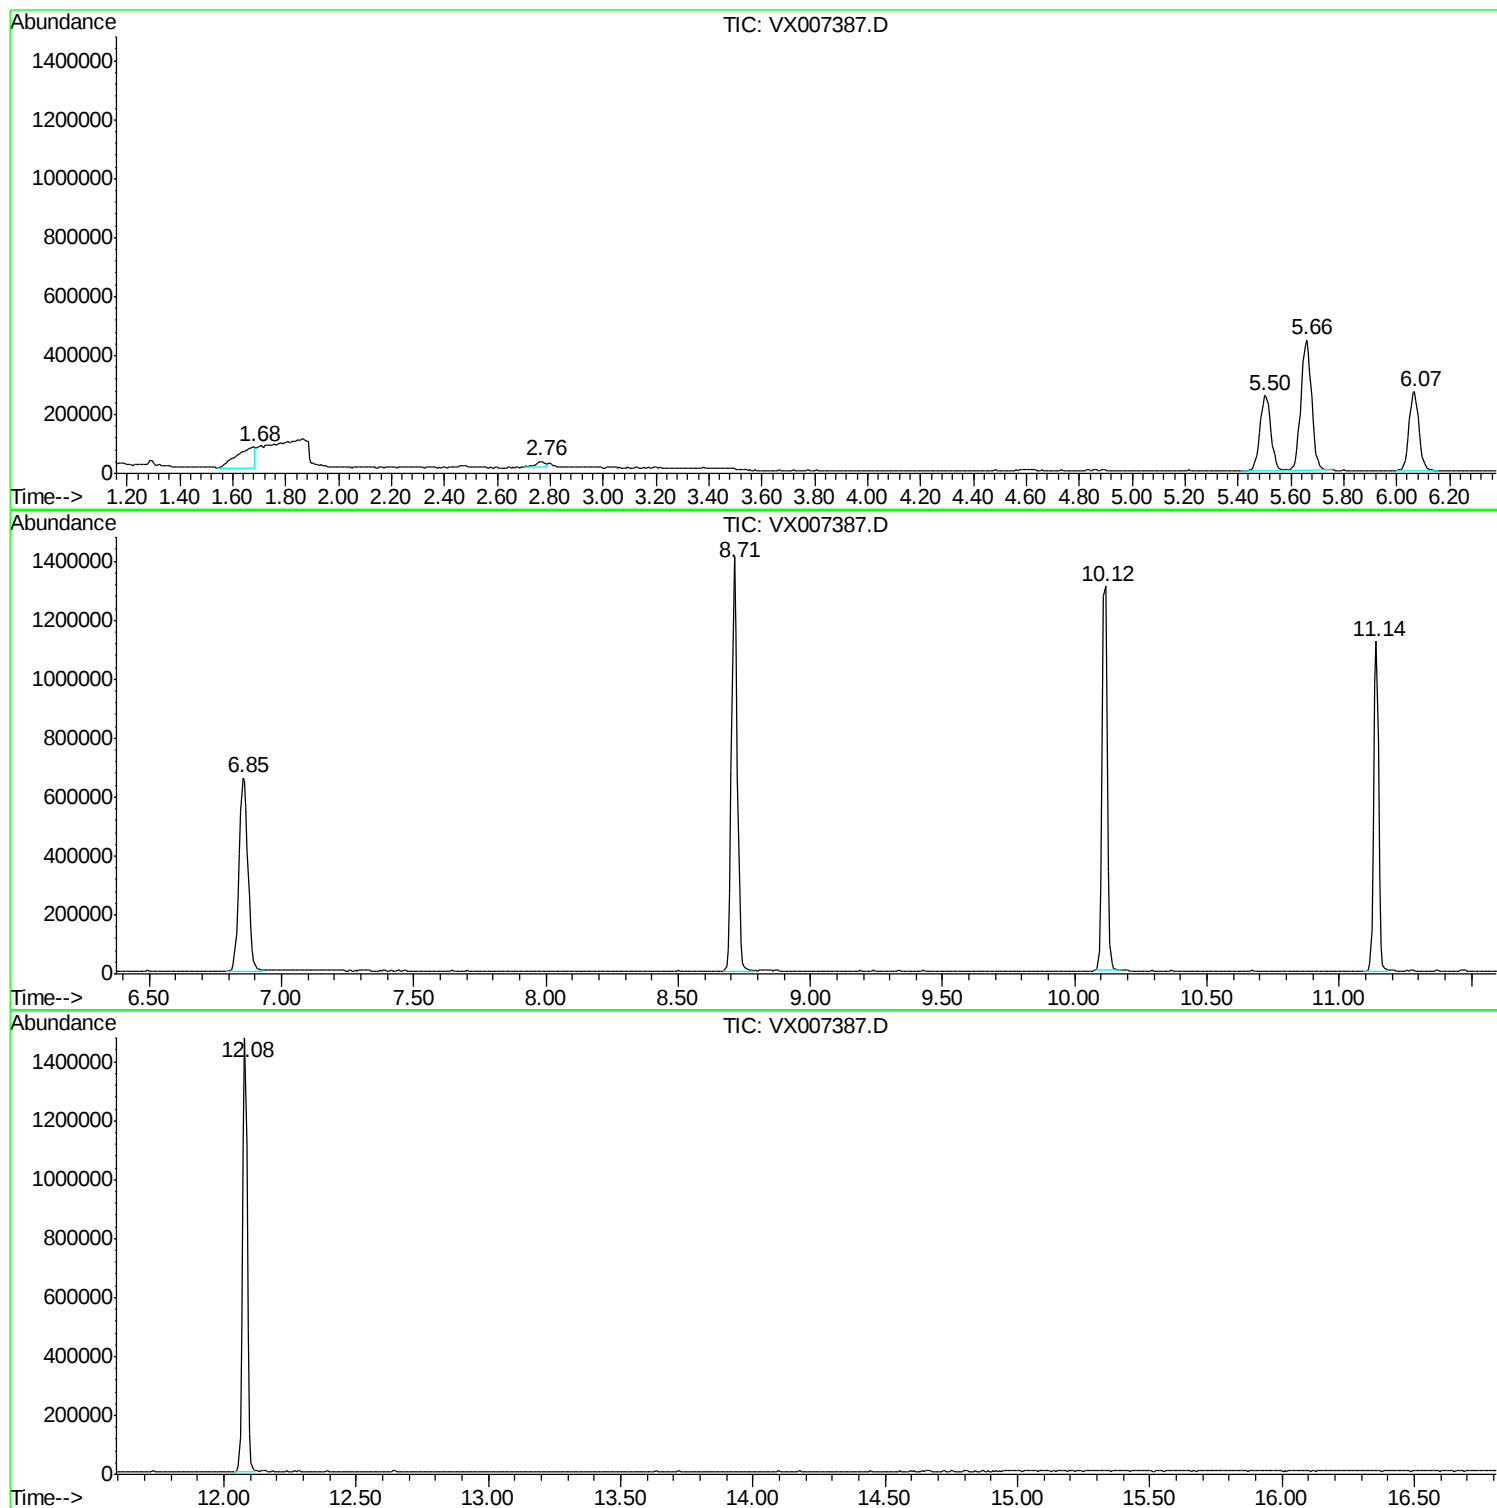

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX020519\
Data File : VX007387.D
Acq On : 05 Feb 2019 19:51
Operator : JC/SP
Sample : K1380-05
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 24 Sample Multiplier: 1










Instrument :
MSVOA_X
ClientSampleId :
KY038PS038-190204

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown1.68 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.		
1.68	13.96 ug/l	342588	Pentafluorobenzene	5.66		
Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Ethene, (2-chloroethoxy)-	106	C4H7ClO	000110-75-8	25	
2	Isopropylthiophosphondiamide	138	C3H11N2PS	1000306-03-6	17	
3	Oxalyl chloride	126	C2Cl2O2	000079-37-8	12	
4	1-Chloroethyl sulfone	190	C4H8Cl2O2S	010038-07-0	12	
5	1,3-Dioxocane, 5,5,6,6,7,7-hexaf...	224	C6H6F6O2	036301-46-9	9	

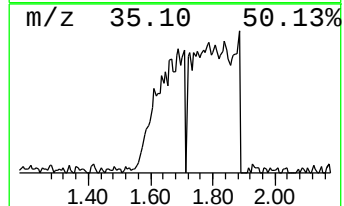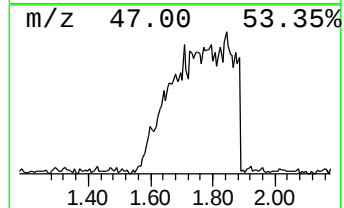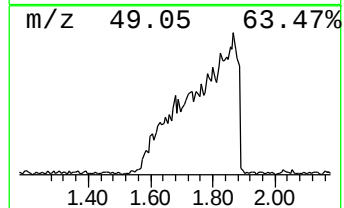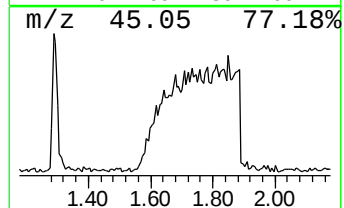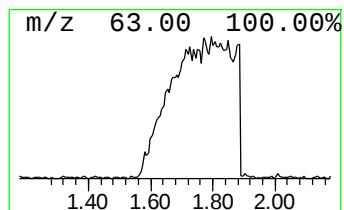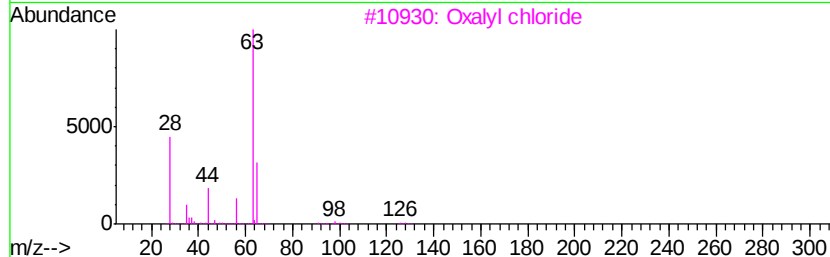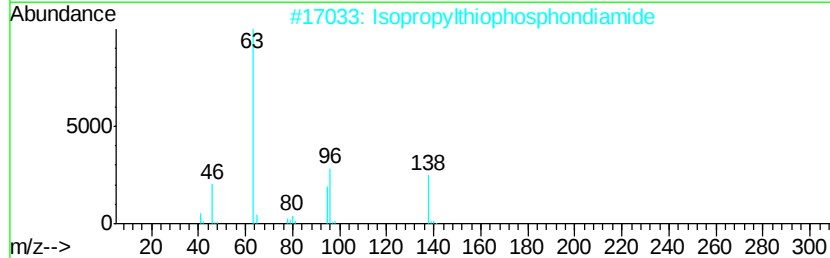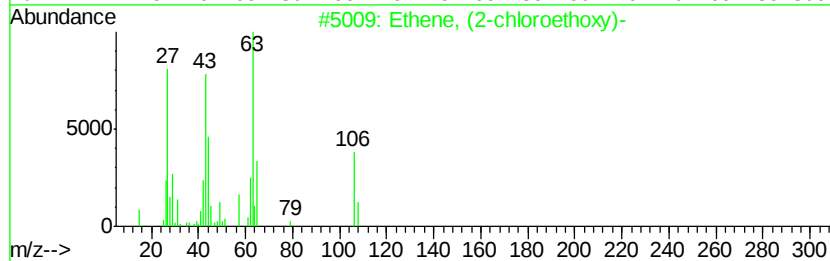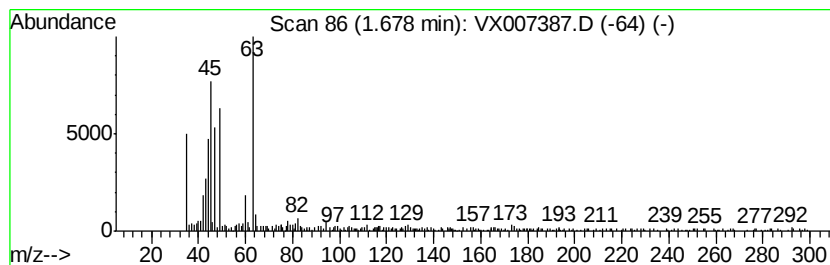

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX020519\
Data File : VX007387.D
Acq On : 05 Feb 2019 19:51
Operator : JC/SP
Sample : K1380-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
KY038PS038-190204

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown1.68	1.68	14.0	ug/l	342588	1	5.66	1226640	50.0