


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX020519\
Data File : VX007364.D
Acq On : 05 Feb 2019 09:08
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
Title : SW846 8260
Last Update : Sat Feb 02 01:32:36 2019

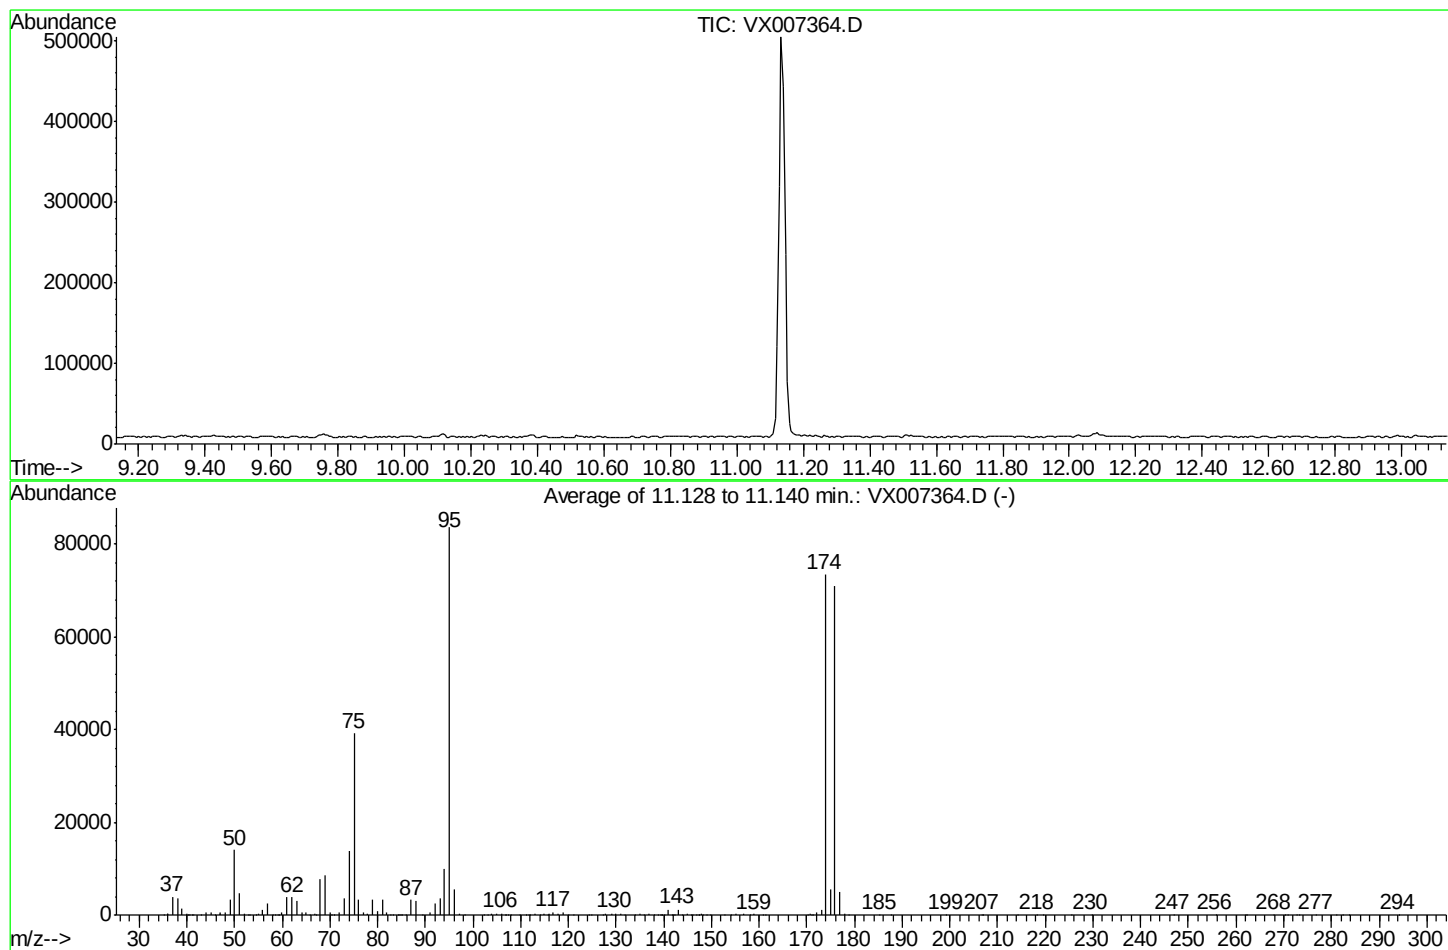

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1627

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	13955	PASS
75	95	30	60	46.8	39085	PASS
95	95	100	100	100.0	83568	PASS
96	95	5	9	6.6	5500	PASS
173	174	0.00	2	1.5	1074	PASS
174	95	50	100	87.7	73293	PASS
175	174	5	9	7.5	5500	PASS
176	174	95	101	96.8	70960	PASS
177	176	5	9	7.2	5085	PASS