

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX020520\
 Data File : VX014813.D
 Acq On : 05 Feb 2020 11:16
 Operator : JC/SP
 Sample : VX0205WBL01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0205WBL01

Quant Time: Feb 06 03:42:13 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA X\METHOD\624X011520W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Wed Jan 15 12:41:12 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.00	128	70928	30.00	ug/l	0.00
28) 1,4-Difluorobenzene	6.85	114	374840	30.00	ug/l	0.00
57) Chlorobenzene-d5	10.10	117	335522	30.00	ug/l	0.00

System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	6.04	65	159441	31.98	ug/l	0.00
Spiked Amount	30.000	Range	50 - 169	Recovery	=	106.60%
60) 4-Bromofluorobenzene	11.13	95	140440	26.16	ug/l	0.00
Spiked Amount	30.000	Range	56 - 143	Recovery	=	87.20%
63) Toluene-d8	8.71	98	447957	29.56	ug/l	0.00
Spiked Amount	30.000	Range	66 - 137	Recovery	=	98.53%


Target Compounds	Ovalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX020520\
Data File : VX014813.D
Acq On : 05 Feb 2020 11:16
Operator : JC/SP
Sample : VX0205WBL01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0205WBL01

Quant Time: Feb 06 03:42:13 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA X\METHOD\624X011520W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Wed Jan 15 12:41:12 2020
Response via : Initial Calibration

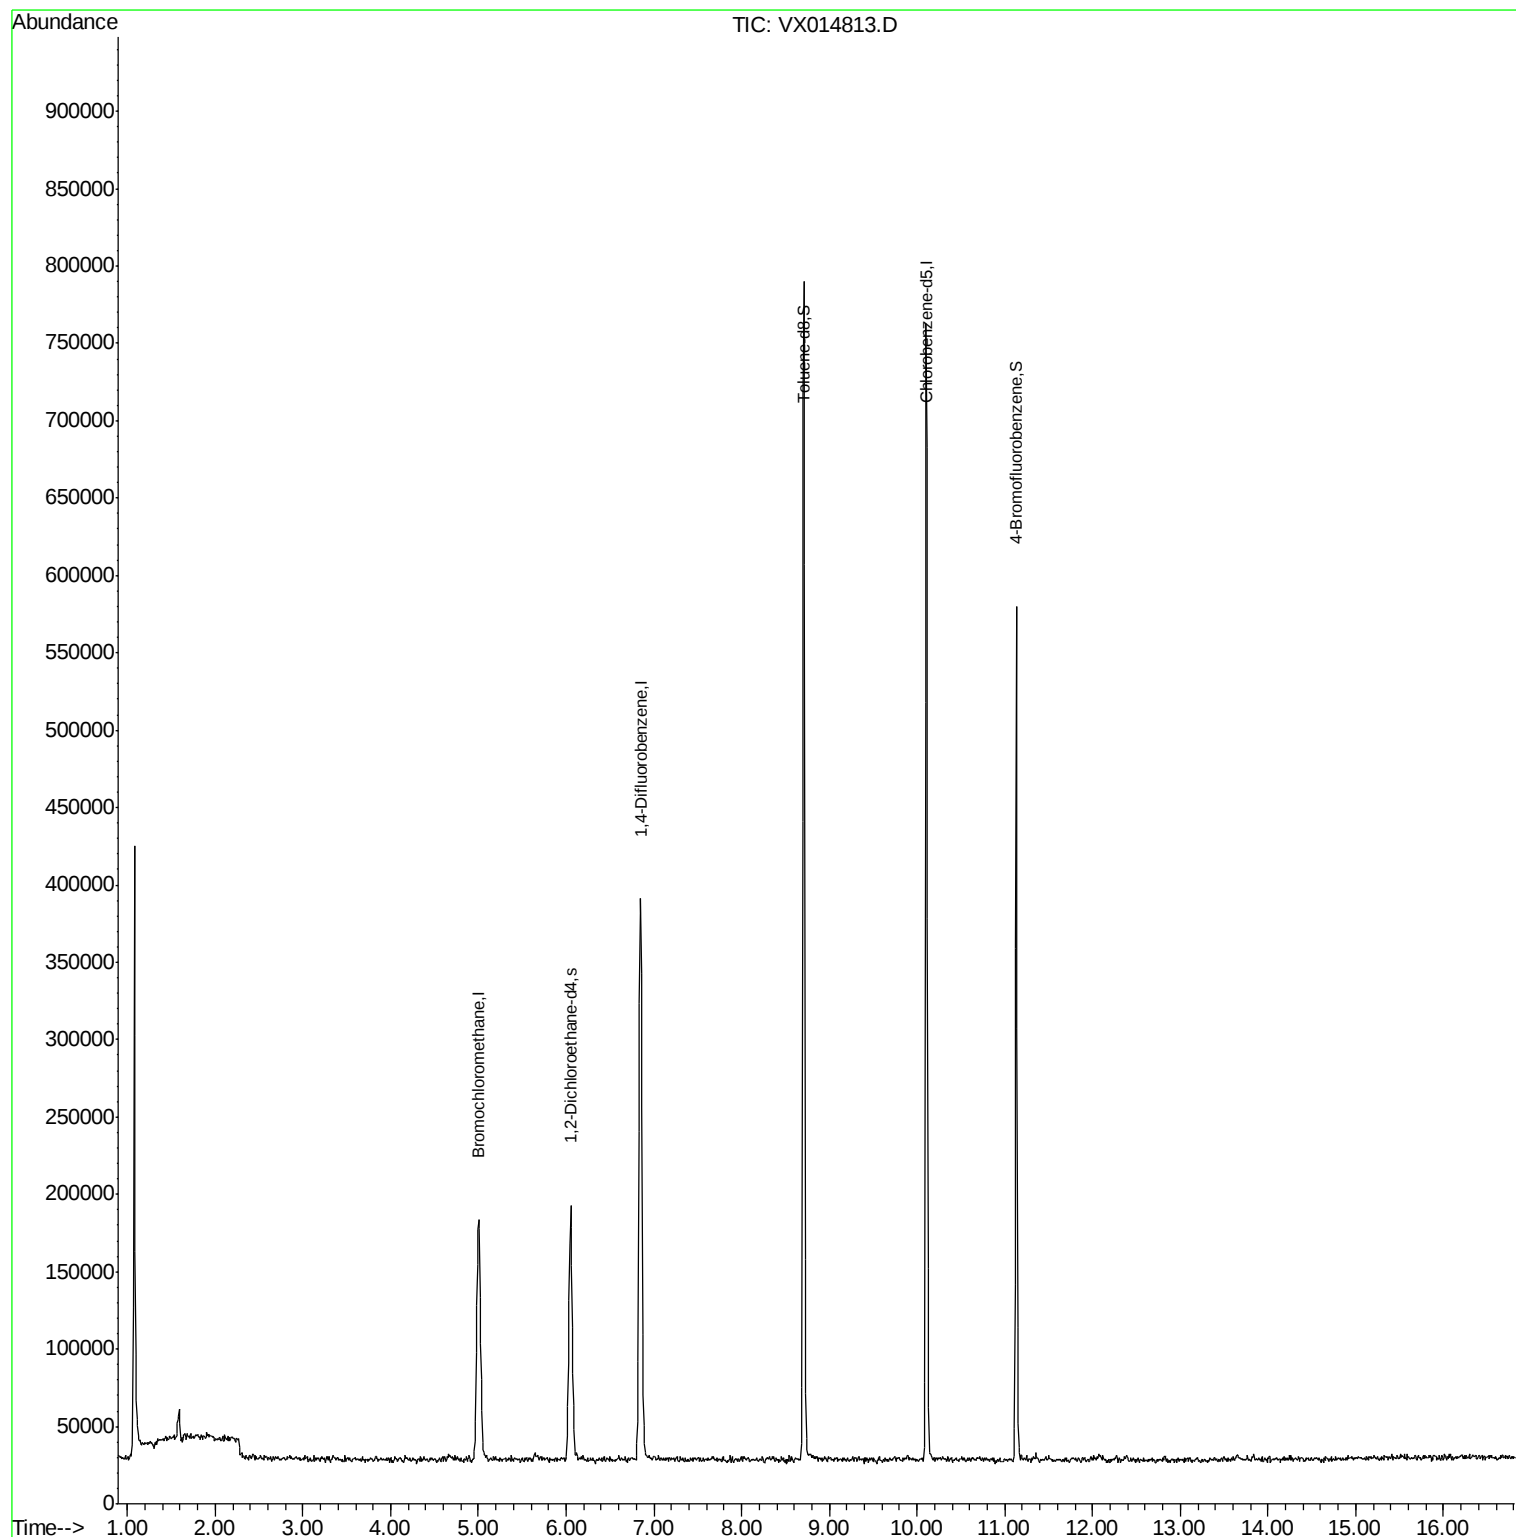

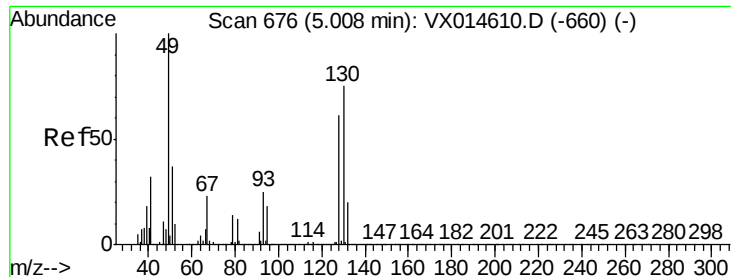

#1

Bromochloromethane

Concen: 30.000 ug/l

RT: 5.00 min Scan# 675

Delta R.T. -0.00 min

Lab File: VX014813.D

Acq: 05 Feb 2020 11:16

Instrument :

MSVOA_X

ClientSampleId :

VX0205WBL01


Tot Ion:128 Resp: 70928

Ion Ratio Lower Upper

128 100

49 160.1 0.0 405.0




130 130.3 0.0 321.5

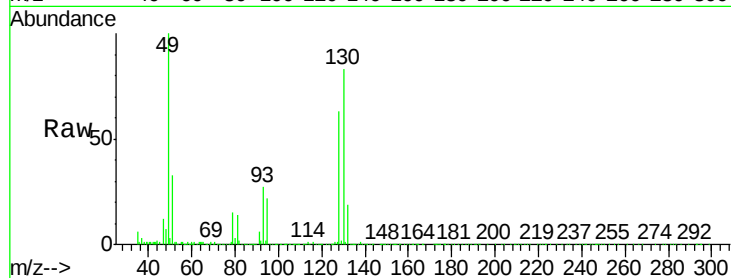

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 49.00 (48.70 to 49.70): VX0

Ion 130.00 (129.70 to 130.70): V

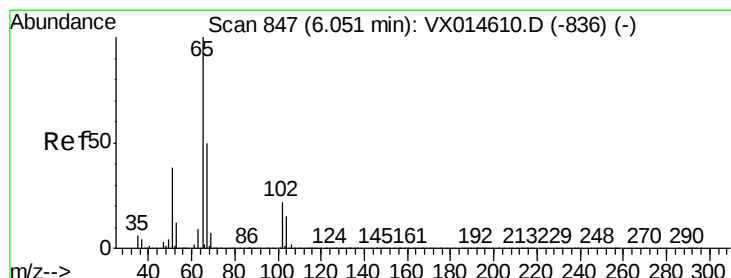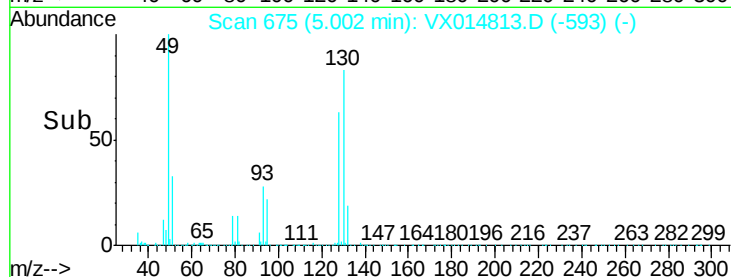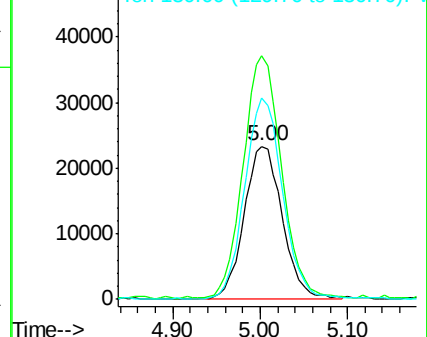

#27

1,2-Dichloroethane-d4

Concen: 31.981 ug/l

RT: 6.04 min Scan# 846

Delta R.T. -0.01 min

Lab File: VX014813.D


Acq: 05 Feb 2020 11:16

Tgt Ion: 65 Resp: 159441

Ion Ratio Lower Upper



65 100


67 52.5 43.1 64.7

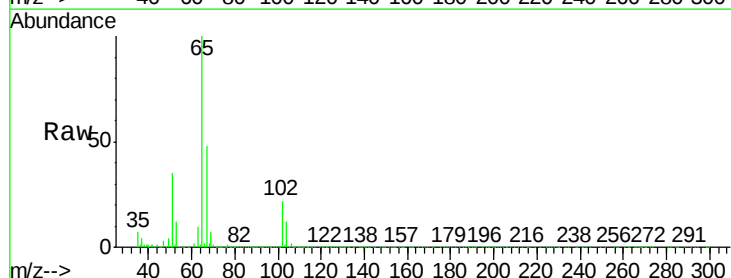

Abundance Ion 65.00 (64.70 to 65.70): VX0

Ion 67.00 (66.70 to 67.70): VX0

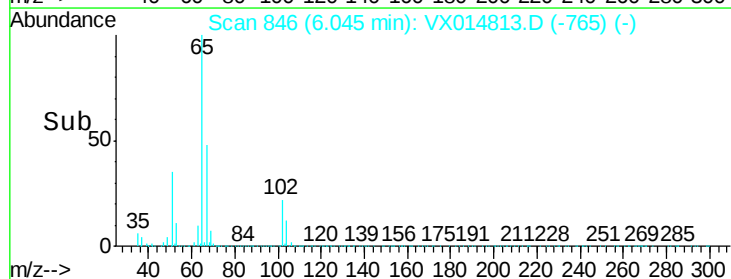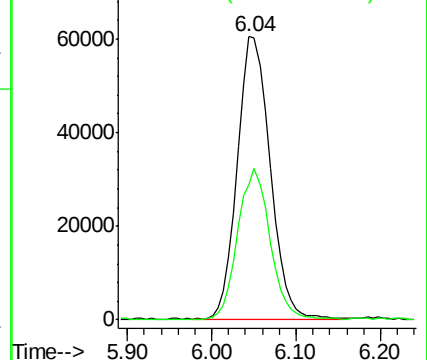

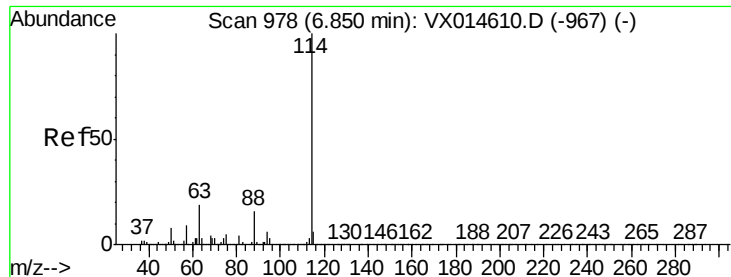

#28

1,4-Difluorobenzene

Concen: 30.000 ug/l

RT: 6.85 min Scan# 978

Delta R.T. -0.00 min

Lab File: VX014813.D

Acq: 05 Feb 2020 11:16

Instrument :

MSVOA_X

ClientSampleId :

VX0205WBL01


Tot Ion:114 Resp: 374840

Ion Ratio Lower Upper

114 100

63 20.8 16.1 24.1




88 15.6 12.5 18.7

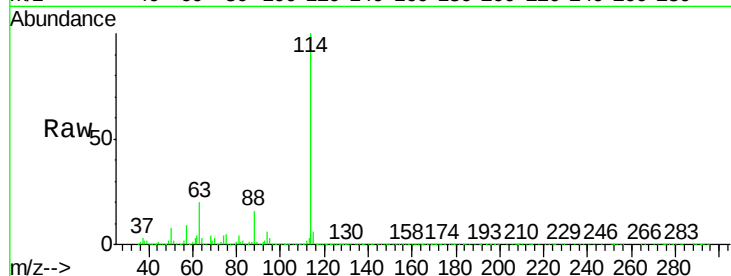

Abundance Ion 114.00 (113.70 to 114.70): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 88.00 (87.70 to 88.70): VX0

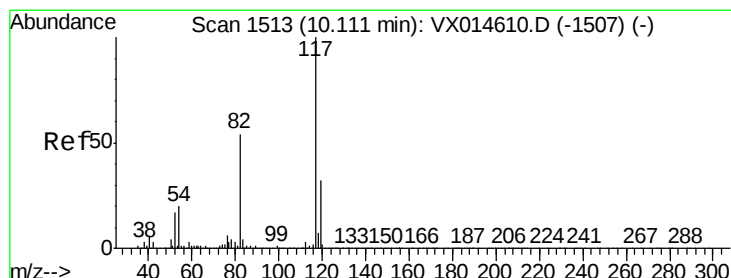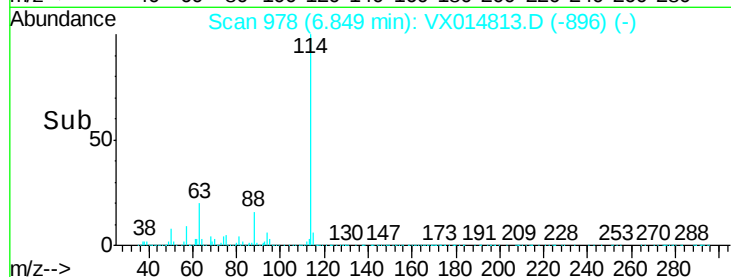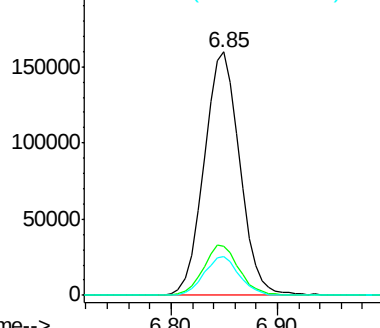

#57

Chlorobenzene-d5

Concen: 30.000 ug/l

RT: 10.10 min Scan# 1512

Delta R.T. -0.01 min

Lab File: VX014813.D

Acq: 05 Feb 2020 11:16


Tgt Ion:117 Resp: 335522

Ion Ratio Lower Upper

117 100

82 53.3 43.8 65.6



119 31.7 25.8 38.6

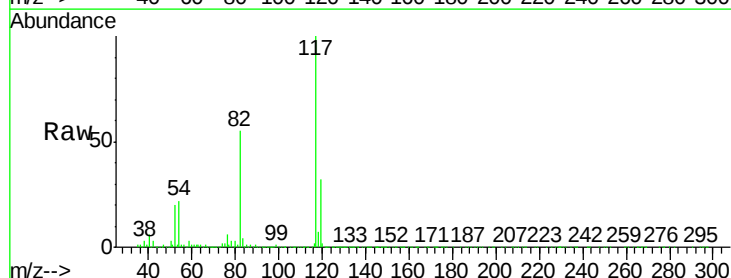


Abundance Ion 117.00 (116.70 to 117.70): V

Ion 82.00 (81.70 to 82.70): VX0

Ion 119.00 (118.70 to 119.70): V



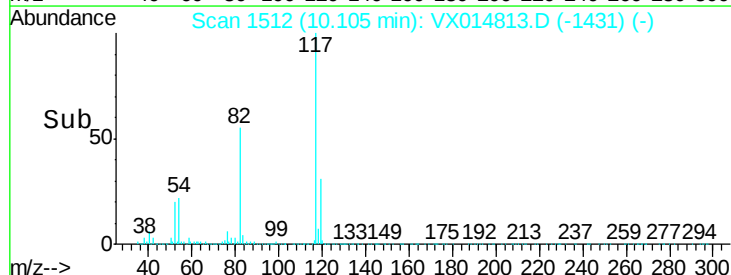
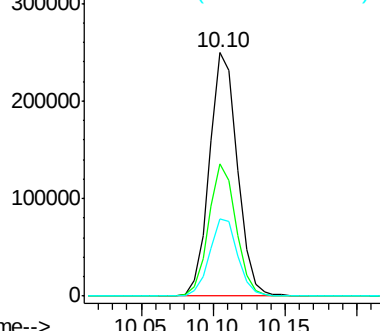


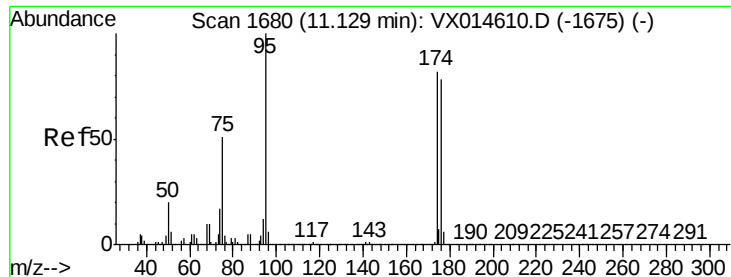

#60
4-Bromofluorobenzene
Concen: 26.157 ug/l
RT: 11.13 min Scan# 1680
Delta R.T. -0.00 min
Lab File: VX014813.D
Acq: 05 Feb 2020 11:16

Instrument :
MSVOA_X
ClientSampled :
VX0205WBL01

Tot Ion	Ratio	Lower	Upper
95	100		
174	90.9	70.2	105.2
176	87.3	68.3	102.5

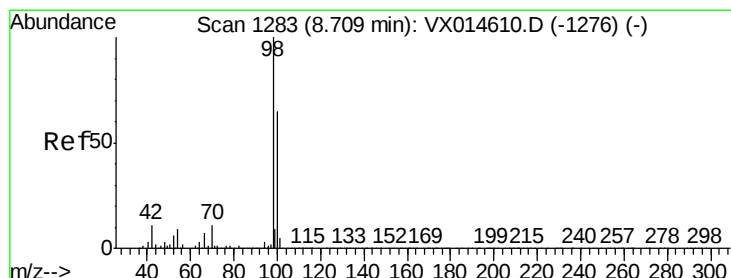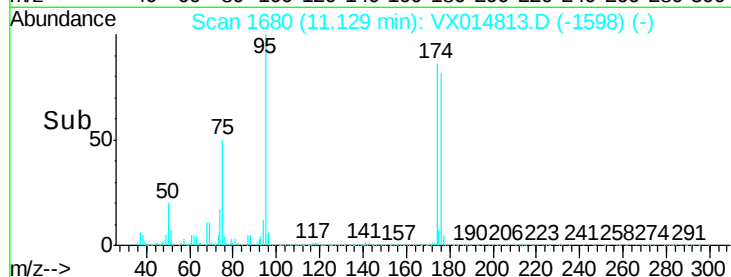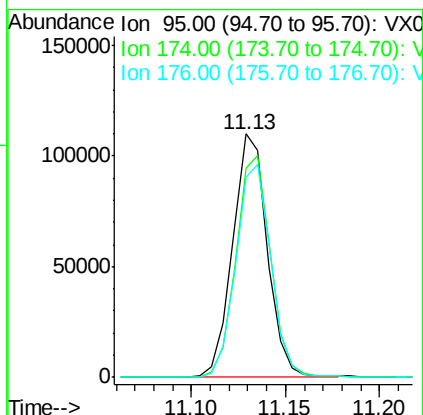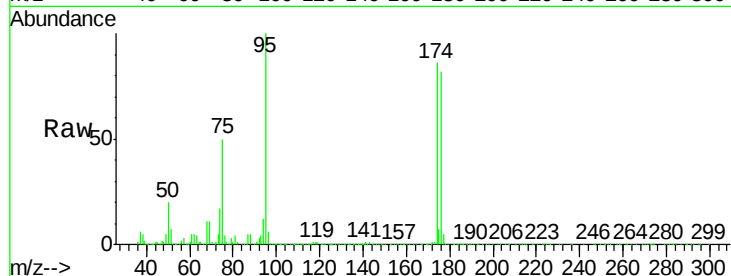

#63
Toluene-d8
Concen: 29.558 ug/l
RT: 8.71 min Scan# 1283
Delta R.T. -0.00 min
Lab File: VX014813.D
Acq: 05 Feb 2020 11:16

Tgt Ion	Ratio	Lower	Upper
98	100		
100	65.2	52.2	78.2

