

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX020520\
 Data File : VX014823.D
 Acq On : 05 Feb 2020 15:31
 Operator : JC/SP
 Sample : L1377-05
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BW-209

Quant Time: Feb 06 03:54:53 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA X\METHOD\624X011520W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Wed Jan 15 12:41:12 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.01	128	67160	30.00	ug/l	0.00
28) 1,4-Difluorobenzene	6.85	114	357027	30.00	ug/l	0.00
57) Chlorobenzene-d5	10.11	117	319390	30.00	ug/l	0.00

System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	6.05	65	144308	30.57	ug/l	0.00
Spiked Amount	30.000	Range	50 - 169	Recovery	=	101.90%
60) 4-Bromofluorobenzene	11.13	95	139615	27.32	ug/l	0.00
Spiked Amount	30.000	Range	56 - 143	Recovery	=	91.07%
63) Toluene-d8	8.71	98	425664	29.51	ug/l	0.00
Spiked Amount	30.000	Range	66 - 137	Recovery	=	98.37%


Target Compounds	Ovalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX020520\
Data File : VX014823.D
Acq On : 05 Feb 2020 15:31
Operator : JC/SP
Sample : L1377-05
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BW-209

Quant Time: Feb 06 03:54:53 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA X\METHOD\624X011520W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Wed Jan 15 12:41:12 2020
Response via : Initial Calibration

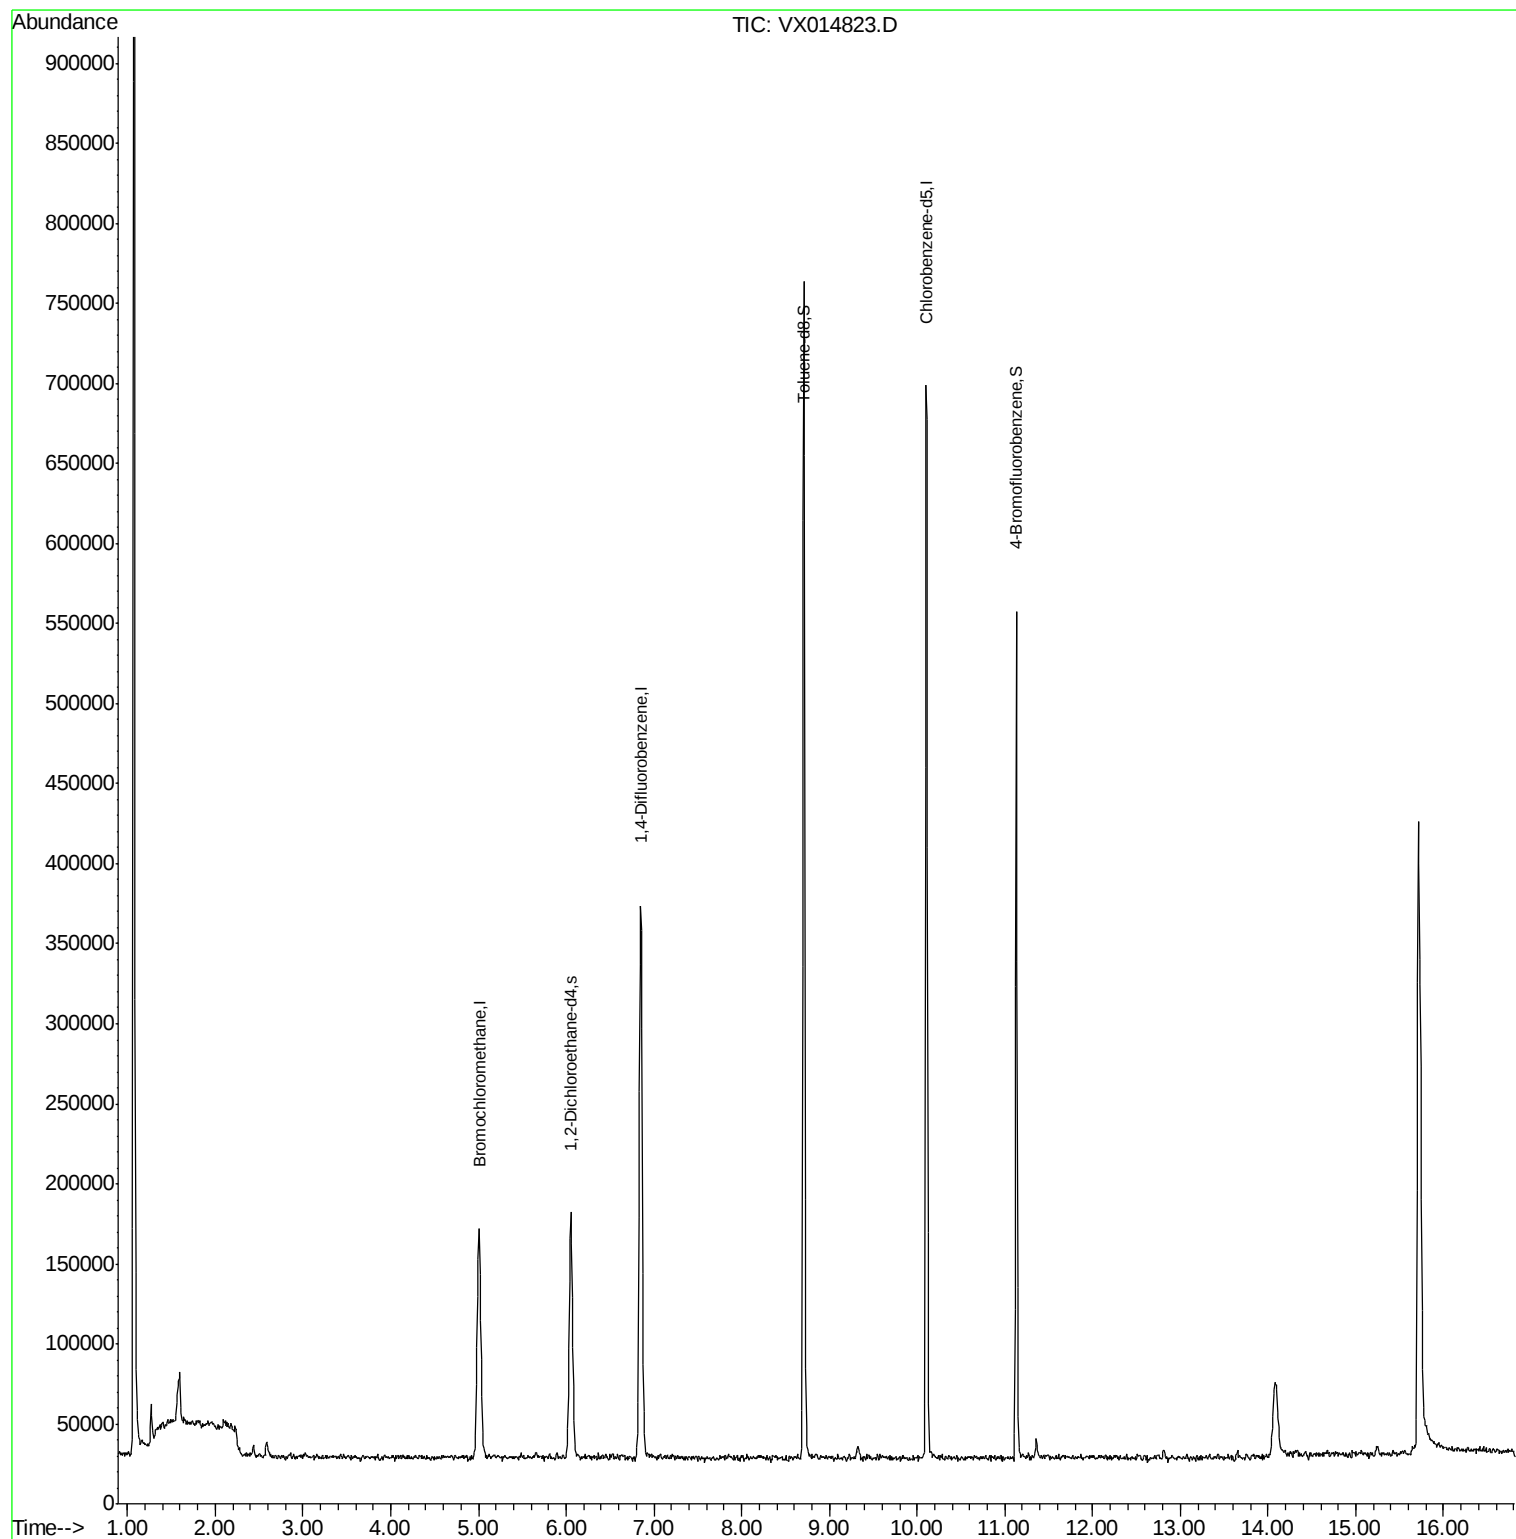

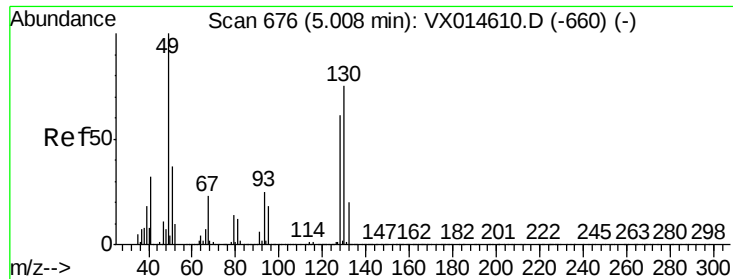

#1

Bromochloromethane

Concen: 30.000 ug/l

RT: 5.01 min Scan# 676

Delta R.T. 0.01 min

Lab File: VX014823.D

Acq: 05 Feb 2020 15:31

Instrument :

MSVOA_X

ClientSampleId :

BW-209


Tot Ion:128 Resp: 67160

Ion Ratio Lower Upper

128 100

49 153.0 0.0 405.0




130 126.5 0.0 321.5

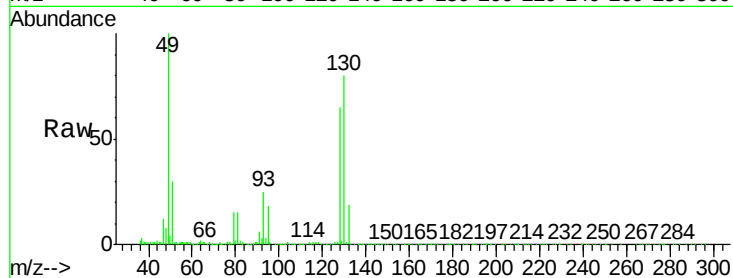

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 49.00 (48.70 to 49.70): VX0

Ion 130.00 (129.70 to 130.70): V

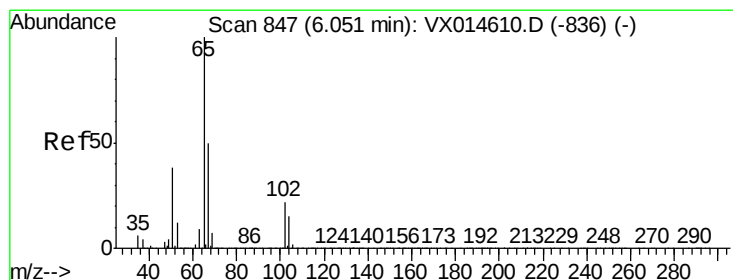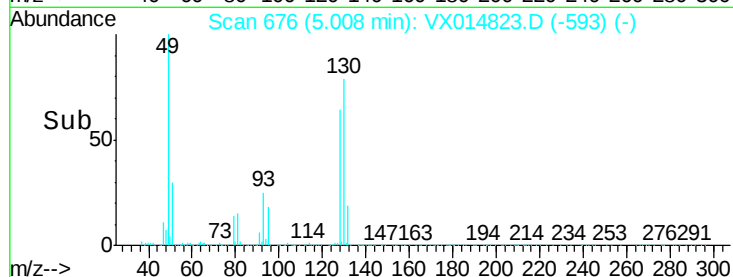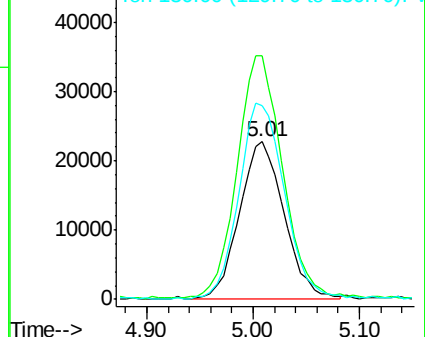

#27

1,2-Dichloroethane-d4

Concen: 30.570 ug/l

RT: 6.05 min Scan# 847

Delta R.T. 0.00 min

Lab File: VX014823.D


Acq: 05 Feb 2020 15:31

Tgt Ion: 65 Resp: 144308

Ion Ratio Lower Upper



65 100


67 53.3 43.1 64.7

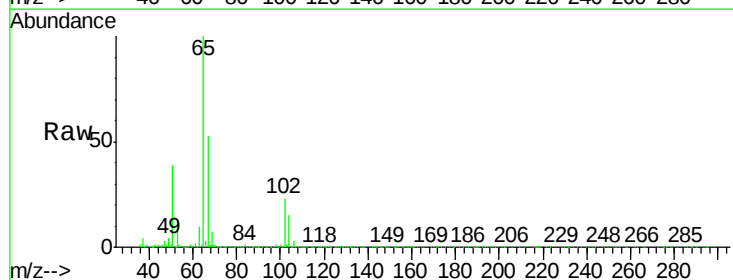

Abundance Ion 65.00 (64.70 to 65.70): VX0

Ion 67.00 (66.70 to 67.70): VX0



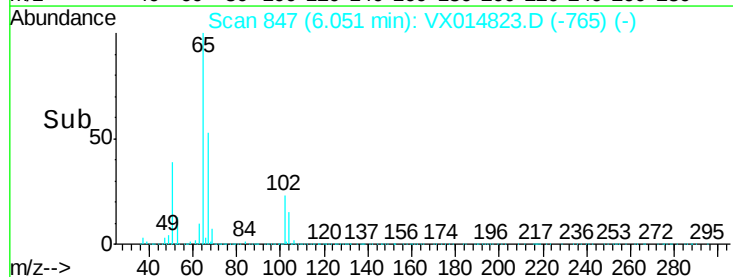
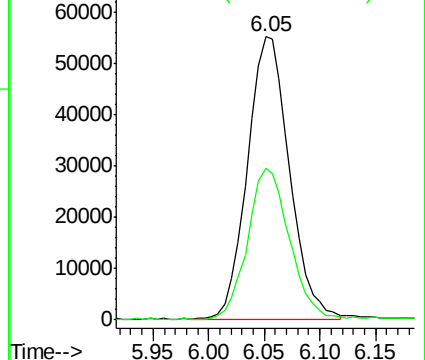


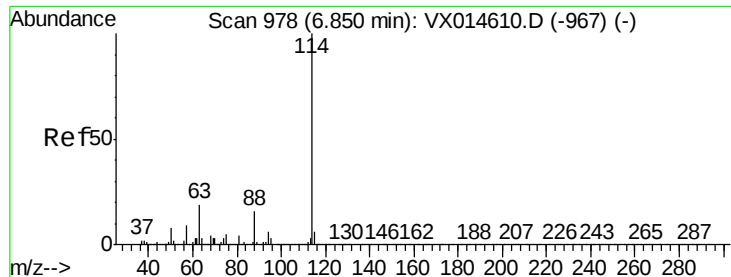

#28
 1,4-Difluorobenzene
 Concen: 30.000 ug/l
 RT: 6.85 min Scan# 978
 Delta R.T. 0.00 min
 Lab File: VX014823.D
 Acq: 05 Feb 2020 15:31




Instrument :
 MSVOA_X
 ClientSampleId :
 BW-209


Tot Ion:	114	Resp:	357027
Ion	Ratio	Lower	Upper
114	100		
63	20.5	16.1	24.1
88	15.4	12.5	18.7

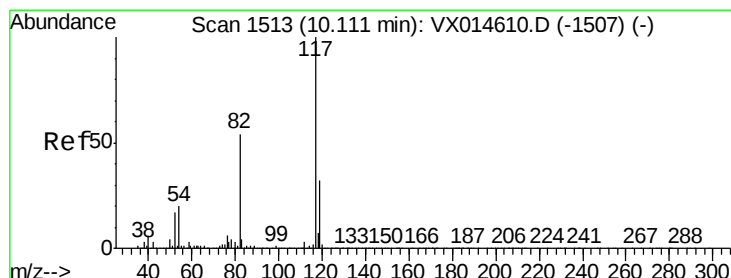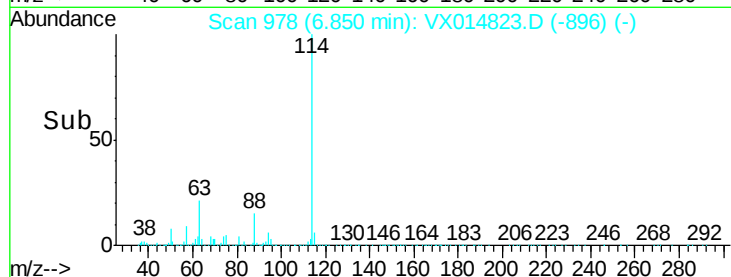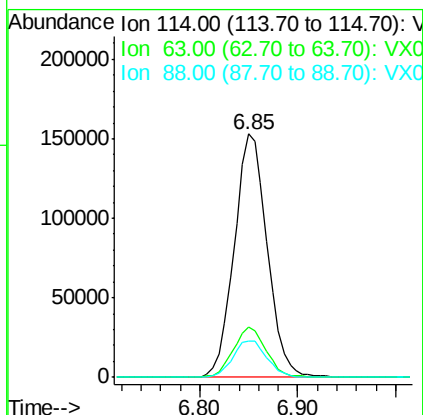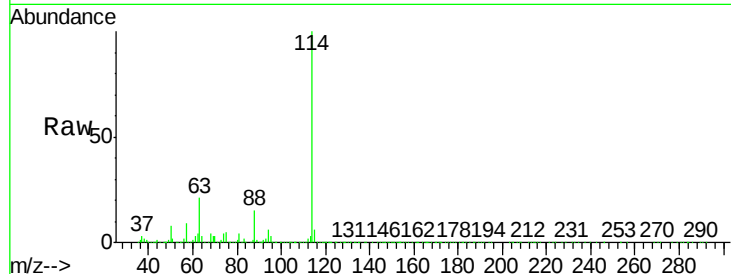

#57
 Chlorobenzene-d5
 Concen: 30.000 ug/l
 RT: 10.11 min Scan# 1513
 Delta R.T. 0.00 min
 Lab File: VX014823.D
 Acq: 05 Feb 2020 15:31

Tgt Ion:	117	Resp:	319390
Ion	Ratio	Lower	Upper
117	100		
82	53.8	43.8	65.6
119	31.8	25.8	38.6


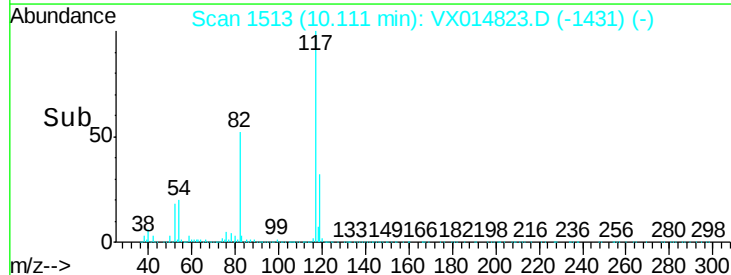
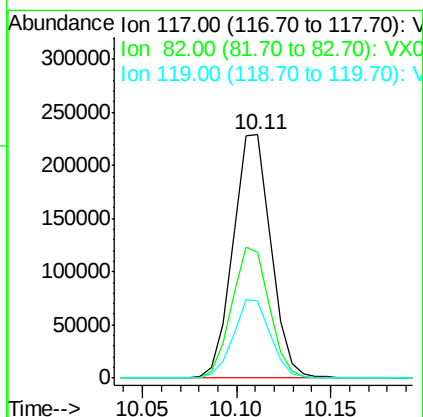
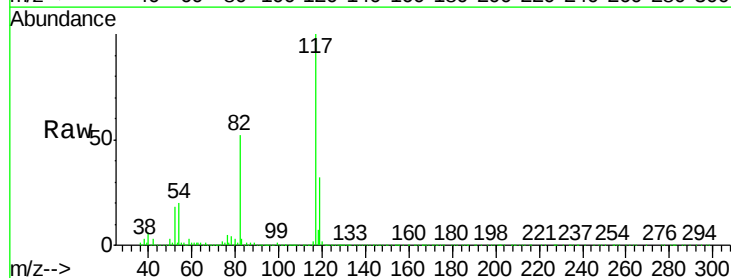


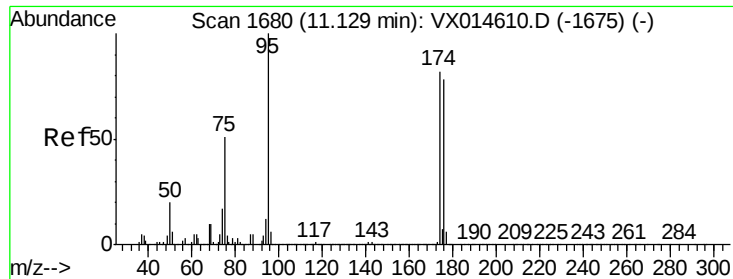

#60
4-Bromofluorobenzene
Concen: 27.317 ug/l
RT: 11.13 min Scan# 1680
Delta R.T. 0.00 min
Lab File: VX014823.D
Acq: 05 Feb 2020 15:31

Instrument :
MSVOA_X
ClientSampled :
BW-209

Tot Ion: 95 Resp: 139615
Ion Ratio Lower Upper
95 100
174 90.7 70.2 105.2
176 87.1 68.3 102.5

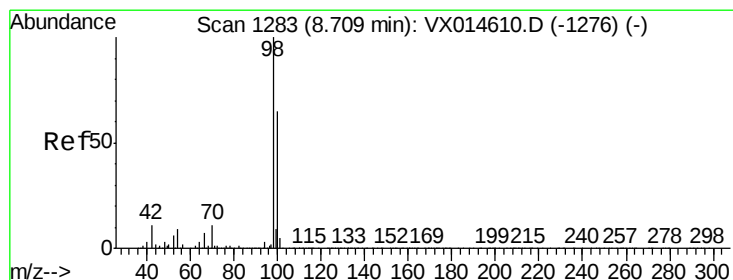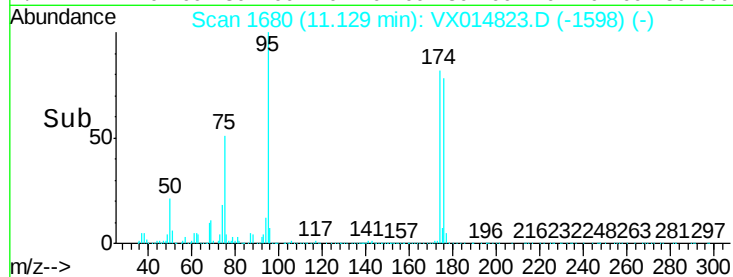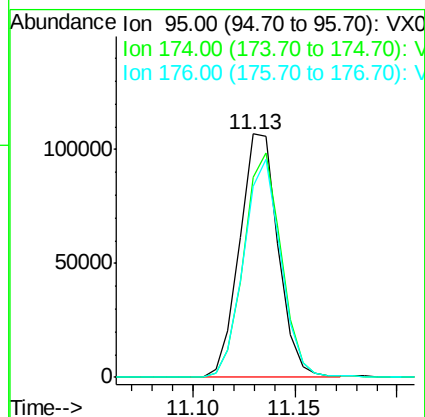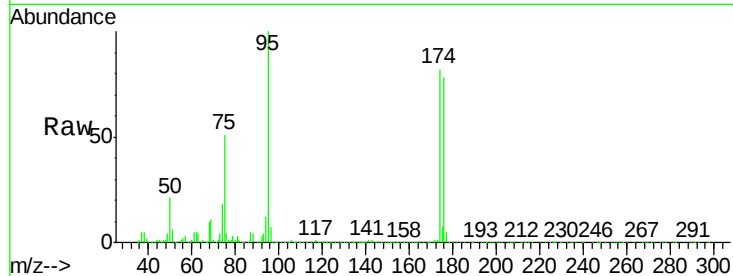

#63
Toluene-d8
Concen: 29.505 ug/l
RT: 8.71 min Scan# 1283
Delta R.T. 0.00 min
Lab File: VX014823.D
Acq: 05 Feb 2020 15:31

Tgt Ion: 98 Resp: 425664
Ion Ratio Lower Upper
98 100
100 65.5 52.2 78.2

