


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX020520\
 Data File : VX014810.D
 Acq On : 05 Feb 2020 09:15
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012220W.M
 Title : SW846 8260
 Last Update : Wed Jan 22 12:35:15 2020

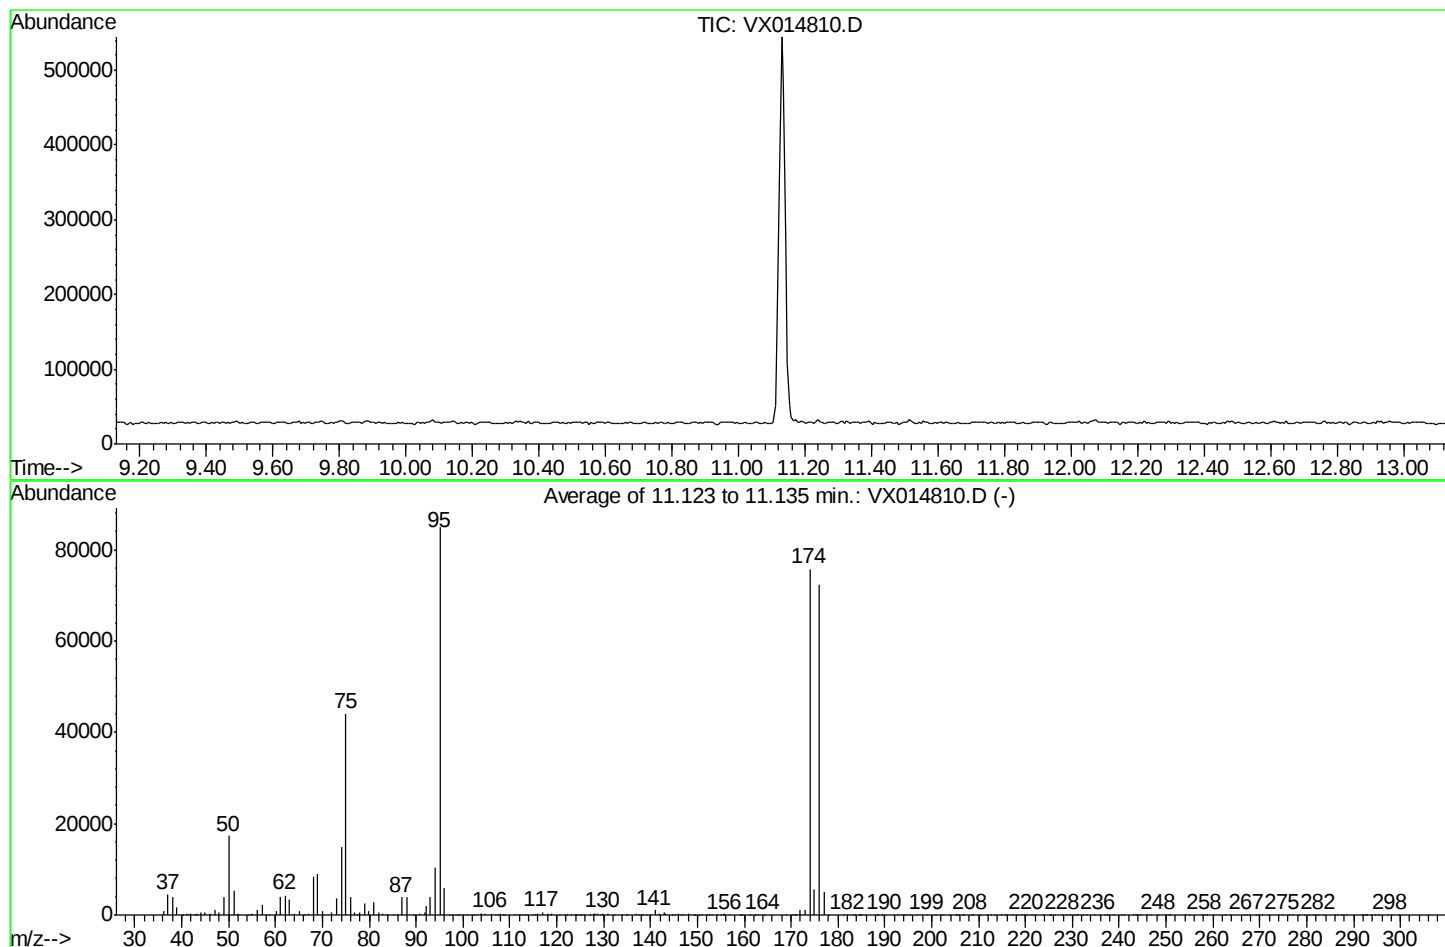

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1671

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	17387	PASS
75	95	30	60	51.9	44053	PASS
95	95	100	100	100.0	84919	PASS
96	95	5	9	6.9	5848	PASS
173	174	0.00	2	1.4	1056	PASS
174	95	50	100	89.3	75818	PASS
175	174	5	9	7.5	5716	PASS
176	174	95	101	95.6	72480	PASS
177	176	5	9	6.9	5009	PASS