

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX020521\  
 Data File : VX020873.D  
 Acq On : 05 Feb 2021 17:54  
 Operator : JC/MD  
 Sample : IBLK  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 16 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 IBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X012521W.M

Title : SW846 8260

Signal : TIC: VX020873.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.464       | 702           | 718         | 733          | rBV2     | 187967         | 537320        | 35.20%          | 6.608%        |
| 2         | 5.629       | 733           | 745         | 761          | rVB      | 300528         | 836786        | 54.81%          | 10.290%       |
| 3         | 6.031       | 801           | 811         | 825          | rBV      | 192161         | 505848        | 33.14%          | 6.220%        |
| 4         | 6.830       | 930           | 942         | 957          | rBV      | 471000         | 1095100       | 71.74%          | 13.467%       |
| 5         | 8.695       | 1241          | 1248        | 1256         | rBV      | 1009049        | 1526571       | 100.00%         | 18.772%       |
| 6         | 10.092      | 1472          | 1477        | 1493         | rVB      | 990020         | 1366956       | 89.54%          | 16.810%       |
| 7         | 11.122      | 1640          | 1646        | 1660         | rBV      | 795335         | 1008254       | 66.05%          | 12.399%       |
| 8         | 12.061      | 1794          | 1800        | 1807         | rBV      | 1020154        | 1255136       | 82.22%          | 15.435%       |




Sum of corrected areas: 8131971

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX020521\  
Data File : VX020873.D  
Acq On : 05 Feb 2021 17:54  
Operator : JC/MD  
Sample : IBLK  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X012521W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

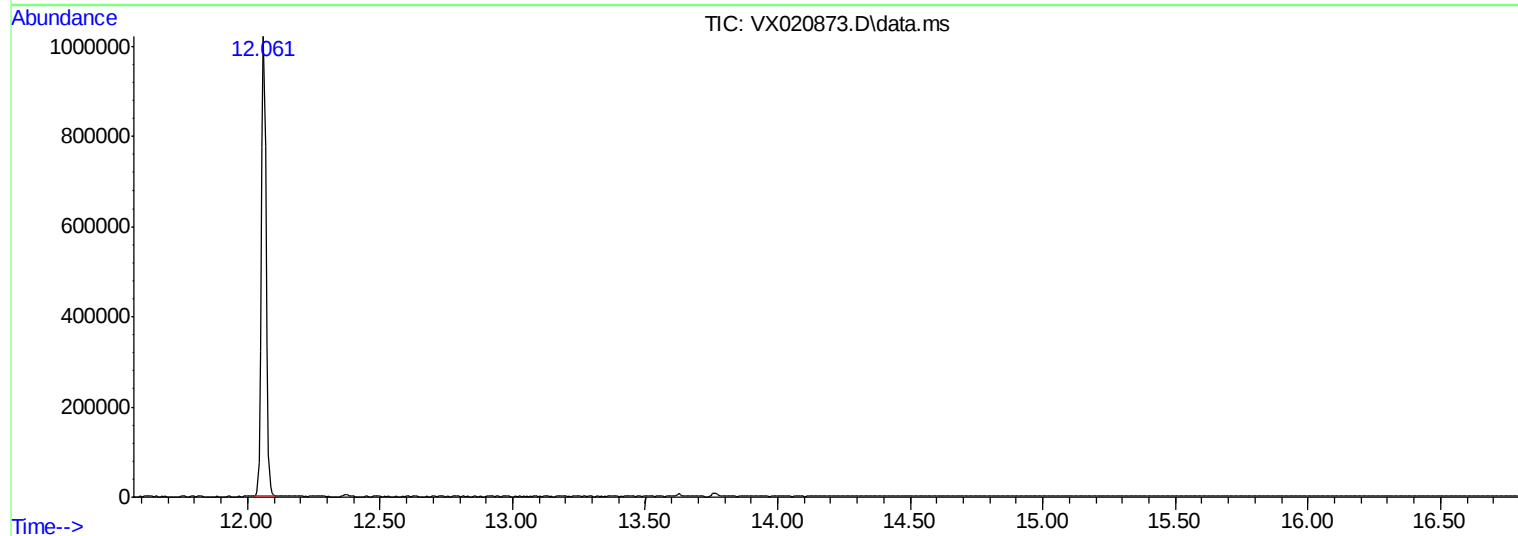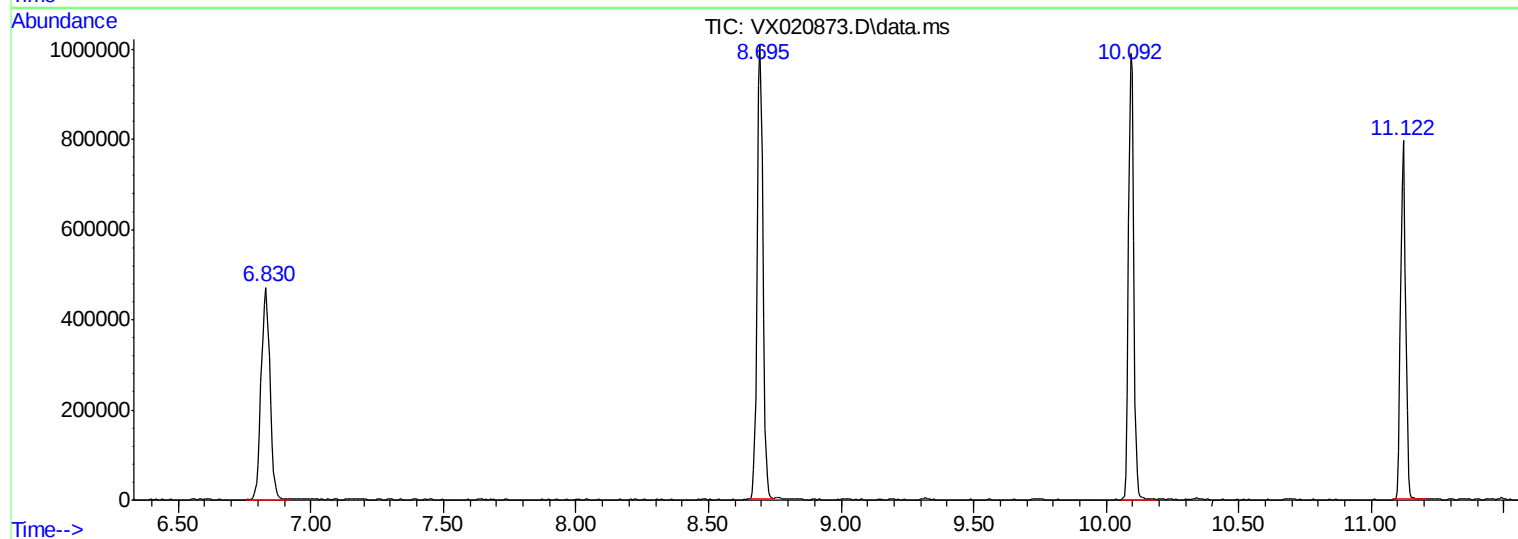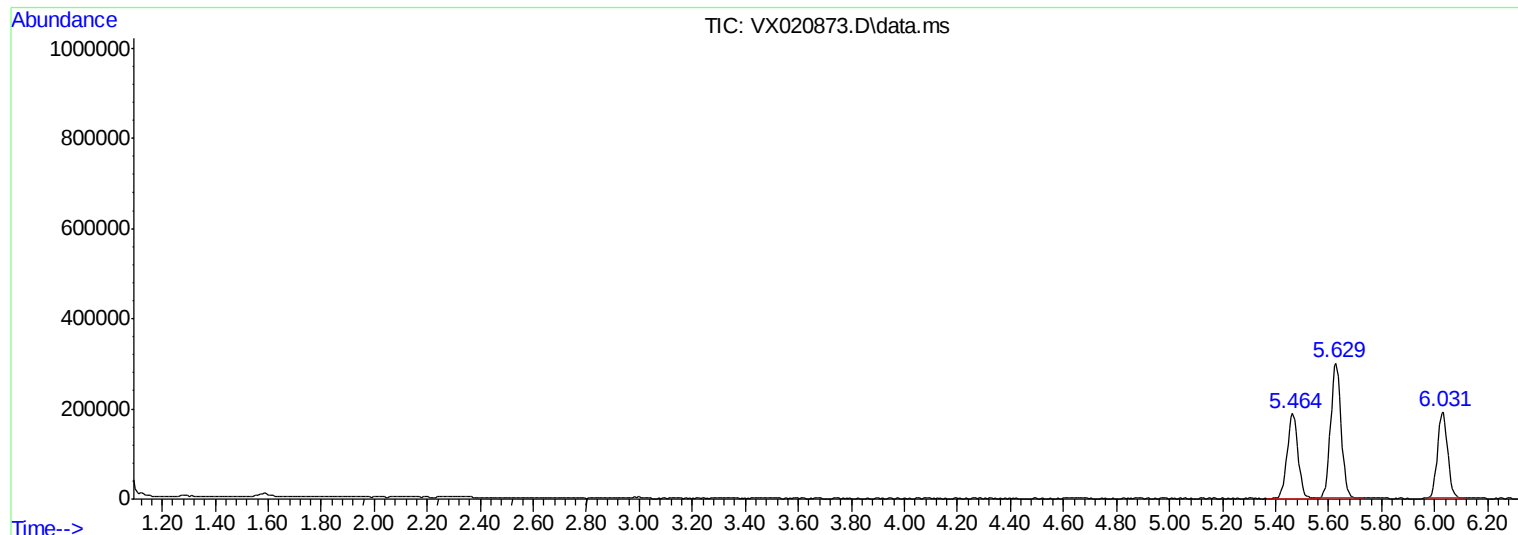

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX020521\  
Data File : VX020873.D  
Acq On : 05 Feb 2021 17:54  
Operator : JC/MD  
Sample : IBLK  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X012521W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX020521\  
Data File : VX020873.D  
Acq On : 05 Feb 2021 17:54  
Operator : JC/MD  
Sample : IBLK  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X012521W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | ---Internal Standard--- |
|------------------|----|---------|-------|----------|-------------------------|
|                  |    |         |       |          | # RT Resp Conc          |

-----