
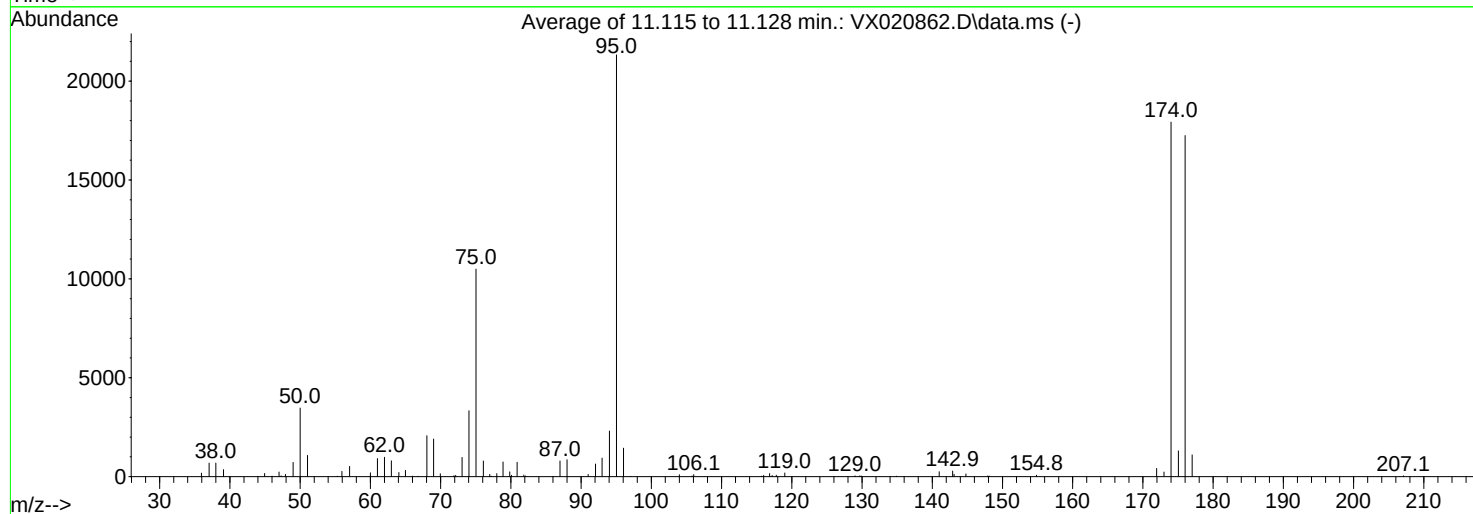


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX020521\  
Data File : VX020862.D  
Acq On : 05 Feb 2021 09:23  
Operator : JC/MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X012521W.M  
Title : SW846 8260  
Last Update : Mon Jan 25 13:38:15 2021

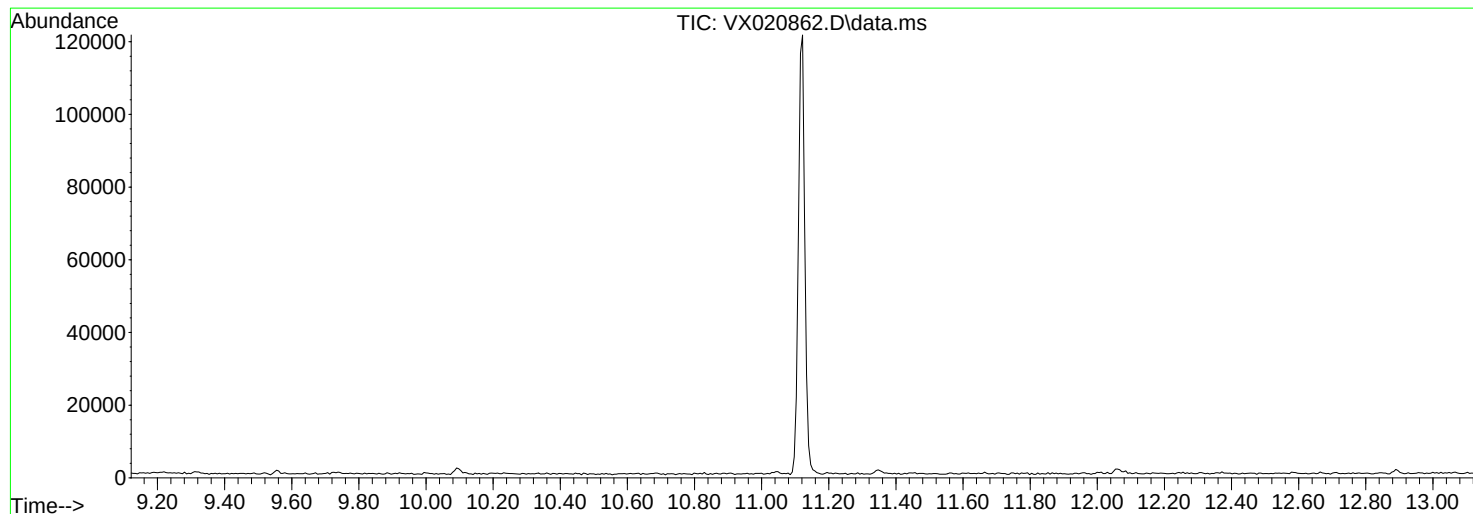

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 16.3         | 3471       | PASS                |
| 75             | 95              | 30              | 60              | 49.2         | 10496      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 21329      | PASS                |
| 96             | 95              | 5               | 9               | 6.7          | 1437       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.3          | 233        | PASS                |
| 174            | 95              | 50              | 100             | 84.0         | 17927      | PASS                |
| 175            | 174             | 5               | 9               | 7.3          | 1304       | PASS                |
| 176            | 174             | 95              | 101             | 96.2         | 17251      | PASS                |
| 177            | 176             | 5               | 9               | 6.4          | 1104       | PASS                |