


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020525\
Data File : VX044832.D
Acq On : 05 Feb 2025 08:02
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011525W.M
Title : SW846 8260
Last Update : Thu Jan 16 01:16:09 2025

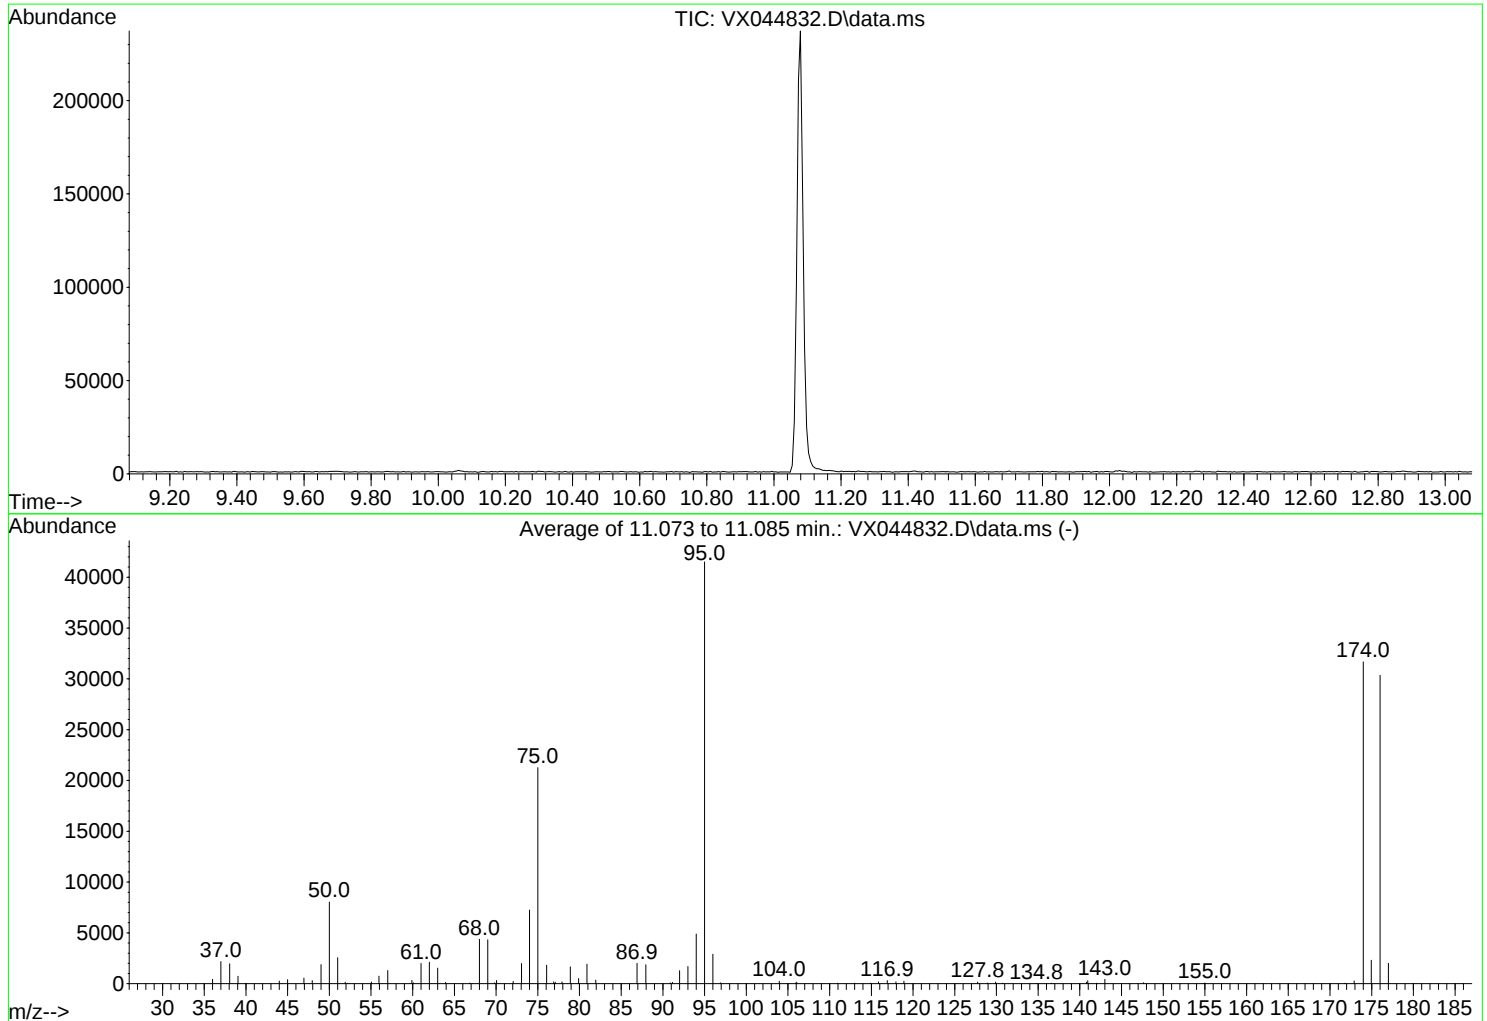

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	8027	PASS
75	95	30	60	51.2	21266	PASS
95	95	100	100	100.0	41515	PASS
96	95	5	9	7.0	2903	PASS
173	174	0.00	2	0.8	267	PASS
174	95	50	100	76.3	31672	PASS
175	174	5	9	7.3	2300	PASS
176	174	95	101	95.8	30349	PASS
177	176	5	9	6.6	1996	PASS