


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX020619\
Data File : VX007389.D
Acq On : 06 Feb 2019 09:22
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
Title : SW846 8260
Last Update : Sat Feb 02 01:32:36 2019

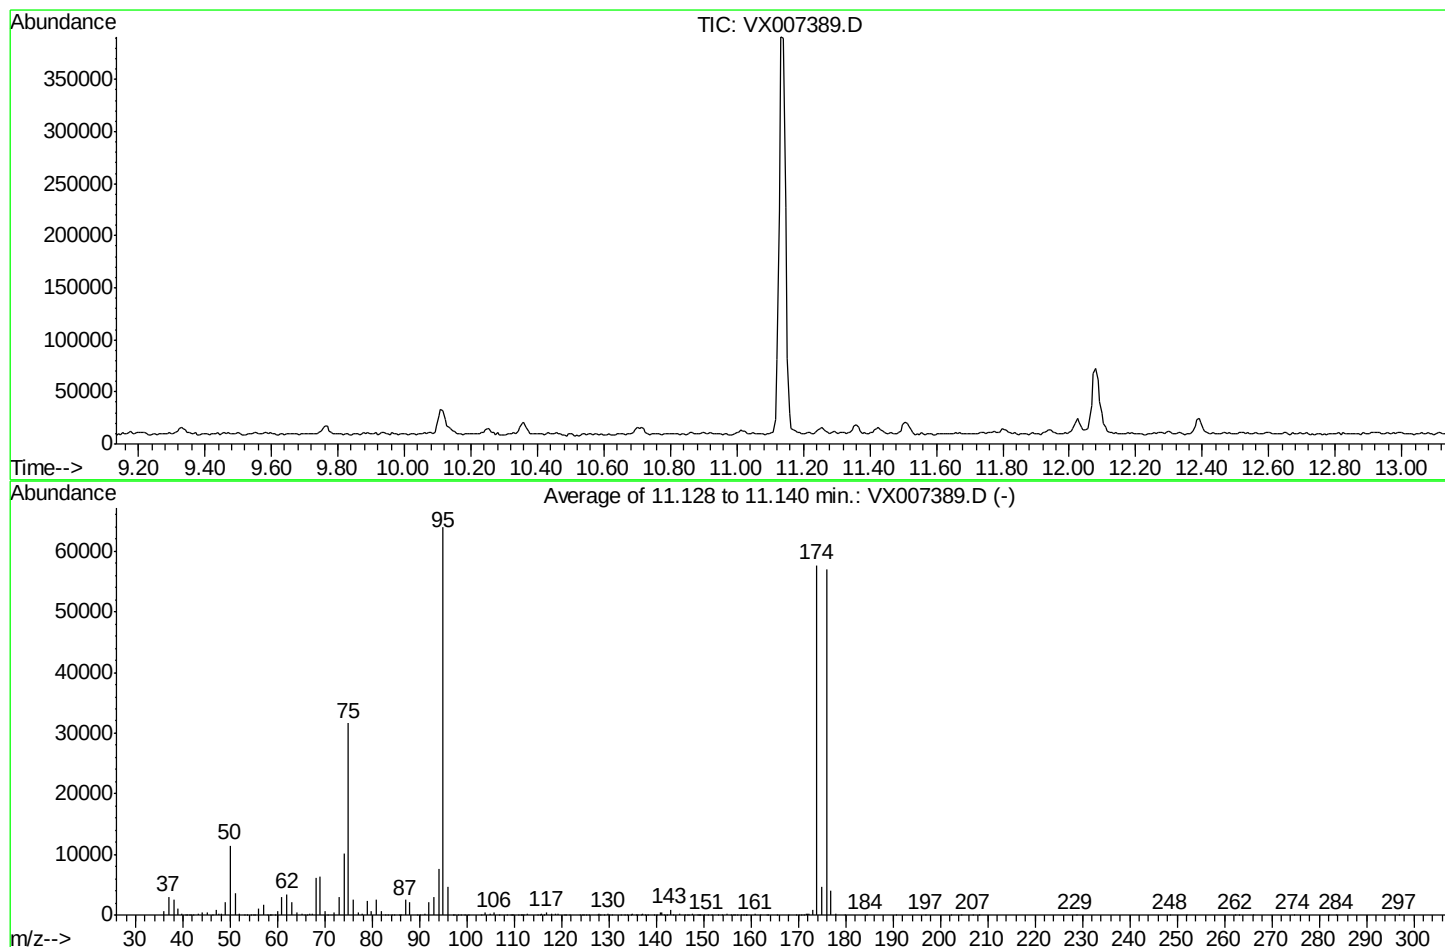

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	11501	PASS
75	95	30	60	49.4	31573	PASS
95	95	100	100	100.0	63946	PASS
96	95	5	9	7.2	4573	PASS
173	174	0.00	2	1.5	845	PASS
174	95	50	100	90.2	57677	PASS
175	174	5	9	8.1	4662	PASS
176	174	95	101	99.0	57085	PASS
177	176	5	9	7.1	4058	PASS