

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX020620\
 Data File : VX014859.D
 Acq On : 06 Feb 2020 19:40
 Operator : JC/SP
 Sample : L1419-03
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Feb 07 00:52:24 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012220W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jan 22 12:35:15 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	476259	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.85	114	738432	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	678568	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.07	152	345002	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.05	65	263901	47.45	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.90%	
35) Dibromofluoromethane	5.49	113	218186	46.83	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.66%	
50) Toluene-d8	8.71	98	877747	49.00	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.00%	
62) 4-Bromofluorobenzene	11.13	95	322256	50.50	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.00%	
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.18	85	441	0.599	ug/l	99
3) Chloromethane	1.32	50	1303	0.202	ug/l #	85
6) Chloroethane	1.71	64	237	Below Cal	#	73
11) Tert butyl alcohol	3.03	59	65100	52.137	ug/l	99
13) Acrolein	2.28	56	2428	2.466	ug/l #	82
14) Allyl chloride	2.70	41	3410	0.401	ug/l #	50
16) Acetone	2.43	43	551852	181.088	ug/l	100
18) Methyl Acetate	2.76	43	25237	2.901	ug/l	93
20) Methylene Chloride	2.85	84	52777	9.357	ug/l	92
25) 2-Butanone	4.66	43	106750	24.444	ug/l	98
29) Tetrahydrofuran	5.14	42	1920	0.741	ug/l #	68
36) 1,1-Dichloropropene	5.65	75	32098	4.678	ug/l #	43
37) Ethyl Acetate	4.83	43	21127	2.688	ug/l #	97
38) Carbon Tetrachloride	5.65	117	42293	6.454	ug/l #	17
39) Methylcyclohexane	7.45	83	2418	0.281	ug/l #	79
40) Benzene	6.13	78	13636	0.643	ug/l	97
41) Methacrylonitrile	5.04	41	387	Below Cal	#	17
43) Isopropyl Acetate	6.47	43	5044	0.392	ug/l #	72
49) 1,4-Dioxane	7.74	88	4878	37.426	ug/l #	84
51) 4-Methyl-2-Pentanone	8.64	43	9738	1.199	ug/l	94
52) Toluene	8.78	92	311900	23.933	ug/l	97
56) Ethyl methacrylate	9.15	69	271	1.813	ug/l #	1
59) 2-Hexanone	9.49	43	5142	0.816	ug/l	90
67) Ethyl Benzene	10.25	91	12768	0.515	ug/l	95
68) m/p-Xylenes	10.36	106	13581	1.446	ug/l	96
69) o-Xylene	10.70	106	7854	0.867	ug/l	89
70) Styrene	10.71	104	7399	0.487	ug/l #	86
76) 1,2,3-Trichloropropane	11.13	75	159674	19.893	ug/l #	39
81) trans-1,4-Dichloro-2-buten	11.13	75	159674	56.611	ug/l #	10
84) 1,2,4-Trimethylbenzene	11.80	105	11386	0.564	ug/l	75
95) Naphthalene	13.83	128	19214	1.711	ug/l #	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX020620\
Data File : VX014859.D
Acq On : 06 Feb 2020 19:40
Operator : JC/SP
Sample : L1419-03
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Feb 07 00:52:24 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X012220W.M
Quant Title : SW846 8260
QLast Update : Wed Jan 22 12:35:15 2020
Response via : Initial Calibration

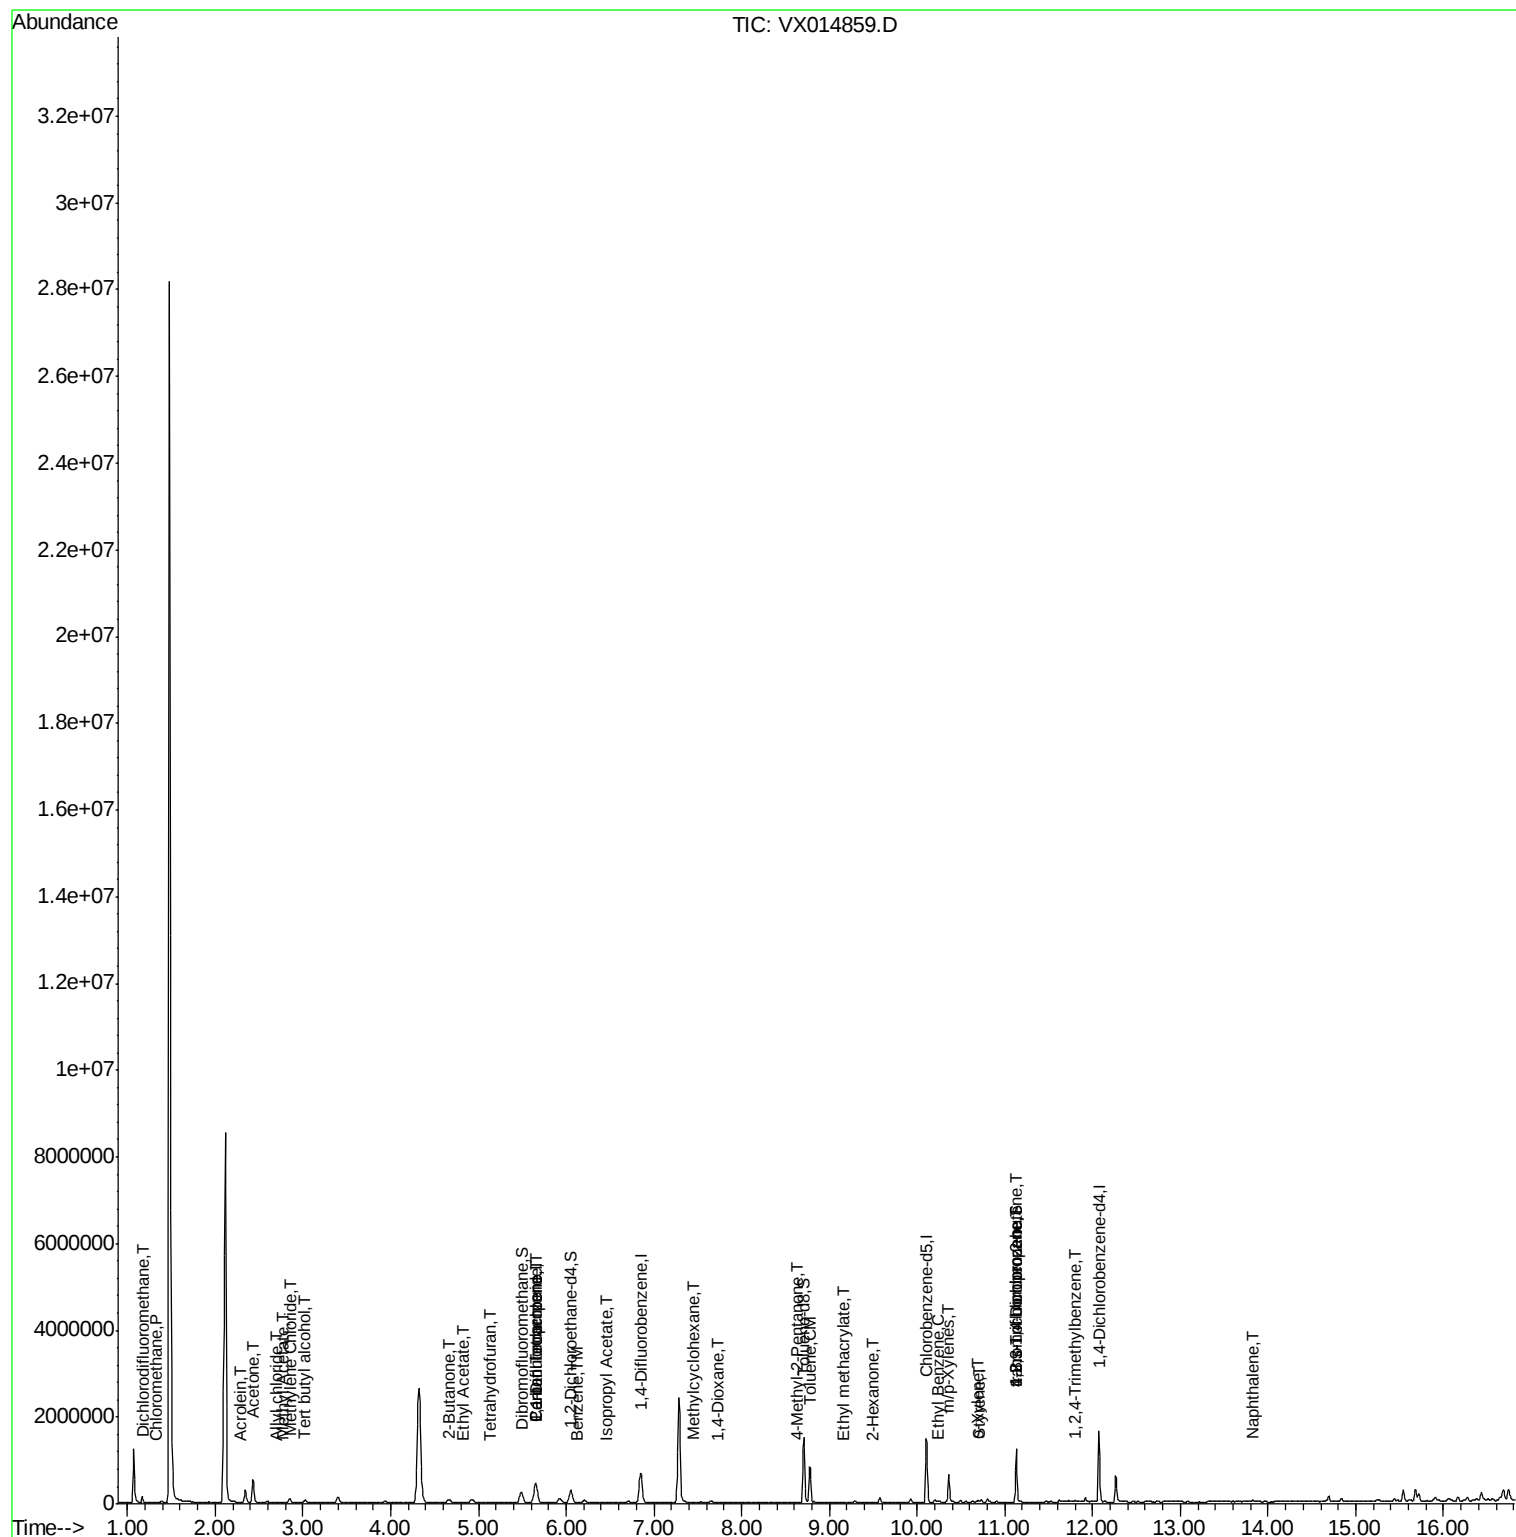




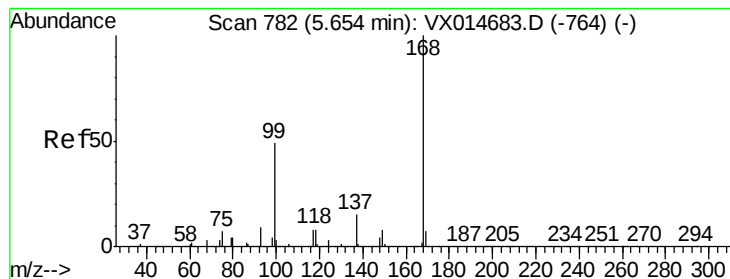


#1

Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.65 min Scan# 782
Delta R.T. 0.00 min
Lab File: VX014859.D
Acq: 06 Feb 2020 19:40

Instrument :
MSVOA_X
ClientSampleId :




Tot Ion:168 Resp: 476259
Ion Ratio Lower Upper
168 100
99 48.8 39.8 59.6

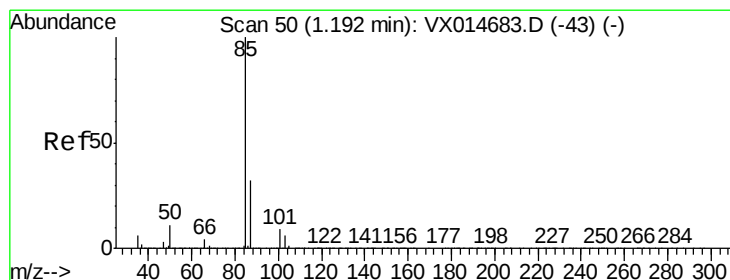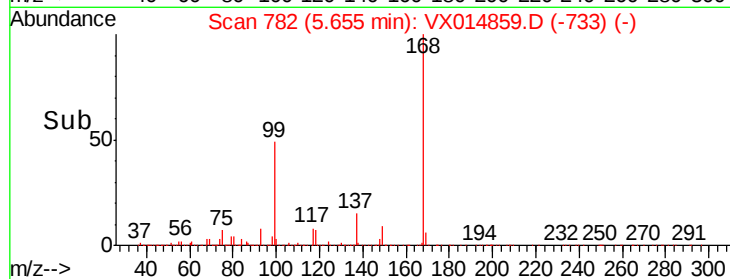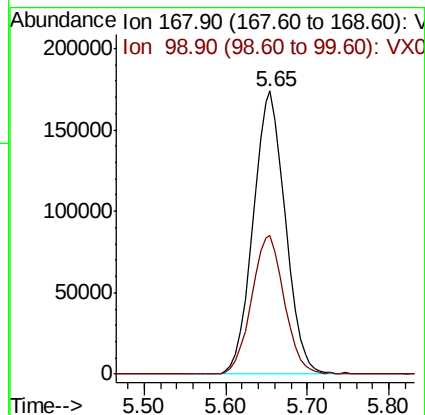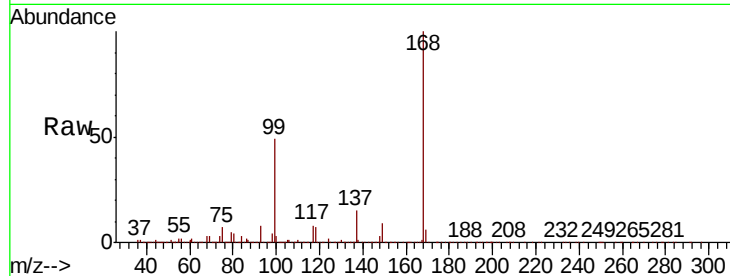


#2

Dichlorodifluoromethane
Concen: 0.599 ug/l
RT: 1.18 min Scan# 48
Delta R.T. -0.01 min
Lab File: VX014859.D
Acq: 06 Feb 2020 19:40

Tgt Ion: 85 Resp: 441
Ion Ratio Lower Upper
85 100
87 31.6 16.2 48.5

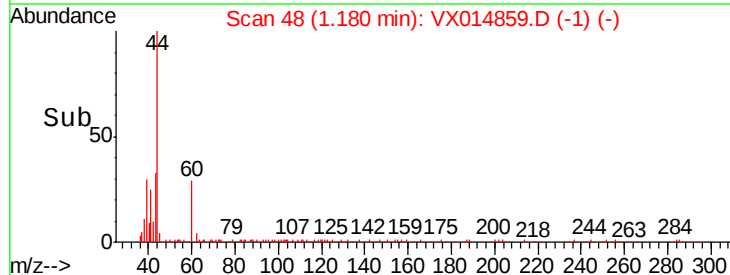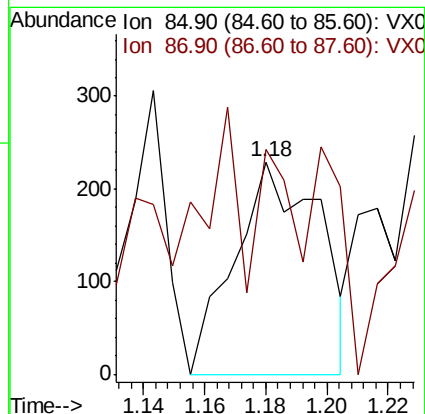

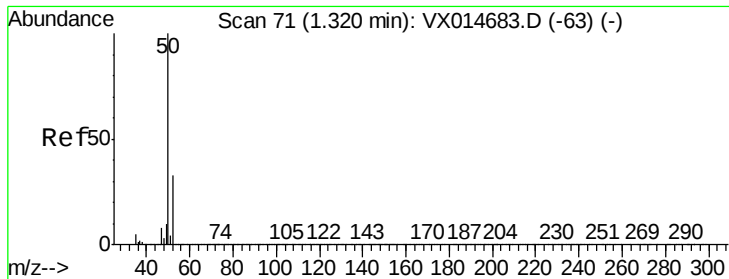

#3

Chloromethane

Concen: 0.202 ug/l

RT: 1.32 min Scan# 71

Delta R.T. 0.00 min

Lab File: VX014859.D

Acq: 06 Feb 2020 19:40


Instrument :
MSVOA_X
ClientSampleId :

Tot Ion: 50 Resp: 1303




Ion Ratio Lower Upper

50 100

52 24.2 26.2 39.2#

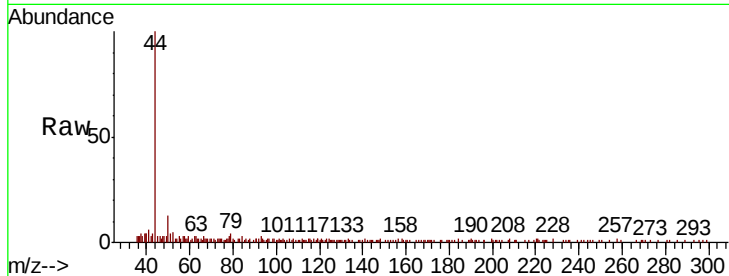

Abundance Ion 49.90 (49.60 to 50.60): VX0
Ion 51.90 (51.60 to 52.60): VX0

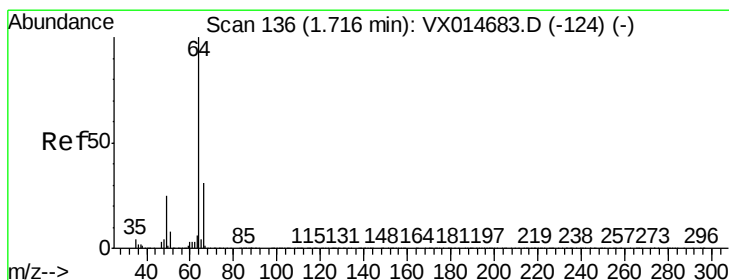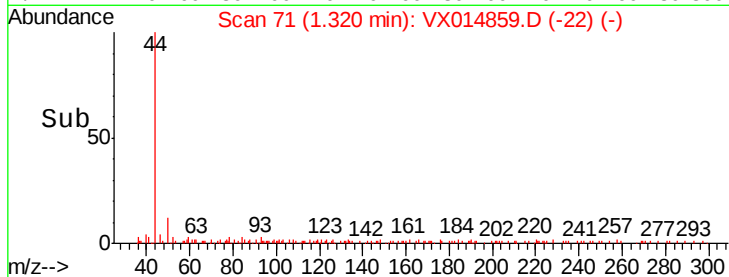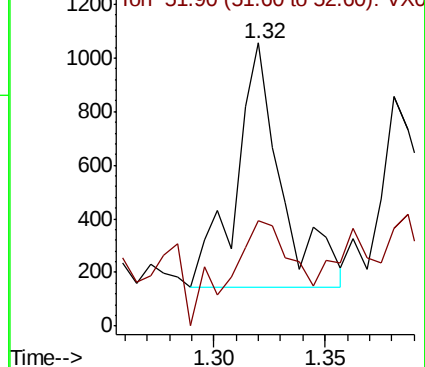

#6

Chloroethane

Concen: Below Cal

RT: 1.71 min Scan# 135

Delta R.T. -0.01 min

Lab File: VX014859.D


Acq: 06 Feb 2020 19:40

Tgt Ion: 64 Resp: 237



Ion Ratio Lower Upper


64 100

66 16.8 25.2 37.8#

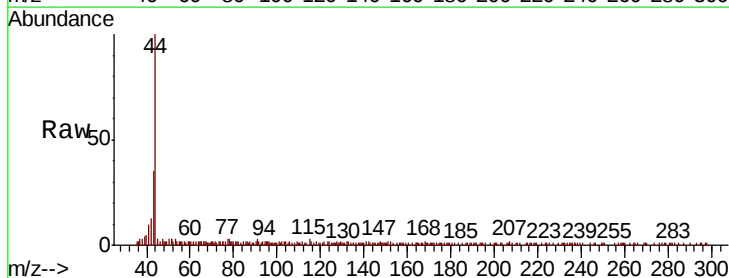

Abundance Ion 63.90 (63.60 to 64.60): VX0
Ion 65.90 (65.60 to 66.60): VX0



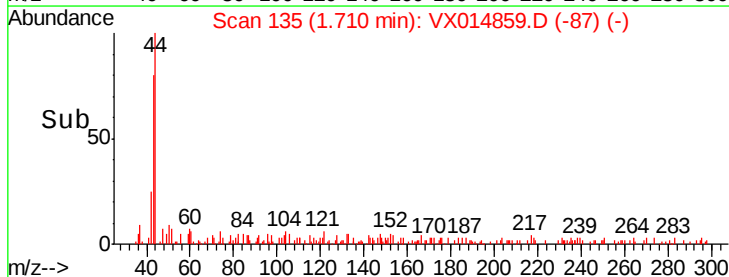
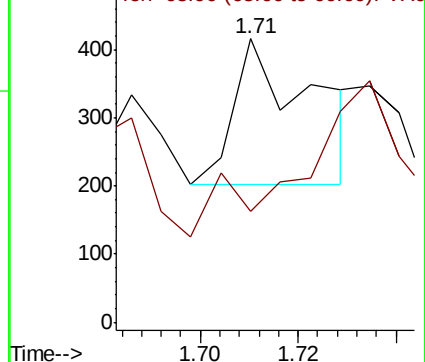


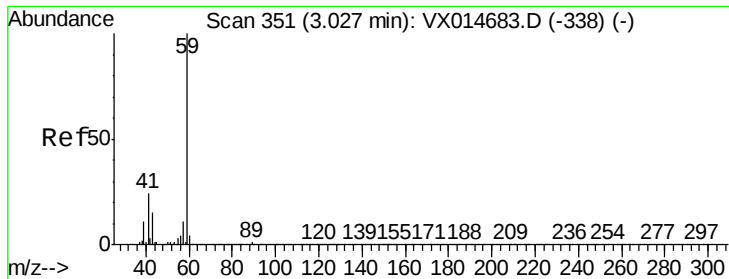

#11
Tert butyl alcohol
Concen: 52.137 ug/l
RT: 3.03 min Scan# 351
Delta R.T. 0.00 min
Lab File: VX014859.D
Acq: 06 Feb 2020 19:40




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion: 59 Resp: 65100
Ion Ratio Lower Upper
59 100
57 10.1 8.3 12.5

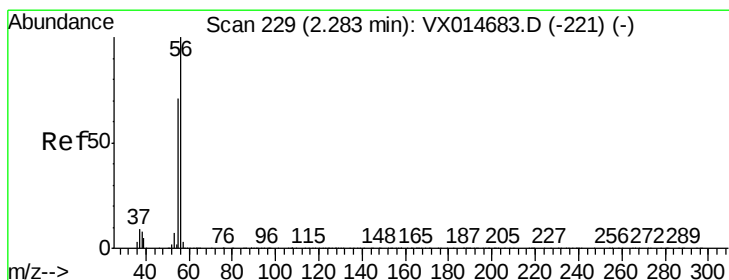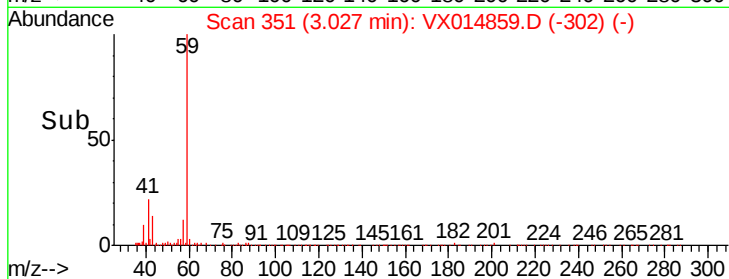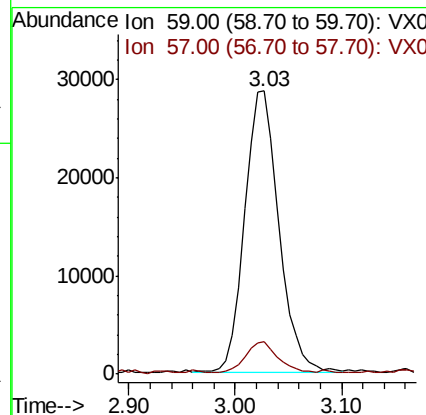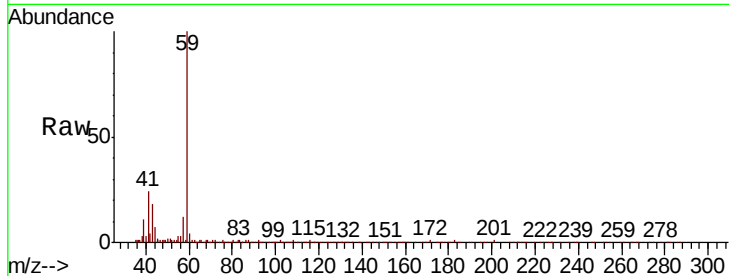

#13
Acrolein
Concen: 2.466 ug/l
RT: 2.28 min Scan# 229
Delta R.T. 0.00 min
Lab File: VX014859.D
Acq: 06 Feb 2020 19:40

Tgt Ion: 56 Resp: 2428
Ion Ratio Lower Upper
56 100
55 56.1 56.6 84.8#


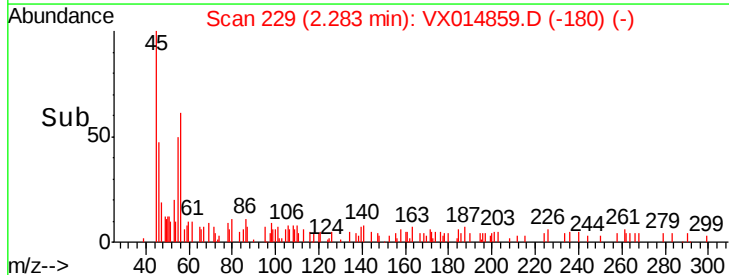
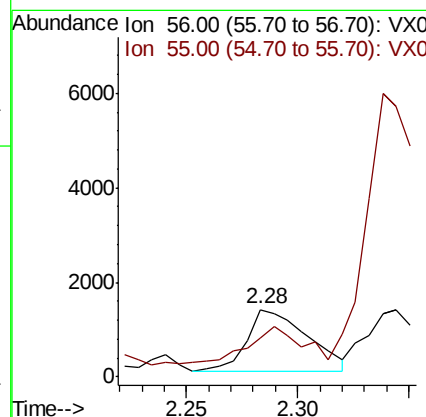
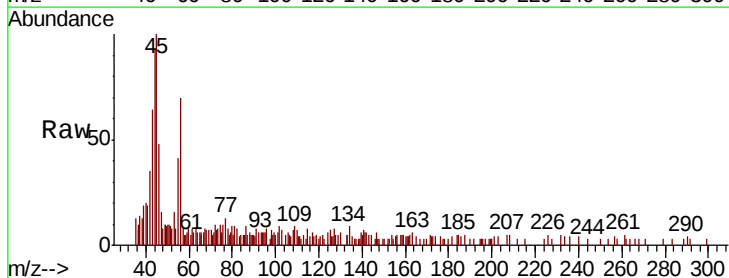


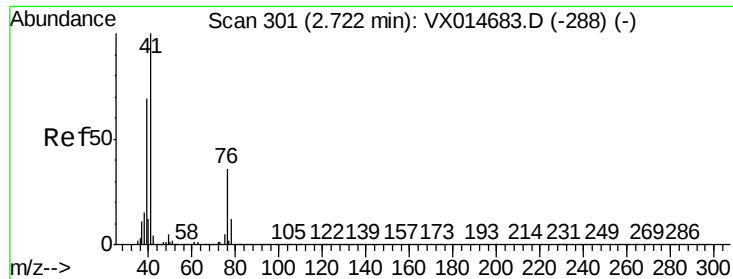

#14
Allvl chloride
Concen: 0.401 ug/l
RT: 2.70 min Scan# 297
Delta R.T. -0.02 min
Lab File: VX014859.D
Acq: 06 Feb 2020 19:40




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion: 41 Resp: 3410
Ion Ratio Lower Upper
41 100
39 28.7 52.0 78.0#
76 0.0 26.0 39.0#

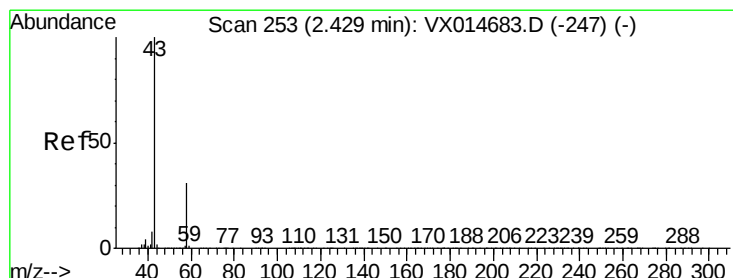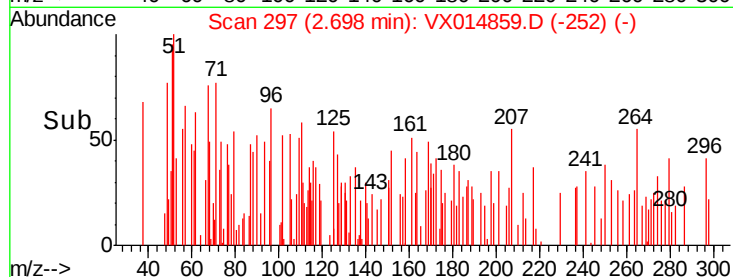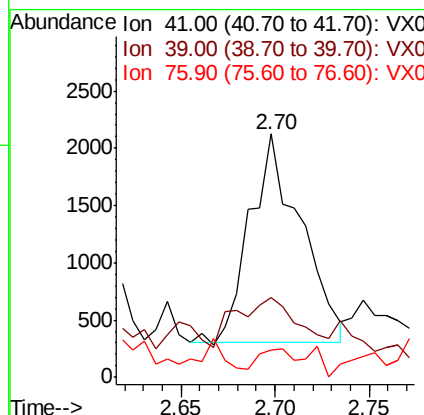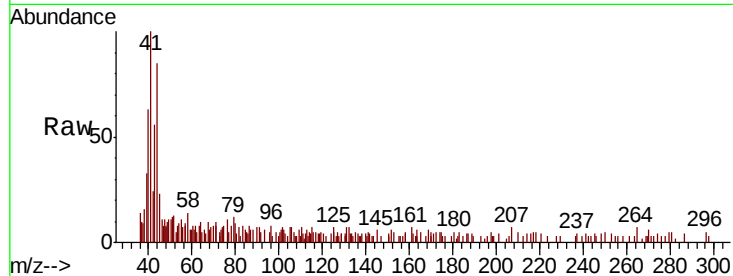

#16
Acetone
Concen: 181.088 ug/l
RT: 2.43 min Scan# 253
Delta R.T. 0.00 min
Lab File: VX014859.D
Acq: 06 Feb 2020 19:40

Tgt Ion: 43 Resp: 551852
Ion Ratio Lower Upper
43 100
58 30.8 24.5 36.7


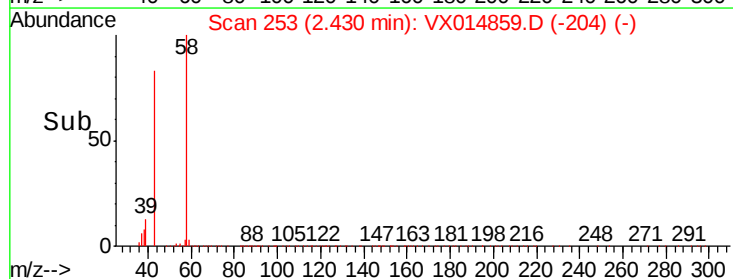
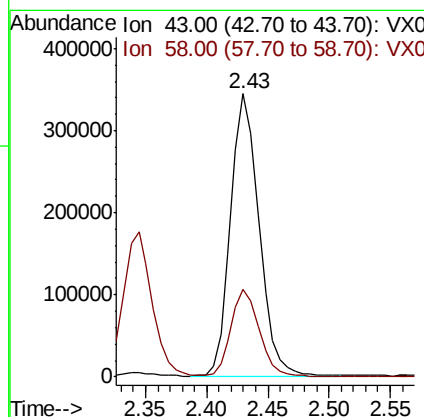
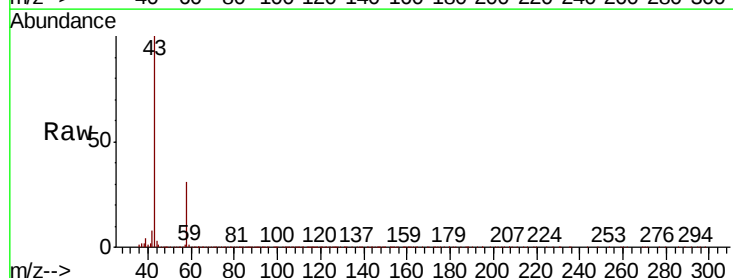


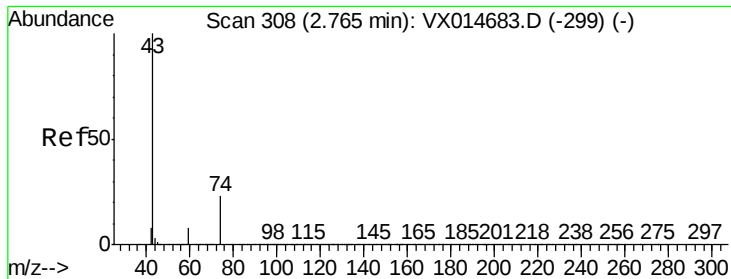

#18
Methyl Acetate
Concen: 2.901 ug/l
RT: 2.76 min Scan# 308
Delta R.T. 0.00 min
Lab File: VX014859.D
Acq: 06 Feb 2020 19:40




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion: 43 Resp: 25237
Ion Ratio Lower Upper
43 100
74 26.5 18.5 27.7

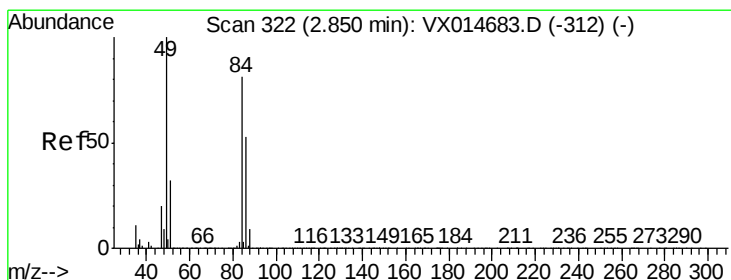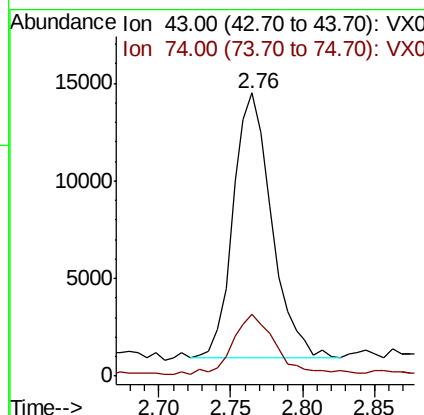

#20
Methylene Chloride
Concen: 9.357 ug/l
RT: 2.85 min Scan# 322
Delta R.T. 0.00 min
Lab File: VX014859.D
Acq: 06 Feb 2020 19:40

Tgt Ion: 84 Resp: 52777
Ion Ratio Lower Upper
84 100
49 112.1 98.2 147.4
51 33.6 31.3 46.9
86 61.1 51.8 77.6

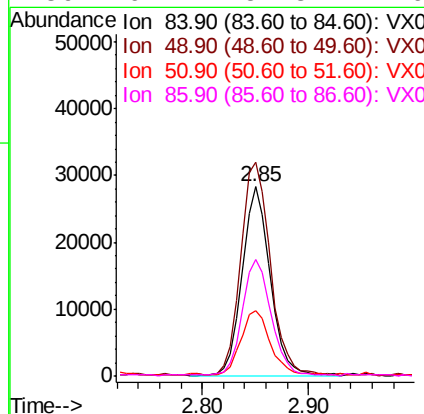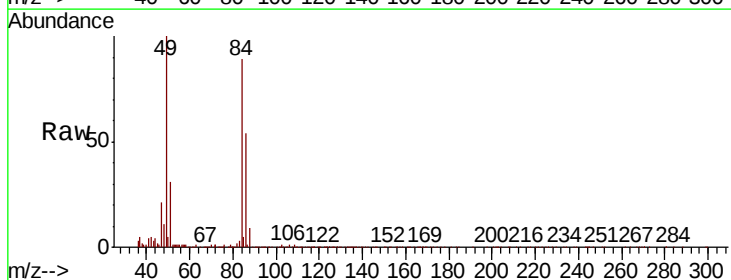



#25

2-Butanone

Concen: 24.444 ug/l

RT: 4.66 min Scan# 619

Delta R.T. 0.01 min

Lab File: VX014859.D

Acq: 06 Feb 2020 19:40





Instrument :
MSVOA_X
ClientSampleId :

Tot Ion: 43 Resp: 106750

Ion Ratio Lower Upper

43 100

72 25.7 19.9 29.9

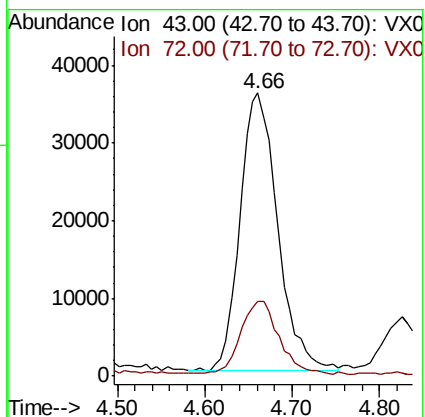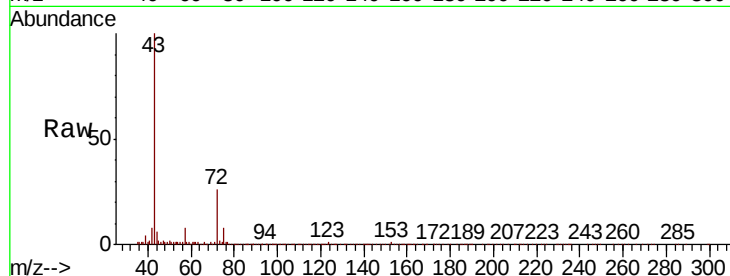

#29

Tetrahydrofuran

Concen: 0.741 ug/l

RT: 5.14 min Scan# 697

Delta R.T. 0.02 min

Lab File: VX014859.D

Acq: 06 Feb 2020 19:40




Tgt Ion: 42 Resp: 1920


Ion Ratio Lower Upper

42 100

72 22.3 35.3 52.9#

71 60.3 33.1 49.7#



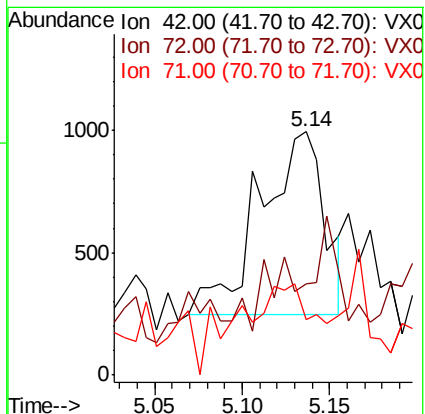





#33
 1,2-Dichloroethane-d4
 Concen: 47.451 ug/l
 RT: 6.05 min Scan# 847
 Delta R.T. 0.00 min
 Lab File: VX014859.D
 Acq: 06 Feb 2020 19:40




Instrument :
 MSVOA_X
 ClientSampleId :


Tot Ion: 65 Resp: 263901
 Ion Ratio Lower Upper
 65 100
 67 51.7 0.0 107.4

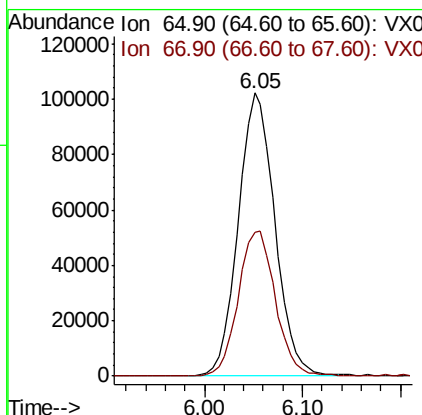

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.85 min Scan# 978
 Delta R.T. 0.00 min
 Lab File: VX014859.D
 Acq: 06 Feb 2020 19:40

Tgt Ion: 114 Resp: 738432
 Ion Ratio Lower Upper
 114 100
 63 20.5 0.0 40.6
 88 14.8 0.0 31.2


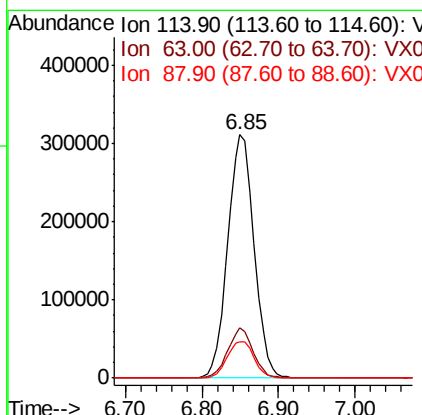




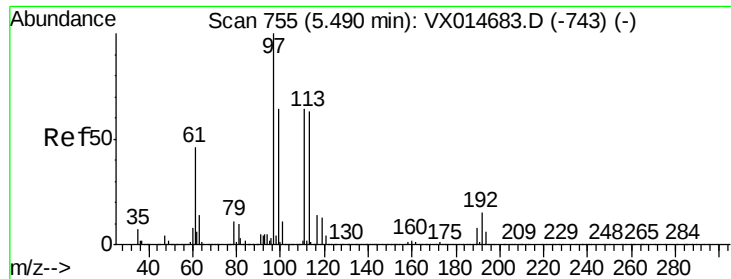

#35
Dibromofluoromethane
Concen: 46.827 ug/l
RT: 5.49 min Scan# 755
Delta R.T. 0.00 min
Lab File: VX014859.D
Acq: 06 Feb 2020 19:40




Instrument :
MSVOA_X
ClientSampled :


Tot Ion	Ratio	Lower	Upper
113	100		
111	102.1	80.7	121.1
192	24.1	18.5	27.7

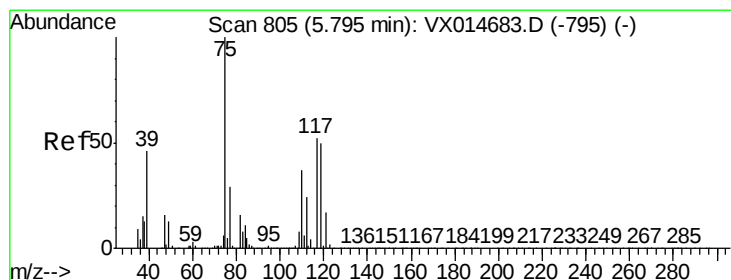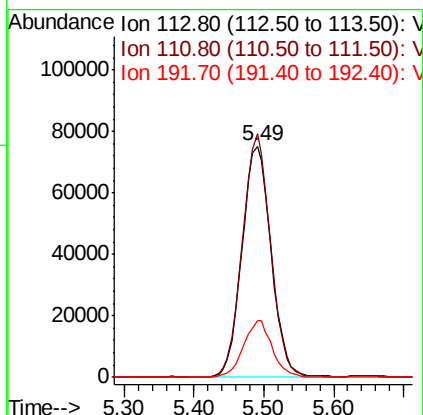

#36
1,1-Dichloropropene
Concen: 4.678 ug/l
RT: 5.65 min Scan# 781
Delta R.T. -0.15 min
Lab File: VX014859.D
Acq: 06 Feb 2020 19:40

Tgt Ion	Ratio	Lower	Upper
75	100		
110	0.0	17.9	53.7#
77	1.8	24.1	36.1#


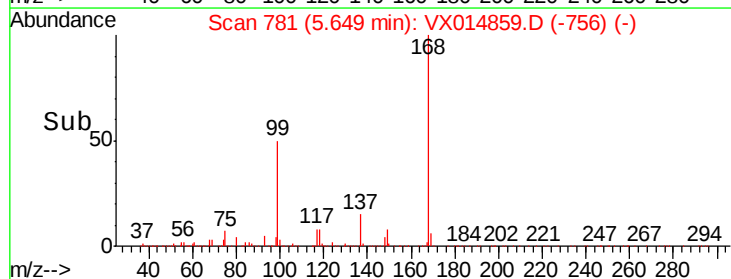
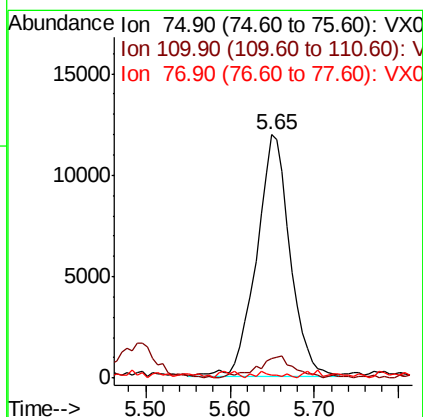
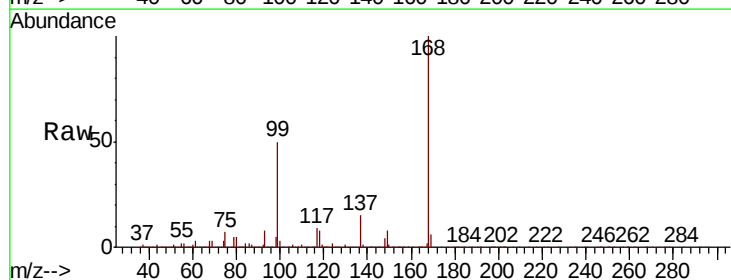


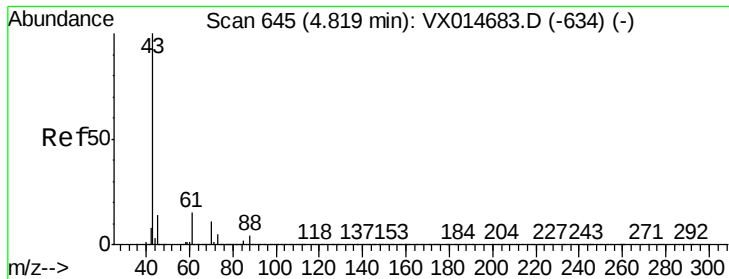

#37
Ethyl Acetate
Concen: 2.688 ug/l
RT: 4.83 min Scan# 646
Delta R.T. 0.01 min
Lab File: VX014859.D
Acq: 06 Feb 2020 19:40




Instrument :
MSVOA_X
ClientSampled :


Tot Ion: 43 Resp: 21127
Ion Ratio Lower Upper
43 100
61 13.2 11.0 16.4
70 12.9 8.5 12.7#

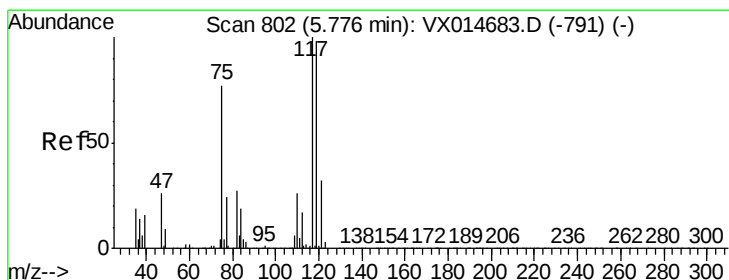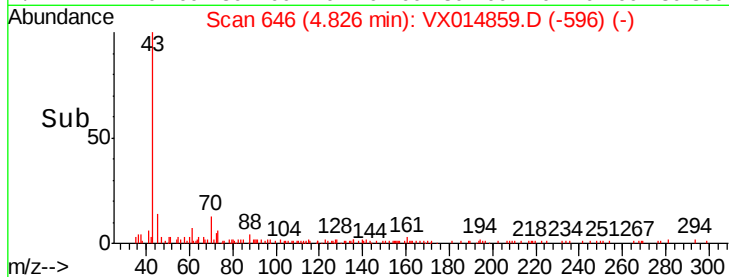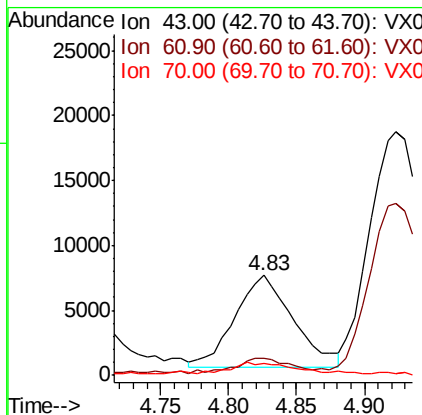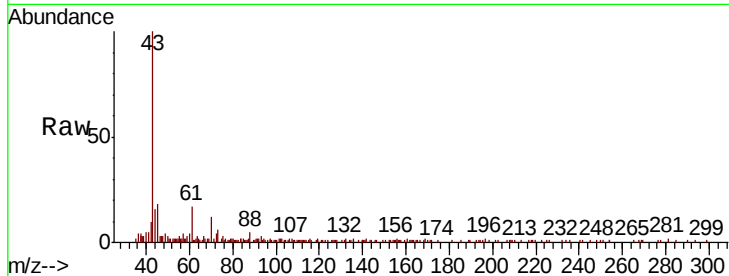

#38
Carbon Tetrachloride
Concen: 6.454 ug/l
RT: 5.65 min Scan# 781
Delta R.T. -0.13 min
Lab File: VX014859.D
Acq: 06 Feb 2020 19:40

Tgt Ion: 117 Resp: 42293
Ion Ratio Lower Upper
117 100
119 6.5 77.9 116.9#
121 0.5 25.4 38.2#


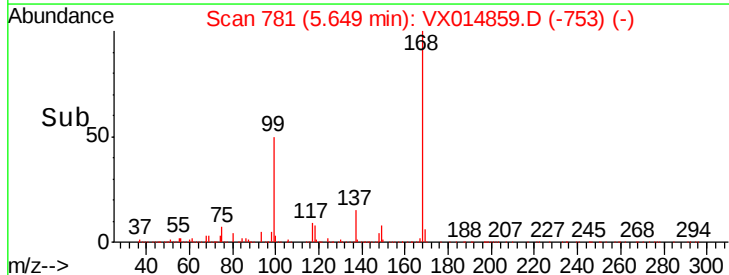
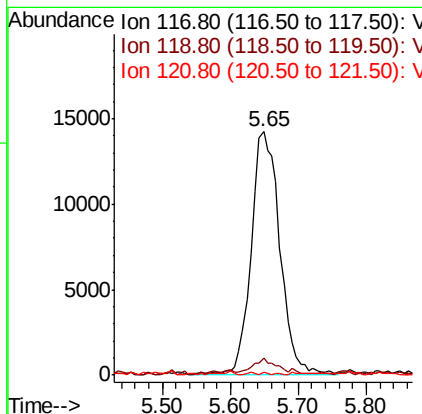
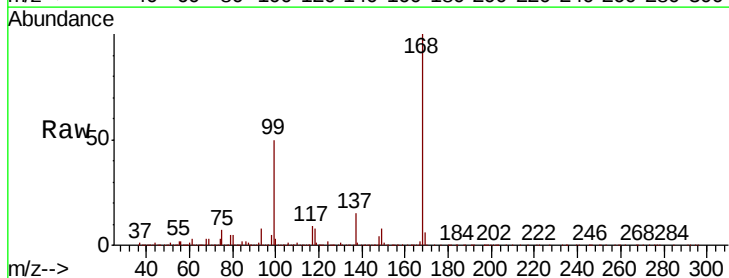




#39
Methvlcvclohexane
Concen: 0.281 ug/l
RT: 7.45 min Scan# 1077
Delta R.T. -0.01 min
Lab File: VX014859.D
Acq: 06 Feb 2020 19:40




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion: 83 Resp: 2418
Ion Ratio Lower Upper
83 100
55 98.2 65.6 98.4
98 32.2 40.2 60.4#

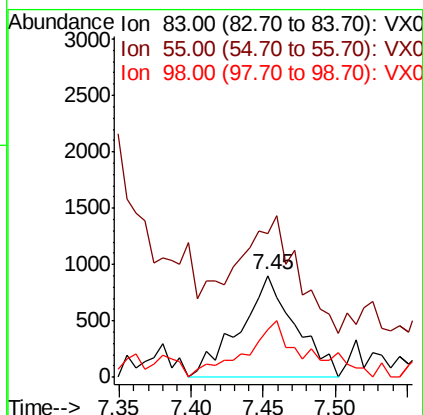

#40
Benzene
Concen: 0.643 ug/l
RT: 6.13 min Scan# 860
Delta R.T. -0.01 min
Lab File: VX014859.D
Acq: 06 Feb 2020 19:40

Tgt Ion: 78 Resp: 13636
Ion Ratio Lower Upper
78 100
77 25.0 18.7 28.1

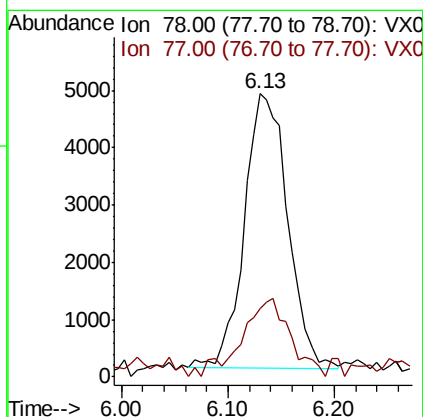



#43

Isopropyl Acetate

Concen: 0.392 ug/l

RT: 6.47 min Scan# 915

Delta R.T. 0.03 min

Lab File: VX014859.D

Acq: 06 Feb 2020 19:40

Instrument :

MSVOA_X

ClientSampleId :





Tot Ion: 43 Resp: 5044

Ion Ratio Lower Upper

43 100

61 6.7 16.2 24.4#

87 2.6 10.5 15.7#

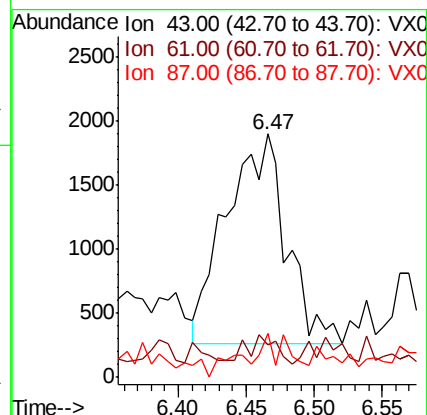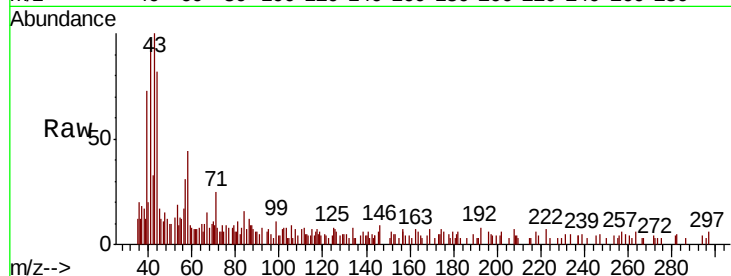

#49

1,4-Dioxane

Concen: 37.426 ug/l

RT: 7.74 min Scan# 1124

Delta R.T. 0.01 min

Lab File: VX014859.D

Acq: 06 Feb 2020 19:40




Tgt Ion: 88 Resp: 4878


Ion Ratio Lower Upper

88 100

43 44.0 26.2 39.2#

58 82.5 56.6 85.0


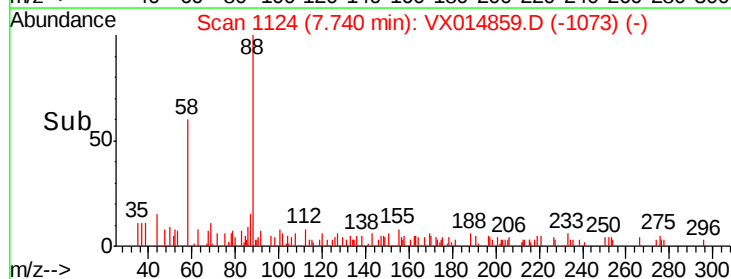
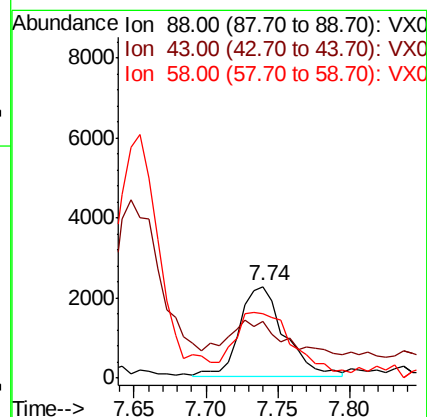





#50
Toluene-d8
Concen: 49.001 ug/l
RT: 8.71 min Scan# 1283
Delta R.T. 0.00 min
Lab File: VX014859.D
Acq: 06 Feb 2020 19:40




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion: 98 Resp: 877747
Ion Ratio Lower Upper
98 100
100 65.8 53.0 79.6

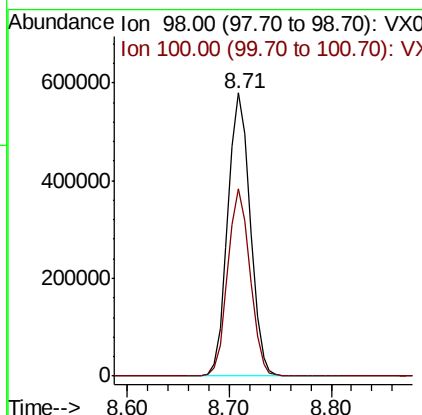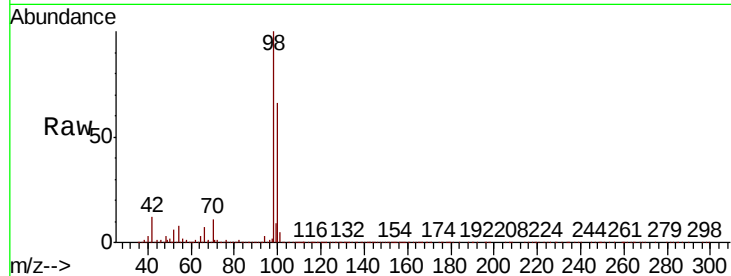

#51
4-Methyl-2-Pentanone
Concen: 1.199 ug/l
RT: 8.64 min Scan# 1271
Delta R.T. 0.00 min
Lab File: VX014859.D
Acq: 06 Feb 2020 19:40

Tgt Ion: 43 Resp: 9738
Ion Ratio Lower Upper
43 100
58 35.6 31.6 47.4

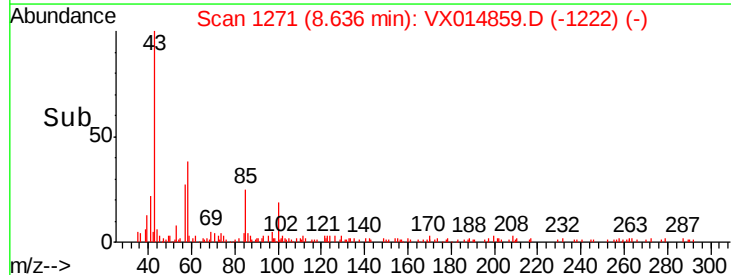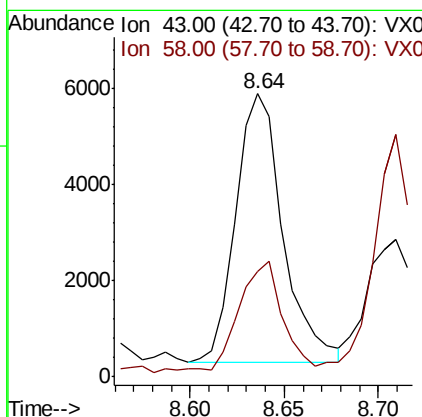

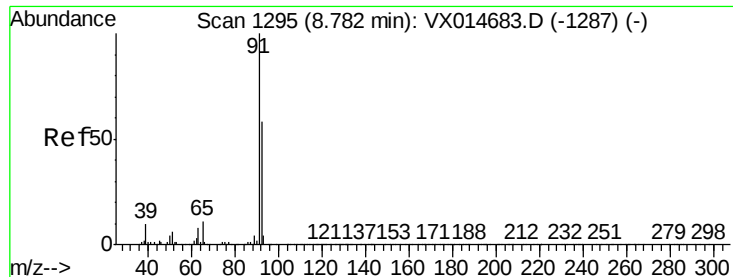

#52

Toluene

Concen: 23.933 ug/l

RT: 8.78 min Scan# 1294

Delta R.T. -0.01 min

Lab File: VX014859.D

Acq: 06 Feb 2020 19:40





Instrument :
MSVOA_X
ClientSampled :

Tot Ion: 92 Resp: 311900

Ion Ratio Lower Upper

92 100

91 173.4 135.9 203.9

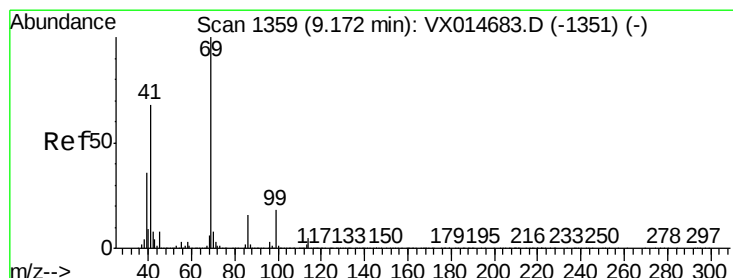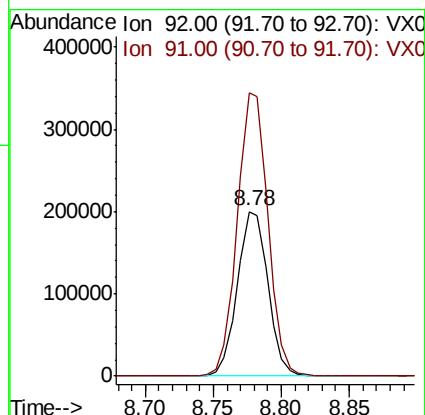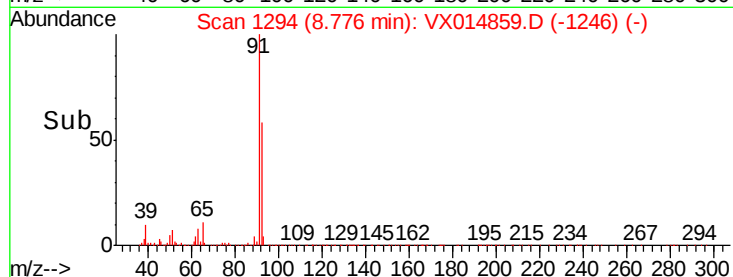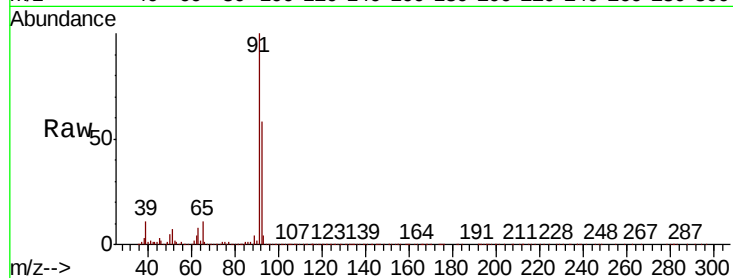

#56

Ethyl methacrylate

Concen: 1.813 ug/l

RT: 9.15 min Scan# 1356

Delta R.T. -0.02 min

Lab File: VX014859.D

Acq: 06 Feb 2020 19:40




Tgt Ion: 69 Resp: 271


Ion Ratio Lower Upper

69 100

41 0.0 54.9 82.3#

39 138.0 29.3 43.9#


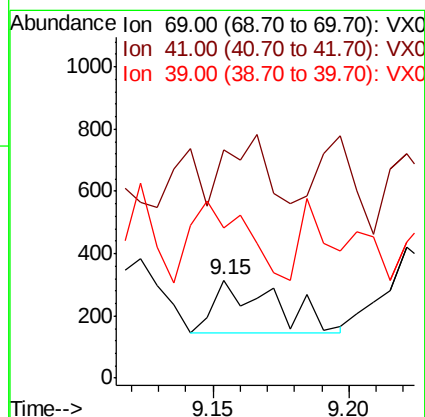
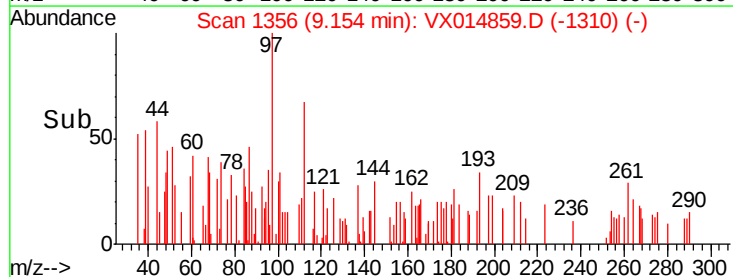
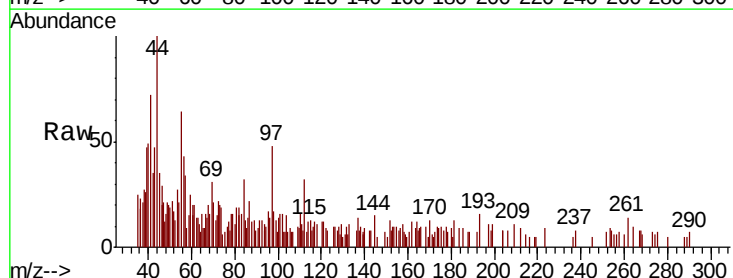




#59
2-Hexanone
Concen: 0.816 ug/l
RT: 9.49 min Scan# 1411
Delta R.T. 0.01 min
Lab File: VX014859.D
Acq: 06 Feb 2020 19:40




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion: 43 Resp: 5142
Ion Ratio Lower Upper
43 100
58 61.6 27.2 81.5

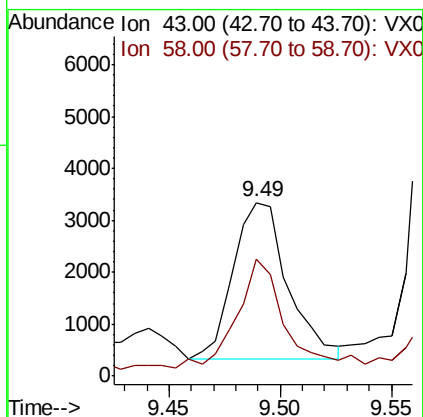

#62
4-Bromofluorobenzene
Concen: 50.503 ug/l
RT: 11.13 min Scan# 1680
Delta R.T. -0.01 min
Lab File: VX014859.D
Acq: 06 Feb 2020 19:40

Tgt Ion: 95 Resp: 322256
Ion Ratio Lower Upper
95 100
174 90.7 0.0 176.0
176 87.9 0.0 172.2



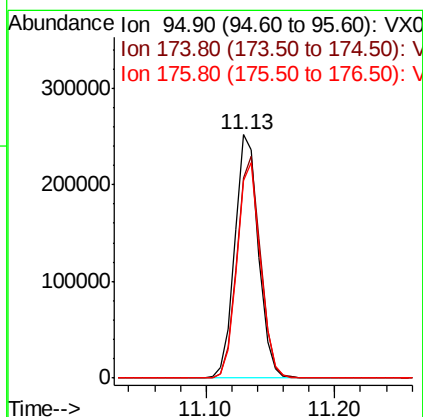





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1512
Delta R.T. -0.01 min
Lab File: VX014859.D
Acq: 06 Feb 2020 19:40




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
117	100		
82	55.4	43.2	64.8
119	32.2	25.8	38.6

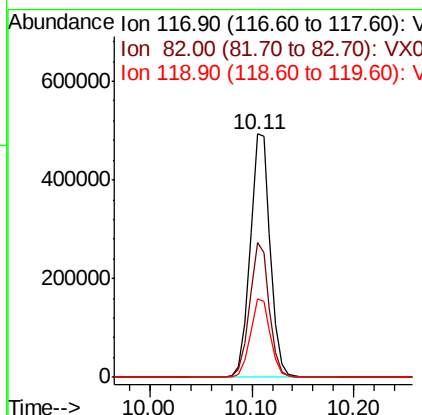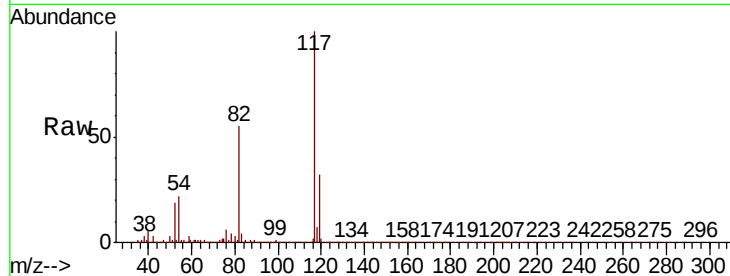

#67
Ethyl Benzene
Concen: 0.515 ug/l
RT: 10.25 min Scan# 1536
Delta R.T. 0.01 min
Lab File: VX014859.D
Acq: 06 Feb 2020 19:40

Tgt Ion	Ratio	Lower	Upper
91	100		
106	33.7	24.9	37.3

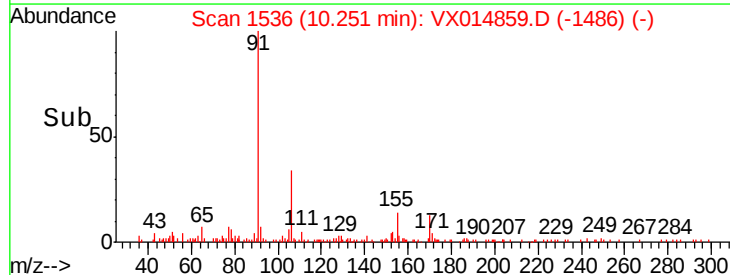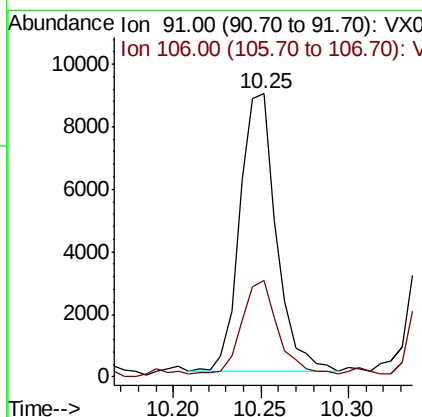



#68

m/p-Xylenes

Concen: 1.446 ug/l

RT: 10.36 min Scan# 1553

Delta R.T. 0.00 min

Lab File: VX014859.D

Acq: 06 Feb 2020 19:40

Instrument :

MSVOA_X


ClientSampleId :

Tot Ion:106 Resp: 13581

Ion Ratio Lower Upper




106 100

91 193.0 159.4 239.2



Abundance Ion 106.00 (105.70 to 106.70): V

Ion 91.00 (90.70 to 91.70): VX0

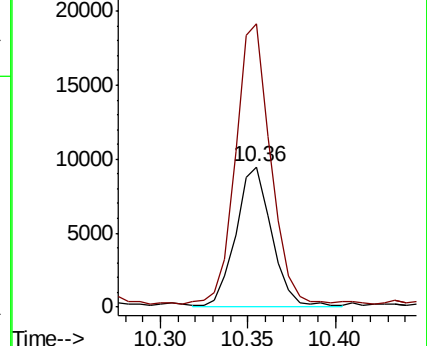

#69

o-Xylene

Concen: 0.867 ug/l

RT: 10.70 min Scan# 1609

Delta R.T. 0.00 min

Lab File: VX014859.D


Acq: 06 Feb 2020 19:40

Tgt Ion:106 Resp: 7854

Ion Ratio Lower Upper



106 100


91 230.1 106.2 318.6



Abundance Ion 106.00 (105.70 to 106.70): V

Ion 91.00 (90.70 to 91.70): VX0



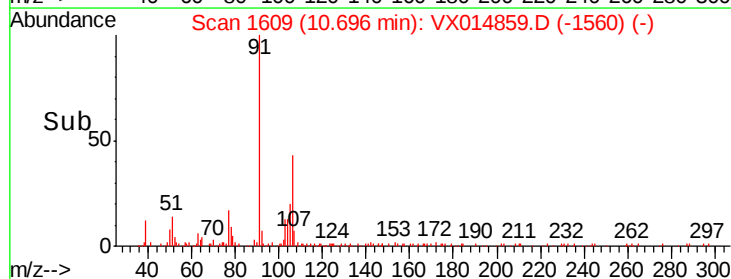
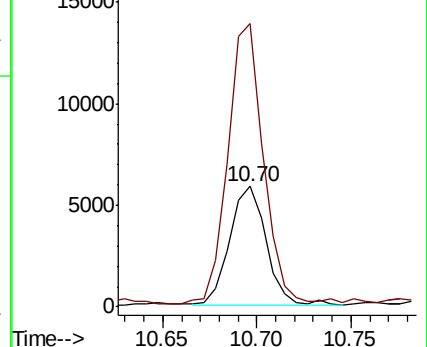


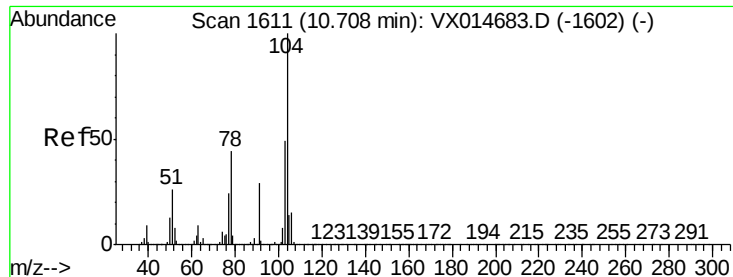

#70
Stvrene
Concen: 0.487 ug/l
RT: 10.71 min Scan# 1611
Delta R.T. 0.00 min
Lab File: VX014859.D
Acq: 06 Feb 2020 19:40




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
104	100		
78	60.5	39.3	58.9#
103	62.1	43.5	65.3

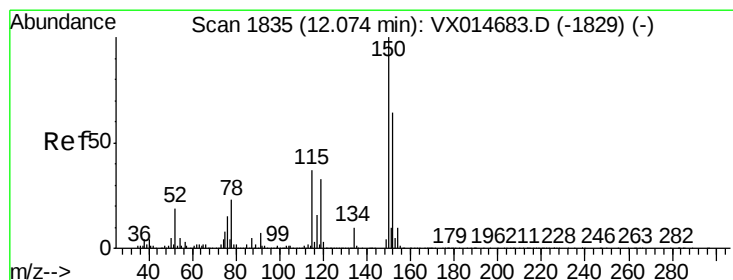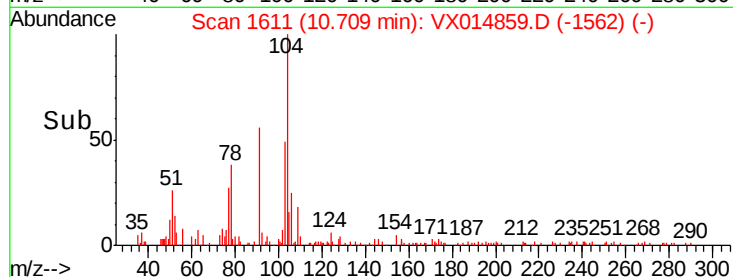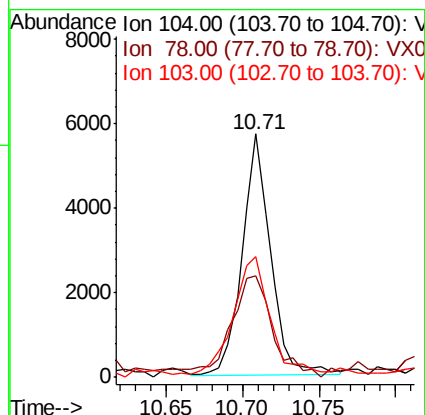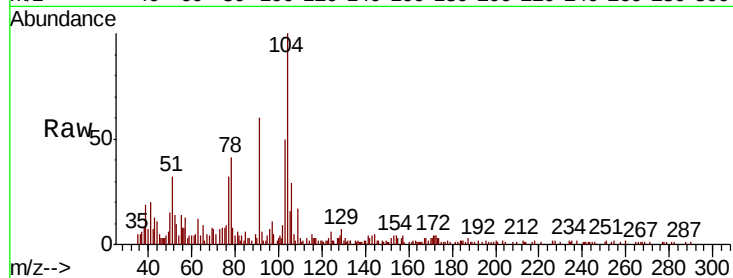

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.07 min Scan# 1835
Delta R.T. 0.00 min
Lab File: VX014859.D
Acq: 06 Feb 2020 19:40

Tgt Ion	Ratio	Lower	Upper
152	100		
115	54.8	39.4	118.1
150	155.1	0.0	351.2

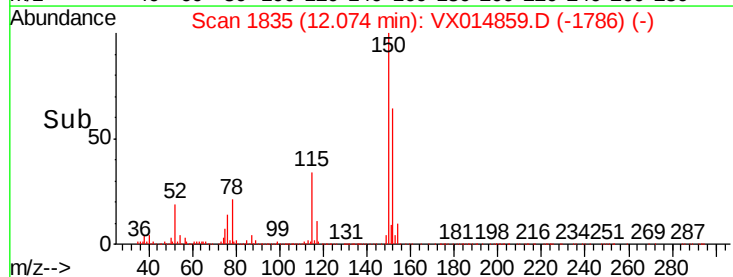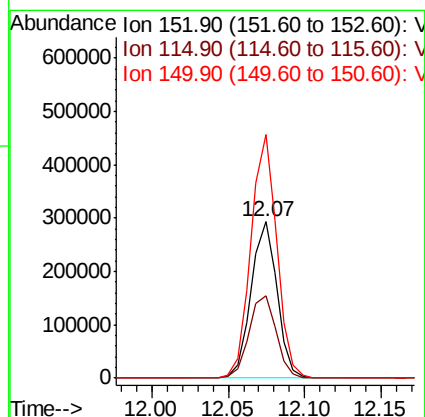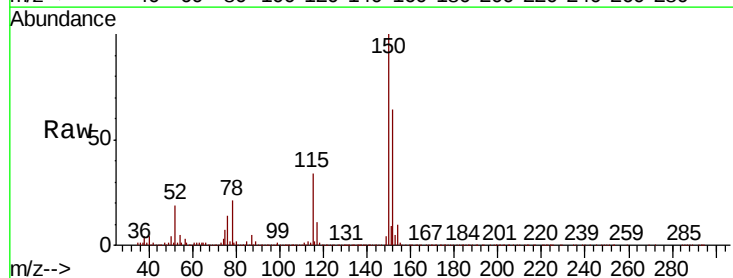



#76

1,2,3-Trichloropropane

Concen: 19.893 ug/l

RT: 11.13 min Scan# 1680

Delta R.T. -0.16 min

Lab File: VX014859.D

Acq: 06 Feb 2020 19:40

Instrument :

MSVOA_X





ClientSampled :

Tot Ion: 75 Resp: 159674

Ion Ratio Lower Upper

75 100

77 1.1 18.7 56.1#

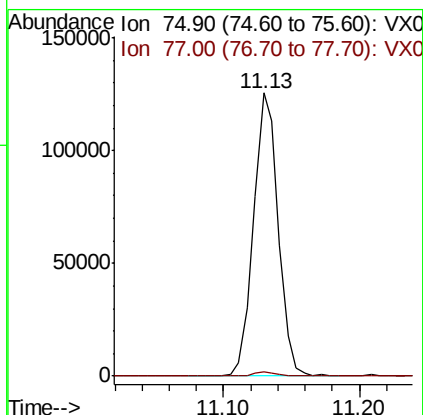

#81

trans-1,4-Dichloro-2-butene

Concen: 56.611 ug/l

RT: 11.13 min Scan# 1680

Delta R.T. 0.06 min

Lab File: VX014859.D

Acq: 06 Feb 2020 19:40




Tgt Ion: 75 Resp: 159674


Ion Ratio Lower Upper

75 100

53 0.0 78.8 118.2#

89 0.0 35.4 53.0#

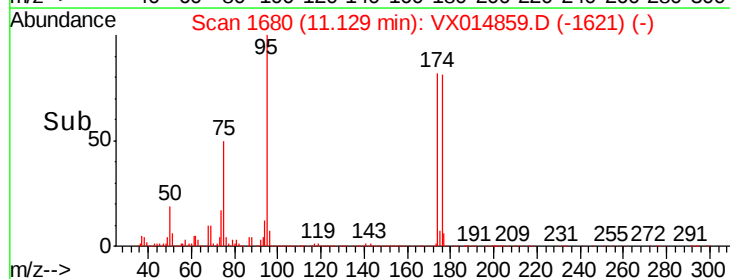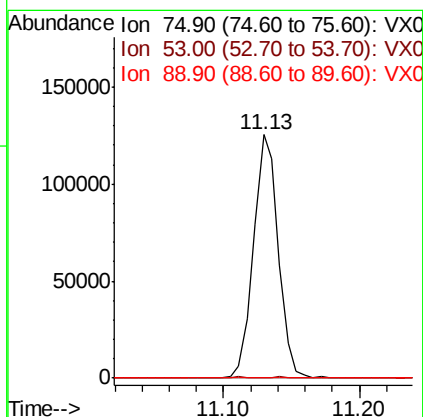



#84

1,2,4-Trimethylbenzene

Concen: 0.564 ug/l

RT: 11.80 min Scan# 1790

Delta R.T. -0.01 min

Lab File: VX014859.D

Acq: 06 Feb 2020 19:40

Instrument :

MSVOA_X


ClientSampleId :

Tot Ion:105 Resp: 11386

Ion Ratio Lower Upper




105 100

120 29.9 23.4 70.0

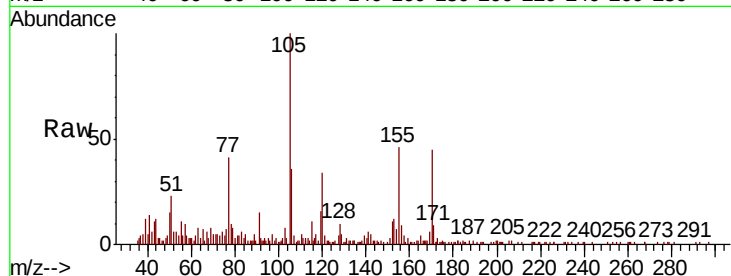

Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

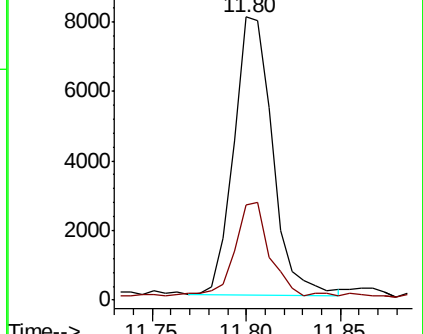

#95

Naphthalene

Concen: 1.711 ug/l

RT: 13.83 min Scan# 2123

Delta R.T. 0.00 min

Lab File: VX014859.D

Acq: 06 Feb 2020 19:40


Tgt Ion:128 Resp: 19214

Ion Ratio Lower Upper

128 100

127 11.3 10.3 15.5

129 13.4 8.6 12.8#



Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

