

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020623\
 Data File : VX034019.D
 Acq On : 06 Feb 2023 10:02
 Operator : JC/MD
 Sample : VX0206MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK612

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M

Title : VOC Analysis

Signal : TIC: VX034019.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	60	rVB	88448	103031	12.43%	1.584%
2	1.666	91	95	114	rVB	63066	86838	10.48%	1.335%
3	2.184	178	180	182	rBV	186	111	0.01%	0.002%
4	2.306	194	200	210	rBV	190384	291390	35.17%	4.481%
5	2.514	230	234	240	rVB	1206	2170	0.26%	0.033%
6	2.642	254	255	258	rBV	178	127	0.02%	0.002%
7	2.788	274	279	285	rVB2	1085	2039	0.25%	0.031%
8	2.873	288	293	294	rBV2	145	202	0.02%	0.003%
9	2.934	299	303	311	rVB4	664	1629	0.20%	0.025%
10	3.014	311	316	318	rBV	133	212	0.03%	0.003%
11	3.087	322	328	333	rBV4	611	1021	0.12%	0.016%
12	3.136	333	336	338	rVB2	108	145	0.02%	0.002%
13	3.203	345	347	351	rVB2	130	156	0.02%	0.002%
14	3.337	366	369	371	rVB2	176	232	0.03%	0.004%
15	3.367	371	374	376	rBV2	173	220	0.03%	0.003%
16	3.495	393	395	398	rVB	163	131	0.02%	0.002%
17	3.538	399	402	404	rBV	142	168	0.02%	0.003%
18	3.617	413	415	418	rBV	197	248	0.03%	0.004%
19	3.690	424	427	430	rVB	191	262	0.03%	0.004%
20	3.837	446	451	454	rBV2	68	125	0.02%	0.002%
21	3.946	465	469	470	rBV2	93	150	0.02%	0.002%
22	4.026	479	482	484	rBV2	147	204	0.02%	0.003%
23	4.215	511	513	518	rVB2	107	138	0.02%	0.002%
24	4.300	525	527	530	rBV2	116	140	0.02%	0.002%
25	4.446	543	551	566	rBV	56652	162803	19.65%	2.503%
26	4.696	590	592	594	rBV	185	152	0.02%	0.002%
27	4.763	602	603	606	rBV	172	185	0.02%	0.003%
28	4.879	621	622	623	rBV	193	113	0.01%	0.002%
29	5.056	638	651	667	rBV	107475	329249	39.73%	5.063%
30	5.208	675	676	678	rBV	183	125	0.02%	0.002%
31	5.391	700	706	708	rBV2	367	680	0.08%	0.010%
32	5.458	716	717	721	rBV2	251	310	0.04%	0.005%
33	5.550	725	732	743	rVB3	756	2376	0.29%	0.037%
34	5.757	764	766	769	rBV2	118	139	0.02%	0.002%
35	5.812	773	775	777	rVB	221	178	0.02%	0.003%
36	5.836	777	779	781	rBV	199	186	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020623\
 Data File : VX034019.D
 Acq On : 06 Feb 2023 10:02
 Operator : JC/MD
 Sample : VX0206MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK612

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
 Title : VOC Analysis

37	5.964	788	800	816	rBV2	279385	828634	100.00%	12.742%
38	6.178	833	835	839	rVB	168	194	0.02%	0.003%
39	6.263	847	849	852	rBV	136	135	0.02%	0.002%
40	6.476	882	884	885	rBV	173	156	0.02%	0.002%
41	6.757	919	930	950	rBV	240989	567980	68.54%	8.734%
42	7.123	983	990	995	rVB6	1381	3093	0.37%	0.048%
43	7.238	1008	1009	1011	rBV	170	119	0.01%	0.002%
44	7.306	1011	1020	1032	rBV	171611	373332	45.05%	5.741%
45	7.415	1036	1038	1043	rVB	162	242	0.03%	0.004%
46	7.488	1043	1050	1054	rBV3	399	879	0.11%	0.014%
47	7.562	1059	1062	1066	rBV	134	196	0.02%	0.003%
48	7.647	1073	1076	1080	rVB	145	180	0.02%	0.003%
49	7.690	1080	1083	1085	rBV2	138	152	0.02%	0.002%
50	7.872	1111	1113	1115	rBV	131	133	0.02%	0.002%
51	8.031	1137	1139	1142	rVB2	147	139	0.02%	0.002%
52	8.324	1180	1187	1200	rBV	121023	194545	23.48%	2.992%
53	8.458	1207	1209	1211	rBV	165	196	0.02%	0.003%
54	8.531	1218	1221	1222	rBV2	122	139	0.02%	0.002%
55	8.647	1233	1240	1256	rBV	446781	707180	85.34%	10.874%
56	8.830	1268	1270	1275	rVB2	285	345	0.04%	0.005%
57	8.945	1284	1289	1299	rBV	84875	126772	15.30%	1.949%
58	9.183	1326	1328	1330	rBV	151	116	0.01%	0.002%
59	9.208	1330	1332	1334	rBV	168	161	0.02%	0.002%
60	9.275	1340	1343	1348	rVB2	766	873	0.11%	0.013%
61	9.384	1355	1361	1379	rBV	236765	355613	42.92%	5.468%
62	9.610	1397	1398	1401	rBV2	278	298	0.04%	0.005%
63	9.695	1409	1412	1413	rBV2	197	175	0.02%	0.003%
64	9.762	1420	1423	1426	rBV2	143	234	0.03%	0.004%
65	9.817	1429	1432	1437	rBV2	135	258	0.03%	0.004%
66	9.903	1444	1446	1449	rBV	161	187	0.02%	0.003%
67	9.988	1457	1460	1462	rBV2	103	146	0.02%	0.002%
68	10.049	1465	1470	1480	rBV	449006	632127	76.29%	9.720%
69	10.201	1492	1495	1498	rVB	689	742	0.09%	0.011%
70	10.305	1508	1512	1516	rVB	818	955	0.12%	0.015%
71	10.366	1520	1522	1526	rBV2	117	128	0.02%	0.002%
72	10.421	1529	1531	1533	rBV	135	139	0.02%	0.002%
73	10.585	1557	1558	1561	rBV	160	179	0.02%	0.003%
74	10.659	1564	1570	1575	rBV3	688	1239	0.15%	0.019%
75	10.713	1578	1579	1581	rBV2	123	129	0.02%	0.002%
76	10.811	1592	1595	1597	rVB2	189	200	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020623\
 Data File : VX034019.D
 Acq On : 06 Feb 2023 10:02
 Operator : JC/MD
 Sample : VX0206MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK612

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
 Title : VOC Analysis

77	10.854	1597	1602	1603	rBV2	149	265	0.03%	0.004%
78	10.963	1617	1620	1626	rVB3	538	812	0.10%	0.012%
79	11.085	1638	1640	1645	rVB2	317	365	0.04%	0.006%
80	11.189	1652	1657	1666	rBV	311498	394757	47.64%	6.070%
81	11.317	1674	1678	1683	rVB3	575	918	0.11%	0.014%
82	11.366	1683	1686	1688	rBV	152	197	0.02%	0.003%
83	11.451	1696	1700	1705	rVV4	701	939	0.11%	0.014%
84	11.713	1740	1743	1745	rVB	368	388	0.05%	0.006%
85	11.750	1746	1749	1753	rVB	790	917	0.11%	0.014%
86	11.786	1753	1755	1757	rBV	100	132	0.02%	0.002%
87	11.969	1781	1785	1788	rBV2	1260	1707	0.21%	0.026%
88	12.024	1788	1794	1807	rVV	499781	647194	78.10%	9.952%
89	12.317	1837	1842	1850	rBV	504788	650531	78.51%	10.003%
90	12.768	1912	1916	1920	rVB3	1222	1666	0.20%	0.026%
91	13.115	1970	1973	1978	rBV2	1575	1870	0.23%	0.029%
92	13.591	2047	2051	2056	rVB	2278	2951	0.36%	0.045%
93	13.780	2078	2082	2087	rVB	2391	2934	0.35%	0.045%
94	13.963	2109	2112	2118	rVB	2202	2767	0.33%	0.043%
95	14.042	2122	2125	2127	rBV2	182	247	0.03%	0.004%
96	14.134	2135	2140	2144	rBV	1179	1692	0.20%	0.026%
97	14.262	2159	2161	2162	rVB	218	116	0.01%	0.002%
98	14.597	2207	2216	2217	rBV4	1588	3130	0.38%	0.048%
99	15.066	2291	2293	2294	rBV	324	179	0.02%	0.003%
100	15.365	2341	2342	2344	rBV	415	346	0.04%	0.005%




Sum of corrected areas: 6503245

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020623\
Data File : VX034019.D
Acq On : 06 Feb 2023 10:02
Operator : JC/MD
Sample : VX0206MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK612

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

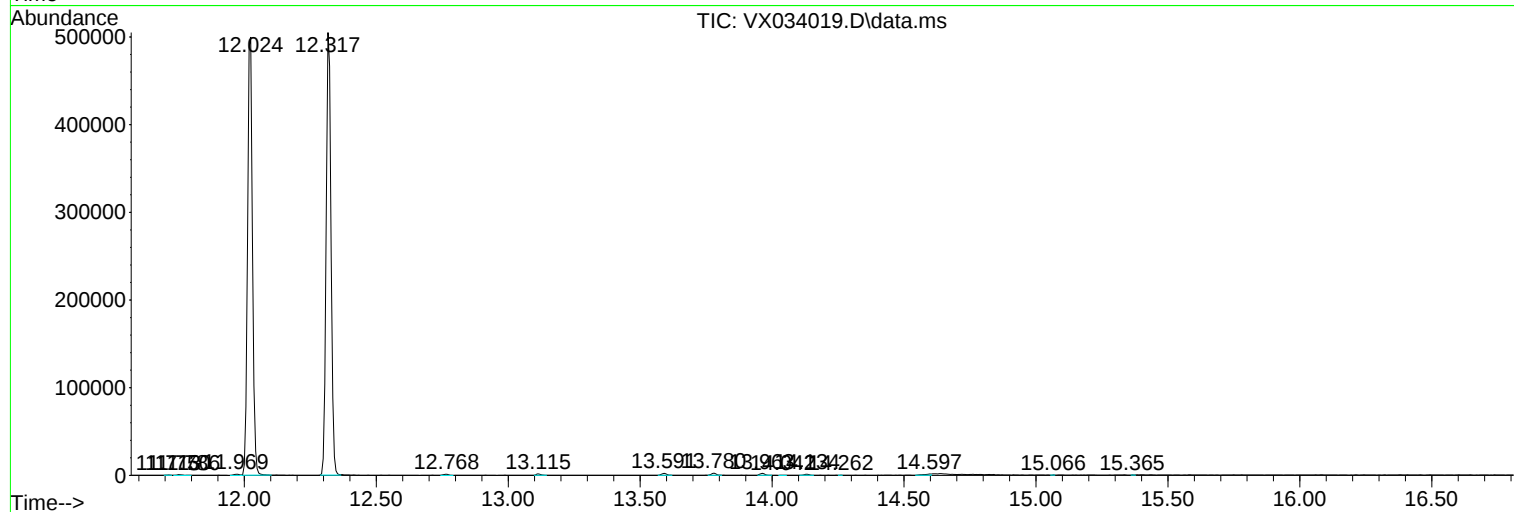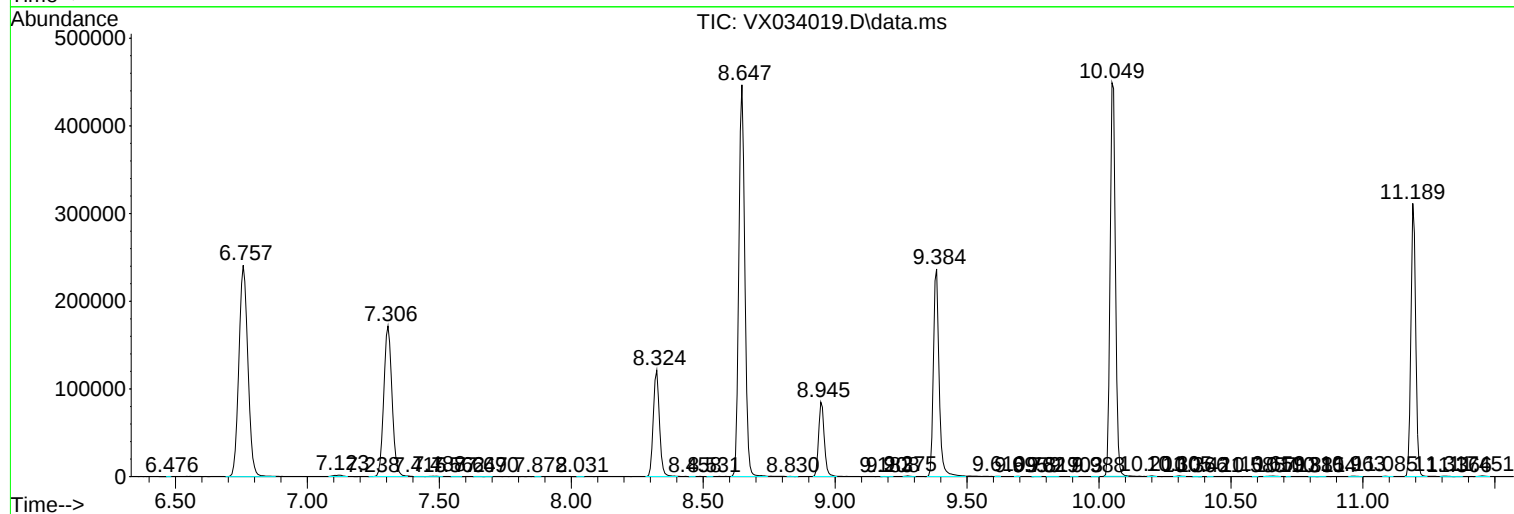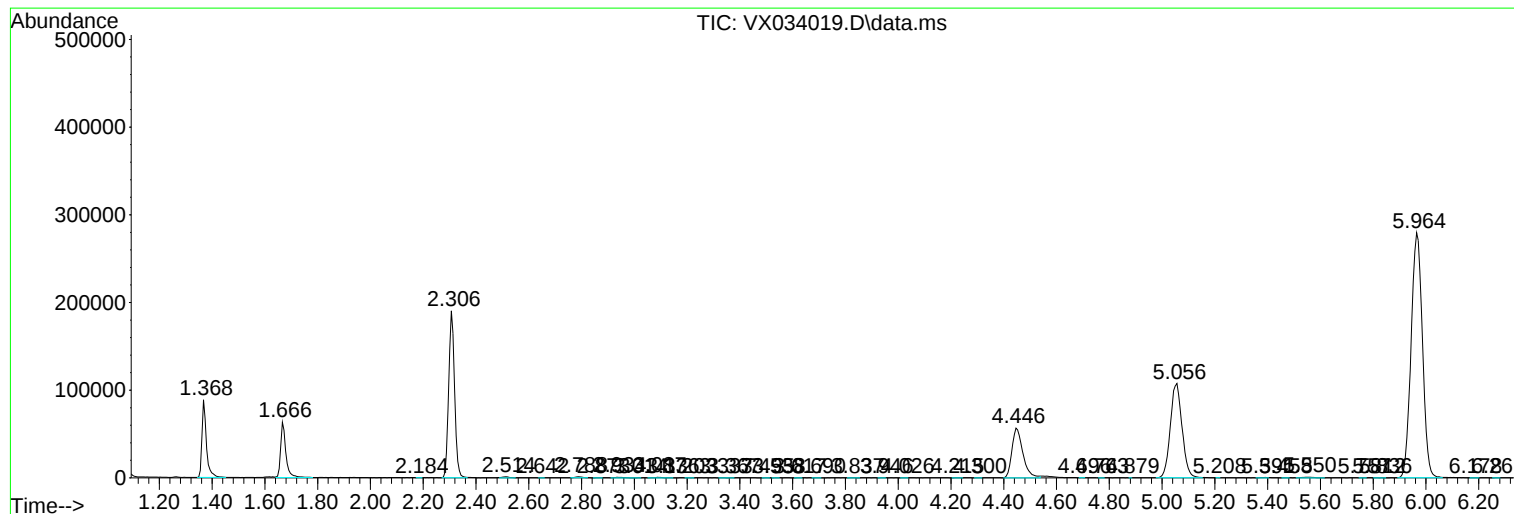

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020623\
Data File : VX034019.D
Acq On : 06 Feb 2023 10:02
Operator : JC/MD
Sample : VX0206MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK612

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020623\
Data File : VX034019.D
Acq On : 06 Feb 2023 10:02
Operator : JC/MD
Sample : VX0206MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK612

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc