

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020623\
 Data File : VX034020.D
 Acq On : 06 Feb 2023 10:25
 Operator : JC/MD
 Sample : VX0206WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK613

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
 Title : VOC Analysis

Signal : TIC: VX034020.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	31	rVB3	1049	969	0.14%	0.018%
2	1.367	42	46	58	rBV	73840	83501	11.99%	1.551%
3	1.666	91	95	113	rVB	48635	69813	10.02%	1.297%
4	2.020	151	153	154	rBV	158	108	0.02%	0.002%
5	2.306	194	200	212	rBV	156109	244135	35.05%	4.536%
6	2.520	229	235	241	rVB2	627	1153	0.17%	0.021%
7	2.642	254	255	257	rBV	167	132	0.02%	0.002%
8	2.757	272	274	275	rBV	100	84	0.01%	0.002%
9	2.788	275	279	286	rVB4	1093	2075	0.30%	0.039%
10	2.843	286	288	290	rBV	176	188	0.03%	0.003%
11	2.898	294	297	299	rBV2	160	154	0.02%	0.003%
12	2.946	299	305	311	rBV3	593	1375	0.20%	0.026%
13	3.093	327	329	332	rBV2	270	273	0.04%	0.005%
14	3.142	335	337	339	rBV	106	119	0.02%	0.002%
15	3.276	356	359	362	rBV2	164	253	0.04%	0.005%
16	3.318	362	366	367	rVV2	92	111	0.02%	0.002%
17	3.404	379	380	382	rBV	150	114	0.02%	0.002%
18	3.477	390	392	395	rVB2	125	109	0.02%	0.002%
19	3.574	405	408	410	rVB2	110	106	0.02%	0.002%
20	3.605	410	413	416	rBV	113	135	0.02%	0.003%
21	3.672	419	424	427	rVB2	199	396	0.06%	0.007%
22	3.702	427	429	430	rBV	206	152	0.02%	0.003%
23	3.958	468	471	472	rBV	122	114	0.02%	0.002%
24	4.013	477	480	484	rBV2	108	219	0.03%	0.004%
25	4.141	500	501	504	rBB	119	94	0.01%	0.002%
26	4.166	504	505	506	rBV	158	96	0.01%	0.002%
27	4.239	516	517	520	rBV	134	126	0.02%	0.002%
28	4.294	524	526	527	rBV	175	114	0.02%	0.002%
29	4.349	533	535	538	rBV	130	172	0.02%	0.003%
30	4.452	543	552	566	rBV	46906	135127	19.40%	2.511%
31	4.800	608	609	611	rBV	117	101	0.01%	0.002%
32	4.891	621	624	625	rBV	114	122	0.02%	0.002%
33	5.056	638	651	667	rBV2	88403	275042	39.49%	5.110%
34	5.342	695	698	699	rBV2	111	116	0.02%	0.002%
35	5.373	699	703	704	rBV	443	563	0.08%	0.010%
36	5.470	716	719	722	rBV	247	288	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020623\
 Data File : VX034020.D
 Acq On : 06 Feb 2023 10:25
 Operator : JC/MD
 Sample : VX0206WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK613

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
 Title : VOC Analysis

37	5.556	726	733	741	rBV2	1609	4204	0.60%	0.078%
38	5.970	789	801	814	rBV2	234590	696465	100.00%	12.940%
39	6.312	855	857	860	rVB	123	106	0.02%	0.002%
40	6.342	860	862	865	rVB	178	168	0.02%	0.003%
41	6.379	865	868	870	rBV	159	189	0.03%	0.004%
42	6.415	872	874	875	rBV	188	98	0.01%	0.002%
43	6.458	880	881	884	rVB	155	100	0.01%	0.002%
44	6.543	893	895	898	rBV2	178	197	0.03%	0.004%
45	6.641	910	911	915	rBV	138	160	0.02%	0.003%
46	6.678	915	917	921	rBV2	88	108	0.02%	0.002%
47	6.757	921	930	943	rBV	197218	476719	68.45%	8.857%
48	7.068	979	981	983	rVB	247	151	0.02%	0.003%
49	7.110	983	988	989	rBV3	1281	1786	0.26%	0.033%
50	7.305	1011	1020	1033	rBV	144410	312588	44.88%	5.808%
51	7.476	1045	1048	1049	rBV	188	206	0.03%	0.004%
52	7.610	1068	1070	1071	rBV	129	107	0.02%	0.002%
53	7.830	1102	1106	1109	rBV2	183	231	0.03%	0.004%
54	7.860	1109	1111	1114	rVB2	174	129	0.02%	0.002%
55	7.952	1125	1126	1128	rVB	217	128	0.02%	0.002%
56	7.982	1128	1131	1135	rBV2	132	221	0.03%	0.004%
57	8.037	1138	1140	1143	rBV2	154	158	0.02%	0.003%
58	8.086	1147	1148	1151	rBV2	156	147	0.02%	0.003%
59	8.324	1181	1187	1198	rBV	99004	158370	22.74%	2.943%
60	8.543	1220	1223	1226	rVB2	166	205	0.03%	0.004%
61	8.567	1226	1227	1228	rBV	226	147	0.02%	0.003%
62	8.647	1234	1240	1251	rBV	372677	585739	84.10%	10.883%
63	8.878	1273	1278	1280	rBV2	160	294	0.04%	0.005%
64	8.951	1284	1290	1298	rBV	66930	100708	14.46%	1.871%
65	9.183	1326	1328	1331	rBV2	116	114	0.02%	0.002%
66	9.275	1339	1343	1346	rVB2	742	871	0.13%	0.016%
67	9.384	1356	1361	1378	rBV	200120	293260	42.11%	5.449%
68	9.957	1453	1455	1457	rVB	111	94	0.01%	0.002%
69	9.976	1457	1458	1459	rBV	186	103	0.01%	0.002%
70	10.055	1465	1471	1481	rBV	373092	527004	75.67%	9.792%
71	10.165	1487	1489	1490	rBV2	183	90	0.01%	0.002%
72	10.195	1492	1494	1498	rVB	425	540	0.08%	0.010%
73	10.311	1509	1513	1517	rVB3	557	837	0.12%	0.016%
74	10.390	1525	1526	1529	rBV2	156	173	0.02%	0.003%
75	10.482	1539	1541	1542	rBV	168	122	0.02%	0.002%
76	10.591	1557	1559	1560	rBV	115	93	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020623\
 Data File : VX034020.D
 Acq On : 06 Feb 2023 10:25
 Operator : JC/MD
 Sample : VX0206WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK613

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
 Title : VOC Analysis

77	10.646	1564	1568	1569	rBV2	401	474	0.07%	0.009%
78	10.756	1584	1586	1587	rBV	124	109	0.02%	0.002%
79	10.774	1587	1589	1590	rVV	192	144	0.02%	0.003%
80	10.963	1617	1620	1626	rVB3	357	576	0.08%	0.011%
81	11.091	1638	1641	1645	rVB2	374	436	0.06%	0.008%
82	11.189	1652	1657	1666	rBV	248017	328862	47.22%	6.110%
83	11.457	1697	1701	1703	rVB2	560	627	0.09%	0.012%
84	11.640	1729	1731	1733	rBV	133	162	0.02%	0.003%
85	11.756	1747	1750	1754	rVB2	451	449	0.06%	0.008%
86	11.890	1769	1772	1776	rBB2	170	233	0.03%	0.004%
87	11.975	1783	1786	1788	rBV2	604	602	0.09%	0.011%
88	12.024	1788	1794	1806	rVV	402595	533070	76.54%	9.904%
89	12.256	1830	1832	1837	rVB2	123	143	0.02%	0.003%
90	12.317	1837	1842	1851	rBV	398955	529589	76.04%	9.840%
91	12.762	1912	1915	1919	rVB3	875	1093	0.16%	0.020%
92	13.109	1970	1972	1976	rVB	412	458	0.07%	0.009%
93	13.591	2048	2051	2055	rBV	864	869	0.12%	0.016%
94	13.743	2074	2076	2078	rBV	206	148	0.02%	0.003%
95	13.786	2079	2083	2089	rVB	560	829	0.12%	0.015%
96	13.963	2110	2112	2117	rVB3	665	786	0.11%	0.015%
97	14.127	2135	2139	2144	rBV2	847	1195	0.17%	0.022%
98	14.225	2154	2155	2157	rBV2	99	99	0.01%	0.002%
99	14.603	2215	2217	2218	rVB	201	102	0.01%	0.002%
100	15.676	2391	2393	2394	rBV	369	192	0.03%	0.004%




Sum of corrected areas: 5382126

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020623\
Data File : VX034020.D
Acq On : 06 Feb 2023 10:25
Operator : JC/MD
Sample : VX0206WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK613

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

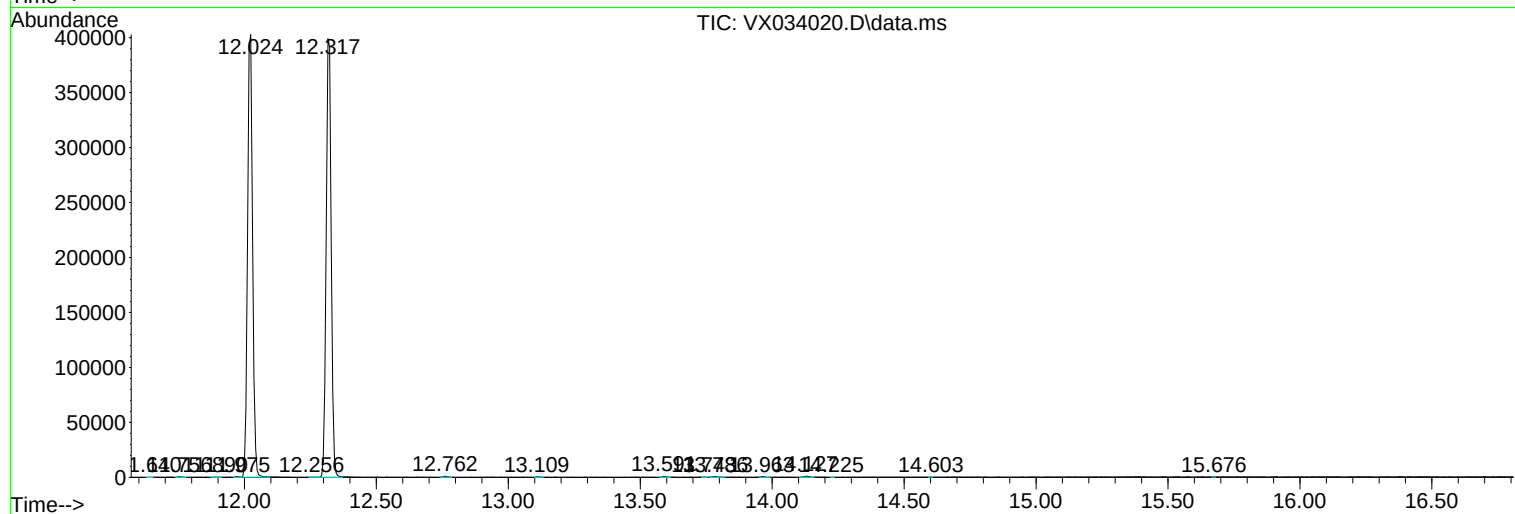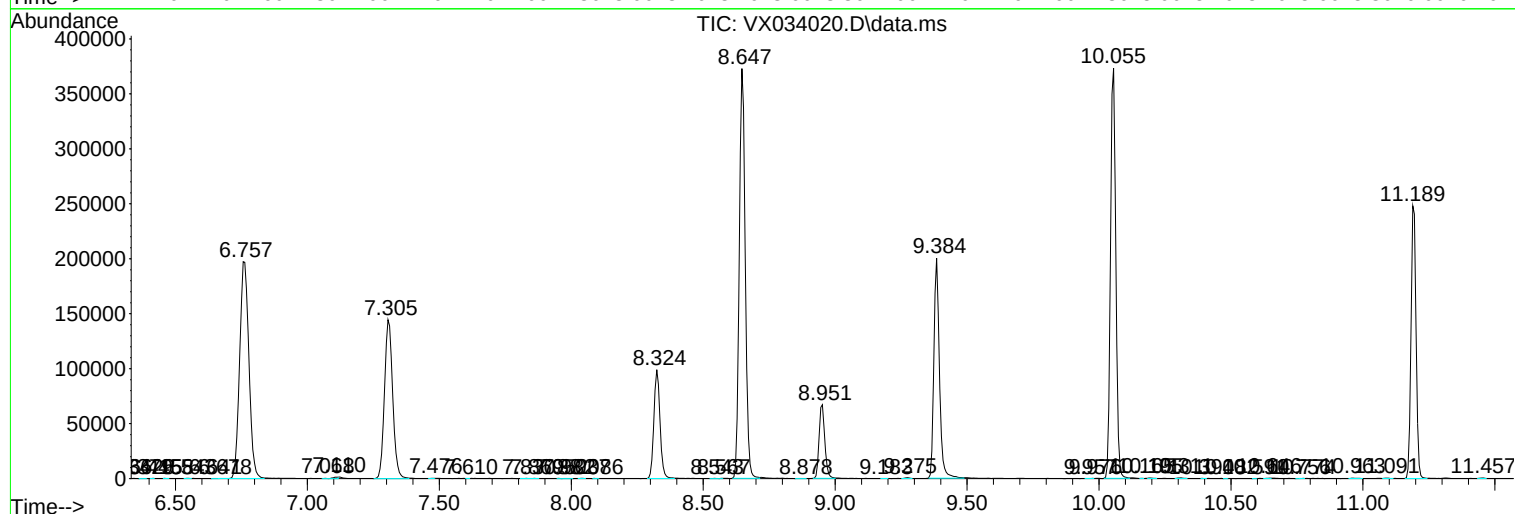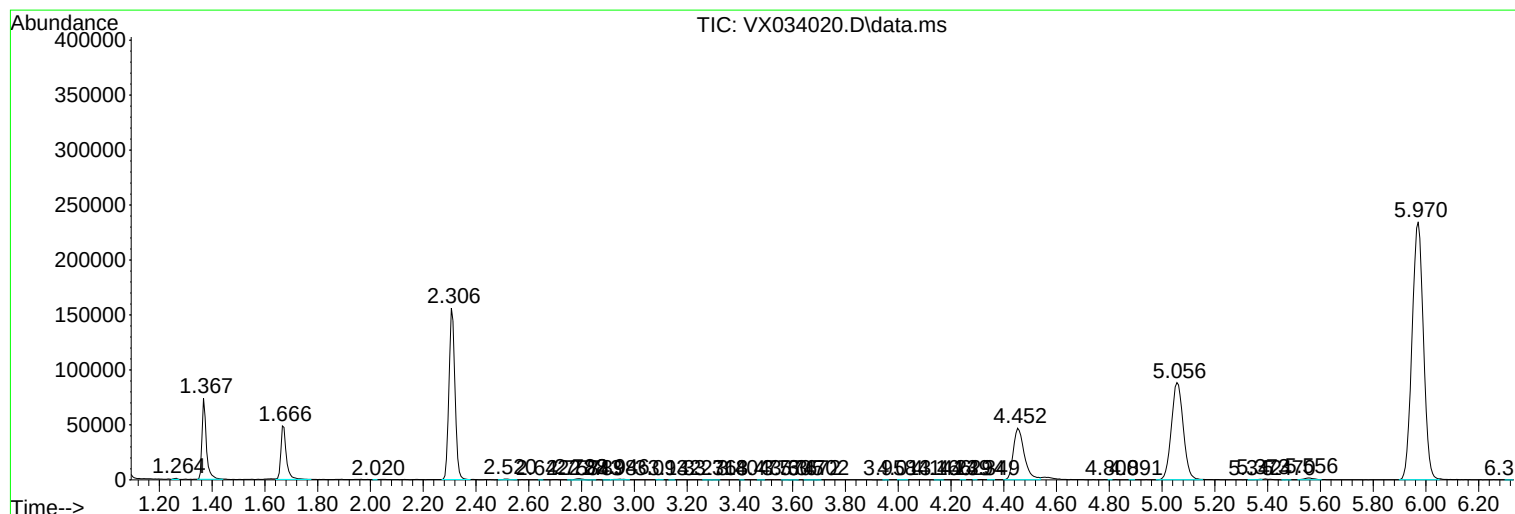

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020623\
Data File : VX034020.D
Acq On : 06 Feb 2023 10:25
Operator : JC/MD
Sample : VX0206WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK613

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020623\
Data File : VX034020.D
Acq On : 06 Feb 2023 10:25
Operator : JC/MD
Sample : VX0206WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK613

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------