


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX020720\
 Data File : VX014861.D
 Acq On : 07 Feb 2020 08:25
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X011520W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Wed Jan 15 12:41:12 2020

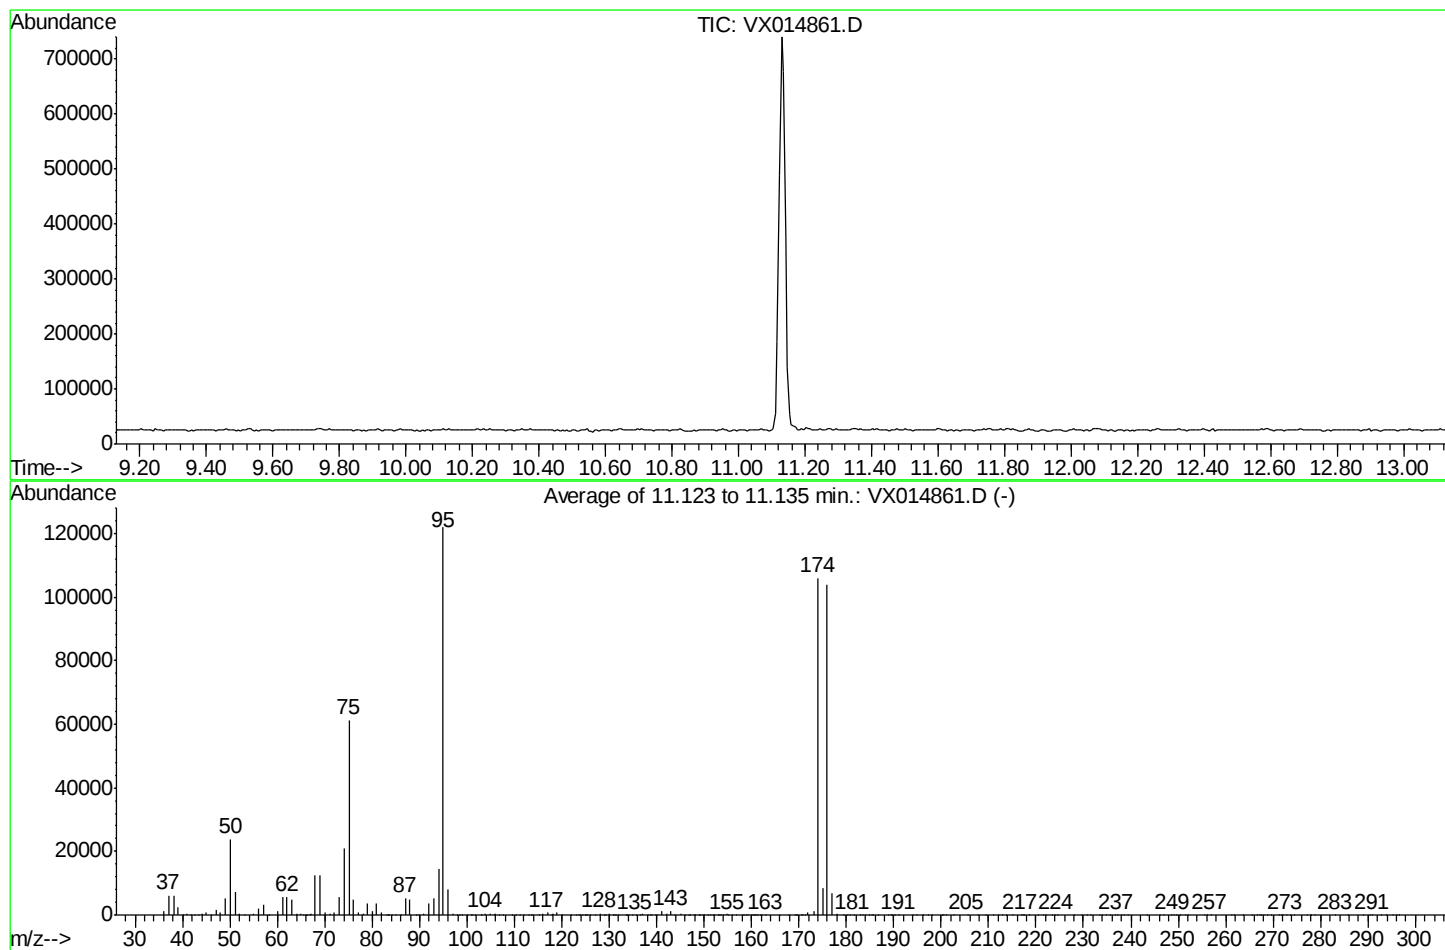

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1674

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	23936	PASS
75	95	30	60	50.3	61353	PASS
95	95	100	100	100.0	121946	PASS
96	95	5	9	6.7	8118	PASS
173	174	0.00	2	1.3	1343	PASS
174	95	50	100	87.0	106096	PASS
175	174	5	9	7.9	8415	PASS
176	174	95	101	97.8	103803	PASS
177	176	5	9	6.7	6991	PASS