

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020722\
 Data File : VX026798.D
 Acq On : 07 Feb 2022 20:30
 Operator : JC/MD
 Sample : N1342-25
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 31540

Manual Integrations
 APPROVED

Reviewed By : John Carlone 02/08/2022
 Supervised By : Mahesh Dadoda 02/08/2022

Quant Time: Feb 07 23:34:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 11 14:45:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	154027	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	241918	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.061	117	195704	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.042	152	96769	50.000	ug/l	0.02
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.970	65	88589	41.173	ug/l	0.01
Spiked Amount 50.000	Range 78 - 117		Recovery =	82.340%		
35) Dibromofluoromethane	5.397	113	70277	44.985	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	89.980%		
50) Toluene-d8	8.659	98	268824	47.752	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	95.500%		
62) 4-Bromofluorobenzene	11.085	95	106778	53.393	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	106.780%		
Target Compounds					Qvalue	
8) Diethyl Ether	2.136	74	1363920	1394.594	ug/l	63
11) Tert butyl alcohol	3.007	59	2038442	6810.315	ug/l #	75
16) Acetone	2.386	43	1229202	1120.253	ug/l	96
18) Methyl Acetate	2.709	43	314973	144.391	ug/l	95
19) Methyl tert-butyl Ether	3.117	73	429756	73.629	ug/l	91
20) Methylene Chloride	2.794	84	2653	1.463	ug/l #	87
25) 2-Butanone	4.562	43	765778	536.655	ug/l	97
29) Tetrahydrofuran	5.013	42	33418	39.432	ug/l	92
31) Cyclohexane	5.476	56	88573	27.909	ug/l	98
37) Ethyl Acetate	4.721	43	39424	15.803	ug/l	96
39) Methylcyclohexane	7.385	83	63014	21.183	ug/l	95
40) Benzene	6.062	78	8945183	1312.264	ug/l	94
43) Isopropyl Acetate	6.348	43	398532	98.894	ug/l	94
49) 1,4-Dioxane	7.696	88	209326	6386.894	ug/l	96
51) 4-Methyl-2-Pentanone	8.586	43	516674	216.158	ug/l	99
52) Toluene	8.738	92	6337242	1516.034	ug/l	87
59) 2-Hexanone	9.445	43	253254	138.432	ug/l	97
67) Ethyl Benzene	10.201	91	514568	68.708	ug/l	100
68) m/p-Xylenes	10.311	106	1492651	532.576	ug/l	95
69) o-Xylene	10.646	106	548130	202.680	ug/l	96
73) Isopropylbenzene	10.969	105	75177	9.478	ug/l	99
78) n-propylbenzene	11.311	91	63170	6.984	ug/l	92
80) 1,3,5-Trimethylbenzene	11.457	105	340727	52.104	ug/l	98
84) 1,2,4-Trimethylbenzene	11.762	105	646535	98.848	ug/l	96
85) sec-Butylbenzene	11.902	105	12799m	1.621	ug/l	
95) Naphthalene	13.780	128	66360	9.641	ug/l #	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020722\
Data File : VX026798.D
Acq On : 07 Feb 2022 20:30
Operator : JC/MD
Sample : N1342-25
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1


Instrument :
MSVOA_X
ClientSampleId :
31540

Manual Integrations
APPROVED

Reviewed By : John Carlone 02/08/2022
Supervised By : Mahesh Dadoda 02/08/2022

Quant Time: Feb 07 23:34:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 11 14:45:13 2022
Response via : Initial Calibration

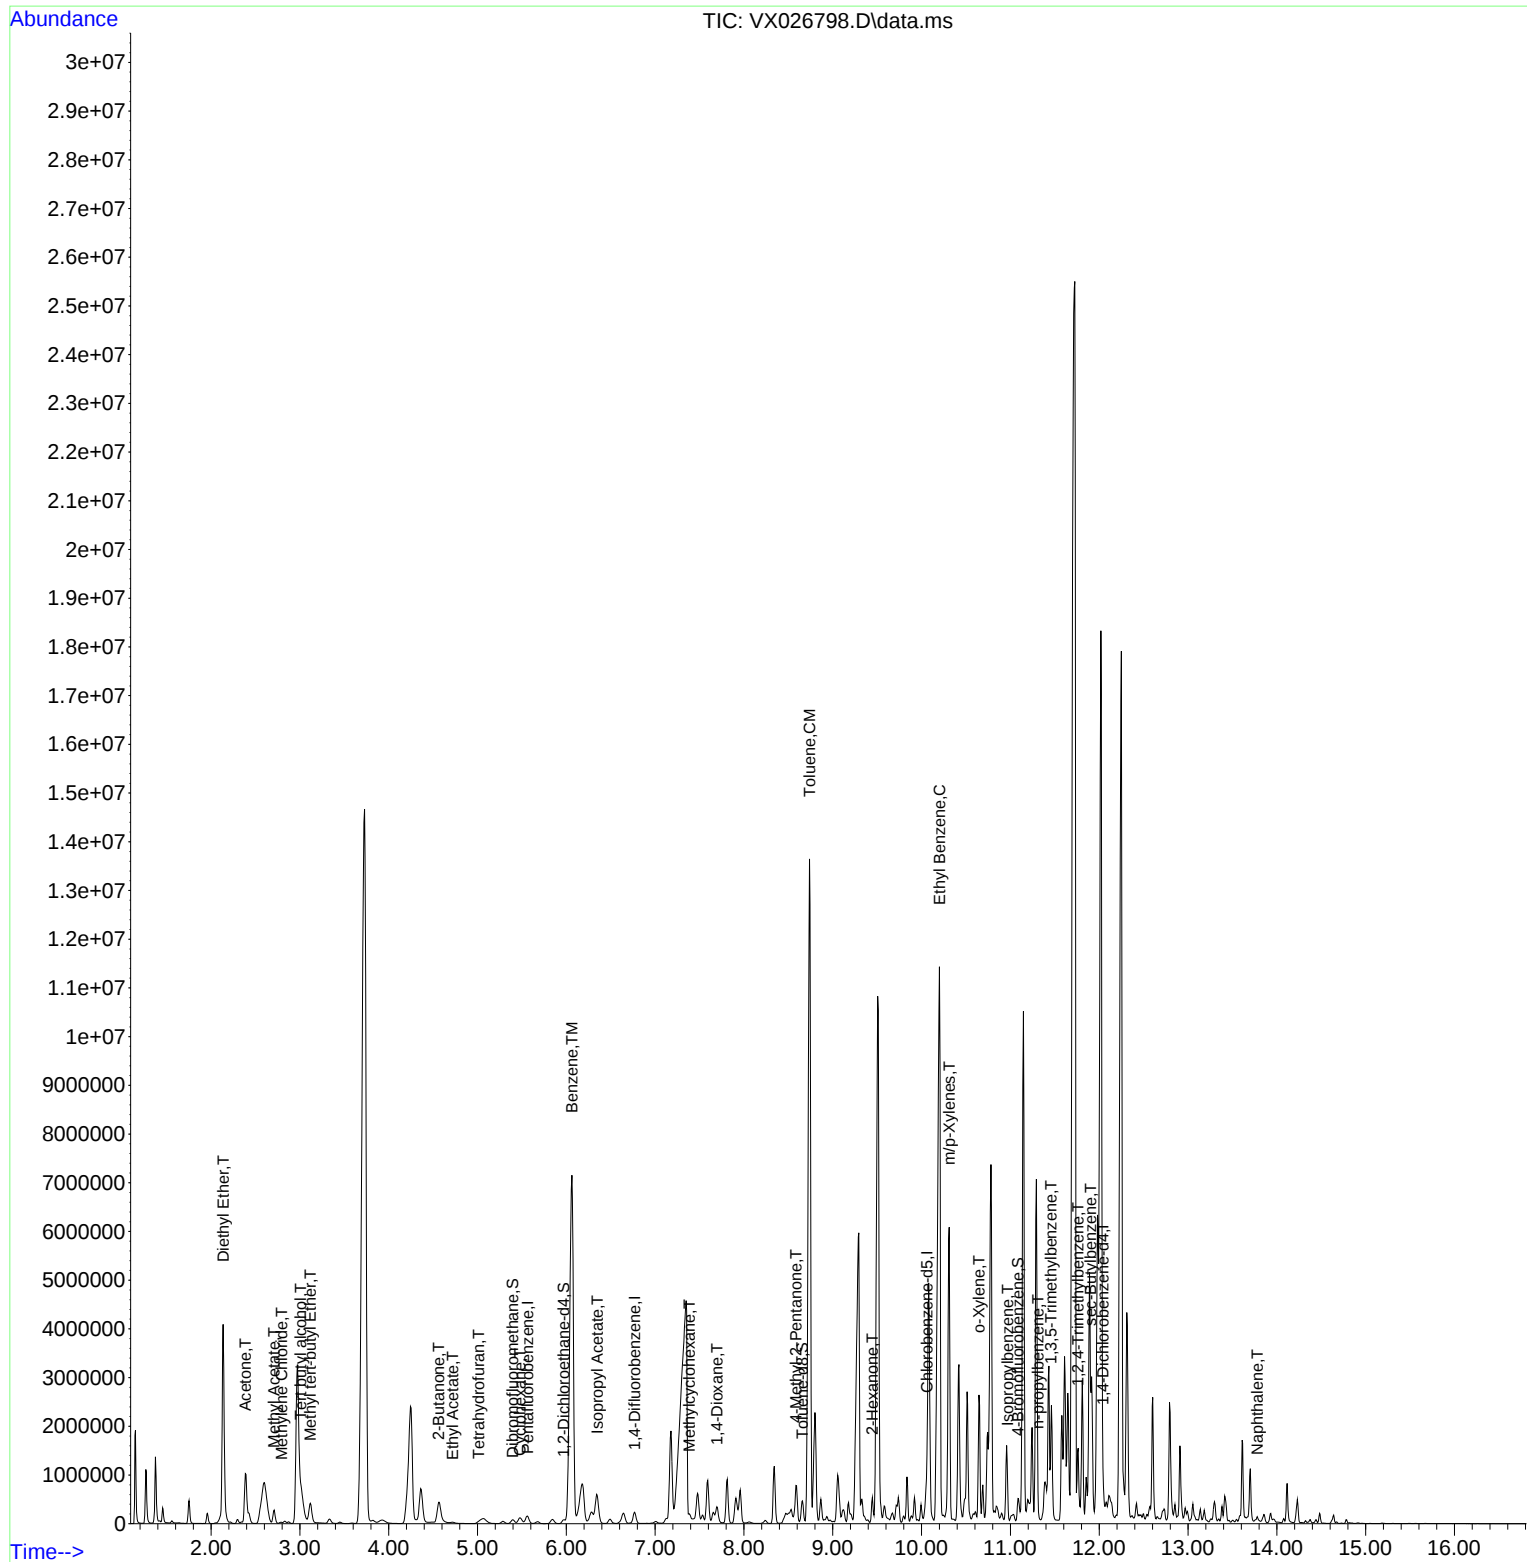

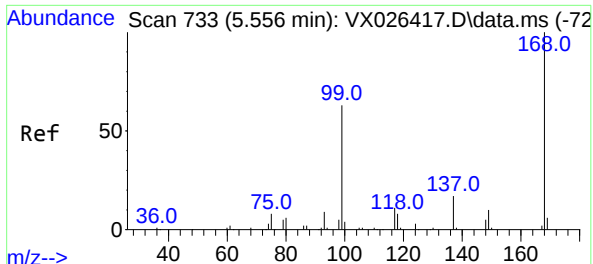





#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX026798.D
Acq: 07 Feb 2022 20:30

Instrument :
MSVOA_X
ClientSampleId :
31540

Tgt Ion:168 Resp: 15402
Ion Ratio Lower Upper
168 100
99 58.2 50.3 75.5




Manual Integrations
APPROVED


Reviewed By :John Carlone 02/08/2022
Supervised By :Mahesh Dadoda 02/08/2022

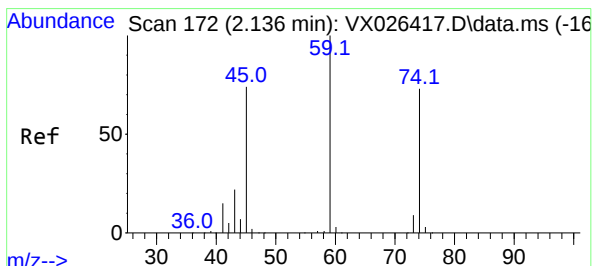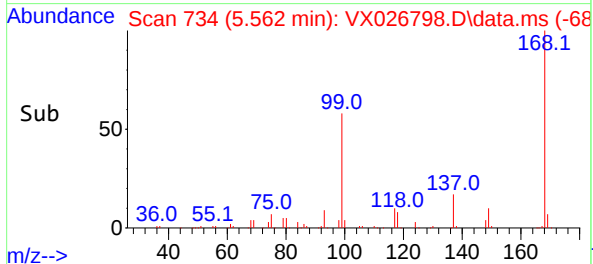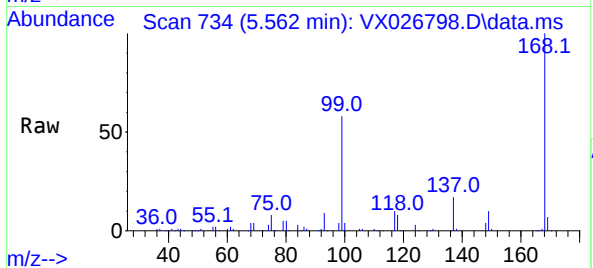

#8
Diethyl Ether
Concen: 1394.594 ug/l
RT: 2.136 min Scan# 172
Delta R.T. -0.000 min
Lab File: VX026798.D
Acq: 07 Feb 2022 20:30

Tgt Ion: 74 Resp: 1363920
Ion Ratio Lower Upper
74 100
45 138.3 50.7 152.1

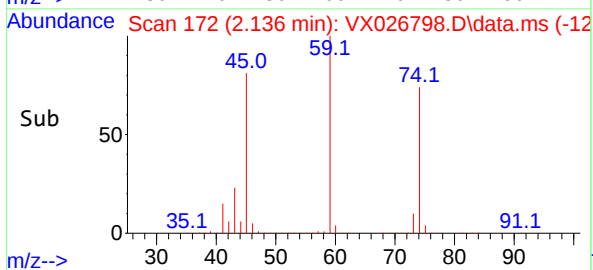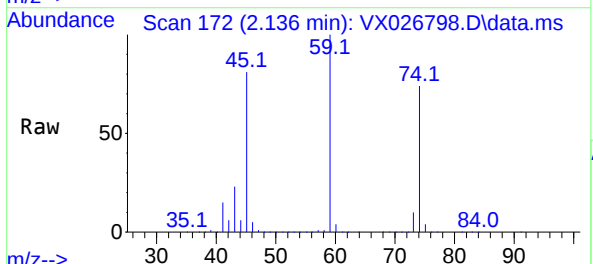



#11

Tert butyl alcohol

Concen: 6810.315 ug/l

RT: 3.007 min Scan# 315

Delta R.T. 0.000 min

Lab File: VX026798.D

Acq: 07 Feb 2022 20:30

Instrument :

MSVOA_X

ClientSampleId :

31540

Tgt Ion: 59 Resp: 203844

Ion Ratio Lower Upper

59 100





57 0.0 7.2 10.8

Manual Integrations

APPROVED

Reviewed By :John Carlone 02/08/2022

Supervised By :Mahesh Dadoda 02/08/2022



#16

Acetone

Concen: 1120.253 ug/l

RT: 2.386 min Scan# 213

Delta R.T. -0.006 min

Lab File: VX026798.D




Acq: 07 Feb 2022 20:30


Tgt Ion: 43 Resp: 1229202

Ion Ratio Lower Upper

43 100

58 30.7 23.0 34.6



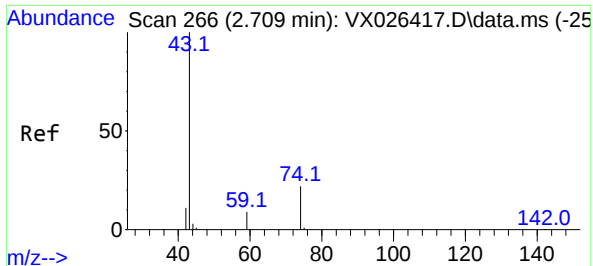

#18

Methyl Acetate

Concen: 144.391 ug/l

RT: 2.709 min Scan# 2

Delta R.T. -0.000 min

Lab File: VX026798.D


Acq: 07 Feb 2022 20:30

Instrument :

MSVOA_X

ClientSampleId :

31540

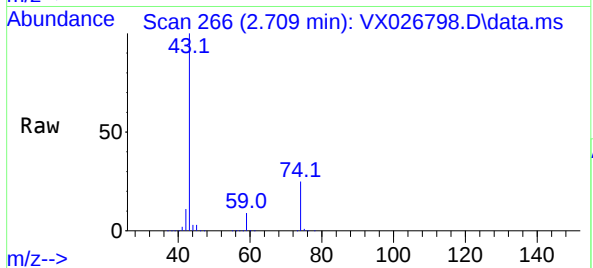

Tgt Ion: 43 Resp: 31497

Ion Ratio Lower Upper

43 100




74 25.4 18.3 27.5

Manual Integrations

APPROVED

Reviewed By :John Carlone 02/08/2022

Supervised By :Mahesh Dadoda 02/08/2022

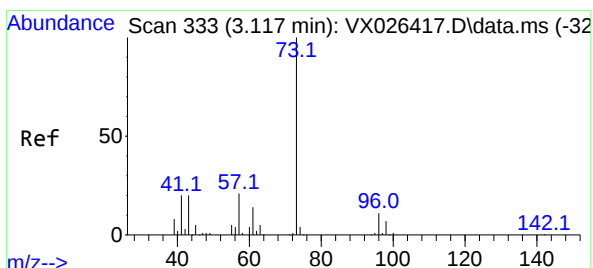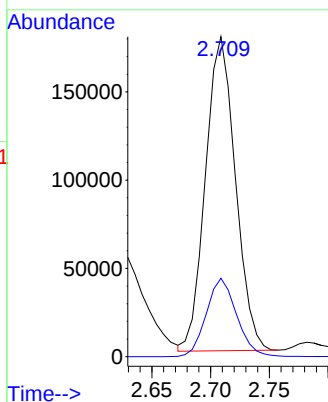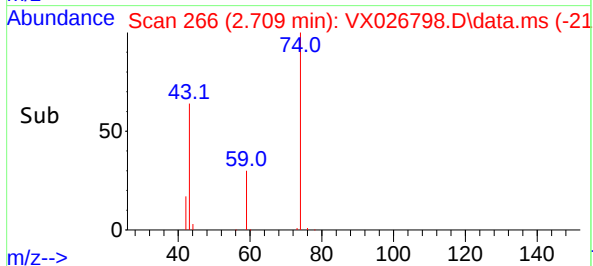

#19

Methyl tert-butyl Ether

Concen: 73.629 ug/l

RT: 3.117 min Scan# 333

Delta R.T. -0.000 min

Lab File: VX026798.D




Acq: 07 Feb 2022 20:30


Tgt Ion: 73 Resp: 429756

Ion Ratio Lower Upper

73 100

57 26.2 17.4 26.2

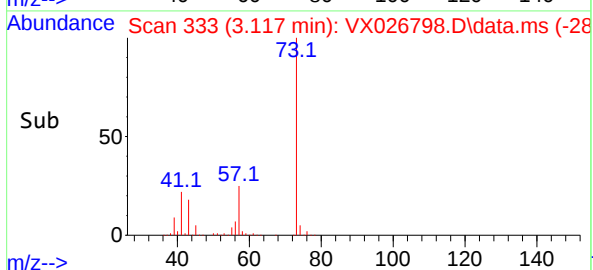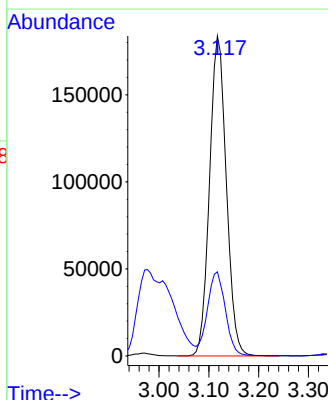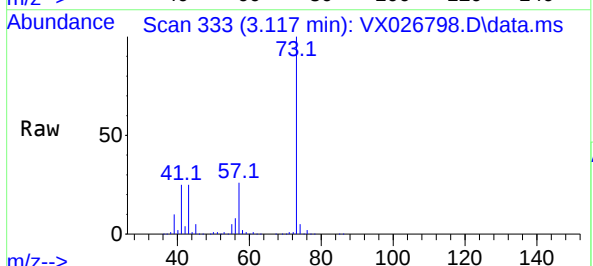




#20
Methylene Chloride
Concen: 1.463 ug/l
RT: 2.794 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX026798.D
Acq: 07 Feb 2022 20:30

Instrument :

MSVOA_X

ClientSampleId :

31540






Tgt Ion: 84 Resp: 265
Ion Ratio Lower Upper
84 100
49 124.9 101.5 152.3
51 39.6 31.2 46.8
86 98.1 51.3 76.9#

Manual Integrations




APPROVED


Reviewed By :John Carlone 02/08/2022
Supervised By :Mahesh Dadoda 02/08/2022

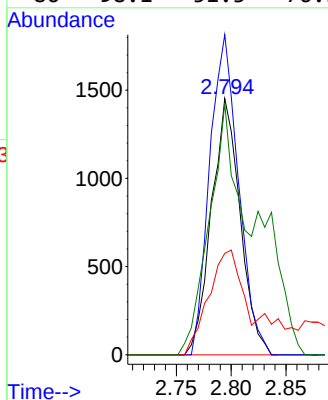

#25
2-Butanone
Concen: 536.655 ug/l
RT: 4.562 min Scan# 570
Delta R.T. -0.000 min
Lab File: VX026798.D
Acq: 07 Feb 2022 20:30

Tgt Ion: 43 Resp: 765778
Ion Ratio Lower Upper
43 100
72 26.9 20.4 30.6

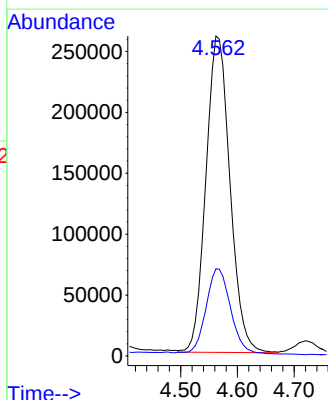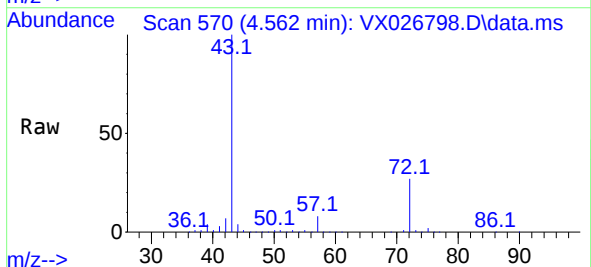



#29

Tetrahydrofuran

Concen: 39.432 ug/l

RT: 5.013 min Scan# 64

Delta R.T. -0.000 min

Lab File: VX026798.D

Acq: 07 Feb 2022 20:30

Instrument :

MSVOA_X

ClientSampleId :

31540

Tgt Ion: 42 Resp: 33418





Ion	Ratio	Lower	Upper
42	100		
72	37.2	34.6	52.0
71	35.6	31.8	47.8

Manual Integrations

APPROVED

Reviewed By :John Carlone 02/08/2022

Supervised By :Mahesh Dadoda 02/08/2022

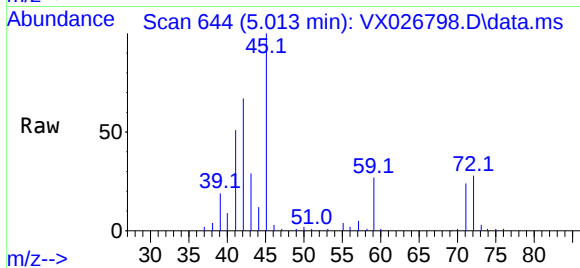

#31

Cyclohexane

Concen: 27.909 ug/l

RT: 5.476 min Scan# 720




Delta R.T. -0.000 min


Lab File: VX026798.D

Acq: 07 Feb 2022 20:30

Tgt Ion: 56 Resp: 88573

Ion	Ratio	Lower	Upper
56	100		
69	31.5	25.8	38.6
84	88.6	68.9	103.3

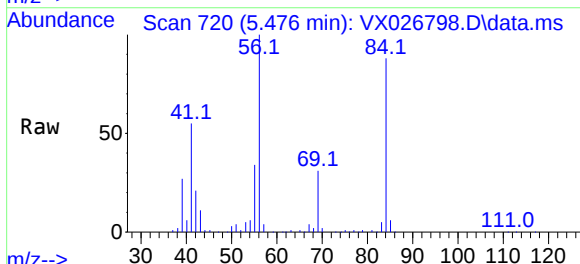



#33

1,2-Dichloroethane-d4

Concen: 41.173 ug/l

RT: 5.970 min Scan# 801

Delta R.T. 0.012 min

Lab File: VX026798.D

Acq: 07 Feb 2022 20:30

Instrument :

MSVOA_X

ClientSampleId :

31540

Tgt Ion: 65 Resp: 88589

Ion Ratio Lower Upper

65 100





67 50.7 0.0 100.8

Manual Integrations

APPROVED

Reviewed By :John Carlone 02/08/2022

Supervised By :Mahesh Dadoda 02/08/2022



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.769 min Scan# 932

Delta R.T. 0.006 min

Lab File: VX026798.D

Acq: 07 Feb 2022 20:30




Tgt Ion:114 Resp: 241918


Ion Ratio Lower Upper

114 100

63 18.7 0.0 42.8

88 16.2 0.0 33.0

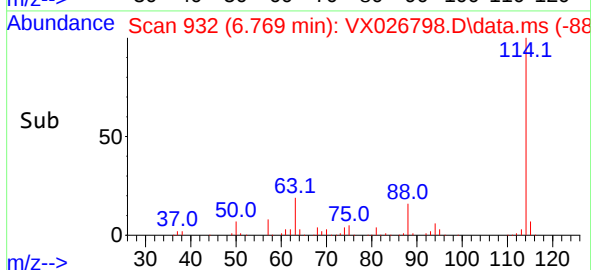

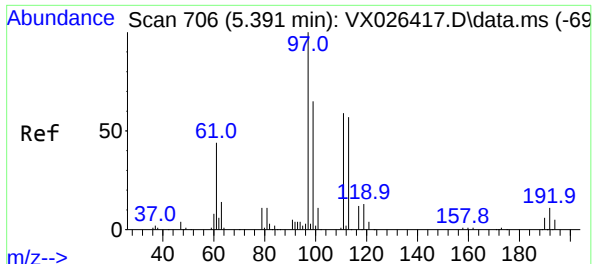

#35

Dibromofluoromethane

Concen: 44.985 ug/l

RT: 5.397 min Scan# 706

Delta R.T. 0.006 min

Lab File: VX026798.D

Acq: 07 Feb 2022 20:30

Instrument :

MSVOA_X

ClientSampleId :

31540

Tgt Ion:113 Resp: 7027

Ion Ratio Lower Upper

113 100

111 101.5 81.2 121.8





192 20.2 15.0 22.4

Manual Integrations

APPROVED

Reviewed By :John Carlone 02/08/2022

Supervised By :Mahesh Dadoda 02/08/2022

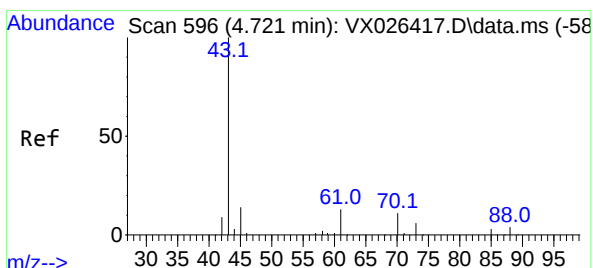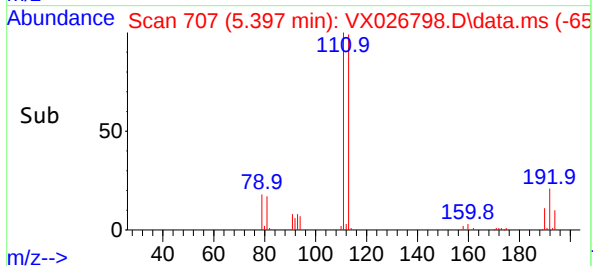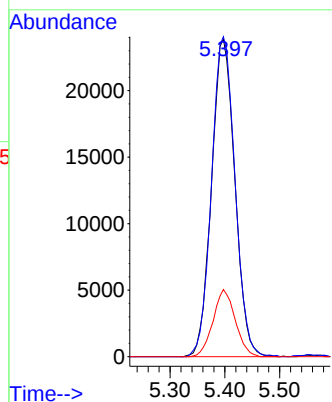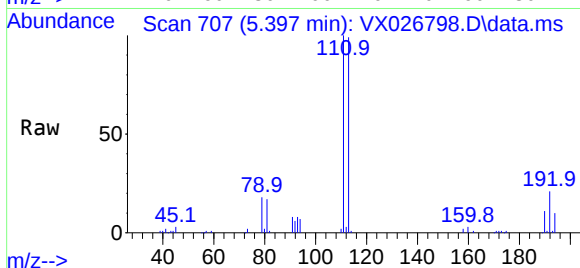

#37

Ethyl Acetate

Concen: 15.803 ug/l

RT: 4.721 min Scan# 596

Delta R.T. -0.000 min

Lab File: VX026798.D

Acq: 07 Feb 2022 20:30




Tgt Ion: 43 Resp: 39424


Ion Ratio Lower Upper

43 100

61 11.4 10.6 16.0

70 9.4 8.5 12.7

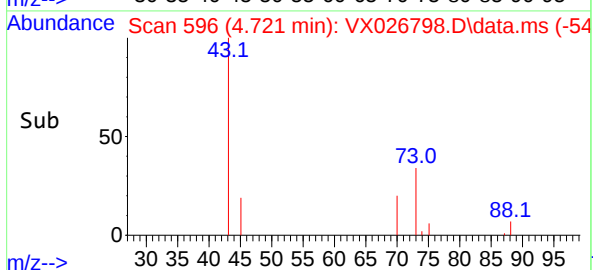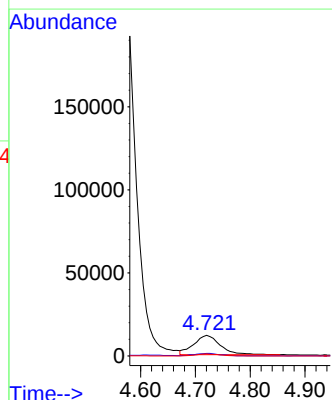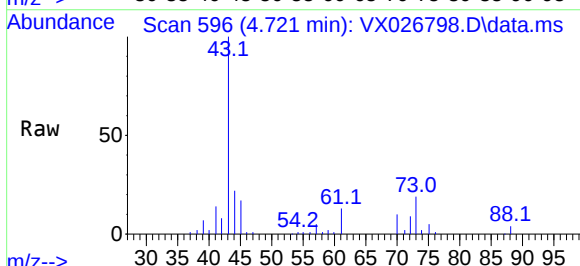

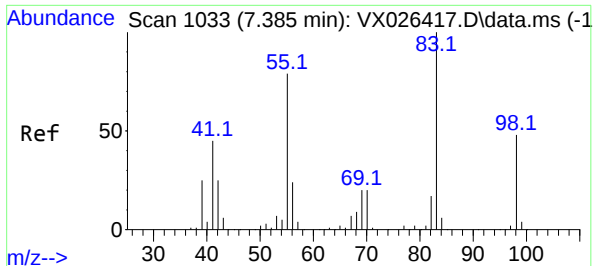

#39

Methylcyclohexane

Concen: 21.183 ug/l

RT: 7.385 min Scan# 1033

Delta R.T. -0.000 min

Lab File: VX026798.D

Acq: 07 Feb 2022 20:30

Instrument :

MSVOA_X

ClientSampleId :

31540

Tgt Ion: 83 Resp: 63014





Ion	Ratio	Lower	Upper
83	100		
55	73.3	63.6	95.4
98	48.3	38.4	57.6

Manual Integrations

APPROVED

Reviewed By :John Carlone 02/08/2022

Supervised By :Mahesh Dadoda 02/08/2022

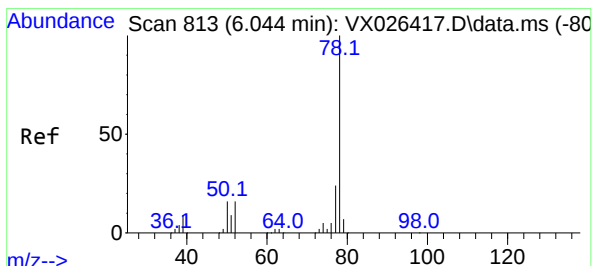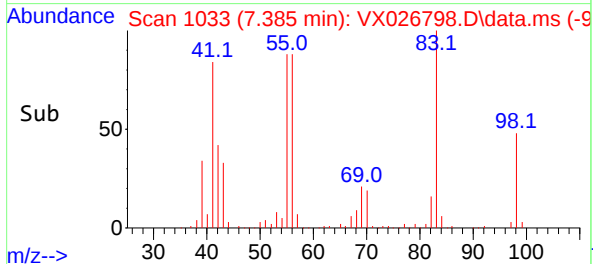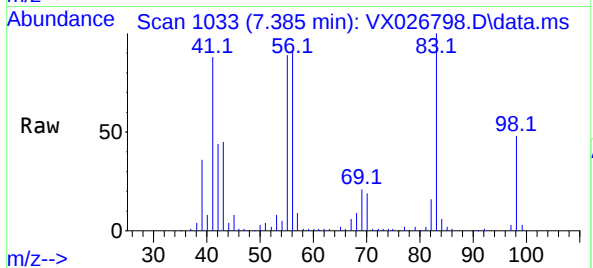

#40

Benzene

Concen: 1312.264 ug/l

RT: 6.062 min Scan# 816




Delta R.T. 0.018 min


Lab File: VX026798.D

Acq: 07 Feb 2022 20:30

Tgt Ion: 78 Resp: 8945183


Ion	Ratio	Lower	Upper
78	100		
77	26.4	18.9	28.3

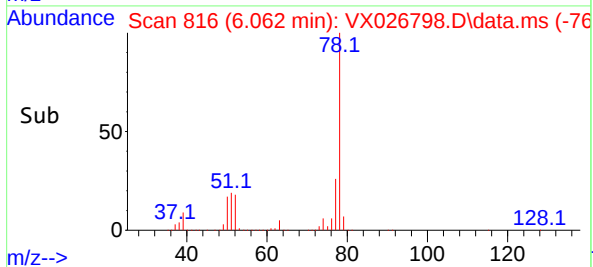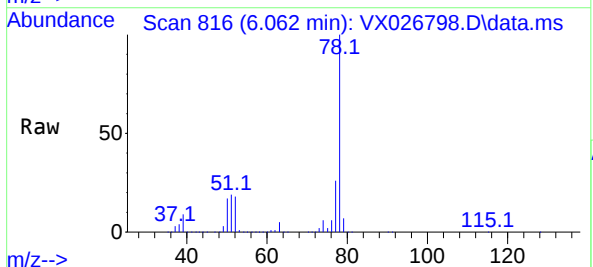



#43
Isopropyl Acetate
Concen: 98.894 ug/l
RT: 6.348 min Scan# 863
Delta R.T. 0.006 min
Lab File: VX026798.D
Acq: 07 Feb 2022 20:30




Instrument :
MSVOA_X
ClientSampleId :
31540




Tgt Ion: 43 Resp: 398532
Ion Ratio Lower Upper
43 100
61 16.7 15.4 23.0
87 10.3 10.2 15.2

Manual Integrations
APPROVED



Reviewed By :John Carlone 02/08/2022
Supervised By :Mahesh Dadoda 02/08/2022




#49
1,4-Dioxane
Concen: 6386.894 ug/l
RT: 7.696 min Scan# 1084
Delta R.T. -0.000 min
Lab File: VX026798.D
Acq: 07 Feb 2022 20:30

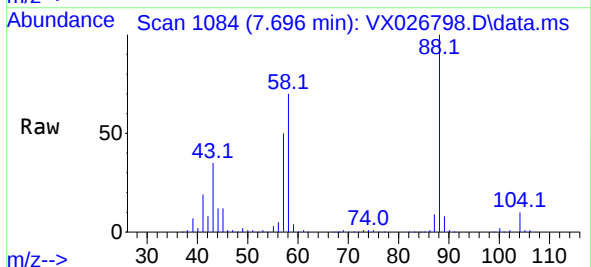


Tgt Ion: 88 Resp: 209326
Ion Ratio Lower Upper
88 100
43 35.4 29.9 44.9
58 76.1 57.8 86.6



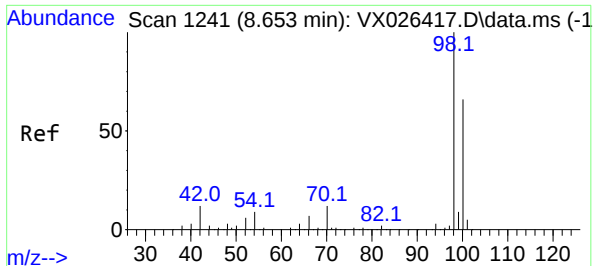

#50
Toluene-d8
Concen: 47.752 ug/l
RT: 8.659 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX026798.D
Acq: 07 Feb 2022 20:30




Instrument :
MSVOA_X
ClientSampleId :
31540

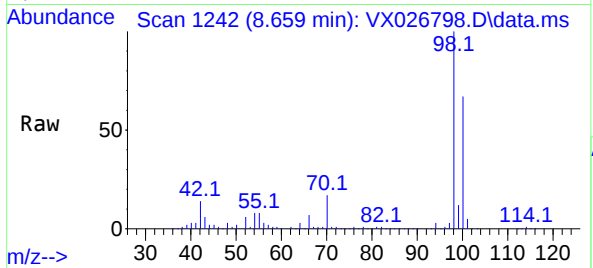


Tgt Ion: 98 Resp: 268824
Ion Ratio Lower Upper
98 100
100 67.5 53.2 79.8

Manual Integrations
APPROVED



Reviewed By :John Carlone 02/08/2022
Supervised By :Mahesh Dadoda 02/08/2022

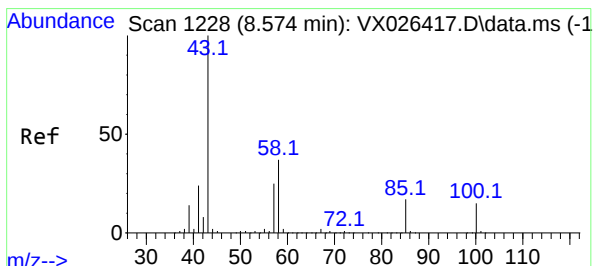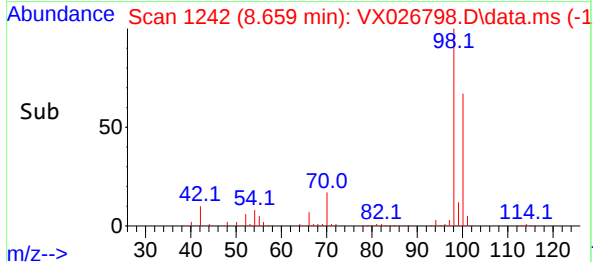


#51
4-Methyl-2-Pentanone
Concen: 216.158 ug/l
RT: 8.586 min Scan# 1230
Delta R.T. 0.012 min
Lab File: VX026798.D
Acq: 07 Feb 2022 20:30

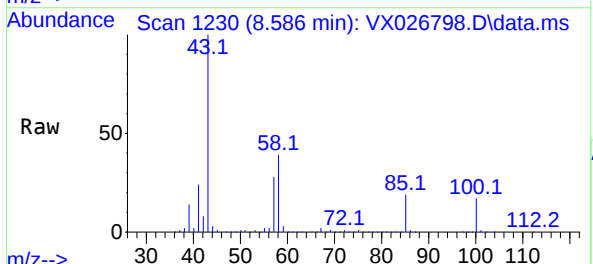


Tgt Ion: 43 Resp: 516674
Ion Ratio Lower Upper
43 100
58 37.8 30.5 45.7

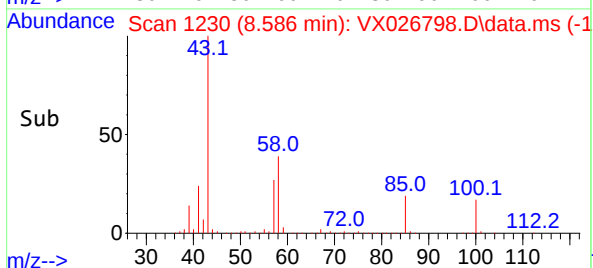



#52
Toluene
Concen: 1516.034 ug/l
RT: 8.738 min Scan# 11
Delta R.T. 0.018 min
Lab File: VX026798.D
Acq: 07 Feb 2022 20:30




Instrument :
MSVOA_X
ClientSampleId :
31540




Tgt Ion: 92 Resp: 633724
Ion Ratio Lower Upper
92 100
91 151.9 135.7 203.5

Manual Integrations
APPROVED



Reviewed By :John Carlone 02/08/2022
Supervised By :Mahesh Dadoda 02/08/2022




#59
2-Hexanone
Concen: 138.432 ug/l
RT: 9.445 min Scan# 1371
Delta R.T. 0.012 min
Lab File: VX026798.D
Acq: 07 Feb 2022 20:30




Tgt Ion: 43 Resp: 253254
Ion Ratio Lower Upper
43 100
58 55.1 26.4 79.2





#62
4-Bromofluorobenzene
Concen: 53.393 ug/l
RT: 11.085 min Scan# 1107
Delta R.T. 0.006 min
Lab File: VX026798.D
Acq: 07 Feb 2022 20:30




Instrument :
MSVOA_X
ClientSampleId :
31540




Tgt Ion: 95 Resp: 106778
Ion Ratio Lower Upper
95 100
174 73.4 0.0 148.6
176 71.5 0.0 141.4

Manual Integrations
APPROVED



Reviewed By :John Carlone 02/08/2022
Supervised By :Mahesh Dadoda 02/08/2022




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.061 min Scan# 1472
Delta R.T. 0.006 min
Lab File: VX026798.D
Acq: 07 Feb 2022 20:30




Tgt Ion:117 Resp: 195704
Ion Ratio Lower Upper
117 100
82 55.0 45.2 67.8
119 32.2 26.2 39.2





#67
Ethyl Benzene
Concen: 68.708 ug/l
RT: 10.201 min Scan# 1495
Delta R.T. 0.006 min
Lab File: VX026798.D
Acq: 07 Feb 2022 20:30




Instrument :
MSVOA_X
ClientSampleId :
31540

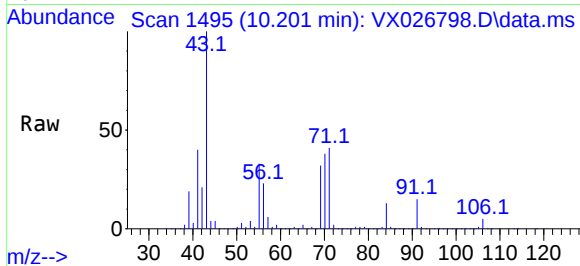


Tgt Ion: 91 Resp: 51456
Ion Ratio Lower Upper
91 100
106 30.9 24.7 37.1

Manual Integrations
APPROVED



Reviewed By :John Carlone 02/08/2022
Supervised By :Mahesh Dadoda 02/08/2022

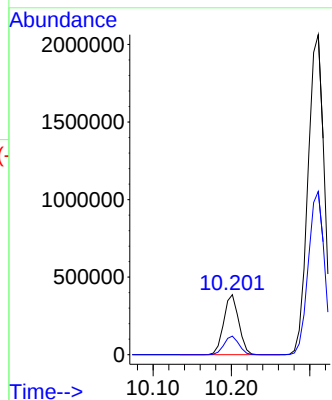


#68
m/p-Xylenes
Concen: 532.576 ug/l
RT: 10.311 min Scan# 1513
Delta R.T. 0.006 min
Lab File: VX026798.D
Acq: 07 Feb 2022 20:30

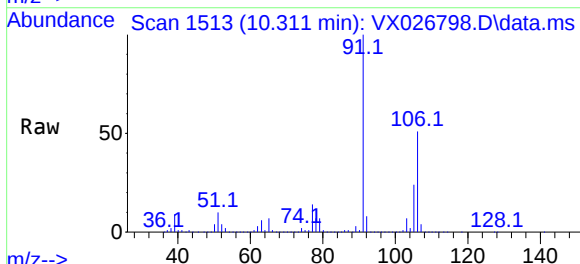

Tgt Ion:106 Resp: 1492651
Ion Ratio Lower Upper
106 100
91 198.3 165.3 247.9

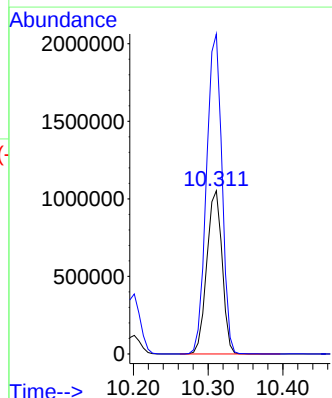







#69
o-Xylene
Concen: 202.680 ug/l
RT: 10.646 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX026798.D
Acq: 07 Feb 2022 20:30

Instrument :
MSVOA_X
ClientSampleId :
31540

Tgt Ion:106 Resp: 548130
Ion Ratio Lower Upper
106 100
91 212.9 109.7 329.0




Manual Integrations
APPROVED


Reviewed By :John Carlone 02/08/2022
Supervised By :Mahesh Dadoda 02/08/2022

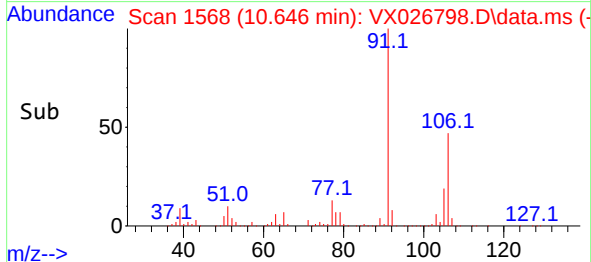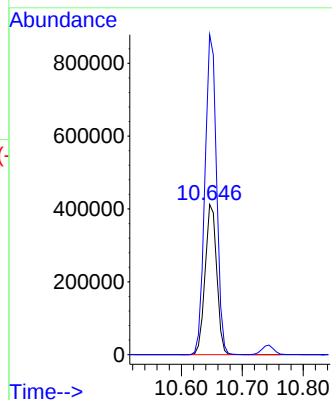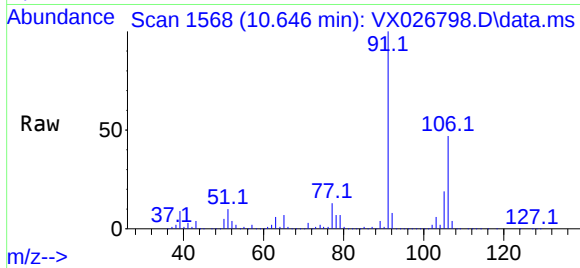

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.042 min Scan# 1797
Delta R.T. 0.018 min
Lab File: VX026798.D
Acq: 07 Feb 2022 20:30


Tgt Ion:152 Resp: 96769
Ion Ratio Lower Upper
152 100
115 62.1 44.2 132.6
150 165.5 0.0 348.2

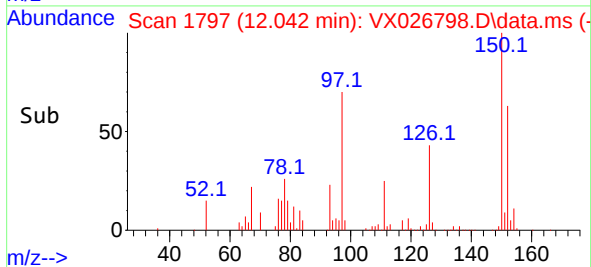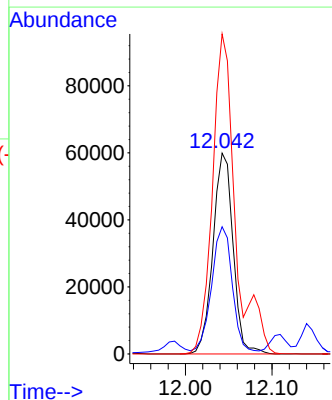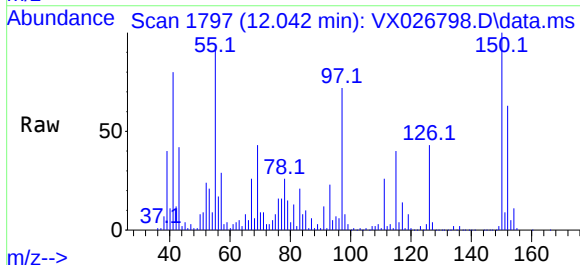



#73
Isopropylbenzene
Concen: 9.478 ug/l
RT: 10.969 min Scan# 1620
Delta R.T. 0.006 min
Lab File: VX026798.D
Acq: 07 Feb 2022 20:30




Instrument :
MSVOA_X
ClientSampleId :
31540

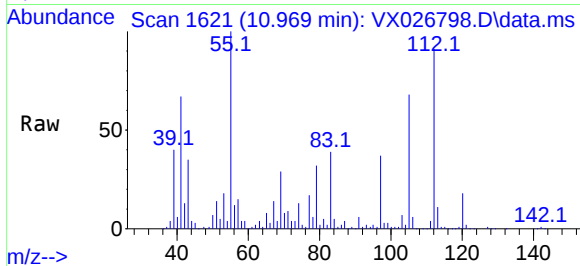


Tgt Ion:105 Resp: 7517
Ion Ratio Lower Upper
105 100
120 26.6 13.1 39.1

Manual Integrations
APPROVED



Reviewed By :John Carlone 02/08/2022
Supervised By :Mahesh Dadoda 02/08/2022




#78
n-propylbenzene
Concen: 6.984 ug/l
RT: 11.311 min Scan# 1677
Delta R.T. 0.006 min
Lab File: VX026798.D
Acq: 07 Feb 2022 20:30

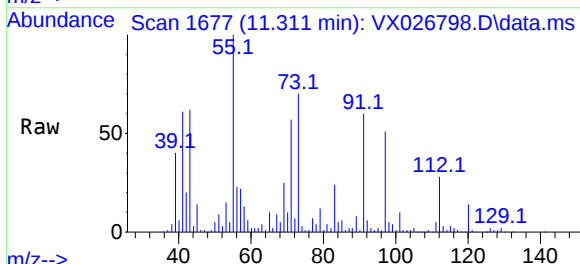

Tgt Ion: 91 Resp: 63170
Ion Ratio Lower Upper
91 100
120 19.0 11.6 34.7









#80
1,3,5-Trimethylbenzene
Concen: 52.104 ug/l
RT: 11.457 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX026798.D
Acq: 07 Feb 2022 20:30

Instrument :
MSVOA_X
ClientSampleId :
31540

Tgt Ion:105 Resp: 34072
Ion Ratio Lower Upper
105 100
120 49.2 24.0 72.0




Manual Integrations
APPROVED


Reviewed By :John Carlone 02/08/2022
Supervised By :Mahesh Dadoda 02/08/2022

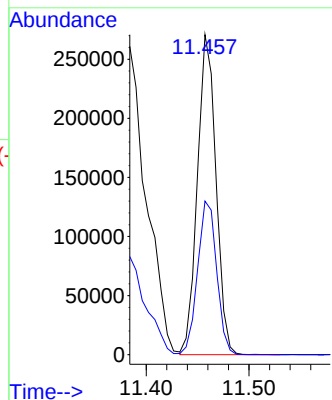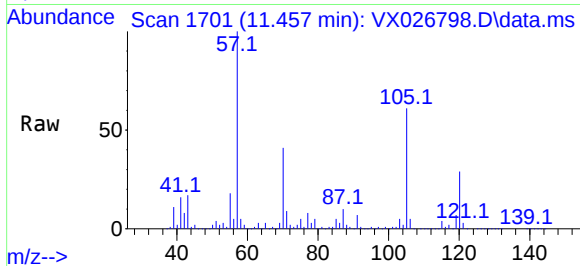

#84
1,2,4-Trimethylbenzene
Concen: 98.848 ug/l
RT: 11.762 min Scan# 1751
Delta R.T. 0.012 min
Lab File: VX026798.D
Acq: 07 Feb 2022 20:30


Tgt Ion:105 Resp: 646535
Ion Ratio Lower Upper
105 100
120 40.9 21.9 65.5

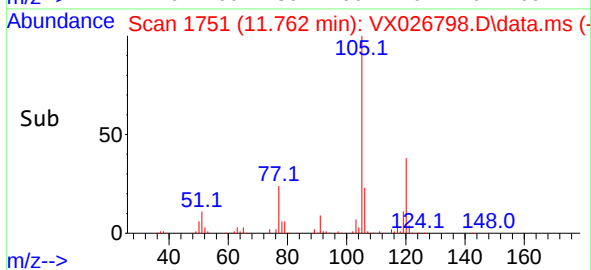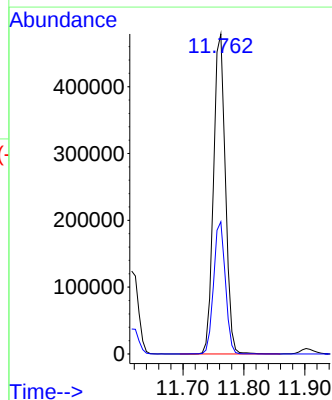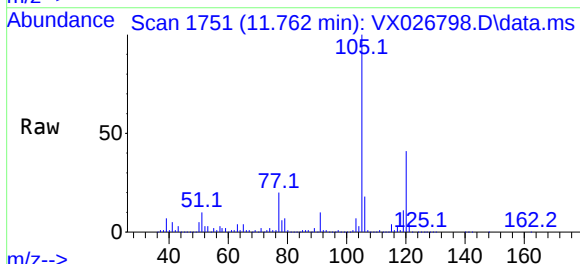



#85
 sec-Butylbenzene
 Concen: 1.621 ug/l m
 RT: 11.902 min Scan# 11
 Delta R.T. 0.012 min
 Lab File: VX026798.D
 Acq: 07 Feb 2022 20:30




Instrument :
 MSVOA_X
 ClientSampleId :
 31540

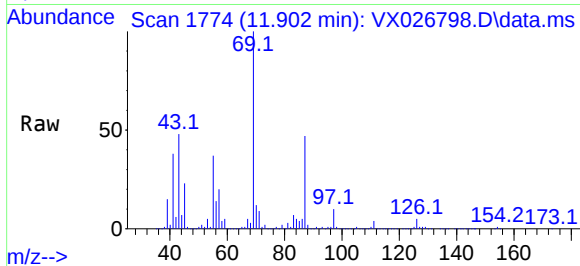


Tgt Ion:105 Resp: 12799
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.1 30.1

Manual Integrations
 APPROVED

Reviewed By :John Carlone 02/08/2022
 Supervised By :Mahesh Dadoda 02/08/2022

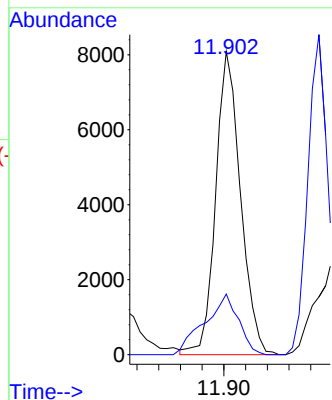

#95
 Naphthalene
 Concen: 9.641 ug/l
 RT: 13.780 min Scan# 2082
 Delta R.T. 0.006 min
 Lab File: VX026798.D
 Acq: 07 Feb 2022 20:30

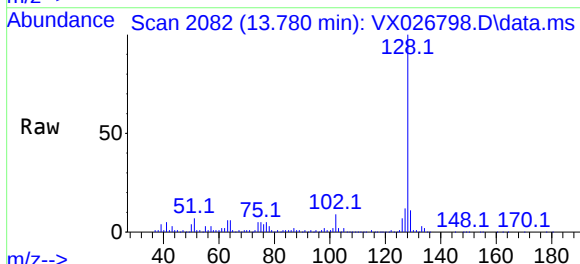

Tgt Ion:128 Resp: 66360
 Ion Ratio Lower Upper
 128 100
 127 13.2 10.3 15.5
 129 13.1 8.7 13.1

