

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020722\
 Data File : VX026784.D
 Acq On : 07 Feb 2022 15:06
 Operator : JC/MD
 Sample : N1399-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 KTS1-GW-MH-02-8-13

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
 Title : SW846 8260

Signal : TIC: VX026784.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.148	7	10	21	rVB2	34094	37361	5.80%	0.934%
2	1.270	26	30	33	rVB2	7437	6770	1.05%	0.169%
3	2.386	209	213	222	rVB	5041	8375	1.30%	0.209%
4	2.563	237	242	255	rVB2	2485	7462	1.16%	0.187%
5	4.568	561	571	584	rBV2	4392	14563	2.26%	0.364%
6	5.391	694	706	720	rBV	74275	214893	33.35%	5.374%
7	5.556	722	733	750	rVB	131090	370458	57.50%	9.264%
8	5.958	790	799	810	rBV	81469	216918	33.67%	5.425%
9	6.769	922	932	945	rBV	200171	478778	74.31%	11.973%
10	8.653	1234	1241	1250	rBV	407496	644274	100.00%	16.111%
11	10.055	1465	1471	1487	rBV	423946	569652	88.42%	14.245%
12	11.079	1634	1639	1646	rBV	331057	426359	66.18%	10.662%
13	11.744	1745	1748	1754	rBV4	4252	6530	1.01%	0.163%
14	12.024	1789	1794	1804	rVB	408978	511226	79.35%	12.784%
15	12.335	1839	1845	1848	rBV6	4428	8159	1.27%	0.204%
16	12.445	1859	1863	1871	rBV8	3801	10972	1.70%	0.274%
17	12.573	1880	1884	1891	rVB8	4439	9592	1.49%	0.240%
18	12.664	1895	1899	1907	rBV6	5558	12569	1.95%	0.314%
19	12.811	1919	1923	1931	rBV2	11998	21447	3.33%	0.536%
20	12.920	1936	1941	1948	rVB3	13176	21345	3.31%	0.534%
21	13.036	1956	1960	1965	rBV7	5074	6584	1.02%	0.165%
22	13.195	1981	1986	1991	rBV6	9118	22342	3.47%	0.559%
23	13.292	1998	2002	2008	rBV5	9896	14268	2.21%	0.357%
24	13.408	2017	2021	2025	rBV2	15613	25138	3.90%	0.629%
25	13.451	2025	2028	2034	rVB5	6220	12770	1.98%	0.319%
26	13.707	2066	2070	2074	rVB3	29418	36686	5.69%	0.917%
27	13.804	2082	2086	2089	rVB4	19855	25740	4.00%	0.644%
28	13.908	2099	2103	2109	rVB8	16691	30777	4.78%	0.770%
29	13.987	2113	2116	2119	rBV3	14470	19540	3.03%	0.489%
30	14.067	2125	2129	2132	rBV4	14019	22019	3.42%	0.551%
31	14.103	2132	2135	2138	rVV	17540	23350	3.62%	0.584%
32	14.140	2138	2141	2144	rVV2	18364	20307	3.15%	0.508%
33	14.213	2151	2153	2157	rVB3	10594	12531	1.94%	0.313%
34	14.304	2165	2168	2171	rBV4	11984	15188	2.36%	0.380%
35	14.426	2185	2188	2194	rVB7	12974	24375	3.78%	0.610%
36	14.548	2206	2208	2210	rBV3	8651	10654	1.65%	0.266%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020722\
Data File : VX026784.D
Acq On : 07 Feb 2022 15:06
Operator : JC/MD
Sample : N1399-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
KTS1-GW-MH-02-8-13

Integration Parameters: RTEINT.P
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
Title : SW846 8260

37	14.627	2217	2221	2226	rBV5	12631	29898	4.64%	0.748%
38	14.755	2239	2242	2245	rBV4	21220	24042	3.73%	0.601%
39	14.932	2268	2271	2273	rBV3	20802	24942	3.87%	0.624%


Sum of corrected areas: 3998854

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020722\
Data File : VX026784.D
Acq On : 07 Feb 2022 15:06
Operator : JC/MD
Sample : N1399-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
KTS1-GW-MH-02-8-13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

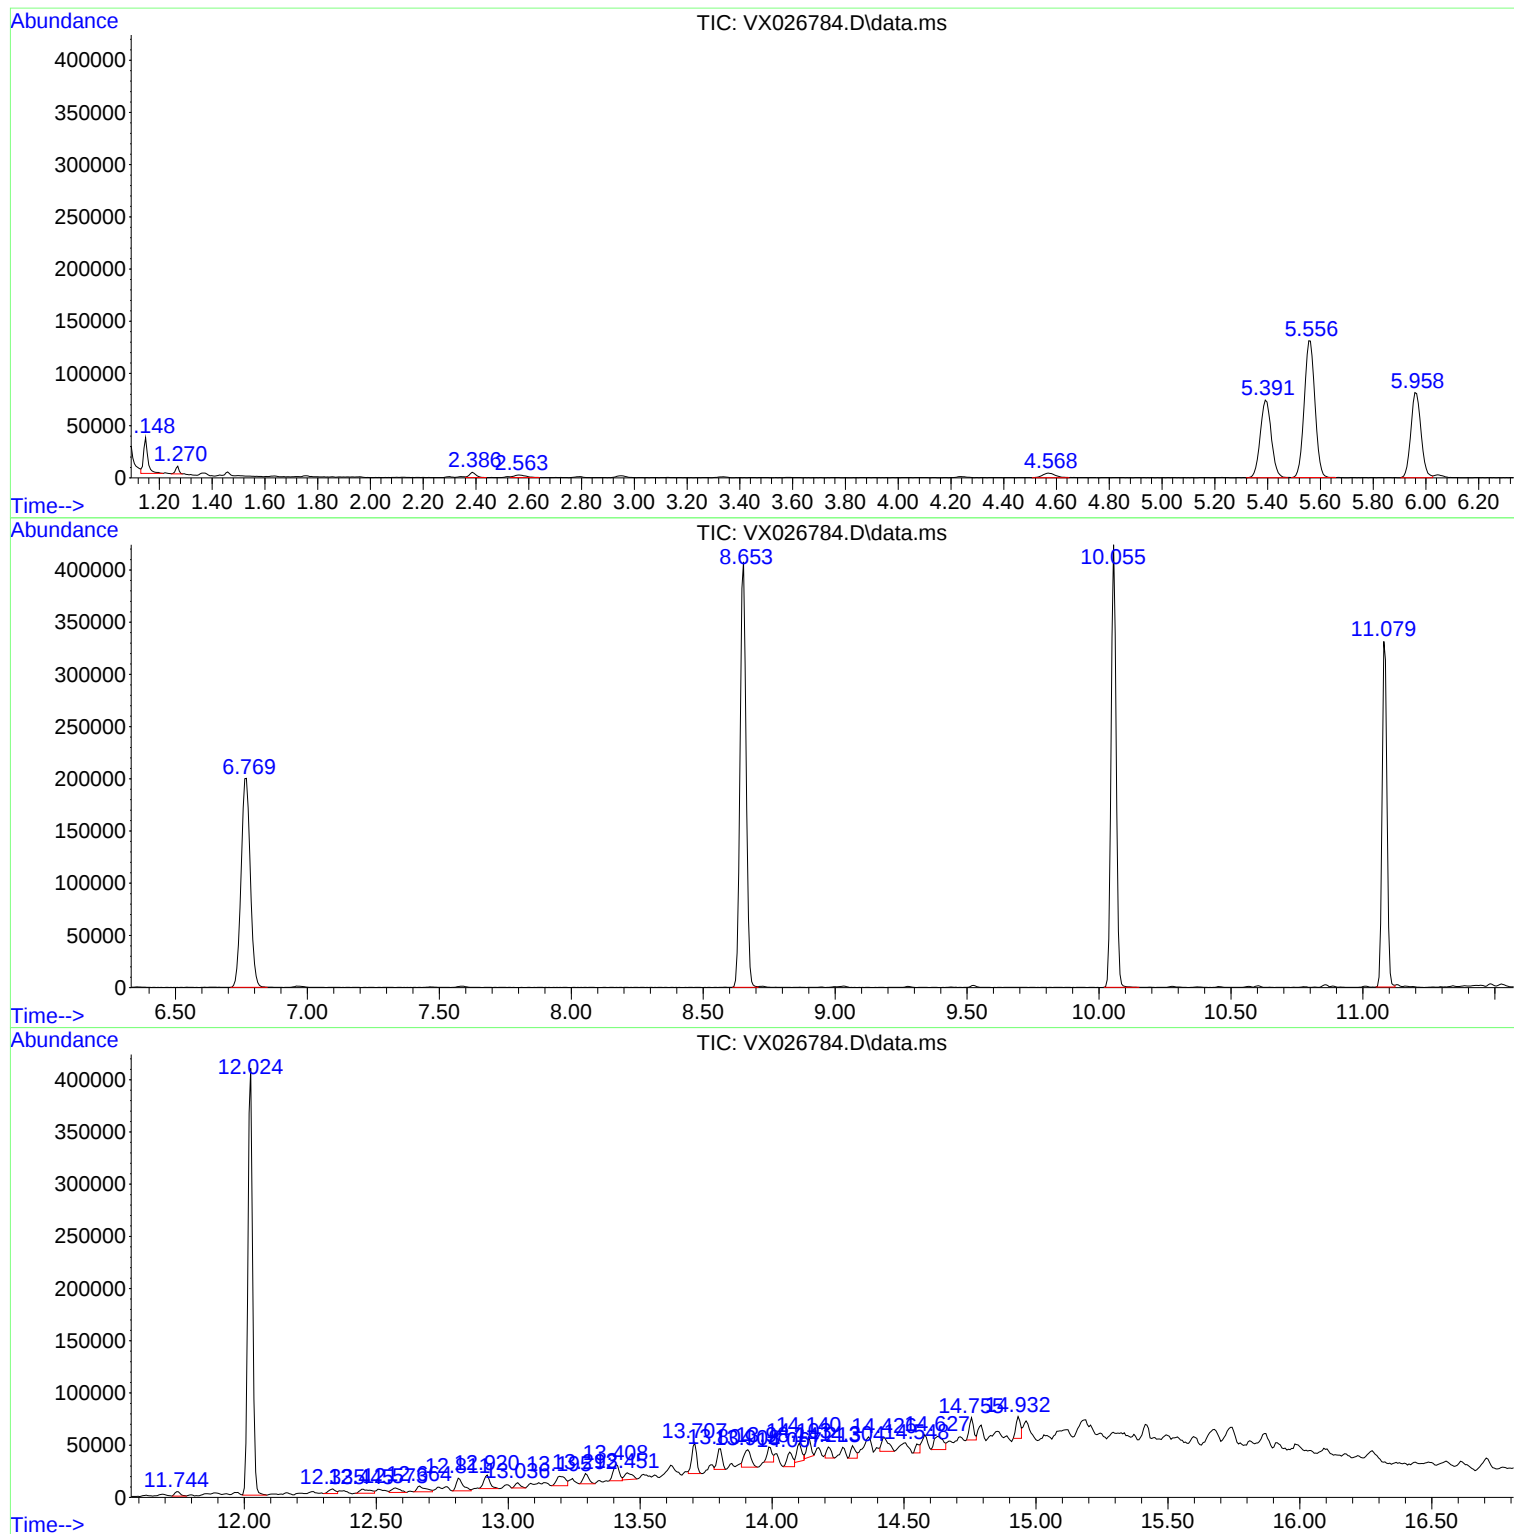

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020722\
Data File : VX026784.D
Acq On : 07 Feb 2022 15:06
Operator : JC/MD
Sample : N1399-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
KTS1-GW-MH-02-8-13










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown1.148 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.148	5.04 ug/l	37361	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopropane	42	C3H6	000075-19-4	40
2			Propene	42	C3H6	000115-07-1	7
3			Cyclopropene	40	C3H4	002781-85-3	2
4			Pyrimidine-2,4(1H,3H)-dione, 5-a...	156	C4H4N4O3	1000270-67-7	2
5			Propane, 2-nitro-	89	C3H7NO2	000079-46-9	2

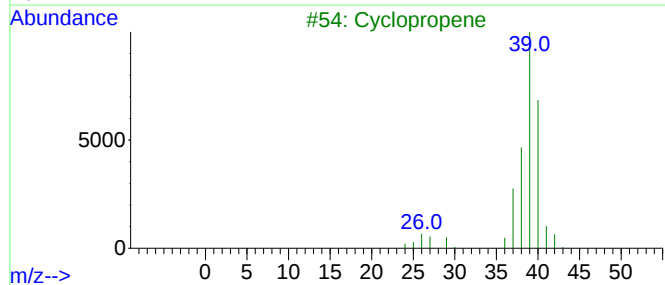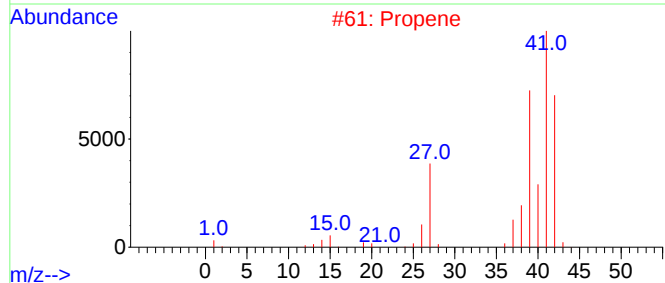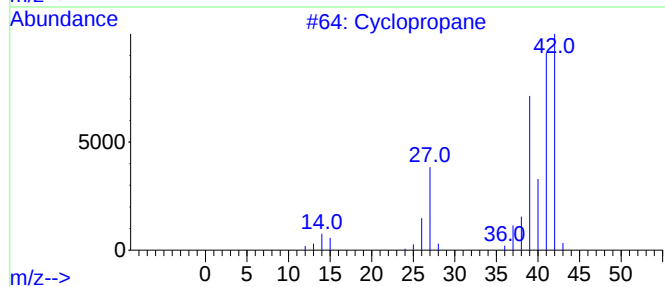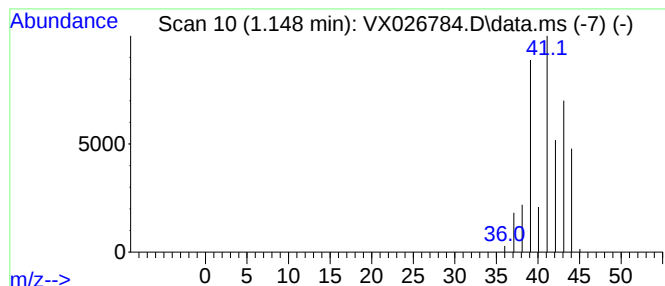

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020722\
Data File : VX026784.D
Acq On : 07 Feb 2022 15:06
Operator : JC/MD
Sample : N1399-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
KTS1-GW-MH-02-8-13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown1.148	1.148	5.0	ug/l	37361	1	5.556	370458	50.0