
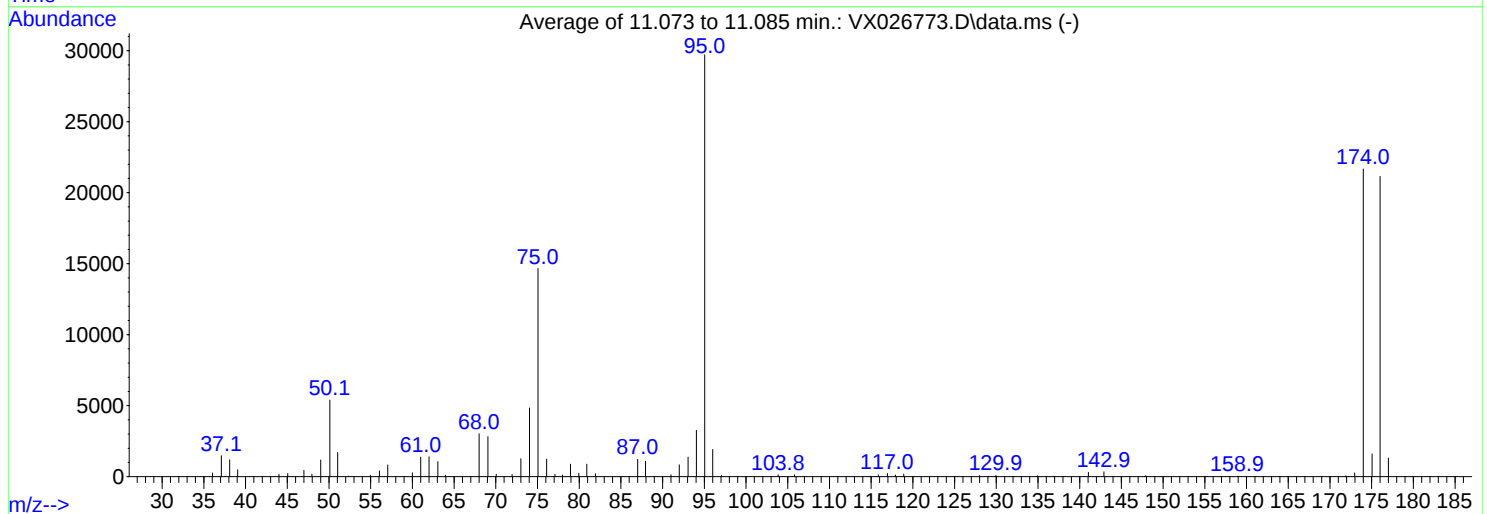


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020722\
Data File : VX026773.D
Acq On : 07 Feb 2022 09:33
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
Title : SW846 8260
Last Update : Tue Jan 11 14:45:13 2022

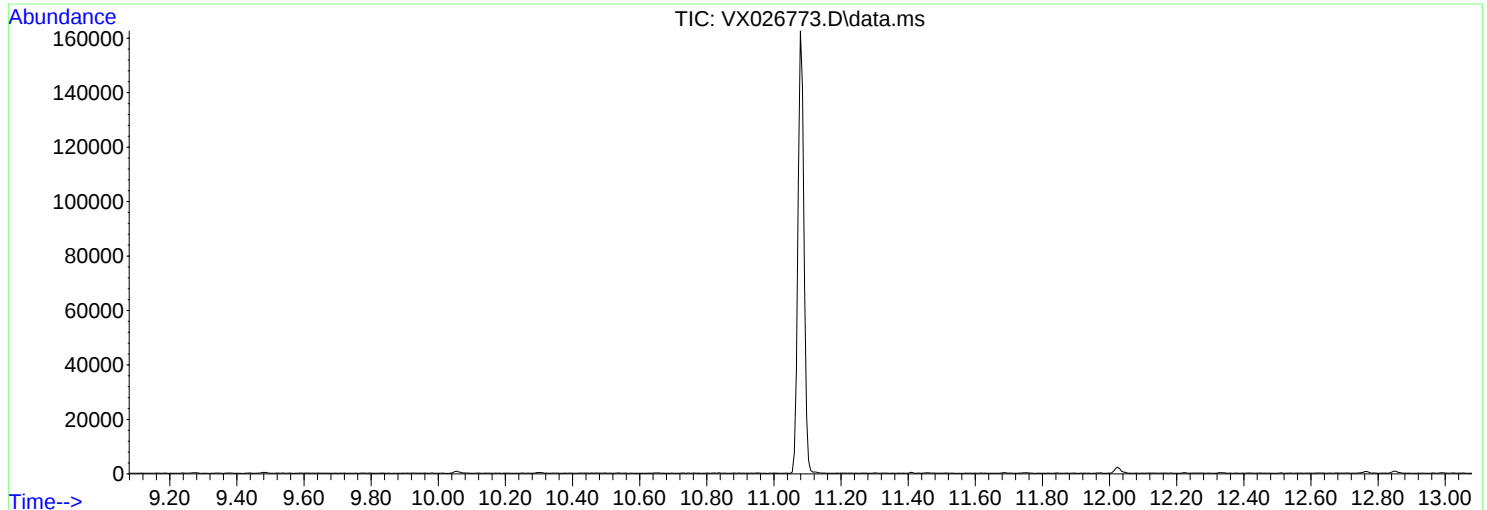

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.2	5396	PASS
75	95	30	60	49.3	14659	PASS
95	95	100	100	100.0	29707	PASS
96	95	5	9	6.5	1918	PASS
173	174	0.00	2	1.2	263	PASS
174	95	50	100	72.9	21669	PASS
175	174	5	9	7.4	1596	PASS
176	174	95	101	97.6	21157	PASS
177	176	5	9	6.2	1312	PASS