

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020723\
 Data File : VX034036.D
 Acq On : 06 Feb 2023 18:38
 Operator : JC/MD
 Sample : 01421-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB-RW10-GW-623-625

Quant Time: Feb 07 00:55:52 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020423W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 03 23:25:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	145144	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	201909	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	177901	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	83075	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	67855	48.494	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	96.980%
35) Dibromofluoromethane	5.385	113	63073	49.084	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.160%
50) Toluene-d8	8.647	98	229250	49.516	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	99.040%
62) 4-Bromofluorobenzene	11.079	95	78320	47.365	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	94.720%
Target Compounds						
16) Acetone	2.380	43	1215	2.056	ug/l	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020723\
Data File : VX034036.D
Acq On : 06 Feb 2023 18:38
Operator : JC/MD
Sample : 01421-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW10-GW-623-625

Quant Time: Feb 07 00:55:52 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020423W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 03 23:25:45 2023
Response via : Initial Calibration




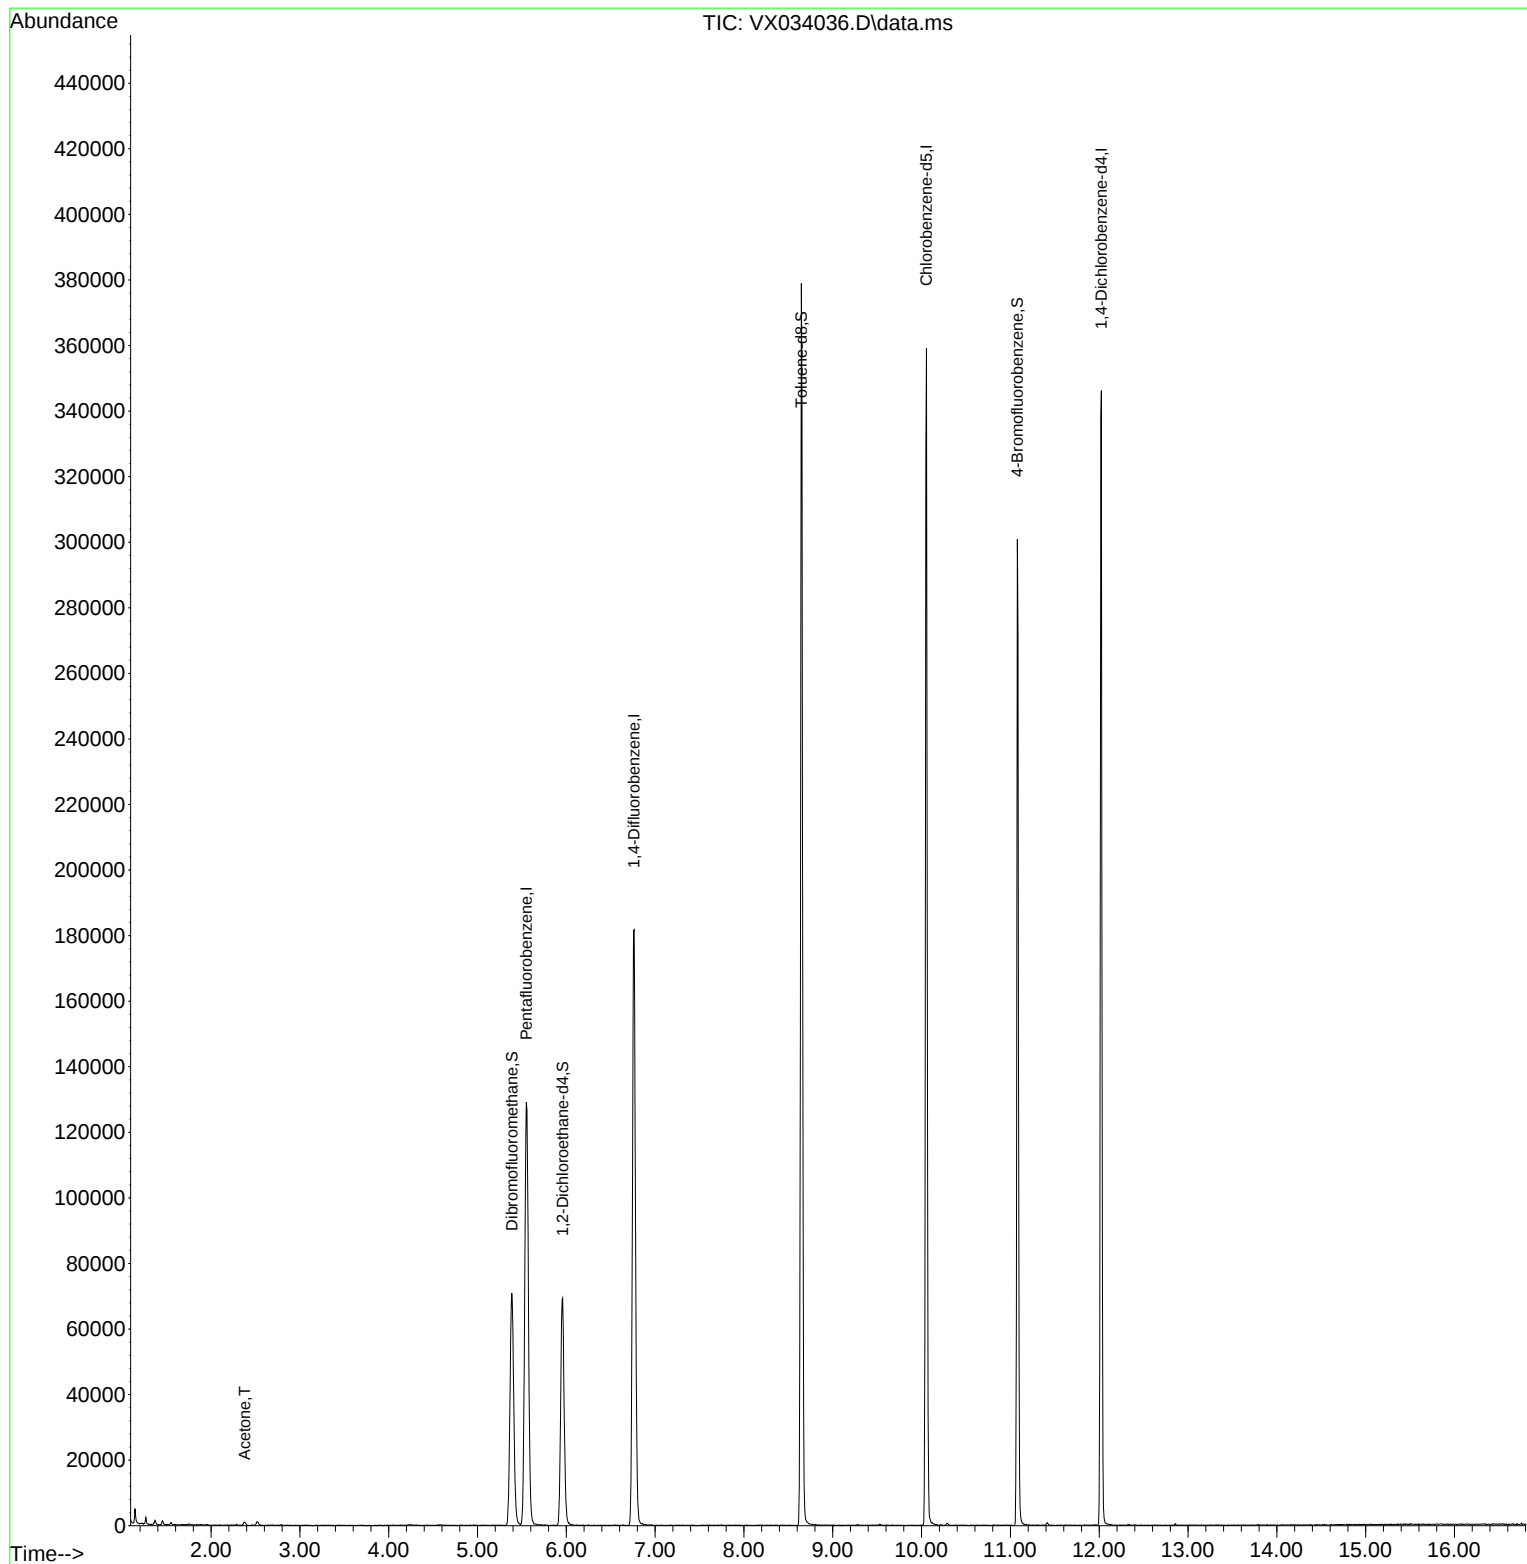


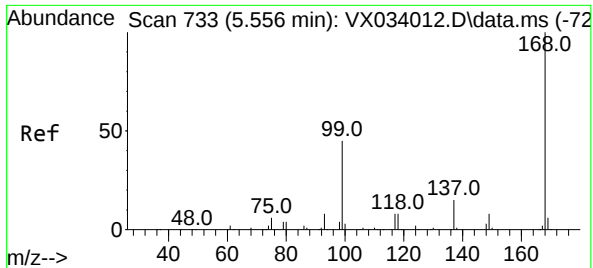

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX034036.D
Acq: 06 Feb 2023 18:38




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW10-GW-623-625


Tgt Ion:168 Resp: 145144
Ion Ratio Lower Upper
168 100
99 48.0 39.6 59.4

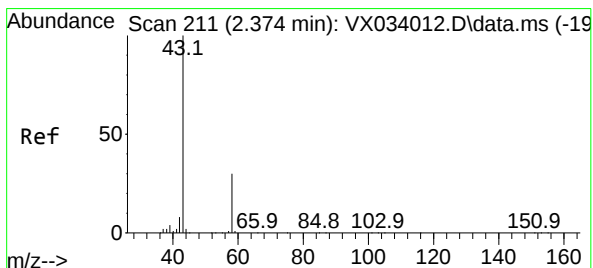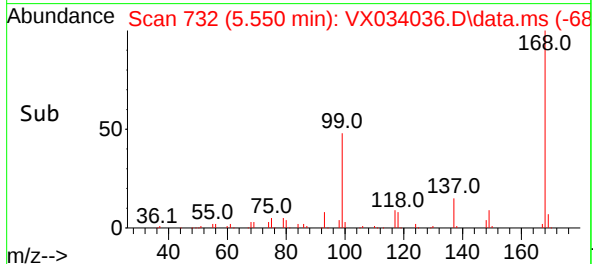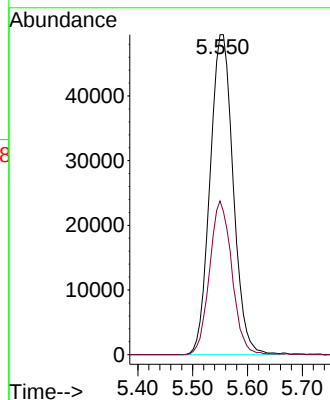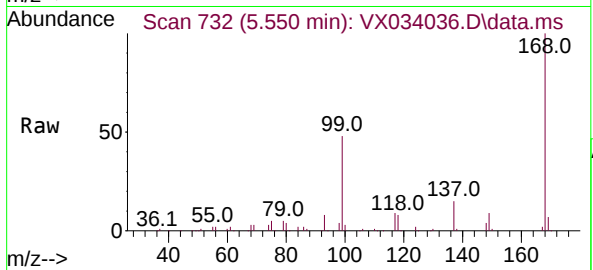

#16
Acetone
Concen: 2.056 ug/l
RT: 2.380 min Scan# 212
Delta R.T. 0.006 min
Lab File: VX034036.D
Acq: 06 Feb 2023 18:38

Tgt Ion: 43 Resp: 1215
Ion Ratio Lower Upper
43 100
58 30.5 22.6 33.8

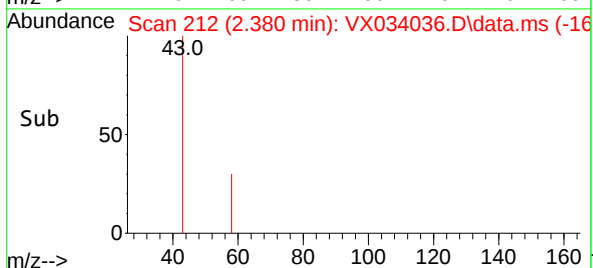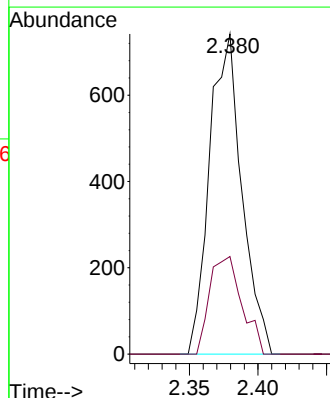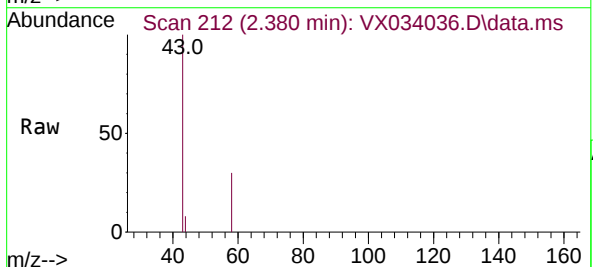

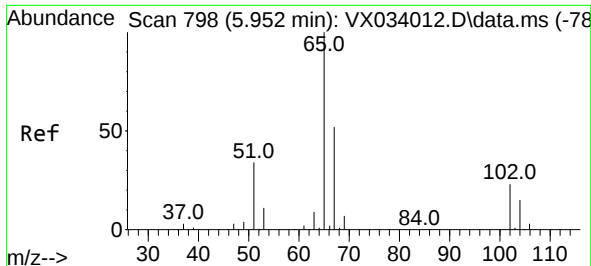

#33

1,2-Dichloroethane-d4

Concen: 48.494 ug/l

RT: 5.958 min Scan# 798

Delta R.T. 0.006 min

Lab File: VX034036.D

Acq: 06 Feb 2023 18:38

Instrument :

MSVOA_X

ClientSampleId :





BP-VPB-RW10-GW-623-625

Tgt Ion: 65 Resp: 67855

Ion Ratio Lower Upper

65 100

67 52.4 0.0 104.8

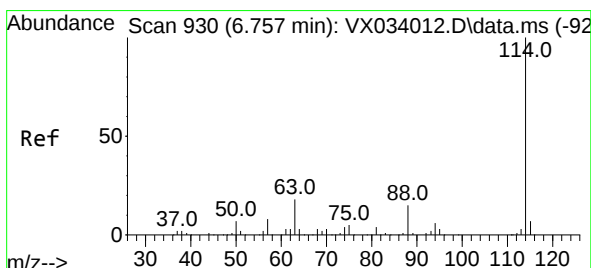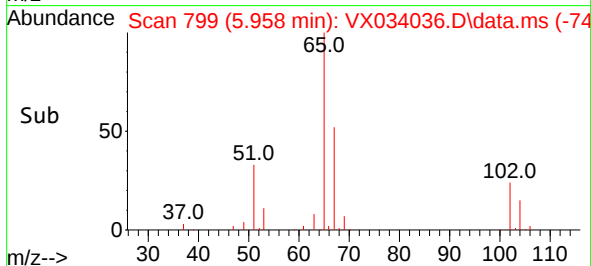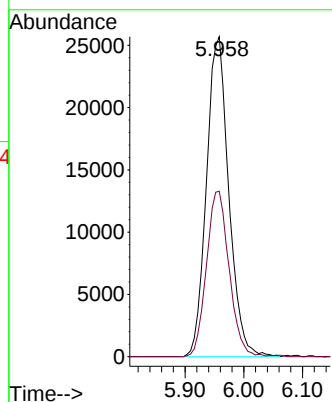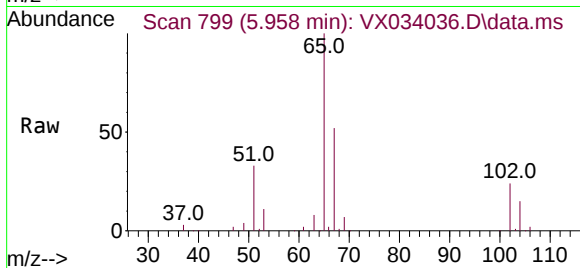

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.006 min

Lab File: VX034036.D

Acq: 06 Feb 2023 18:38




Tgt Ion: 114 Resp: 201909


Ion Ratio Lower Upper

114 100

63 17.5 0.0 37.4

88 14.6 0.0 30.6


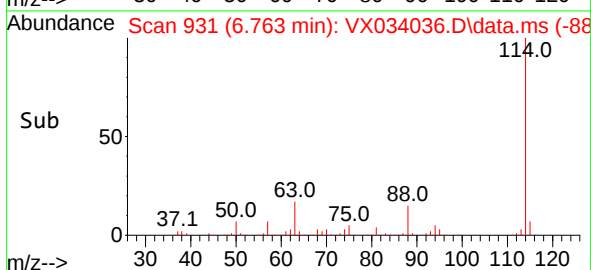
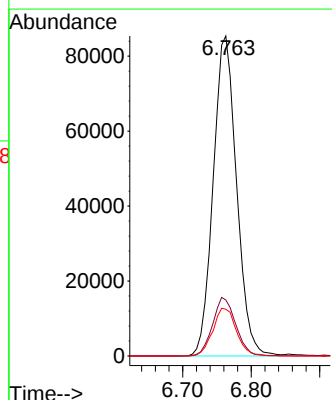
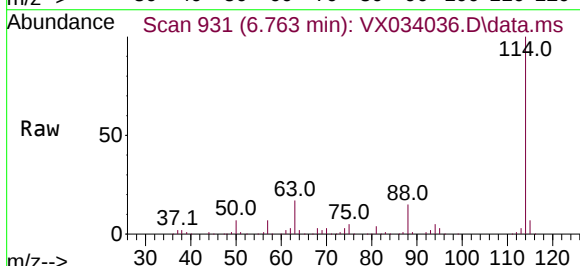


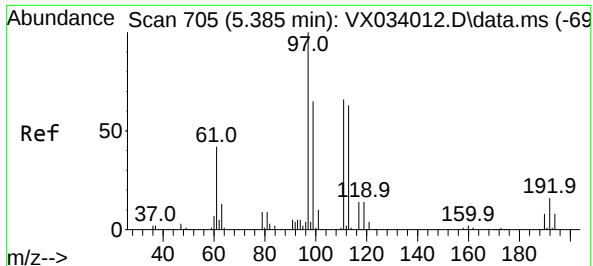

#35
Dibromofluoromethane
Concen: 49.084 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX034036.D
Acq: 06 Feb 2023 18:38




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW10-GW-623-625


Tgt Ion:113 Resp: 63073
Ion Ratio Lower Upper
113 100
111 101.8 83.0 124.6
192 25.0 19.0 28.4

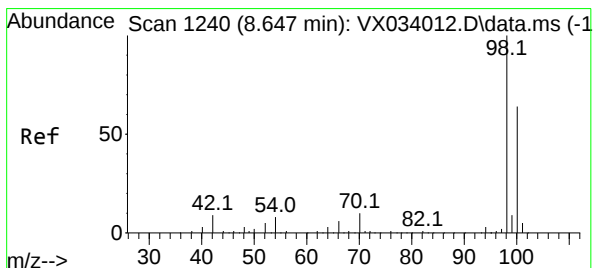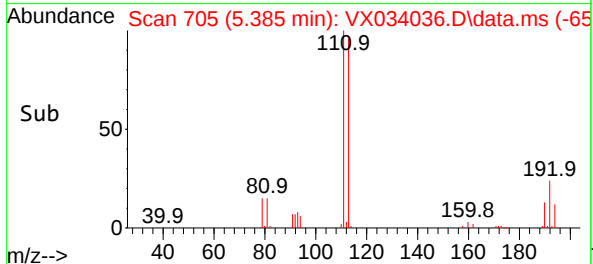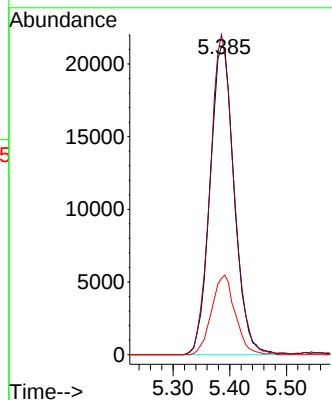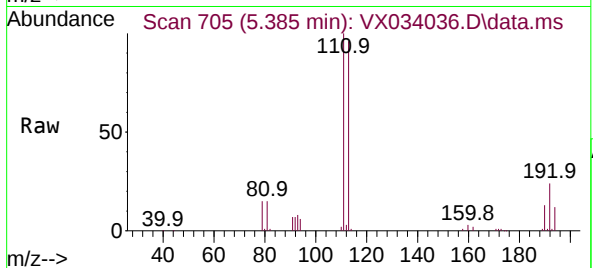

#50
Toluene-d8
Concen: 49.516 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.000 min
Lab File: VX034036.D
Acq: 06 Feb 2023 18:38

Tgt Ion: 98 Resp: 229250
Ion Ratio Lower Upper
98 100
100 66.5 53.6 80.4


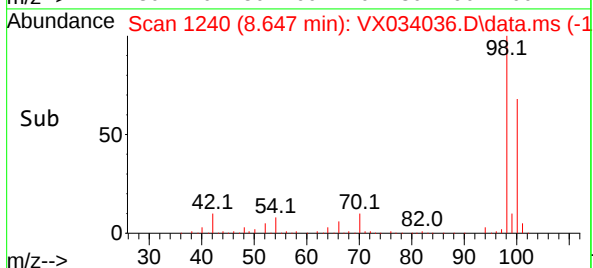
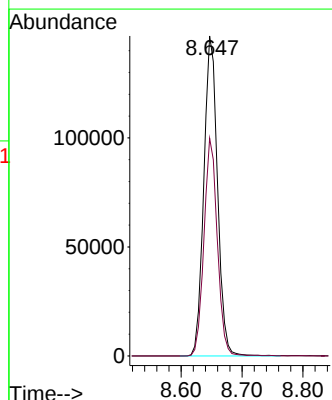
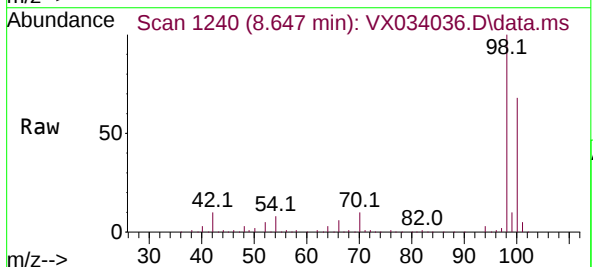


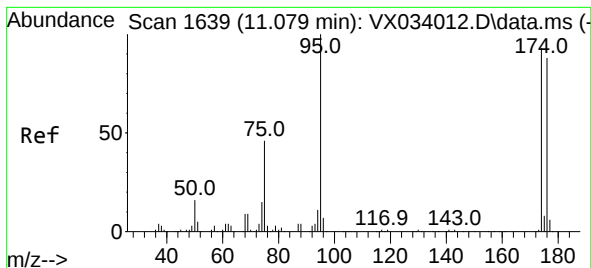

#62
4-Bromofluorobenzene
Concen: 47.365 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX034036.D
Acq: 06 Feb 2023 18:38




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW10-GW-623-625


Tgt Ion: 95 Resp: 78320
Ion Ratio Lower Upper
95 100
174 97.6 0.0 184.4
176 94.7 0.0 178.8

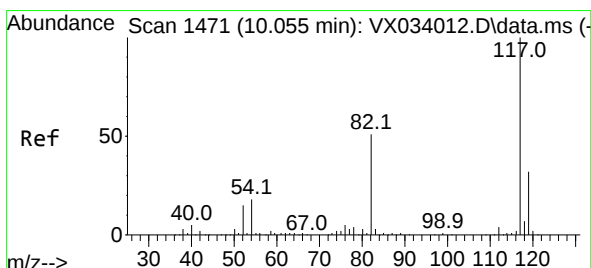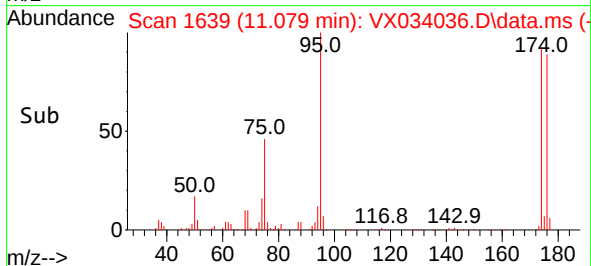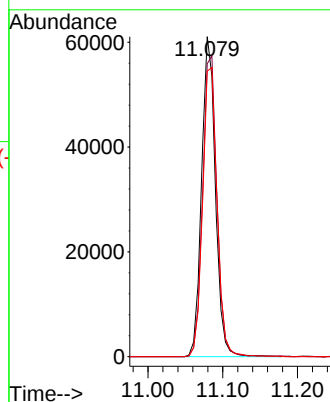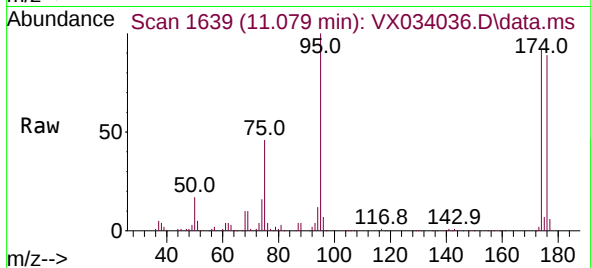

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX034036.D
Acq: 06 Feb 2023 18:38

Tgt Ion: 117 Resp: 177901
Ion Ratio Lower Upper
117 100
82 50.2 40.6 60.8
119 31.8 25.6 38.4

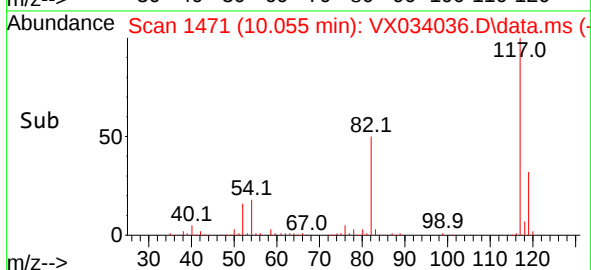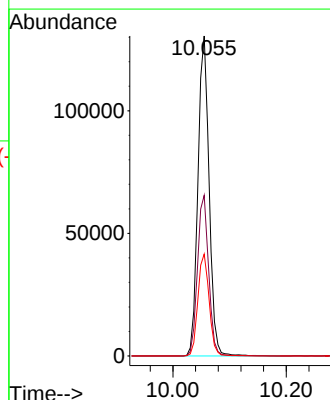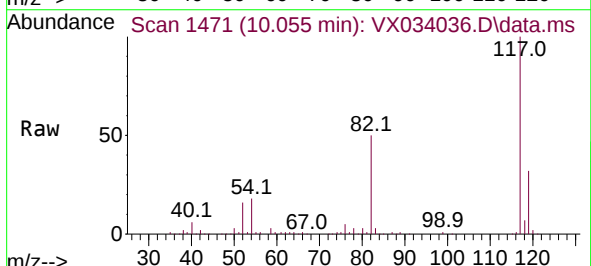

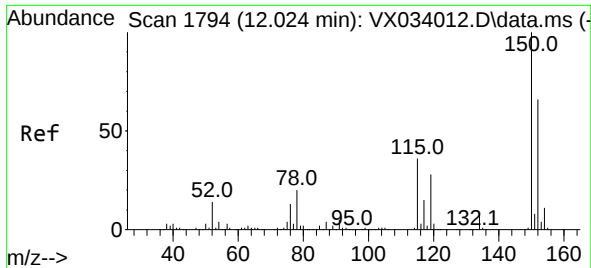

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX034036.D


Acq: 06 Feb 2023 18:38

Instrument :

MSVOA_X

ClientSampleId :

BP-VPB-RW10-GW-623-625

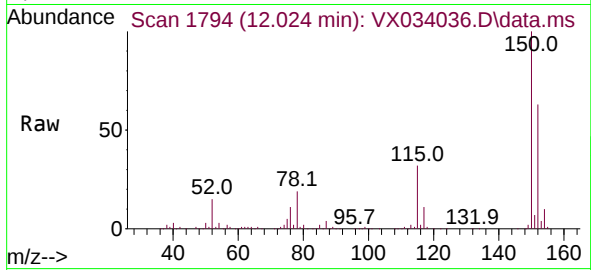

Tgt Ion:152 Resp: 83075

Ion Ratio Lower Upper

152 100

115 53.4 38.7 116.1

150 157.6 0.0 348.2

