

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020723\
 Data File : VX034038.D
 Acq On : 06 Feb 2023 19:25
 Operator : JC/MD
 Sample : 01308-23
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TRIP-BLANK

Quant Time: Feb 07 00:56:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020423W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 03 23:25:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	143396	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	200763	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	179768	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	87270	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	67249	48.646	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	97.300%
35) Dibromofluoromethane	5.385	113	63021	49.323	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.640%
50) Toluene-d8	8.647	98	227738	49.470	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	98.940%
62) 4-Bromofluorobenzene	11.079	95	79252	48.202	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	96.400%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020723\
Data File : VX034038.D
Acq On : 06 Feb 2023 19:25
Operator : JC/MD
Sample : 01308-23
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TRIP-BLANK

Quant Time: Feb 07 00:56:59 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020423W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 03 23:25:45 2023
Response via : Initial Calibration




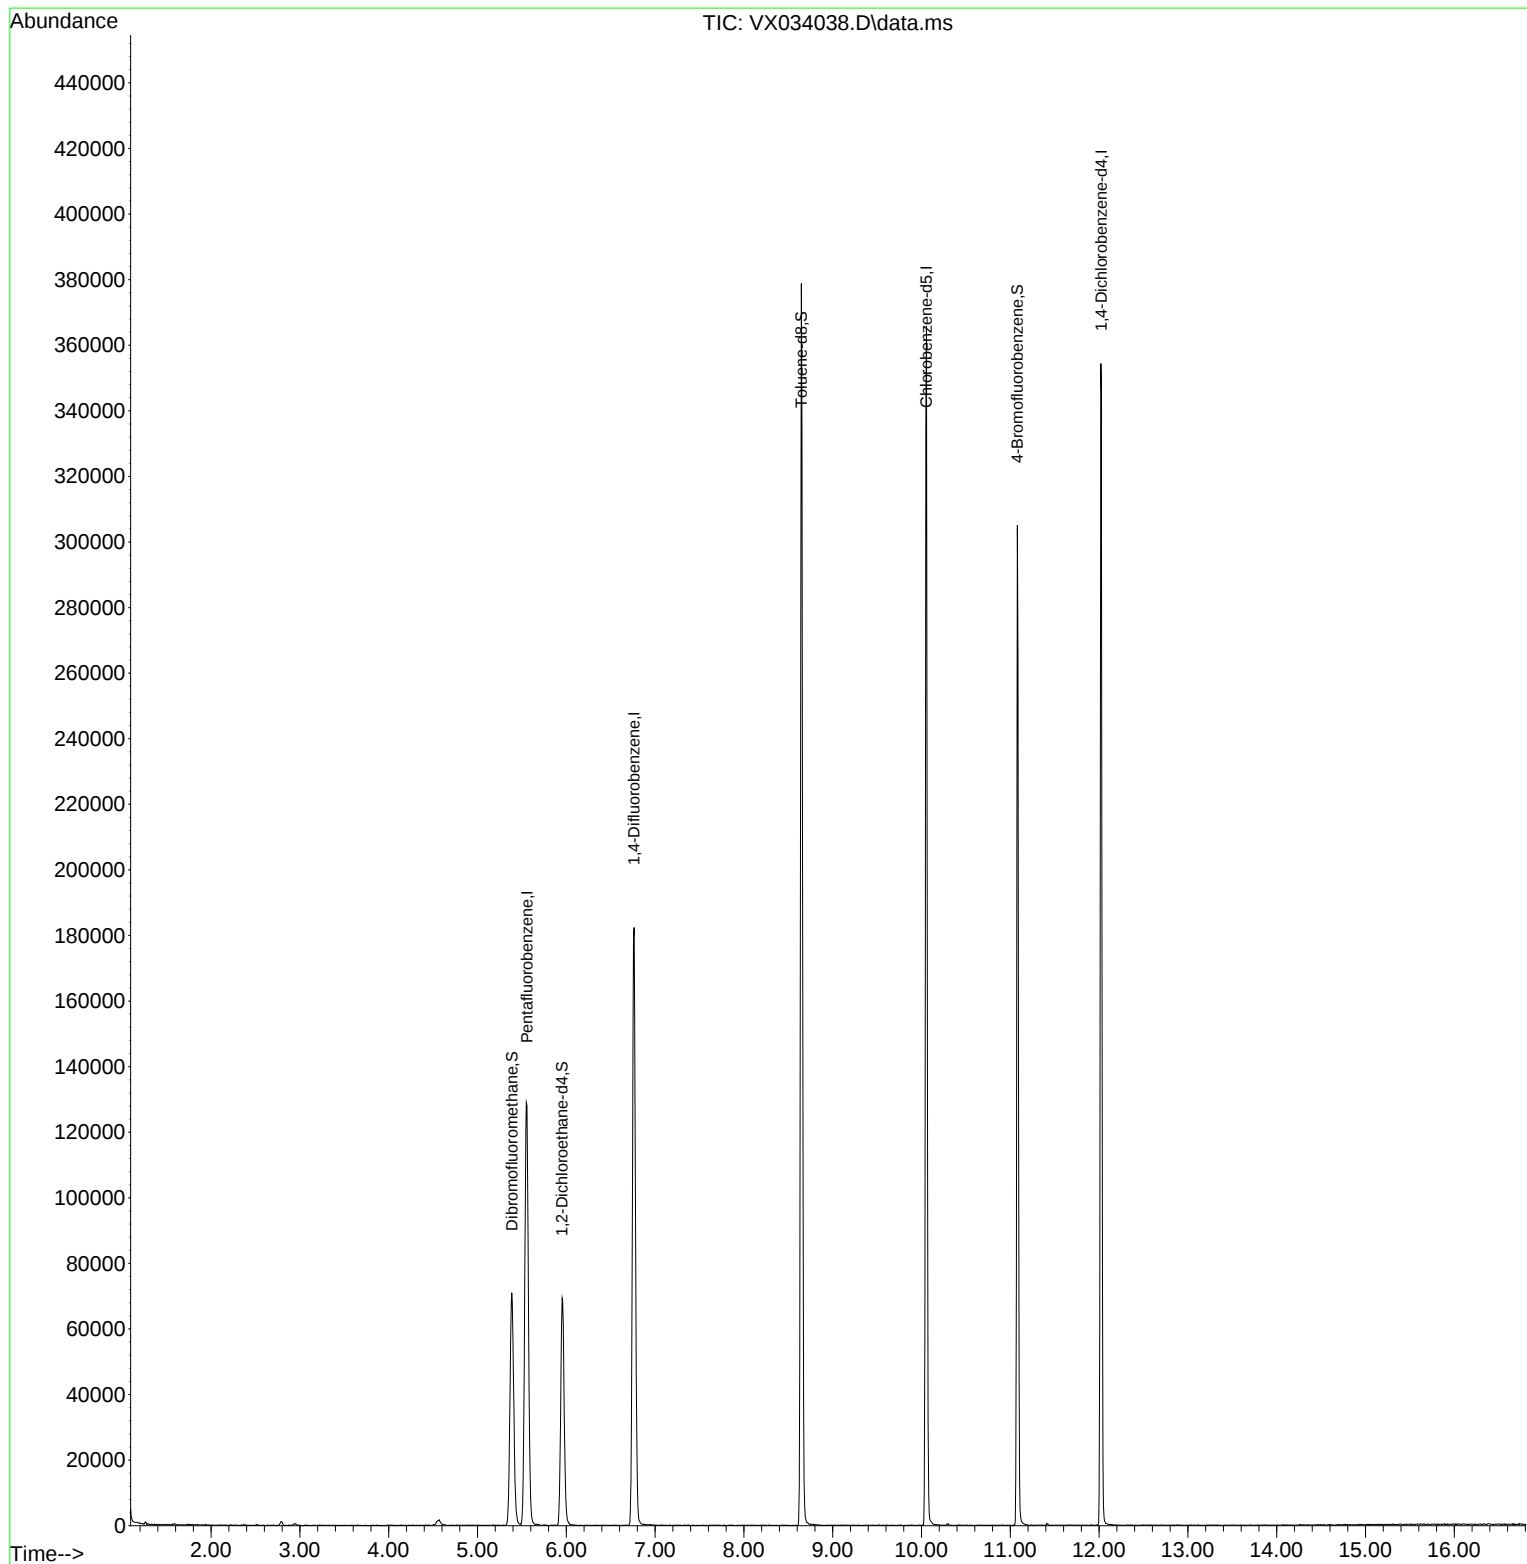


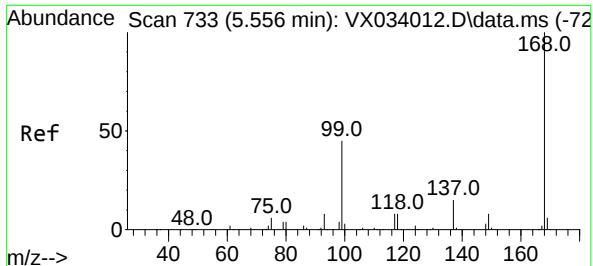

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.000 min
Lab File: VX034038.D
Acq: 06 Feb 2023 19:25




Instrument :
MSVOA_X
ClientSampleId :
TRIP-BLANK


Tgt Ion:168 Resp: 143396
Ion Ratio Lower Upper
168 100
99 47.6 39.6 59.4

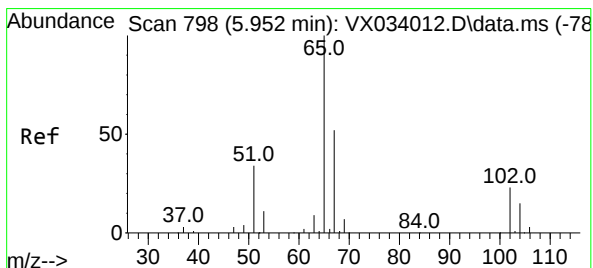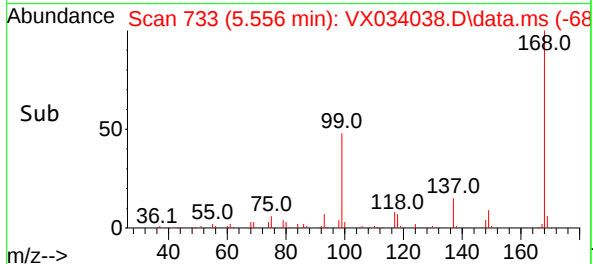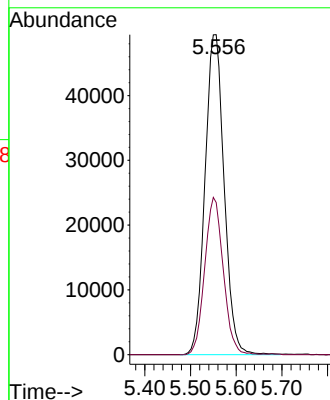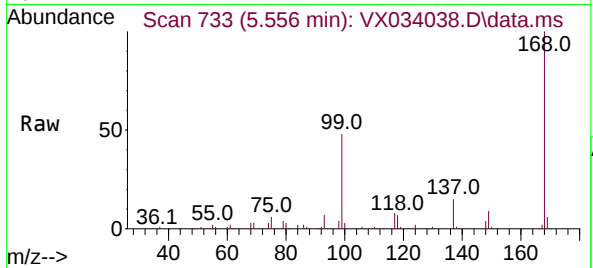

#33
1,2-Dichloroethane-d4
Concen: 48.646 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX034038.D
Acq: 06 Feb 2023 19:25

Tgt Ion: 65 Resp: 67249
Ion Ratio Lower Upper
65 100
67 52.4 0.0 104.8

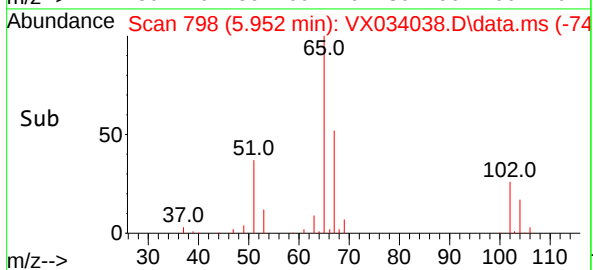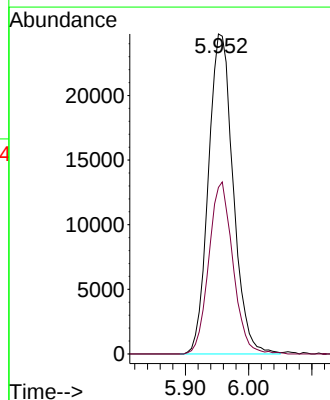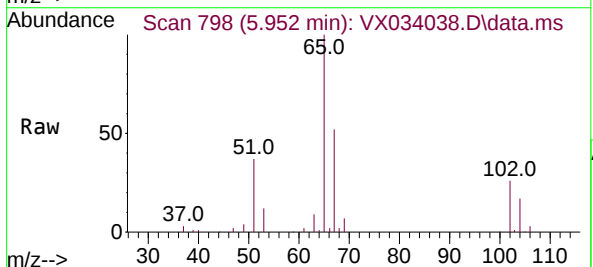

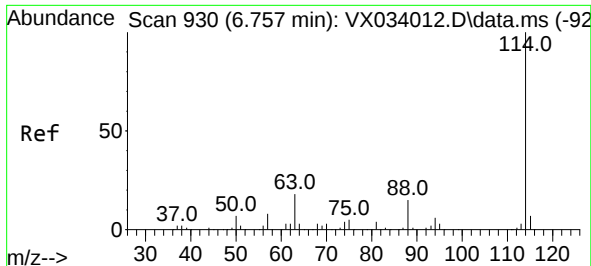

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 91

Delta R.T. 0.006 min

Lab File: VX034038.D

Acq: 06 Feb 2023 19:25

Instrument :

MSVOA_X

ClientSampleId :

TRIP-BLANK





Tgt Ion:114 Resp: 200763

Ion Ratio Lower Upper

114 100

63 18.3 0.0 37.4

88 15.3 0.0 30.6

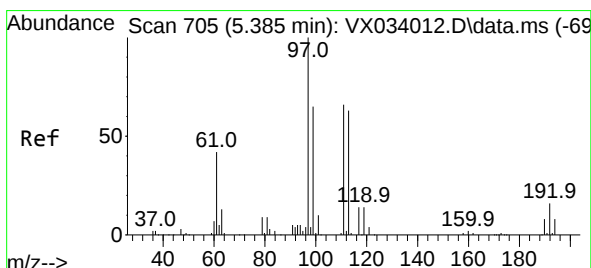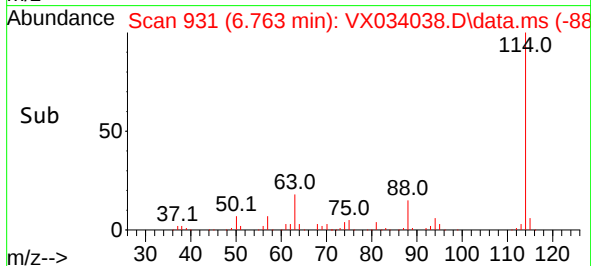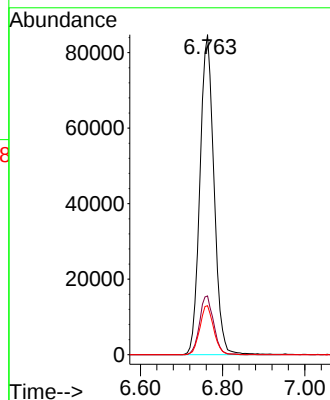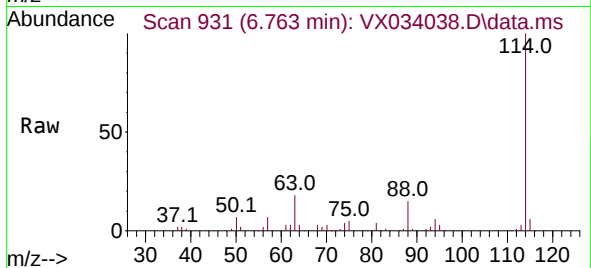

#35

Dibromofluoromethane

Concen: 49.323 ug/l

RT: 5.385 min Scan# 705

Delta R.T. 0.000 min

Lab File: VX034038.D

Acq: 06 Feb 2023 19:25




Tgt Ion:113 Resp: 63021


Ion Ratio Lower Upper

113 100

111 100.8 83.0 124.6

192 25.0 19.0 28.4


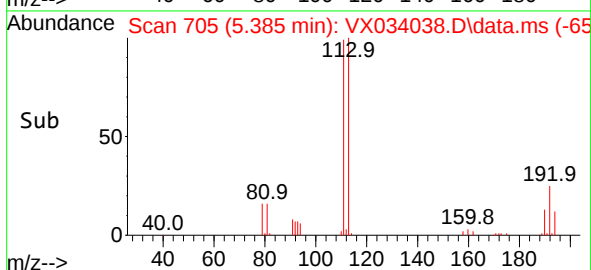
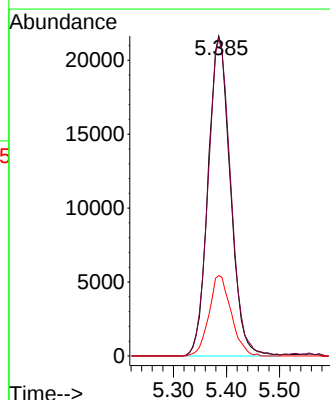
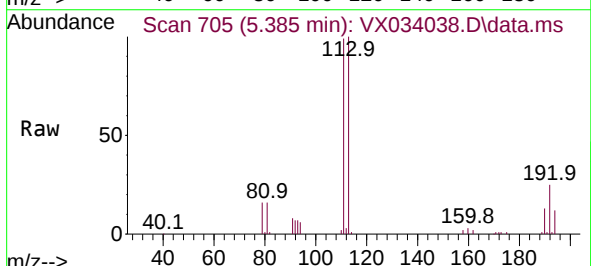


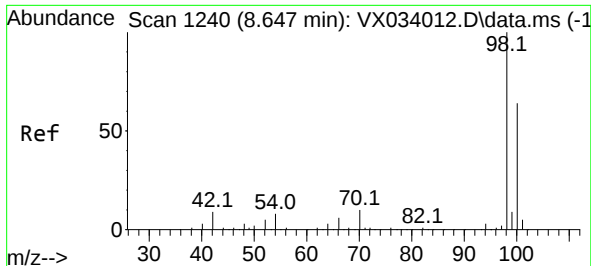

#50
Toluene-d8
Concen: 49.470 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX034038.D
Acq: 06 Feb 2023 19:25




Instrument :
MSVOA_X
ClientSampleId :
TRIP-BLANK


Tgt Ion: 98 Resp: 227738
Ion Ratio Lower Upper
98 100
100 67.6 53.6 80.4

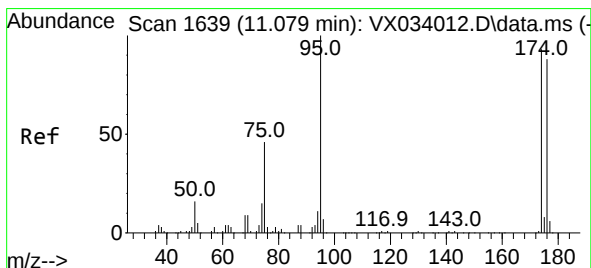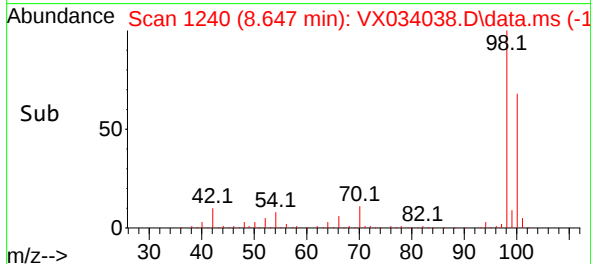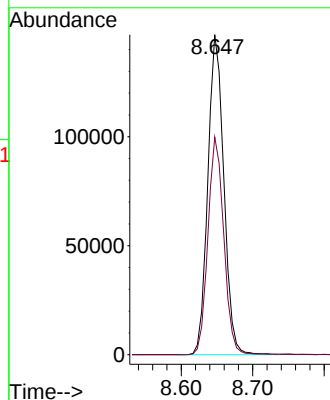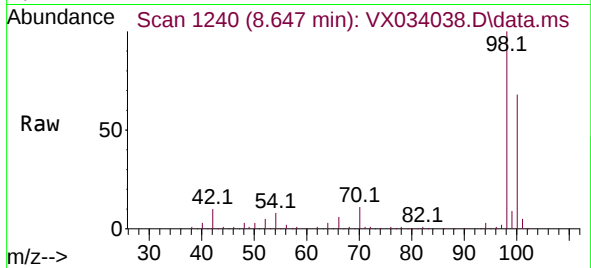

#62
4-Bromofluorobenzene
Concen: 48.202 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX034038.D
Acq: 06 Feb 2023 19:25

Tgt Ion: 95 Resp: 79252
Ion Ratio Lower Upper
95 100
174 97.3 0.0 184.4
176 96.5 0.0 178.8


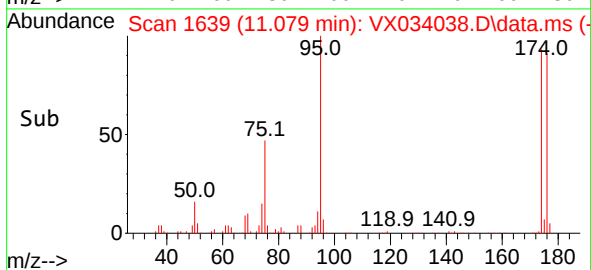
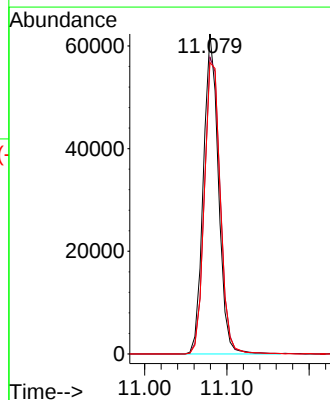
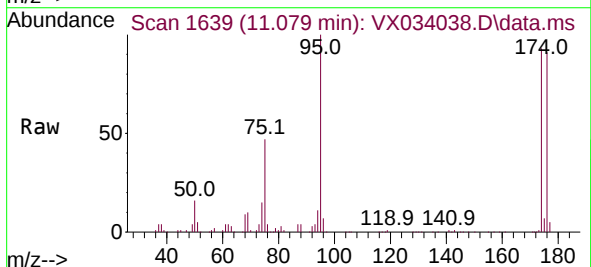


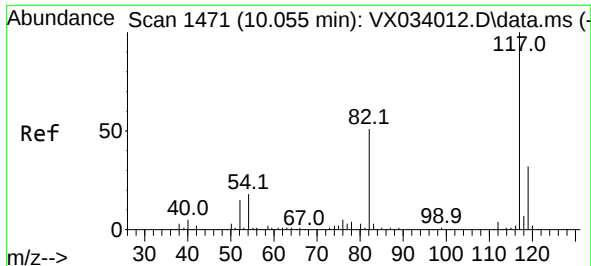

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX034038.D
Acq: 06 Feb 2023 19:25

Instrument :
MSVOA_X
ClientSampleId :
TRIP-BLANK

Tgt Ion:117 Resp: 179768
Ion Ratio Lower Upper
117 100
82 49.4 40.6 60.8
119 31.6 25.6 38.4

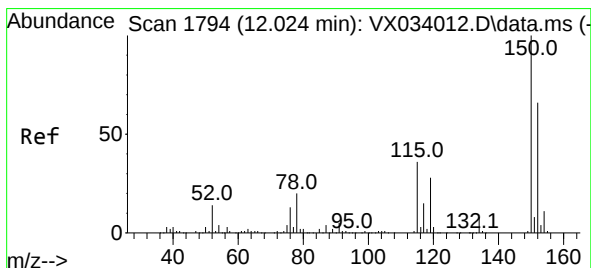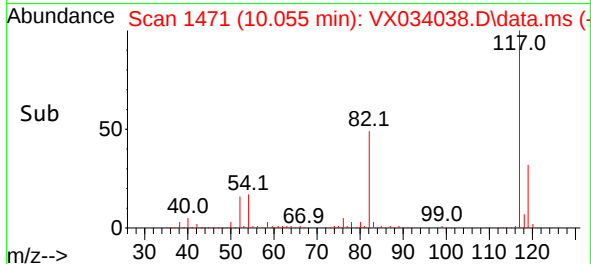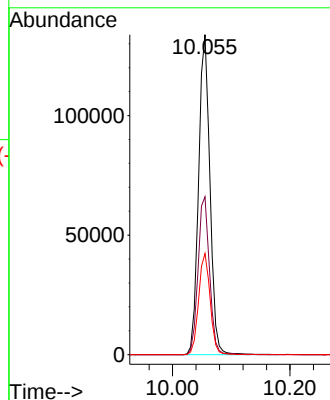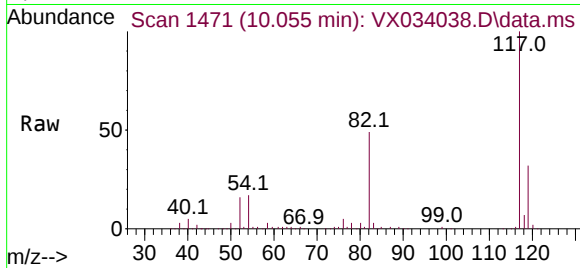

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX034038.D
Acq: 06 Feb 2023 19:25

Tgt Ion:152 Resp: 87270
Ion Ratio Lower Upper
152 100
115 53.5 38.7 116.1
150 157.2 0.0 348.2

