

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020723\
 Data File : VX034042.D
 Acq On : 06 Feb 2023 20:57
 Operator : JC/MD
 Sample : 01442-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB-2023-2-2

Quant Time: Feb 07 00:58:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020423W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 03 23:25:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	140633	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	198783	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	177816	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	89972	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	67145	49.525	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	99.060%
35) Dibromofluoromethane	5.385	113	61934	48.955	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	97.920%
50) Toluene-d8	8.647	98	223667	49.070	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	98.140%
62) 4-Bromofluorobenzene	11.079	95	80290	49.320	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	98.640%


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020723\
Data File : VX034042.D
Acq On : 06 Feb 2023 20:57
Operator : JC/MD
Sample : 01442-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-2023-2-2

Quant Time: Feb 07 00:58:37 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020423W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 03 23:25:45 2023
Response via : Initial Calibration

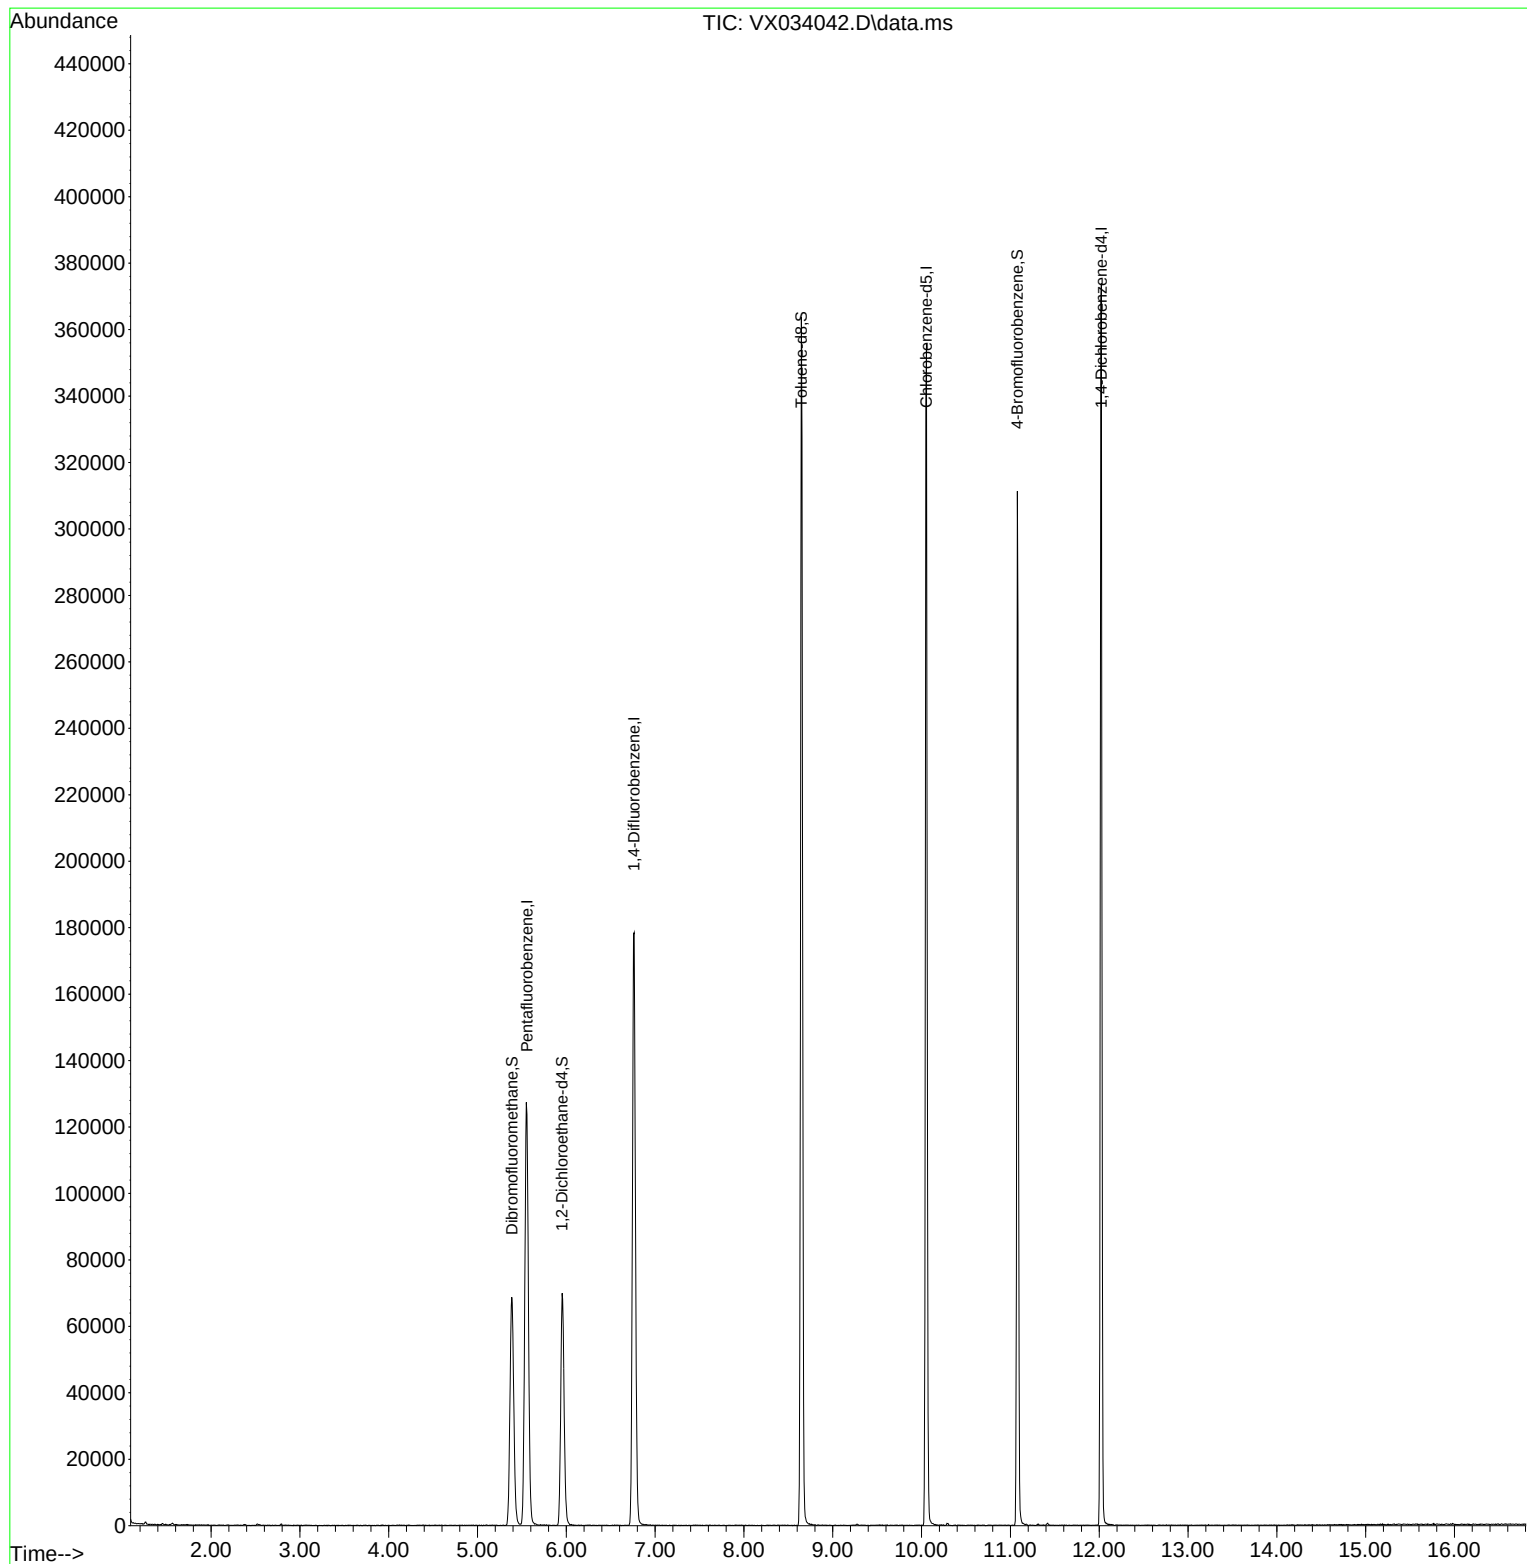

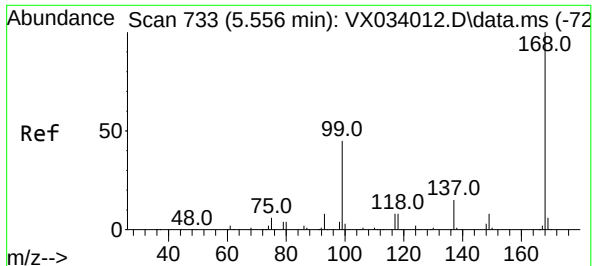


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 713
Delta R.T. -0.000 min
Lab File: VX034042.D
Acq: 06 Feb 2023 20:57

Instrument :




MSVOA_X

ClientSampleId :

TB-2023-2-2



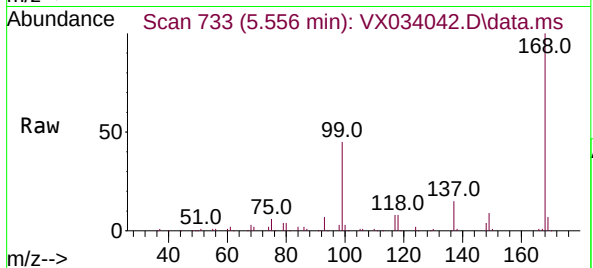



Tgt Ion:168 Resp: 140633
Ion Ratio Lower Upper
168 100
99 45.0 39.6 59.4

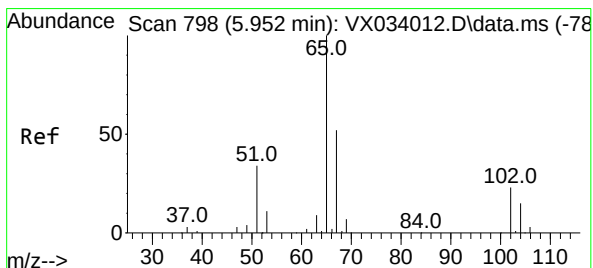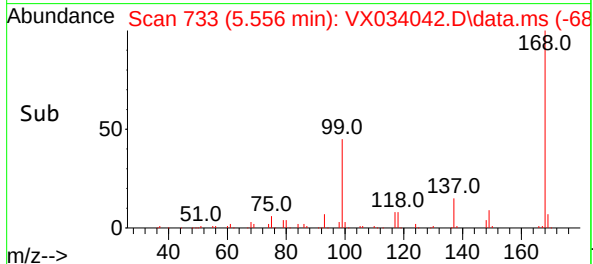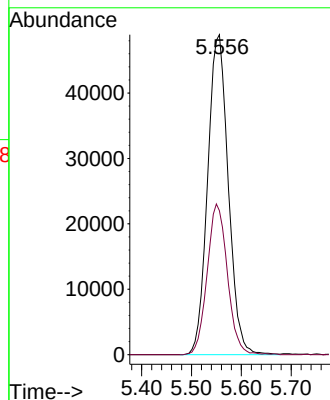

#33
1,2-Dichloroethane-d4
Concen: 49.525 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX034042.D
Acq: 06 Feb 2023 20:57

Tgt Ion: 65 Resp: 67145
Ion Ratio Lower Upper
65 100
67 52.0 0.0 104.8


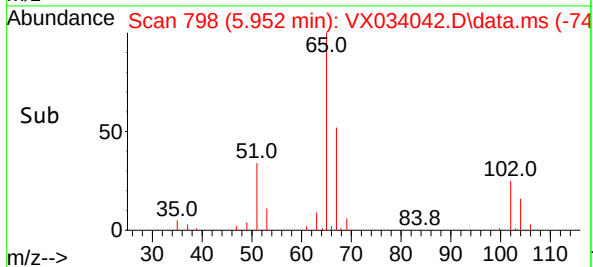
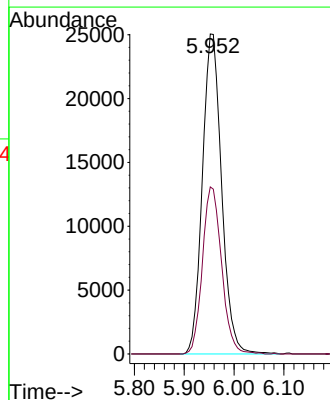
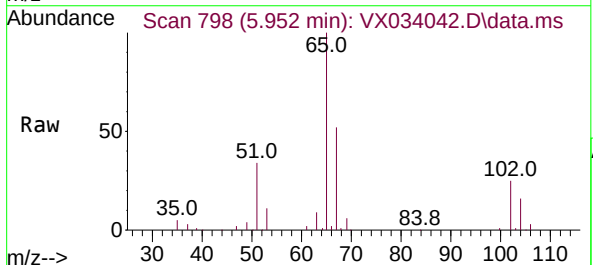


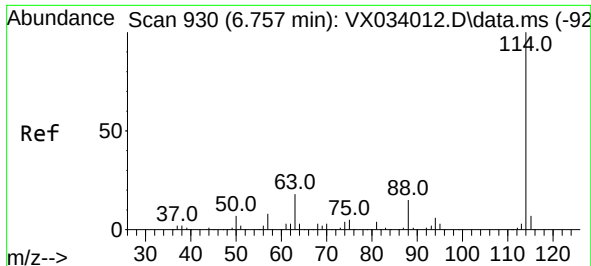

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.006 min
Lab File: VX034042.D
Acq: 06 Feb 2023 20:57




Instrument :
MSVOA_X
ClientSampleId :
TB-2023-2-2


Tgt Ion:114 Resp: 198783
Ion Ratio Lower Upper
114 100
63 17.4 0.0 37.4
88 14.6 0.0 30.6

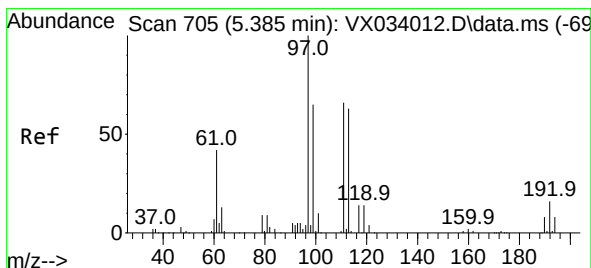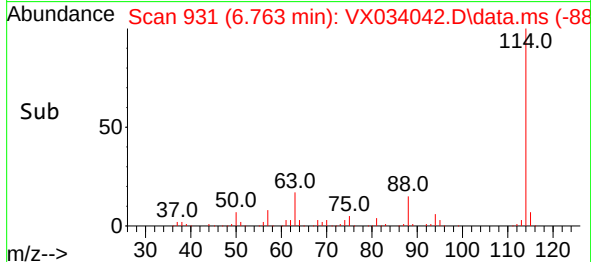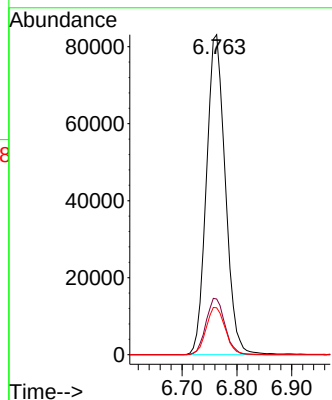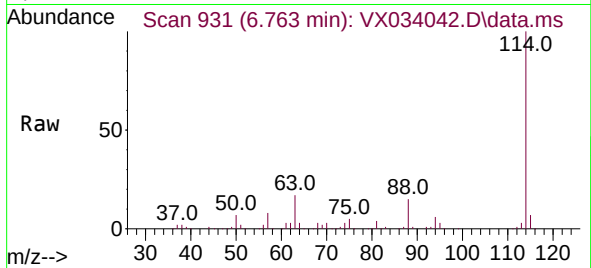

#35
Dibromofluoromethane
Concen: 48.955 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX034042.D
Acq: 06 Feb 2023 20:57

Tgt Ion:113 Resp: 61934
Ion Ratio Lower Upper
113 100
111 102.0 83.0 124.6
192 25.2 19.0 28.4


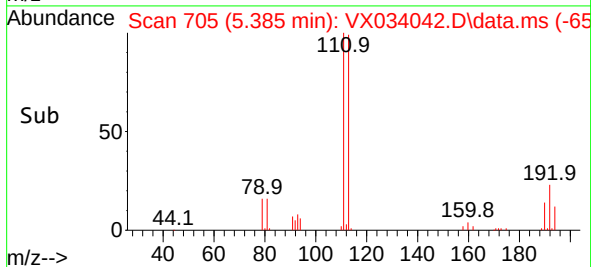
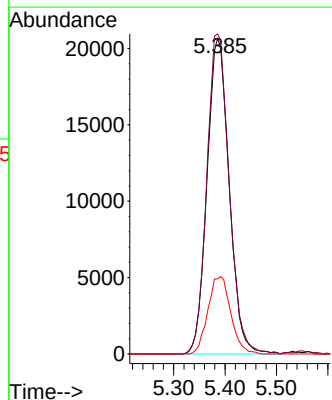
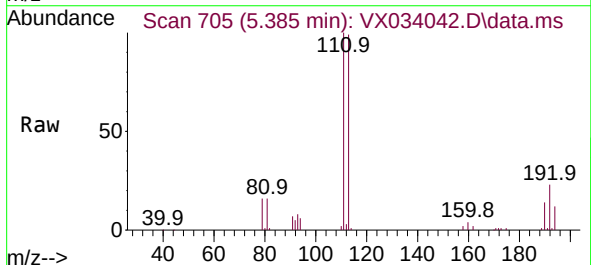


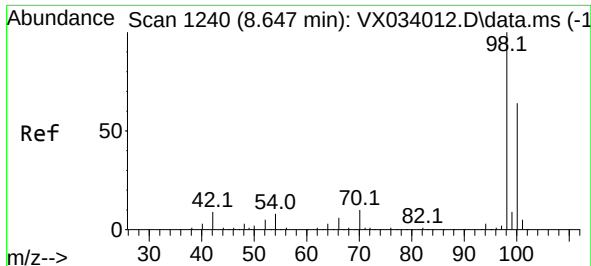

#50
Toluene-d8
Concen: 49.070 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX034042.D
Acq: 06 Feb 2023 20:57




Instrument :
MSVOA_X
ClientSampleId :
TB-2023-2-2


Tgt Ion: 98 Resp: 223667
Ion Ratio Lower Upper
98 100
100 66.9 53.6 80.4

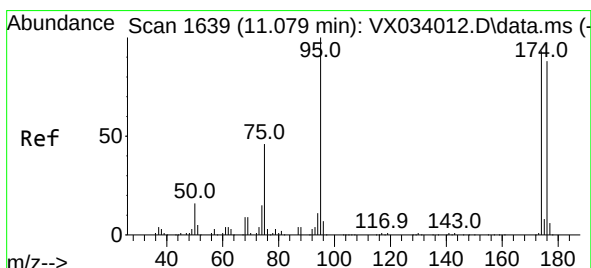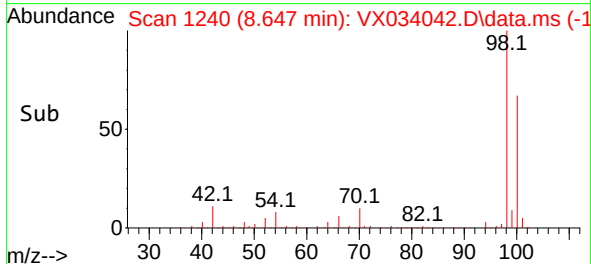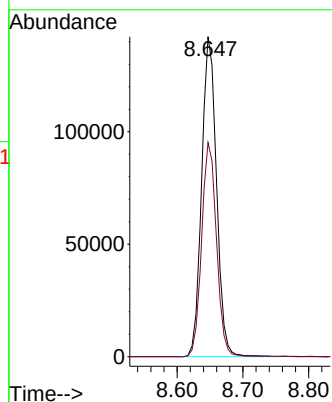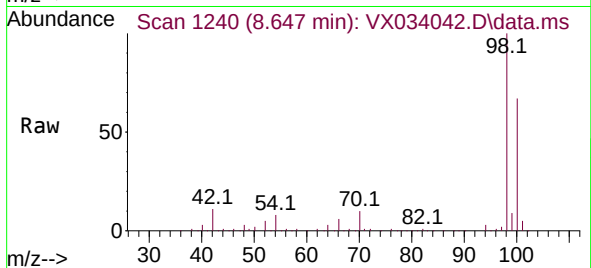

#62
4-Bromofluorobenzene
Concen: 49.320 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX034042.D
Acq: 06 Feb 2023 20:57

Tgt Ion: 95 Resp: 80290
Ion Ratio Lower Upper
95 100
174 97.6 0.0 184.4
176 95.5 0.0 178.8


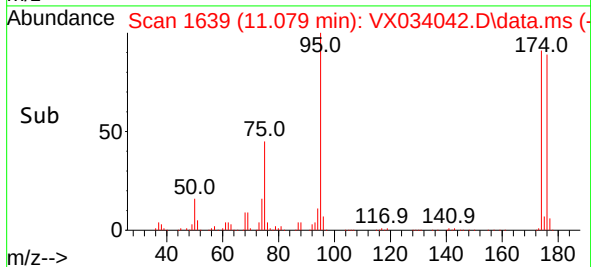
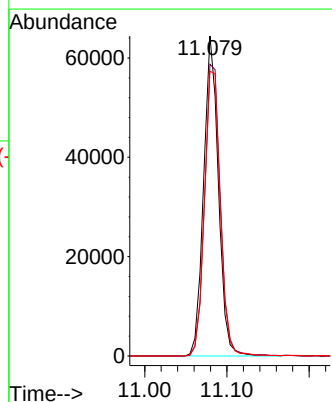
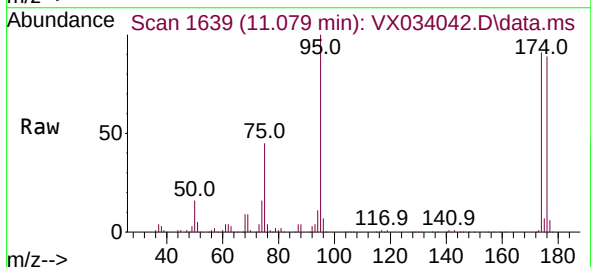


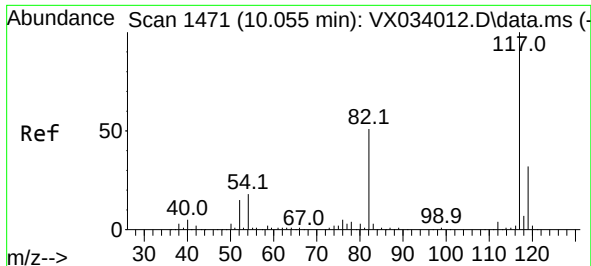

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX034042.D
Acq: 06 Feb 2023 20:57

Instrument :
MSVOA_X
ClientSampleId :
TB-2023-2-2

Tgt Ion:117 Resp: 177816
Ion Ratio Lower Upper
117 100
82 49.1 40.6 60.8
119 32.3 25.6 38.4

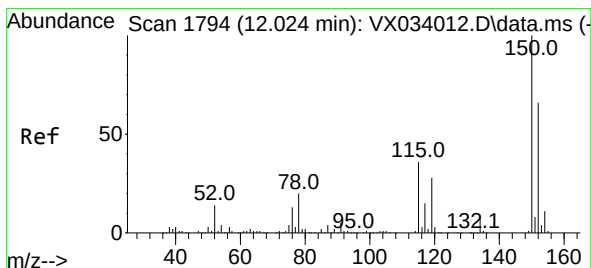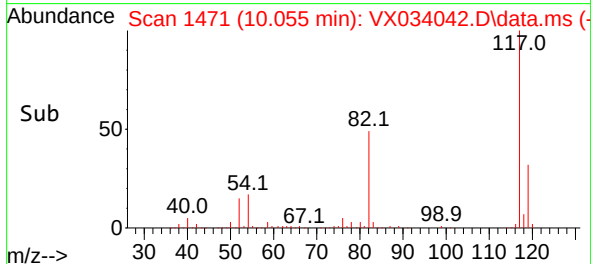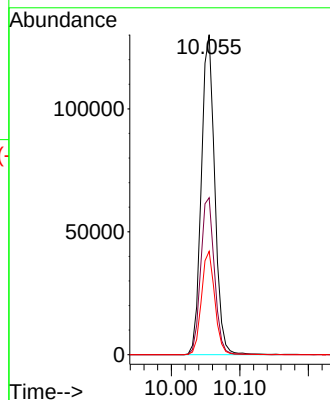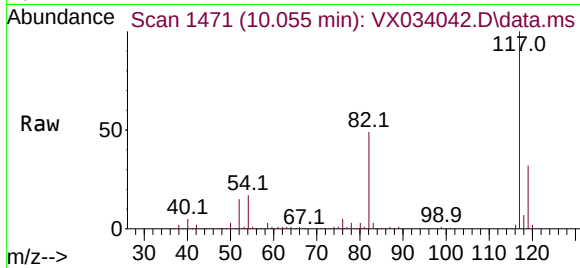

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX034042.D
Acq: 06 Feb 2023 20:57

Tgt Ion:152 Resp: 89972
Ion Ratio Lower Upper
152 100
115 52.9 38.7 116.1
150 155.8 0.0 348.2

