

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020723\
 Data File : VX034043.D
 Acq On : 06 Feb 2023 21:21
 Operator : JC/MD
 Sample : 01442-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EB-2023-2-3

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020423W.M

Title : SW846 8260

Signal : TIC: VX034043.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	34	rVB	10028	8741	1.58%	0.291%
2	2.947	298	305	315	rBV	3687	8638	1.56%	0.287%
3	4.556	559	569	581	rBV	3730	12258	2.22%	0.408%
4	5.385	695	705	722	rBV2	67124	196281	35.52%	6.528%
5	5.550	722	732	748	rVV	123126	346903	62.78%	11.537%
6	5.958	789	799	815	rBV	67774	178631	32.33%	5.941%
7	6.763	921	931	949	rBV	169206	409302	74.08%	13.612%
8	8.647	1233	1240	1251	rBV	354493	552550	100.00%	18.376%
9	10.055	1465	1471	1479	rBV	336658	470217	85.10%	15.638%
10	11.079	1634	1639	1652	rBV	292777	376955	68.22%	12.536%
11	12.024	1788	1794	1804	rBV	346232	446418	80.79%	14.846%




Sum of corrected areas: 3006894

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020723\
Data File : VX034043.D
Acq On : 06 Feb 2023 21:21
Operator : JC/MD
Sample : 01442-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-2023-2-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020423W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

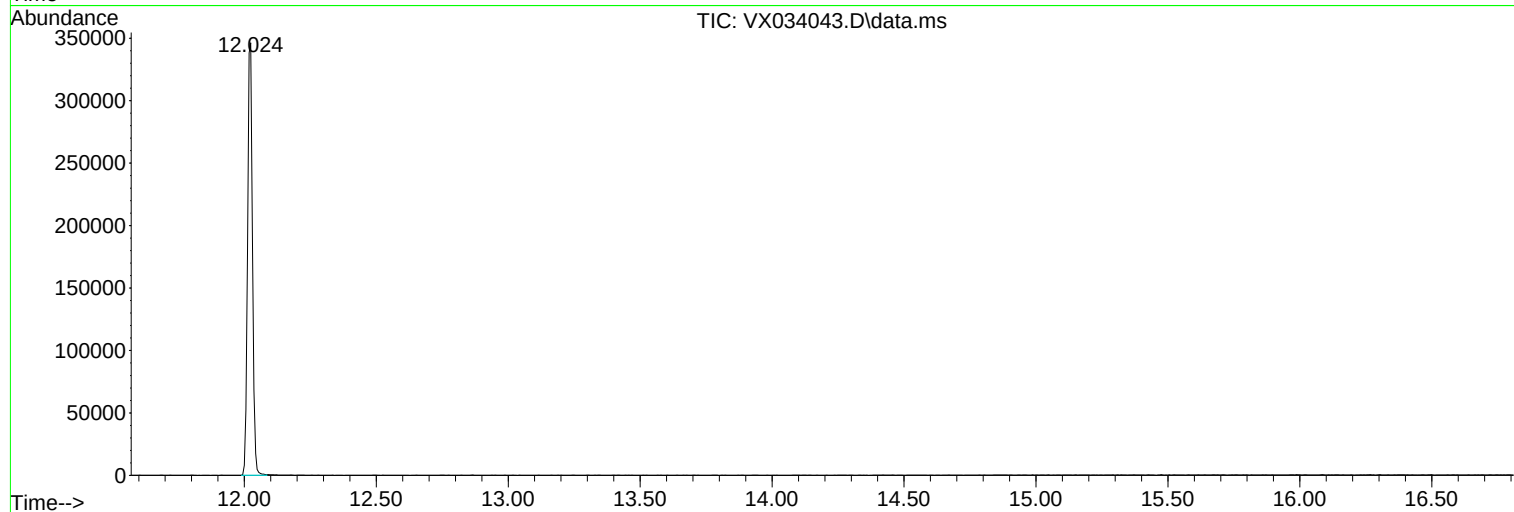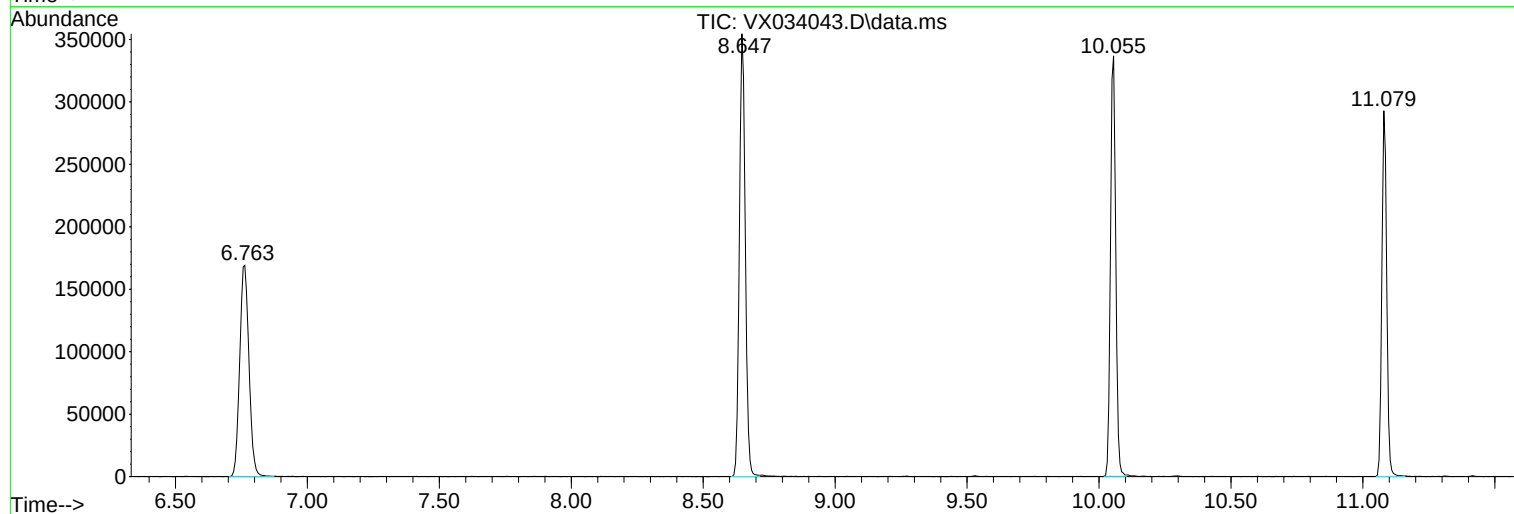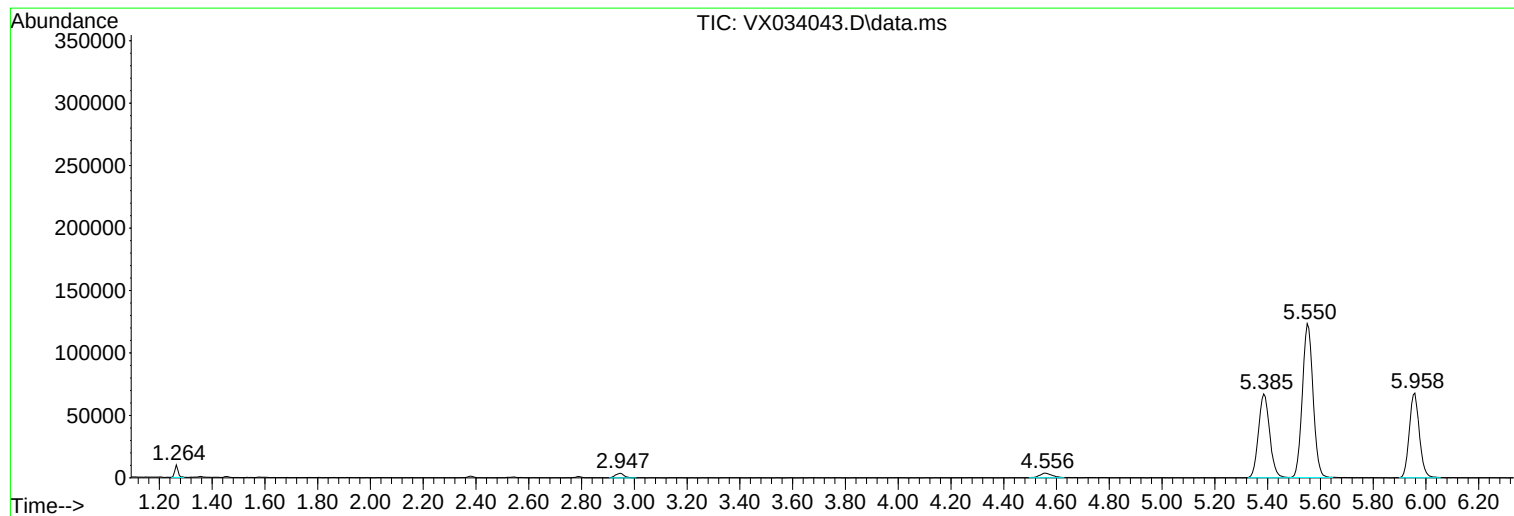

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020723\
Data File : VX034043.D
Acq On : 06 Feb 2023 21:21
Operator : JC/MD
Sample : 01442-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-2023-2-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020423W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020723\
Data File : VX034043.D
Acq On : 06 Feb 2023 21:21
Operator : JC/MD
Sample : 01442-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-2023-2-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020423W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------