
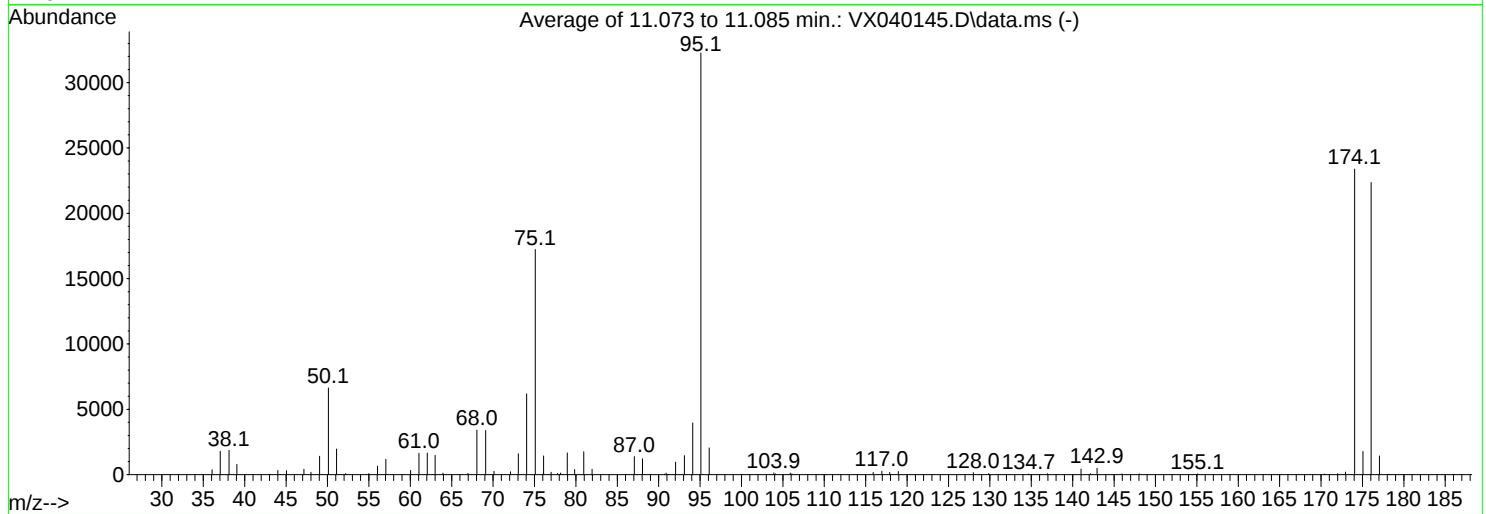


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020724\
Data File : VX040145.D
Acq On : 07 Feb 2024 08:33
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X013024W.M
Title : SW846 8260
Last Update : Thu Feb 01 05:44:39 2024

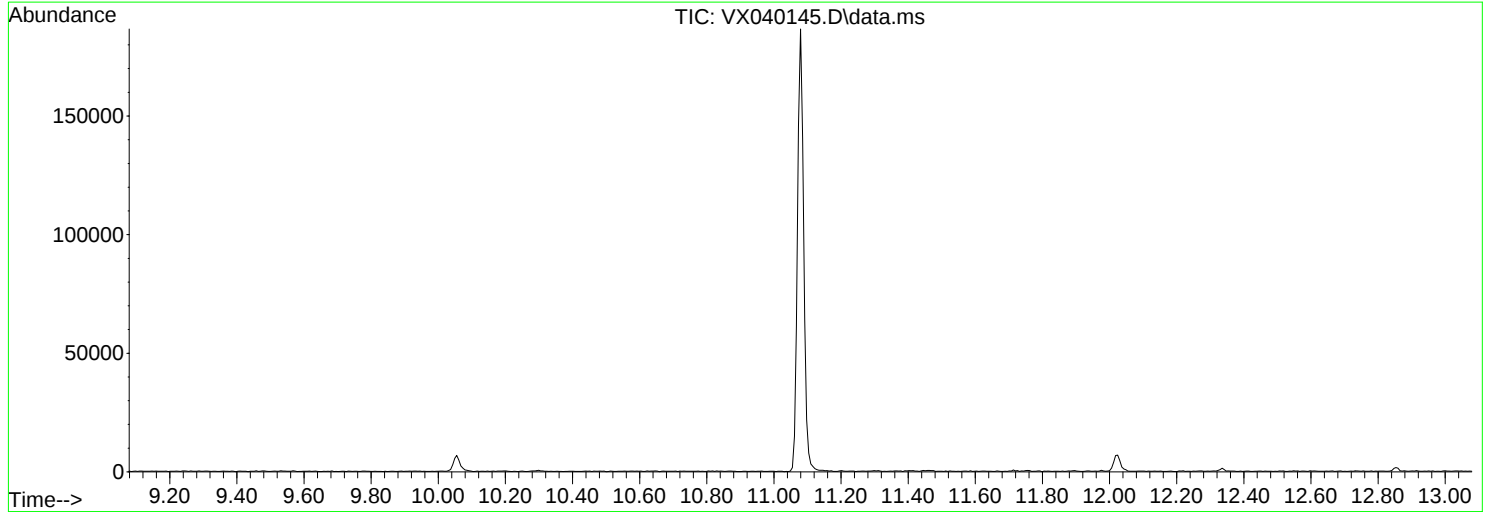

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.6	6641	PASS
75	95	30	60	53.4	17231	PASS
95	95	100	100	100.0	32277	PASS
96	95	5	9	6.3	2049	PASS
173	174	0.00	2	0.9	199	PASS
174	95	50	100	72.5	23387	PASS
175	174	5	9	7.6	1780	PASS
176	174	95	101	95.6	22355	PASS
177	176	5	9	6.4	1434	PASS