


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020821\
Data File : VX020875.D
Acq On : 08 Feb 2021 09:57
Operator : JC/MD
Sample : BFB66
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB66

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM020821WMA.M
Title : VOC Analysis
Last Update : Mon Feb 08 17:06:55 2021

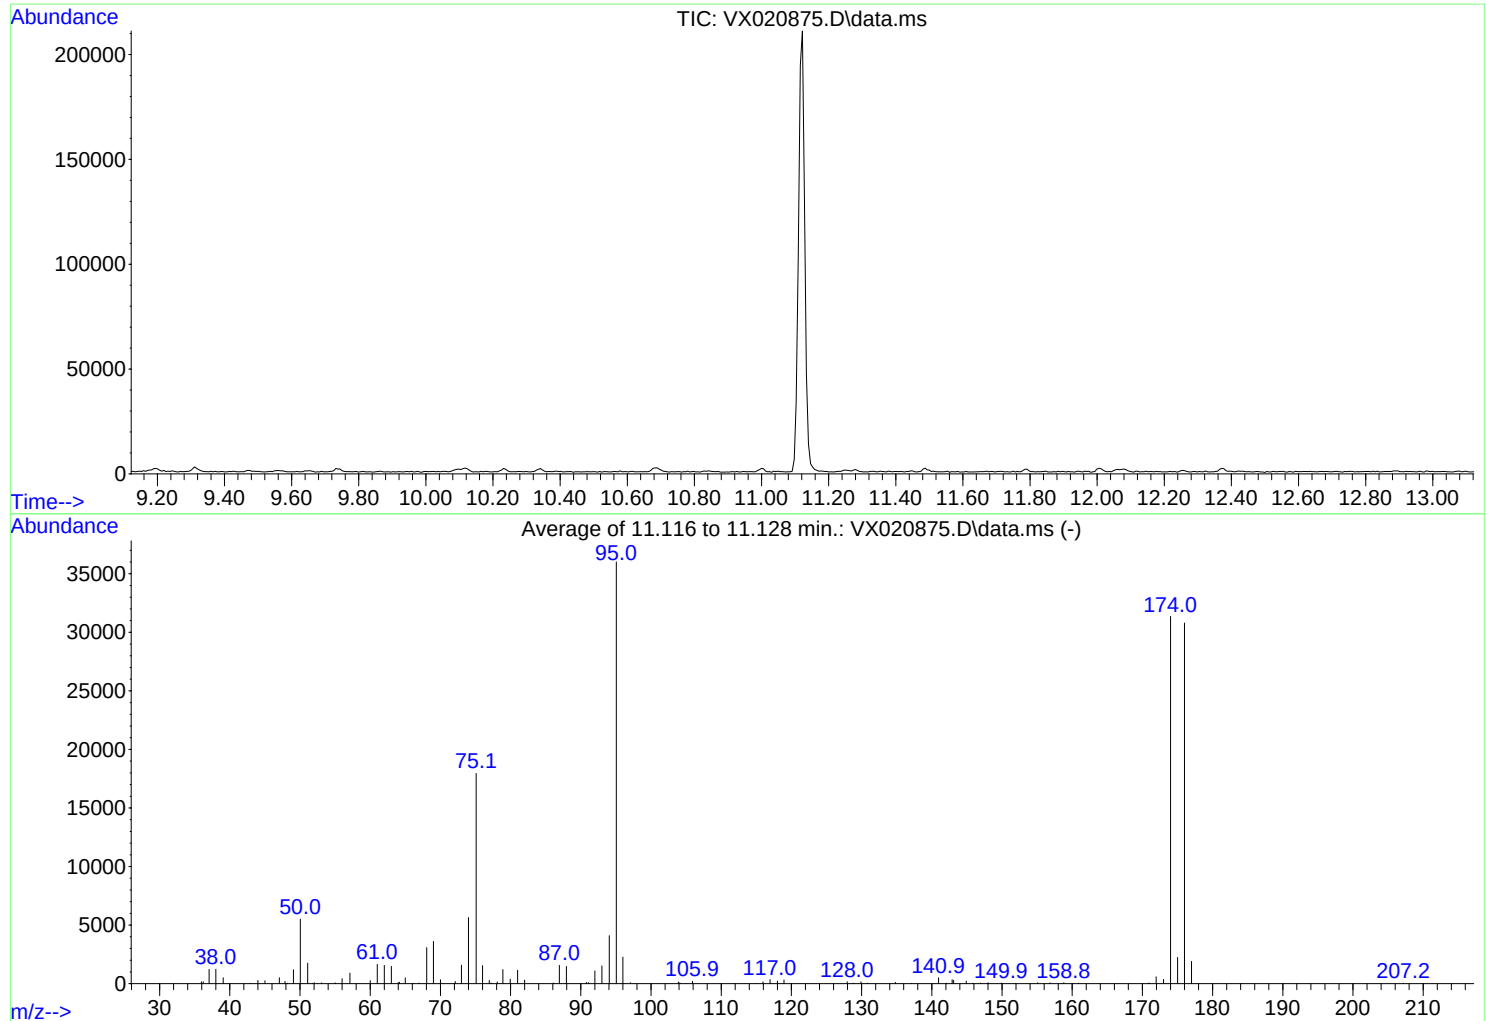

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1639

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	5501	PASS
75	95	30	80	49.8	17955	PASS
95	95	100	100	100.0	36019	PASS
96	95	5	9	6.3	2275	PASS
173	174	0.00	2	1.2	361	PASS
174	95	50	120	87.0	31352	PASS
175	174	5	9	7.2	2246	PASS
176	174	95	101	98.2	30792	PASS
177	176	5	9	6.2	1904	PASS

m/z	Abundance
36.00	349.0
37.10	1510.0
38.00	1454.0
39.10	695.0
40.00	446.0
44.00	724.0
45.00	280.0
47.10	782.0
47.80	283.0
49.00	1711.0
50.10	6718.0
51.10	2213.0
52.10	163.0
53.10	98.0
55.00	115.0
55.90	443.0
57.10	1205.0
58.30	58.0
60.00	305.0
61.00	1763.0
62.00	1824.0
63.00	1864.0
64.00	297.0
64.90	580.0
68.10	3587.0
69.00	4047.0
70.00	352.0
72.10	212.0
73.00	1620.0
74.00	6866.0
75.10	20760.0
76.00	2069.0
77.00	352.0
78.10	254.0
78.80	1256.0
79.90	458.0
81.00	1334.0
82.00	293.0
86.90	1808.0
88.00	1908.0
90.80	138.0
91.20	153.0
92.10	1471.0
93.00	1877.0
94.00	4298.0
95.00	41544.0
96.00	2694.0
97.10	101.0
103.90	216.0
105.00	62.0
105.90	260.0
115.90	128.0
117.00	366.0
118.00	264.0
119.00	324.0
127.90	158.0
129.90	162.0
130.80	51.0
134.90	104.0
137.10	81.0
141.00	592.0
142.10	53.0
142.90	615.0
144.90	288.0
145.90	73.0
146.90	93.0
147.90	142.0
149.90	98.0
155.10	62.0
156.90	87.0
158.80	101.0
170.80	100.0
171.90	514.0
173.00	401.0
174.00	29144.0
175.00	2249.0
176.00	30680.0
177.00	1956.0

Instrument :
MSVOA_X
ClientSampleId :
BFB66

m/z	Abundance
36.20	407.0
37.00	1342.0
38.00	1431.0
39.00	537.0
40.00	477.0
42.90	70.0
44.10	884.0
45.00	374.0
47.00	423.0
47.90	193.0
49.10	1162.0
50.00	6405.0
51.10	1933.0
52.00	93.0
53.00	96.0
55.00	103.0
56.00	400.0
57.10	1017.0
60.10	274.0
61.00	2017.0
62.00	1875.0
63.00	1534.0
64.20	271.0
65.00	577.0
66.10	74.0
67.00	121.0
68.00	3617.0
69.00	4085.0
70.00	405.0
72.10	219.0
73.00	2037.0
74.00	6554.0
75.10	21176.0
76.00	1617.0
76.90	454.0
78.10	121.0
78.90	1527.0
80.00	448.0
81.00	1375.0
82.00	435.0
86.20	106.0
86.90	1656.0
88.00	1664.0
90.80	187.0
92.00	1186.0
93.00	1643.0
94.10	5450.0
95.10	41784.0
96.00	2671.0
97.00	89.0
103.90	211.0
105.90	258.0
115.00	63.0
116.00	165.0
116.90	450.0
118.00	322.0
119.00	327.0
128.00	159.0
128.80	112.0
129.90	156.0
130.90	67.0
134.80	157.0
140.90	515.0
142.10	60.0
143.10	870.0
144.90	213.0
145.80	70.0
147.00	63.0
148.10	95.0
149.90	72.0
151.90	63.0
155.10	109.0
156.80	53.0
158.80	99.0
160.90	54.0
171.00	120.0
171.90	717.0
173.00	325.0
174.00	39264.0
175.00	2856.0
176.00	36272.0
177.00	2291.0

Instrument :
MSVOA_X
ClientSampleId :
BFB66

m/z	Abundance
35.80	121.0
36.20	104.0
37.00	805.0
38.00	821.0
39.00	307.0
39.90	356.0
44.00	883.0
45.00	93.0
47.00	325.0
47.90	120.0
48.20	118.0
49.10	692.0
50.00	3381.0
51.00	1105.0
51.80	79.0
56.10	439.0
57.10	488.0
59.90	212.0
61.00	1148.0
62.00	966.0
63.00	1018.0
64.10	101.0
65.10	335.0
66.90	61.0
68.00	2030.0
69.10	2698.0
70.00	226.0
72.10	152.0
73.10	1074.0
74.10	3504.0
75.10	11929.0
76.00	946.0
77.20	161.0
78.10	96.0
79.00	830.0
80.00	247.0
80.90	757.0
82.00	193.0
86.10	75.0
87.00	1225.0
87.80	833.0
91.00	102.0
91.90	623.0
93.00	1036.0
94.10	2561.0
95.00	24728.0
96.10	1461.0
97.00	75.0
104.10	187.0
105.80	101.0
115.90	148.0
116.90	221.0
118.00	61.0
118.90	285.0
127.90	195.0
129.90	174.0
134.70	66.0
140.90	412.0
142.90	407.0
144.80	149.0
148.00	106.0
155.10	81.0
156.80	71.0
158.80	62.0
160.90	70.0
170.90	59.0
172.00	554.0
173.00	358.0
174.00	25648.0
175.10	1634.0
176.00	25424.0
177.00	1465.0
207.20	85.0

Instrument :
MSVOA_X
ClientSampleId :
BFB66

m/z	Abundance
40.00	478.0
44.00	558.0

Instrument :
MSVOA_X
ClientSampleId :
BFB66