

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX020822\  
Data File : VX026844.D  
Acq On : 09 Feb 2022 00:29  
Operator : JC/MD  
Sample : N1425-05 50X  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 37 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
20722

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X020822W.M

Title : SW846 8260

Signal : TIC: VX026844.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.459       | 57            | 61          | 67           | rBV      | 10812          | 12145         | 1.80%           | 0.338%        |
| 2         | 5.391       | 695           | 706         | 720          | rBV      | 77991          | 224305        | 33.16%          | 6.244%        |
| 3         | 5.556       | 722           | 733         | 748          | rVB      | 137620         | 390023        | 57.65%          | 10.857%       |
| 4         | 5.958       | 788           | 799         | 812          | rBV      | 85312          | 228089        | 33.72%          | 6.349%        |
| 5         | 6.763       | 921           | 931         | 945          | rBV      | 213381         | 511286        | 75.58%          | 14.232%       |
| 6         | 8.653       | 1234          | 1241        | 1250         | rBV      | 431188         | 676514        | 100.00%         | 18.831%       |
| 7         | 10.055      | 1465          | 1471        | 1488         | rBV      | 442533         | 587449        | 86.83%          | 16.352%       |
| 8         | 11.079      | 1634          | 1639        | 1652         | rBV      | 326667         | 430254        | 63.60%          | 11.977%       |
| 9         | 11.573      | 1711          | 1720        | 1725         | rBV      | 9254           | 11838         | 1.75%           | 0.330%        |
| 10        | 12.024      | 1788          | 1794        | 1802         | rBV      | 408765         | 511812        | 75.65%          | 14.247%       |
| 11        | 13.140      | 1973          | 1977        | 1985         | rBV2     | 5545           | 8745          | 1.29%           | 0.243%        |




Sum of corrected areas: 3592460

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX020822\  
Data File : VX026844.D  
Acq On : 09 Feb 2022 00:29  
Operator : JC/MD  
Sample : N1425-05 50X  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 37 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
20722

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X020822W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

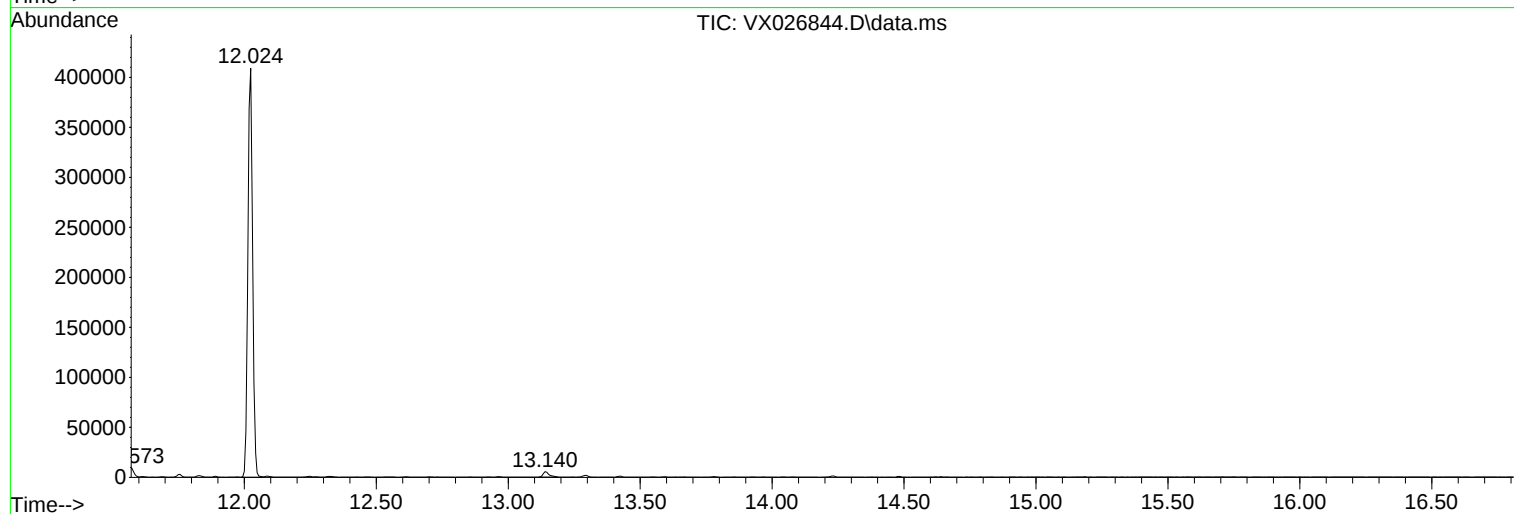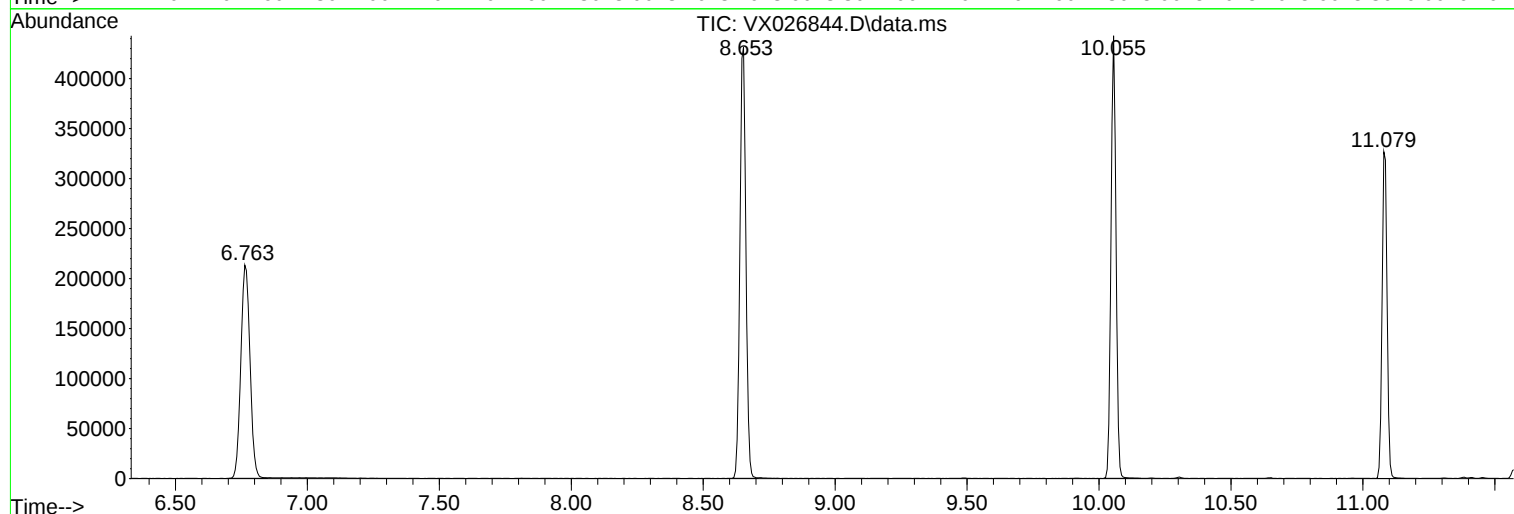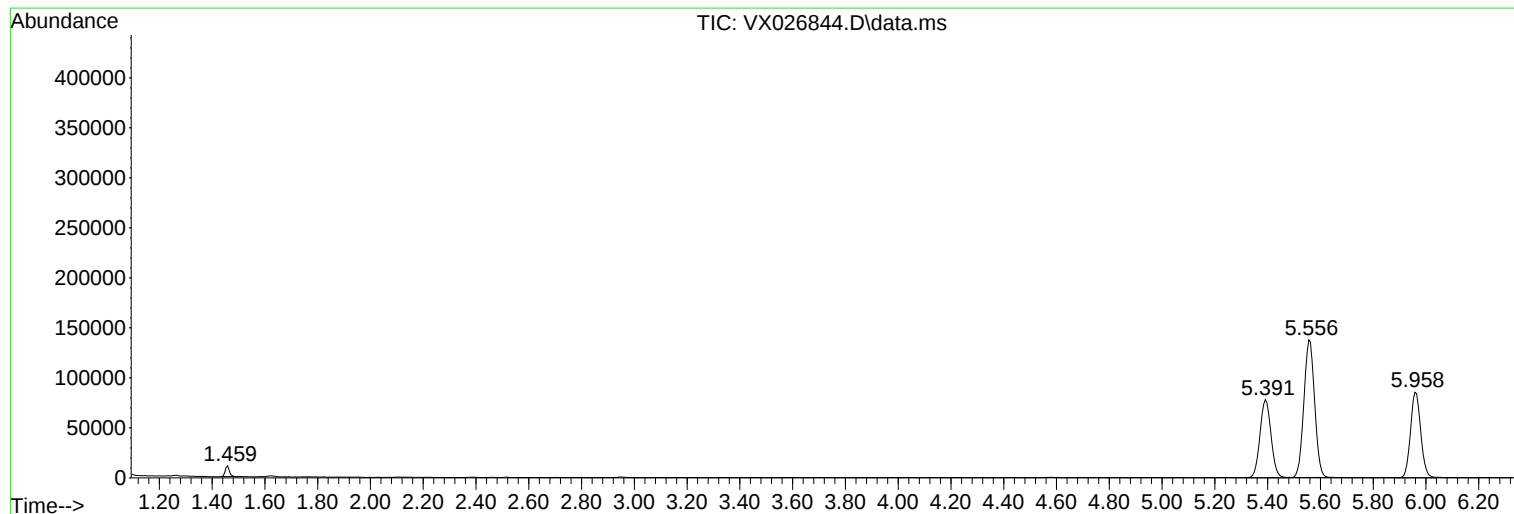

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX020822\  
Data File : VX026844.D  
Acq On : 09 Feb 2022 00:29  
Operator : JC/MD  
Sample : N1425-05 50X  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 37 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
20722

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X020822W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX020822\  
Data File : VX026844.D  
Acq On : 09 Feb 2022 00:29  
Operator : JC/MD  
Sample : N1425-05 50X  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 37 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
20722

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X020822W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |