

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020822\
 Data File : VX026845.D
 Acq On : 09 Feb 2022 00:52
 Operator : JC/MD
 Sample : N1425-07 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 31380

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
 Title : SW846 8260

Signal : TIC: VX026845.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.391	694	706	722	rBV	81706	236853	33.25%	5.688%
2	5.556	722	733	749	rVB	146992	410690	57.66%	9.862%
3	5.958	787	799	818	rBV	89515	240694	33.79%	5.780%
4	6.763	921	931	947	rBV	225200	537195	75.42%	12.900%
5	8.653	1234	1241	1248	rBV	454764	712240	100.00%	17.104%
6	8.720	1248	1252	1261	rVB	6950	11084	1.56%	0.266%
7	10.055	1465	1471	1490	rBV	461413	612528	86.00%	14.709%
8	10.195	1490	1494	1500	rVB	13021	16353	2.30%	0.393%
9	10.299	1506	1511	1518	rBV	44849	61640	8.65%	1.480%
10	10.640	1562	1567	1575	rBV	28462	37661	5.29%	0.904%
11	11.079	1634	1639	1654	rVB	351185	443501	62.27%	10.650%
12	11.305	1672	1676	1682	rBV	6183	7706	1.08%	0.185%
13	11.378	1683	1688	1696	rVV	26178	45701	6.42%	1.097%
14	11.451	1696	1700	1708	rVB	12178	14957	2.10%	0.359%
15	11.616	1722	1727	1732	rVB	15024	17718	2.49%	0.425%
16	11.750	1744	1749	1755	rBV	49315	61203	8.59%	1.470%
17	12.024	1788	1794	1800	rBV	429281	526611	73.94%	12.646%
18	12.091	1800	1805	1809	rVB	19640	25038	3.52%	0.601%
19	12.244	1825	1830	1833	rBV	19563	25525	3.58%	0.613%
20	12.317	1838	1842	1849	rVB3	7509	11674	1.64%	0.280%
21	12.615	1887	1891	1894	rBV	6054	7156	1.00%	0.172%
22	12.701	1901	1905	1916	rVB2	7000	9806	1.38%	0.235%
23	13.170	1978	1982	1986	rVB	9261	12485	1.75%	0.300%
24	13.292	1998	2002	2011	rVB2	22234	29710	4.17%	0.713%
25	13.420	2019	2023	2029	rVB	19165	24171	3.39%	0.580%
26	14.231	2149	2156	2160	rBV2	10450	15972	2.24%	0.384%
27	14.481	2193	2197	2202	rVB2	6901	8350	1.17%	0.201%




Sum of corrected areas: 4164222

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020822\
Data File : VX026845.D
Acq On : 09 Feb 2022 00:52
Operator : JC/MD
Sample : N1425-07 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
31380

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

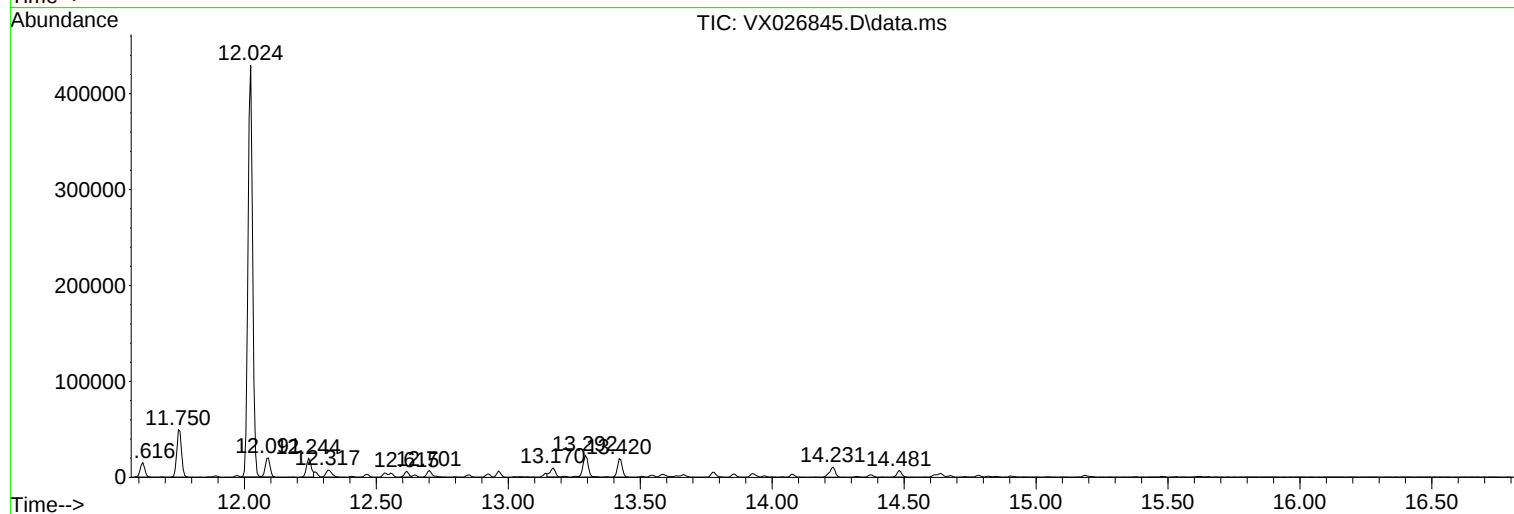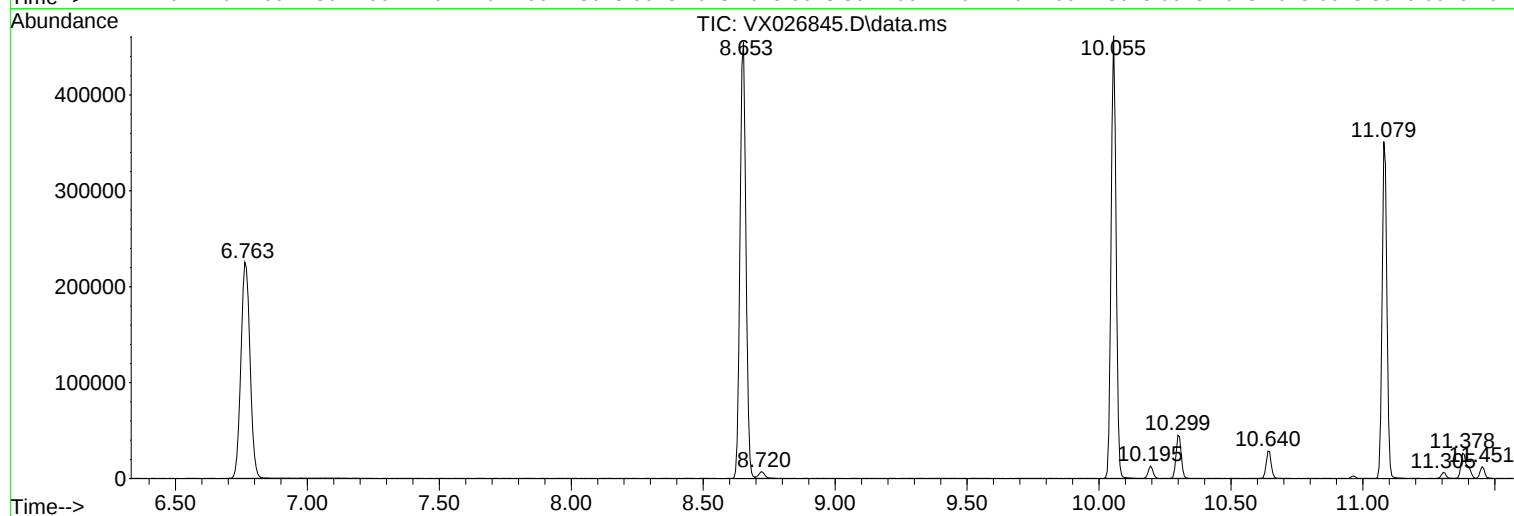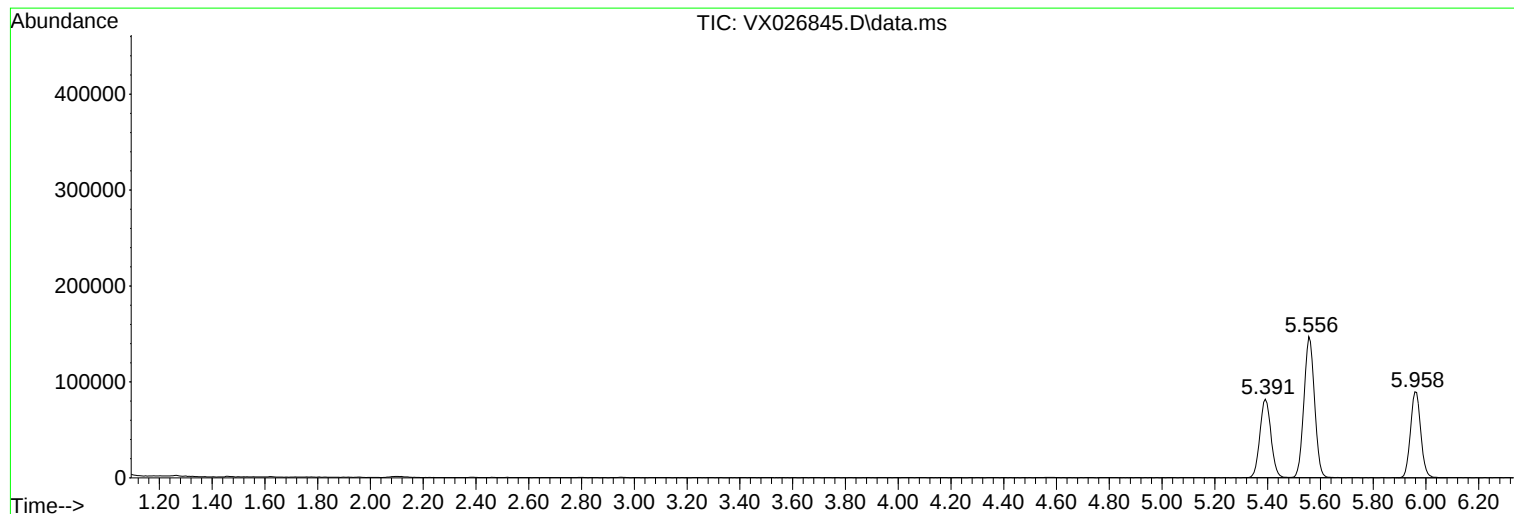

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020822\
Data File : VX026845.D
Acq On : 09 Feb 2022 00:52
Operator : JC/MD
Sample : N1425-07 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
31380

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020822\
Data File : VX026845.D
Acq On : 09 Feb 2022 00:52
Operator : JC/MD
Sample : N1425-07 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
31380

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------